

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
 Data File : BP014622.D
 Acq On : 08 Apr 2023 01:09
 Operator : CG/JU
 Sample : 02225-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Quant Time: Apr 08 01:47:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 00:45:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	135694	20.000	ng/u1	0.00
20) Naphthalene-d8	10.799	136	616289	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.634	164	416797	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.392	188	902774	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	657211	20.000	ng/u1	0.00
88) Perylene-d12	23.980	264	666494	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	22930	6.553	ng/uL	0.00
4) Pyridine-d5	3.793	84	294272	32.817	ng/u1	0.00
7) Phenol-d5	7.146	99	420718	33.619	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	302551	37.681	ng/u1	0.00
11) 2-Chlorophenol-d4	7.505	132	313099	34.616	ng/u1	0.00
15) 4-Methylphenol-d8	8.699	113	366304	36.288	ng/u1	0.00
21) Nitrobenzene-d5	9.158	128	167559	33.679	ng/u1	0.00
24) 2-Nitrophenol-d4	9.881	143	192689	33.823	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	320799	30.920	ng/u1	0.00
31) 4-Chloroaniline-d4	10.946	131	463072	33.884	ng/u1	0.00
46) Dimethylphthalate-d6	14.040	166	1244308	36.820	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	1322784	35.275	ng/u1	0.00
54) 4-Nitrophenol-d4	14.863	143	127966	25.065	ng/u1	0.00
60) Fluorene-d10	15.628	176	1030456	36.564	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	198913	29.944	ng/u1	0.00
73) Anthracene-d10	17.492	188	1617890	37.031	ng/u1	0.00
81) Pyrene-d10	19.722	212	1761798	39.910	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.816	264	1336117	37.732	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.399	88	14997	3.900 ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014622.D
Acq On : 08 Apr 2023 01:09
Operator : CG/JU
Sample : 02225-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0


Quant Time: Apr 08 01:47:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

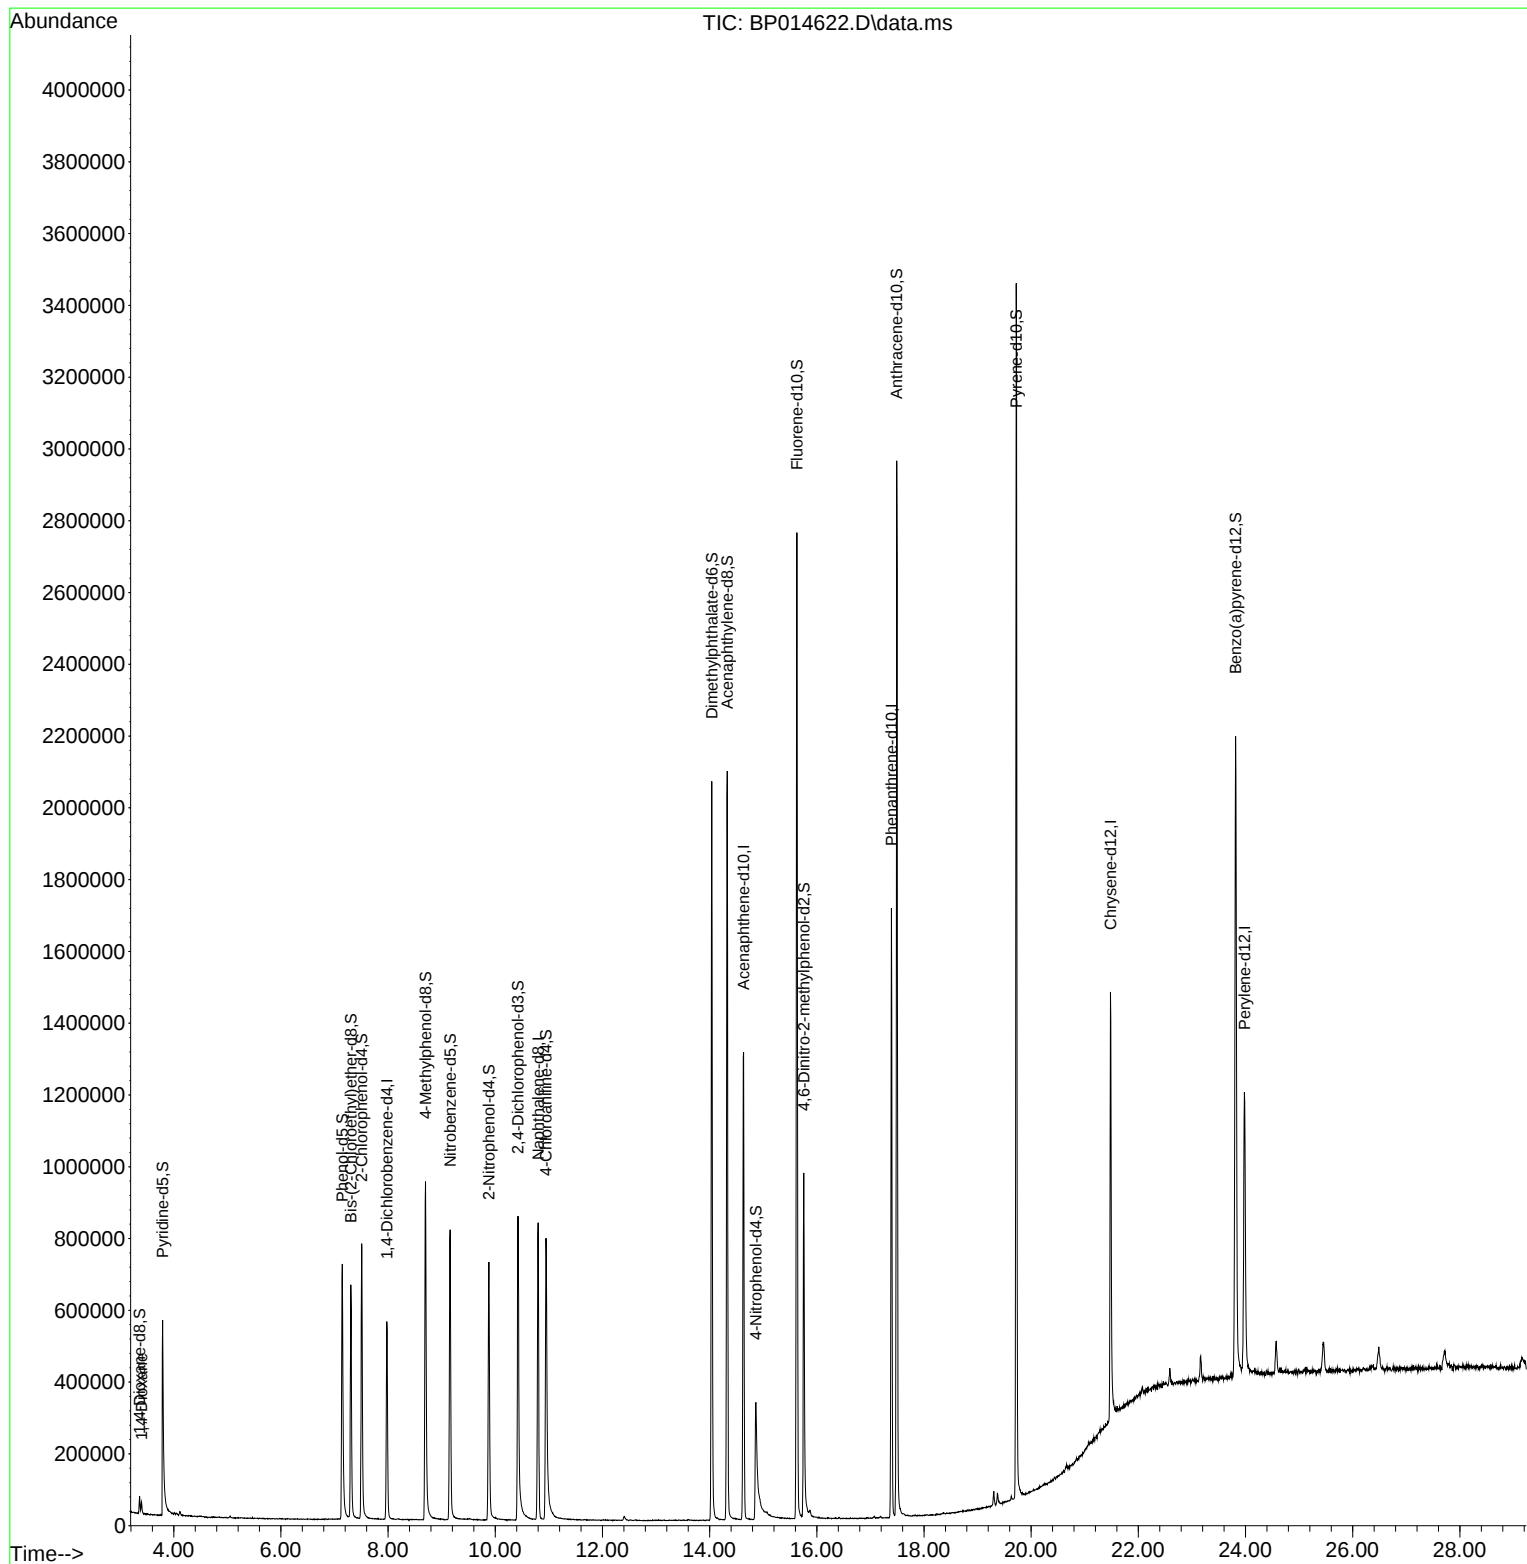

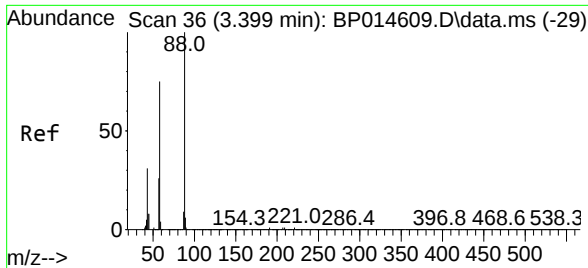

#2
 1,4-Dioxane
 Concen: 3.900 ng/uL
 RT: 3.399 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: BP014622.D
 Acq: 08 Apr 2023 01:09

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

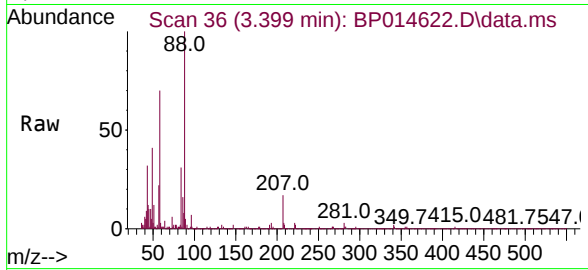

Tgt Ion:	88	Resp:	14997
Ion	Ratio	Lower	Upper
88	100		
43	31.9	24.4	36.6
58	69.7	57.4	86.0

