

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
 Data File : BP014619.D
 Acq On : 07 Apr 2023 23:28
 Operator : CG/JU
 Sample : 02225-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	20	24	27	rBV	46657	63384	1.30%	0.159%
2	3.364	27	30	33	rVV	37722	46825	0.96%	0.118%
3	3.399	33	36	44	rVB	61998	76490	1.57%	0.192%
4	4.016	136	141	145	rVB3	8926	14013	0.29%	0.035%
5	4.116	154	158	166	rVB3	10602	18477	0.38%	0.046%
6	4.646	244	248	254	rBV9	6319	14442	0.30%	0.036%
7	5.046	314	316	320	rVB4	4524	5509	0.11%	0.014%
8	5.387	370	374	380	rVB3	9887	16011	0.33%	0.040%
9	6.358	537	539	545	rVB7	3285	5032	0.10%	0.013%
10	7.152	666	674	686	rBV2	93286	216065	4.44%	0.543%
11	7.305	694	700	718	rBV	541725	870424	17.88%	2.187%
12	7.510	727	735	750	rBV	484542	881574	18.11%	2.215%
13	7.663	760	761	768	rVB7	2656	5442	0.11%	0.014%
14	7.975	807	814	826	rBV	508650	852355	17.51%	2.142%
15	8.087	831	833	839	rVB7	3441	5025	0.10%	0.013%
16	8.699	930	937	955	rBV	320053	647429	13.30%	1.627%
17	9.157	1008	1015	1038	rBV	648874	1155528	23.74%	2.904%
18	9.522	1072	1077	1086	rVB4	8237	13572	0.28%	0.034%
19	9.881	1129	1138	1157	rBV	537055	975407	20.04%	2.451%
20	10.428	1224	1231	1254	rBV	541702	1245657	25.59%	3.130%
21	10.798	1286	1294	1306	rVB	720180	1228239	25.23%	3.086%
22	10.957	1315	1321	1336	rBV	159888	414337	8.51%	1.041%
23	12.022	1496	1502	1507	rVB6	6212	10849	0.22%	0.027%
24	12.204	1528	1533	1539	rVB9	5616	11152	0.23%	0.028%
25	12.404	1559	1567	1575	rBV6	10150	26049	0.54%	0.065%
26	13.357	1722	1729	1734	rVB6	3526	7177	0.15%	0.018%
27	13.428	1734	1741	1748	rBV5	9520	17376	0.36%	0.044%
28	13.610	1770	1772	1779	rVB8	3322	5445	0.11%	0.014%
29	14.039	1836	1845	1858	rBV	1558613	2228984	45.79%	5.601%
30	14.328	1884	1894	1907	rBV	1716241	2529283	51.96%	6.356%
31	14.510	1921	1925	1929	rVB5	7918	10272	0.21%	0.026%
32	14.634	1939	1946	1960	rBV	1096378	1646197	33.82%	4.137%
33	14.916	1989	1994	1995	rBV3	18901	26650	0.55%	0.067%
34	15.381	2068	2073	2082	rVB3	11260	24445	0.50%	0.061%
35	15.457	2082	2086	2090	rVB6	10792	14042	0.29%	0.035%
36	15.628	2108	2115	2129	rBV	2224424	3231574	66.39%	8.120%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
 Data File : BP014619.D
 Acq On : 07 Apr 2023 23:28
 Operator : CG/JU
 Sample : 02225-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.757	2131	2137	2152	rVV	715673	1205583	24.77%	3.029%
38	15.869	2154	2156	2164	rVB6	16848	26369	0.54%	0.066%
39	15.998	2173	2178	2190	rVB	68051	116922	2.40%	0.294%
40	16.322	2230	2233	2237	rBV4	7727	11074	0.23%	0.028%
41	17.069	2357	2360	2363	rVB5	4073	5616	0.12%	0.014%
42	17.128	2366	2370	2375	rVV5	6563	7895	0.16%	0.020%
43	17.392	2409	2415	2426	rBV	1410399	1955722	40.18%	4.914%
44	17.492	2426	2432	2446	rBV	2535798	3697504	75.96%	9.291%
45	17.663	2459	2461	2467	rVB5	6987	12520	0.26%	0.031%
46	18.039	2524	2525	2529	rVB4	6566	6332	0.13%	0.016%
47	18.269	2559	2564	2572	rBV2	51736	101717	2.09%	0.256%
48	18.333	2573	2575	2580	rVB2	8426	11870	0.24%	0.030%
49	18.663	2629	2631	2635	rVB5	4836	4938	0.10%	0.012%
50	19.304	2736	2740	2746	rBV	37558	50133	1.03%	0.126%
51	19.369	2748	2751	2760	rVV2	27501	53709	1.10%	0.135%
52	19.498	2770	2773	2780	rBV8	21824	47537	0.98%	0.119%
53	19.722	2805	2811	2827	rBV	3153067	4430061	91.01%	11.132%
54	21.169	3054	3057	3065	rVB3	80741	154458	3.17%	0.388%
55	21.480	3105	3110	3121	rBV	1342096	2129153	43.74%	5.350%
56	23.821	3500	3508	3521	rBV	2388295	4867754	100.00%	12.232%
57	23.986	3529	3536	3549	rVB	1084891	2337701	48.02%	5.874%




Sum of corrected areas: 39795300

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014619.D
Acq On : 07 Apr 2023 23:28
Operator : CG/JU
Sample : 02225-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

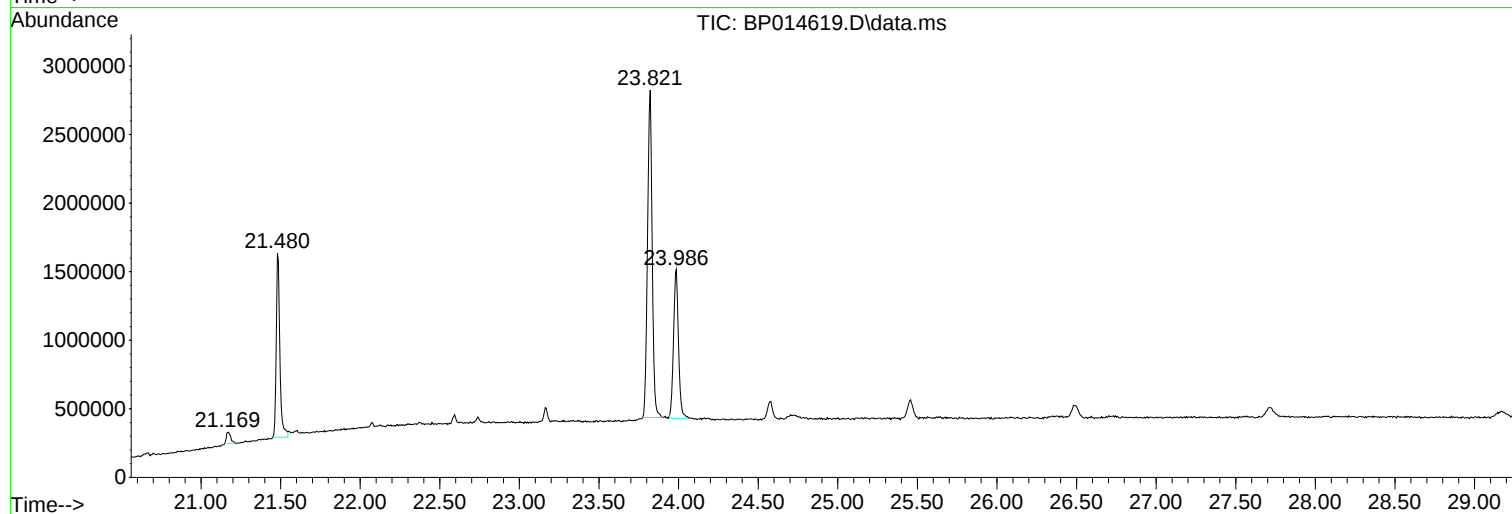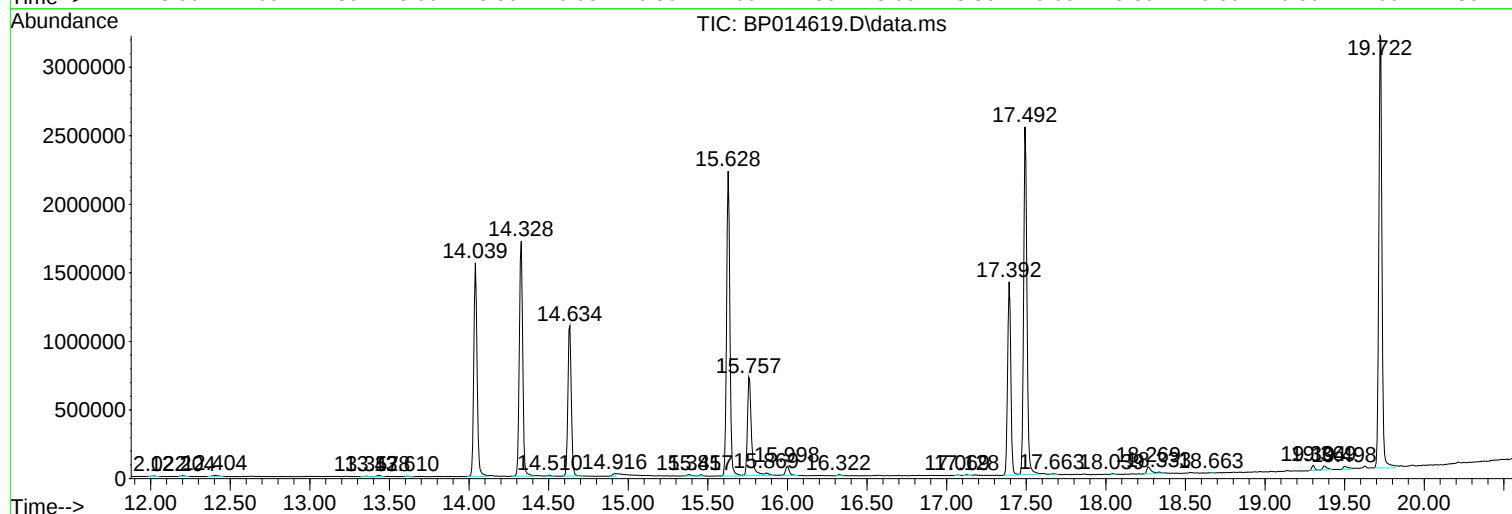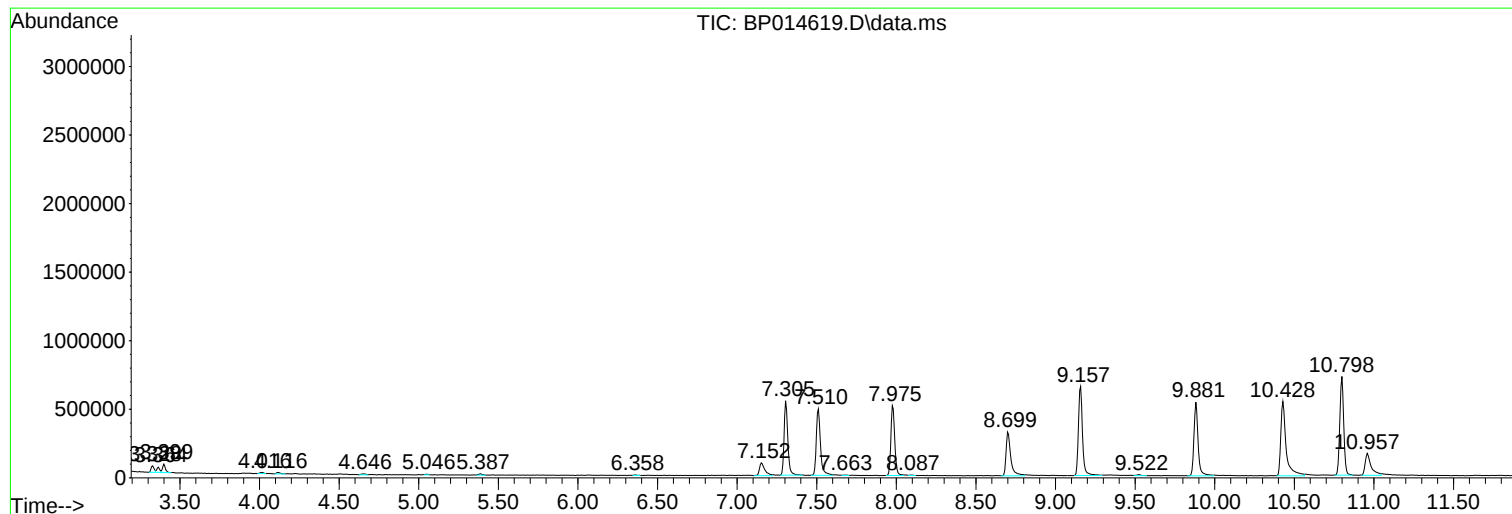

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014619.D
Acq On : 07 Apr 2023 23:28
Operator : CG/JU
Sample : 02225-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014619.D
Acq On : 07 Apr 2023 23:28
Operator : CG/JU
Sample : 02225-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc