

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
 Data File : BP014620.D
 Acq On : 08 Apr 2023 00:02
 Operator : CG/JU
 Sample : 02225-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	26	30	33	rBV	34463	44373	0.98%	0.119%
2	3.399	33	36	42	rVB	22749	33981	0.75%	0.091%
3	4.017	138	141	145	rVB3	5285	7481	0.16%	0.020%
4	4.117	154	158	166	rVB2	10712	15714	0.35%	0.042%
5	5.046	312	316	318	rBV5	6143	7687	0.17%	0.021%
6	6.364	536	540	544	rBV7	3240	5006	0.11%	0.013%
7	7.152	669	674	688	rBV	88899	199032	4.37%	0.533%
8	7.305	694	700	717	rBV	526176	865082	19.01%	2.316%
9	7.511	729	735	751	rBV	476648	866609	19.05%	2.320%
10	7.975	807	814	833	rBV	490470	847341	18.62%	2.269%
11	8.705	931	938	959	rBV	304384	635901	13.98%	1.703%
12	9.158	1008	1015	1033	rBV	630416	1136282	24.97%	3.042%
13	9.516	1074	1076	1083	rVB7	3973	5917	0.13%	0.016%
14	9.881	1131	1138	1157	rBV	525342	958965	21.08%	2.568%
15	10.210	1189	1194	1199	rBV9	3799	7921	0.17%	0.021%
16	10.428	1224	1231	1261	rBV	487710	1232570	27.09%	3.300%
17	10.799	1286	1294	1307	rBV	714185	1206689	26.52%	3.231%
18	10.963	1316	1322	1346	rBV	82841	262280	5.76%	0.702%
19	11.146	1351	1353	1359	rVB7	4078	6410	0.14%	0.017%
20	12.022	1495	1502	1507	rVB9	3771	7711	0.17%	0.021%
21	12.404	1562	1567	1568	rBV4	7917	8981	0.20%	0.024%
22	13.440	1737	1743	1746	rBV8	2703	4641	0.10%	0.012%
23	13.604	1769	1771	1780	rVB9	3040	4879	0.11%	0.013%
24	14.040	1836	1845	1857	rBV	1480914	2074785	45.60%	5.555%
25	14.328	1882	1894	1913	rBV	1534959	2427231	53.35%	6.499%
26	14.634	1939	1946	1960	rBV	1042096	1601323	35.19%	4.287%
27	14.928	1989	1996	2005	rBV	15215	58974	1.30%	0.158%
28	15.410	2071	2078	2081	rBV9	3641	8269	0.18%	0.022%
29	15.628	2108	2115	2131	rBV	2038969	2975453	65.40%	7.967%
30	15.757	2131	2137	2151	rVV	601304	1035481	22.76%	2.772%
31	15.869	2154	2156	2161	rVB4	12201	16267	0.36%	0.044%
32	15.998	2173	2178	2187	rVB2	23704	40437	0.89%	0.108%
33	16.204	2208	2213	2216	rBV7	4122	6880	0.15%	0.018%
34	17.392	2409	2415	2425	rBV	1347911	1910430	41.99%	5.115%
35	17.492	2426	2432	2448	rVV	2278403	3323900	73.05%	8.900%
36	17.757	2472	2477	2483	rBV3	12401	22906	0.50%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014620.D
Acq On : 08 Apr 2023 00:02
Operator : CG/JU
Sample : 02225-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	18.275	2562	2565	2570	rBV7	14897	30536	0.67%	0.082%
38	19.304	2736	2740	2745	rBV2	34847	51159	1.12%	0.137%
39	19.375	2748	2752	2758	rVV	26925	52032	1.14%	0.139%
40	19.598	2787	2790	2793	rBV3	20734	30574	0.67%	0.082%
41	19.722	2805	2811	2826	rBV	2835856	4063943	89.32%	10.881%
42	21.480	3105	3110	3121	rBV2	1375286	2238186	49.19%	5.993%
43	23.816	3500	3507	3518	rBV2	2185894	4549865	100.00%	12.182%
44	23.980	3529	3535	3556	rVB2	1054608	2458685	54.04%	6.583%




Sum of corrected areas: 37348769

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014620.D
Acq On : 08 Apr 2023 00:02
Operator : CG/JU
Sample : 02225-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

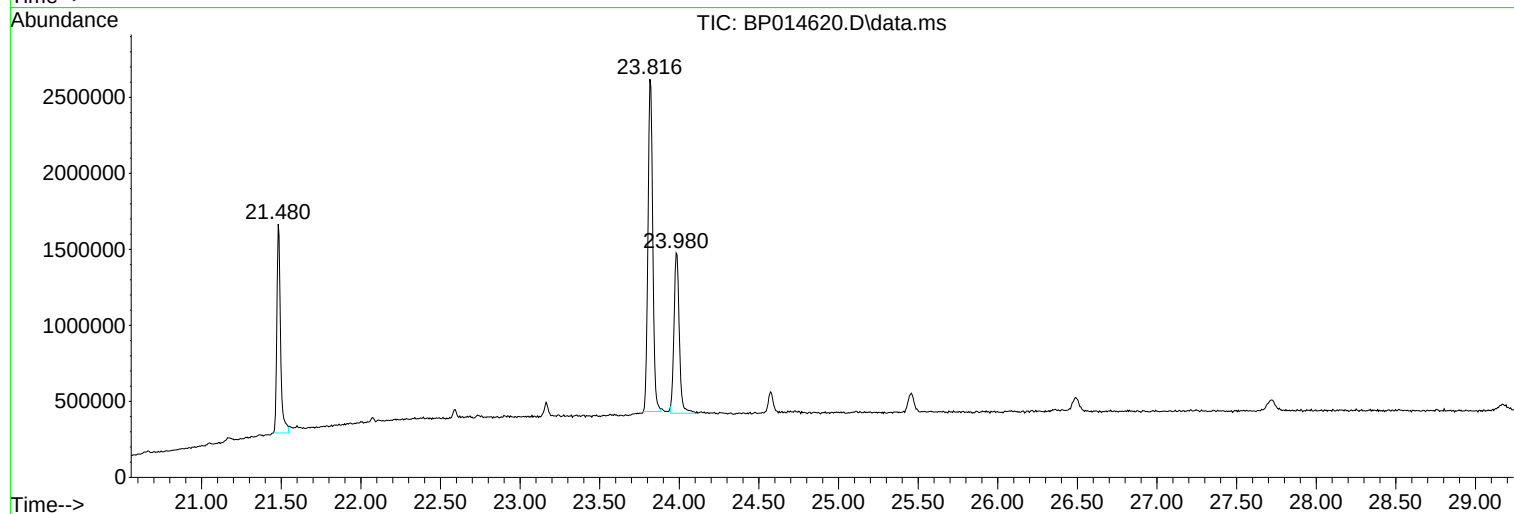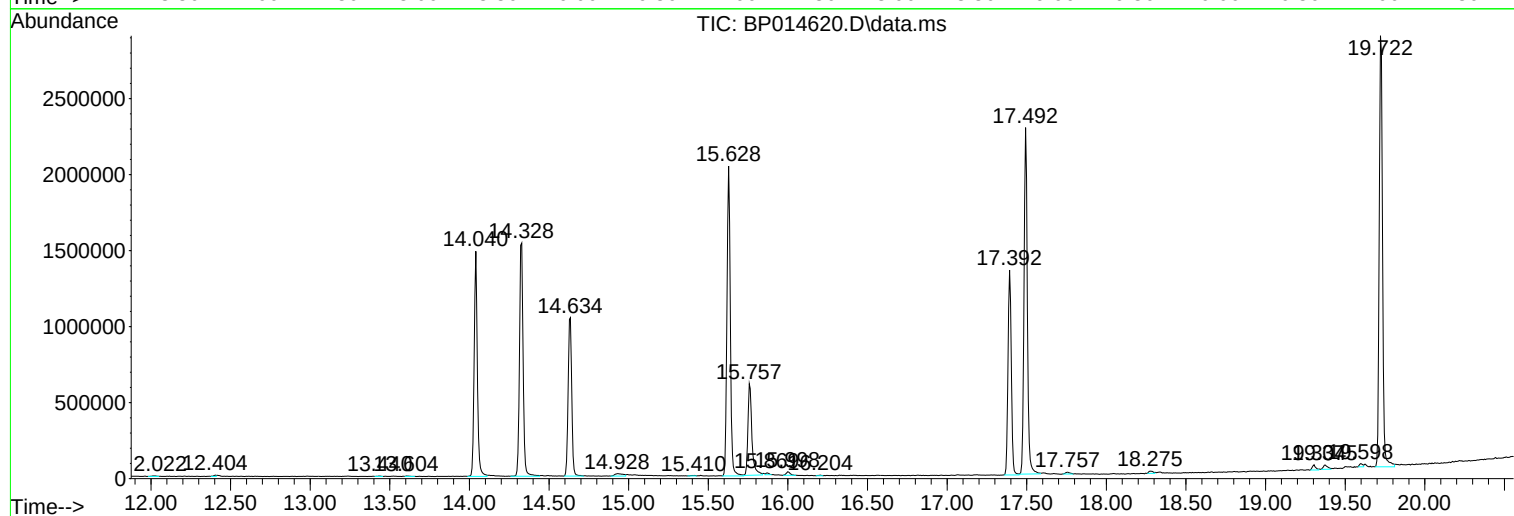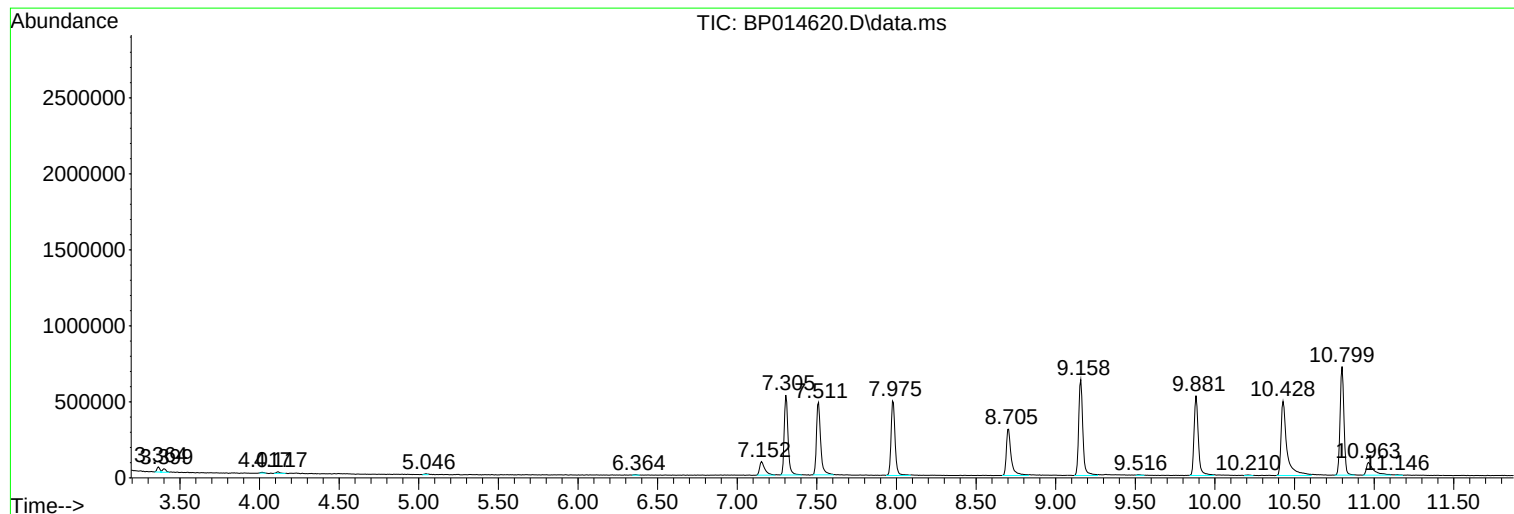

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014620.D
Acq On : 08 Apr 2023 00:02
Operator : CG/JU
Sample : 02225-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014620.D
Acq On : 08 Apr 2023 00:02
Operator : CG/JU
Sample : 02225-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc