




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009721.D
 Acq On : 08 Apr 2022 17:04
 Operator : CG/JU
 Sample : N2182-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

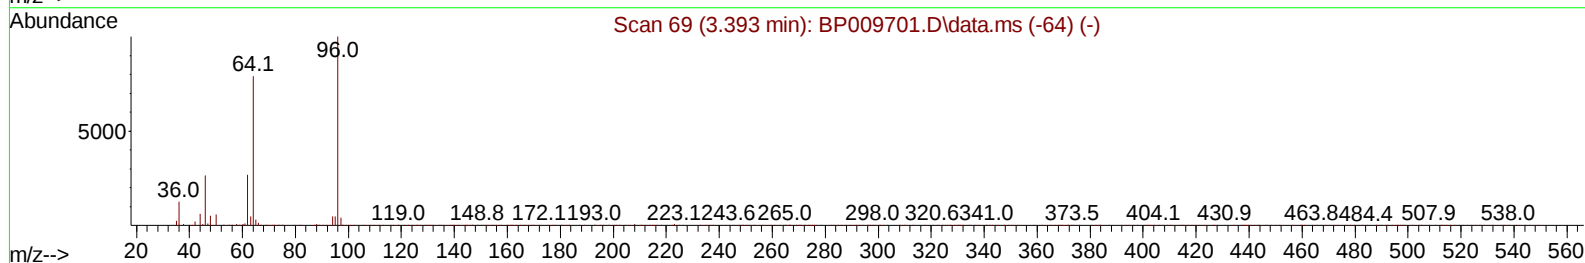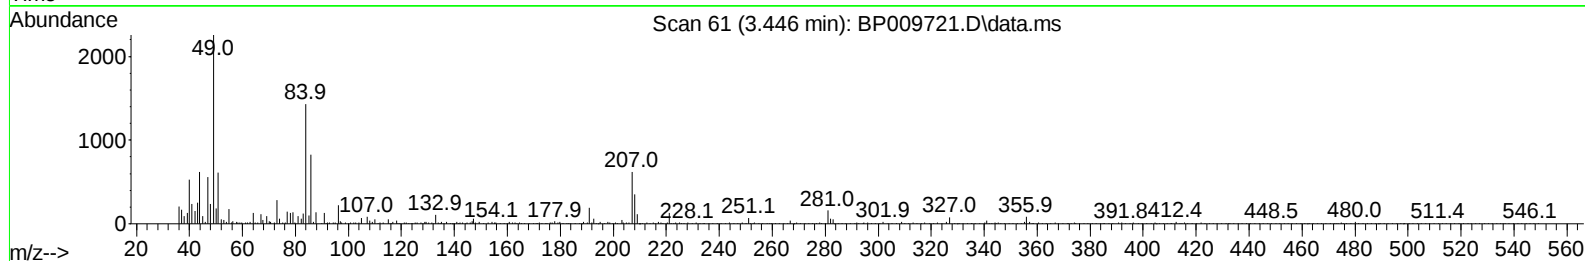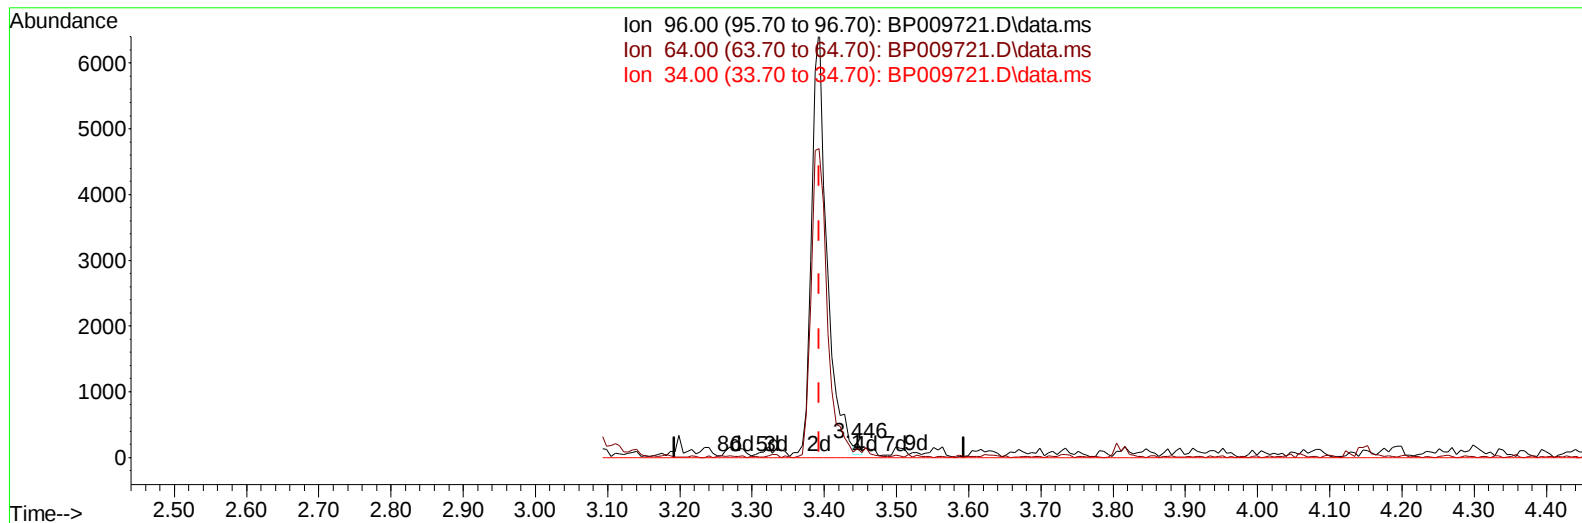

TIC: BP009721.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.446min (+ 0.053) 0.04 ng/uL

response 83

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	58.64
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009721.D
 Acq On : 08 Apr 2022 17:04
 Operator : CG/JU
 Sample : N2182-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

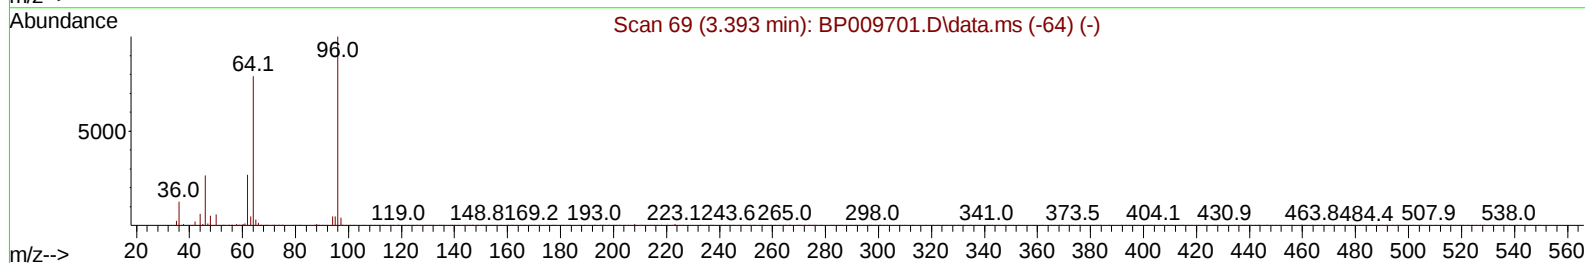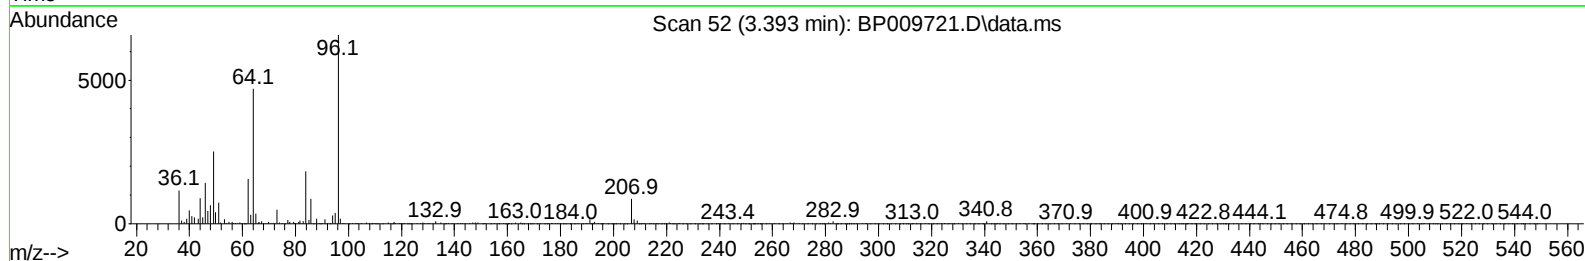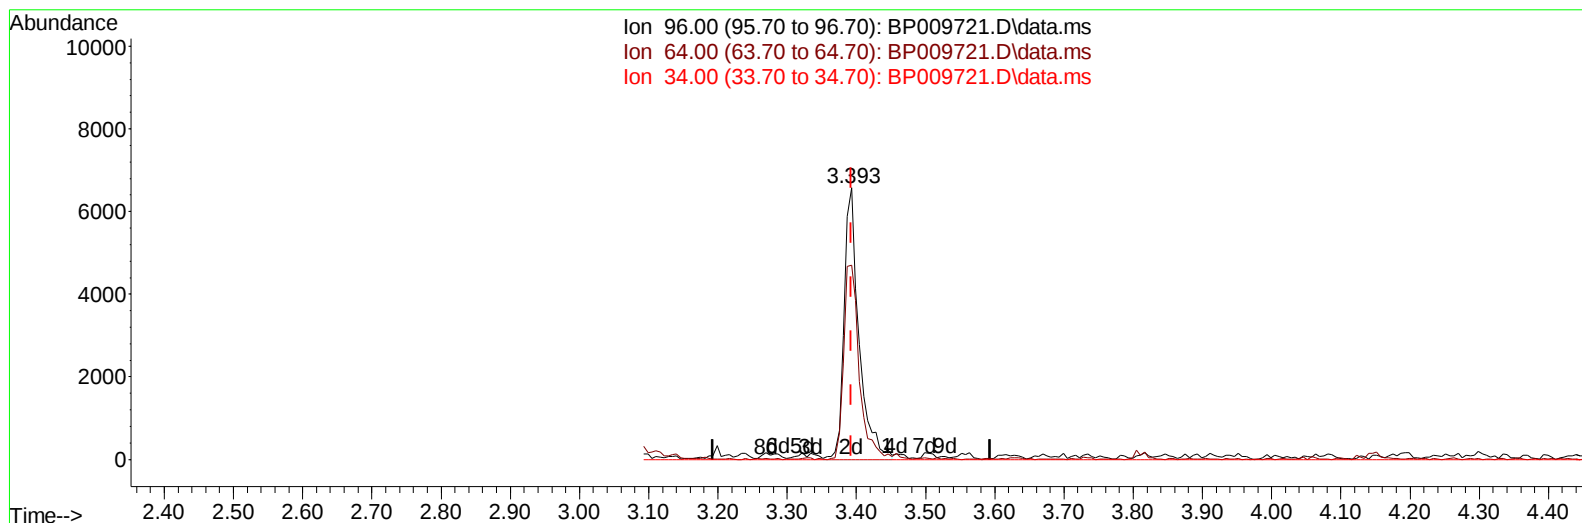

TIC: BP009721.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.393min (-0.000) 5.05 ng/uL m

response 9854

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	71.50#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009721.D
 Acq On : 08 Apr 2022 17:04
 Operator : CG/JU
 Sample : N2182-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

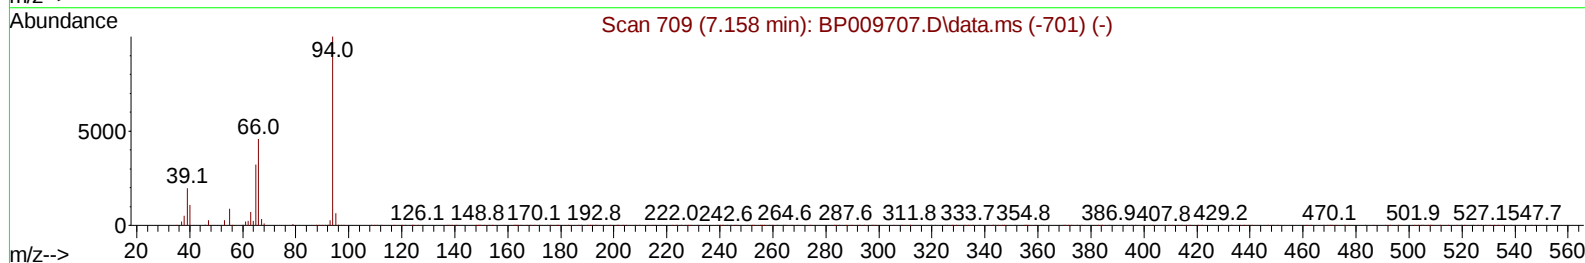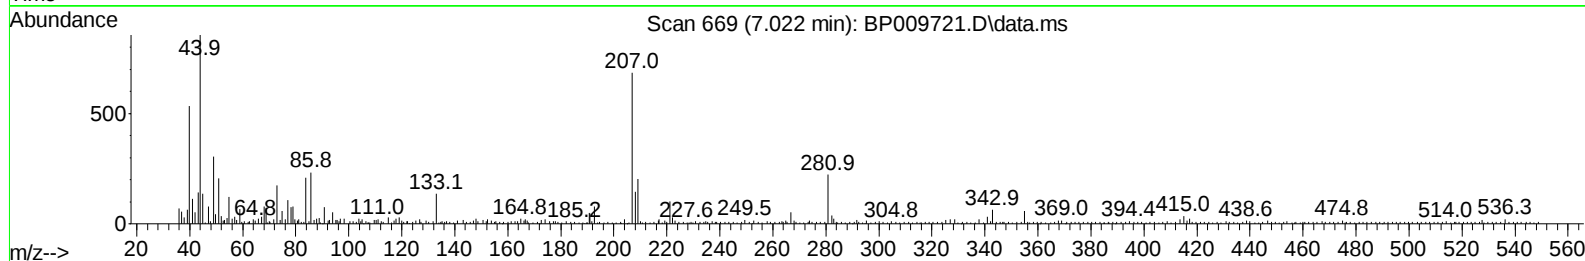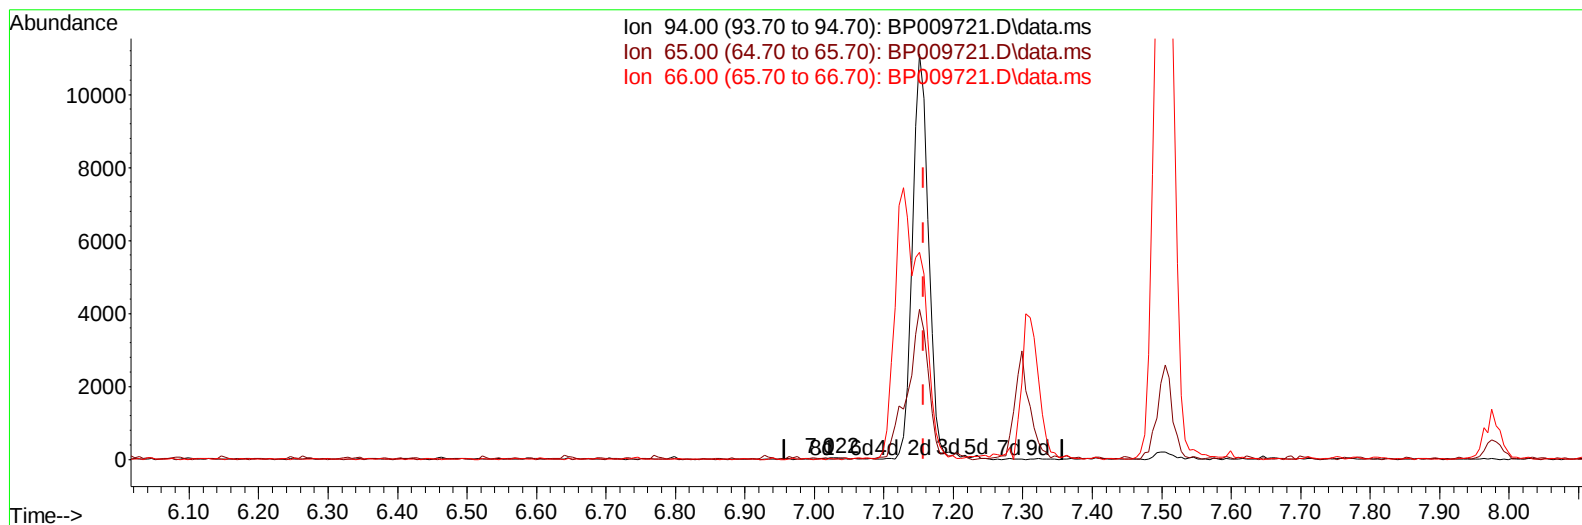

TIC: BP009721.D\data.ms

(8) Phenol

7.022min (-0.135) 0.01 ng/u1

response 61

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	23.80	28.30
66.00	43.20	41.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009721.D
 Acq On : 08 Apr 2022 17:04
 Operator : CG/JU
 Sample : N2182-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

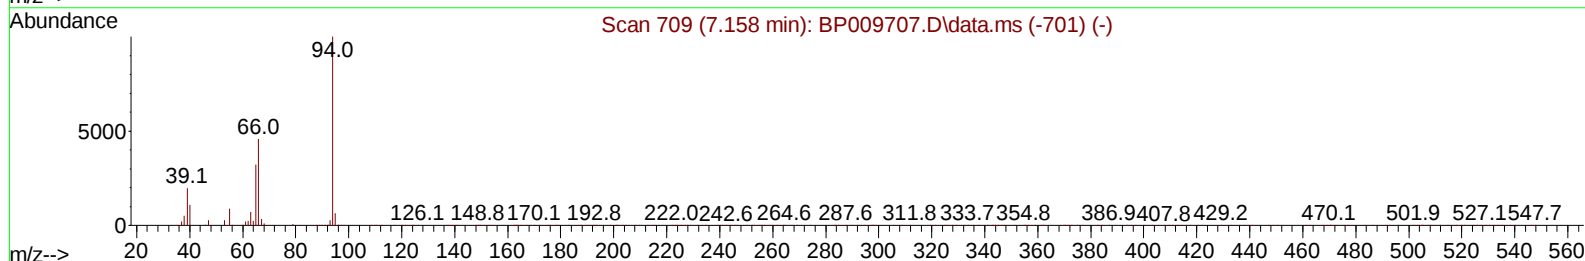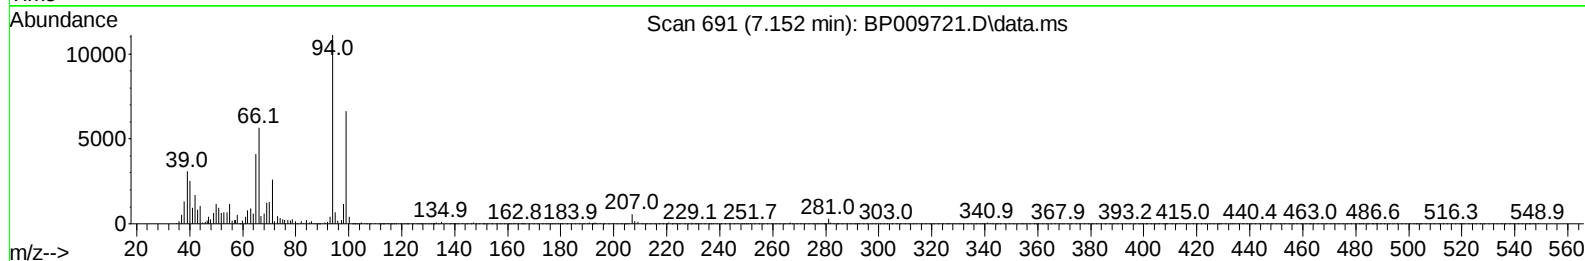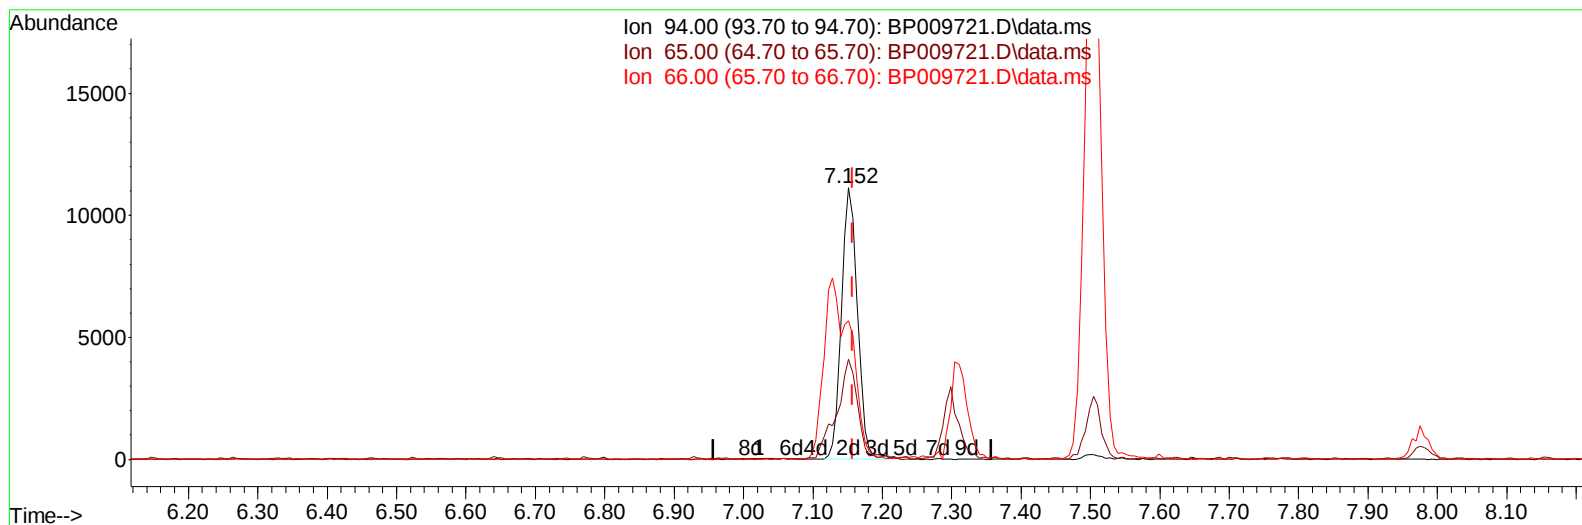

TIC: BP009721.D\data.ms

(8) Phenol

7.152min (-0.006) 2.34 ng/ul m

response 17863

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	23.80	36.93#
66.00	43.20	51.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009721.D
Acq On : 08 Apr 2022 17:04
Operator : CG/JU
Sample : N2182-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 07 19:16:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

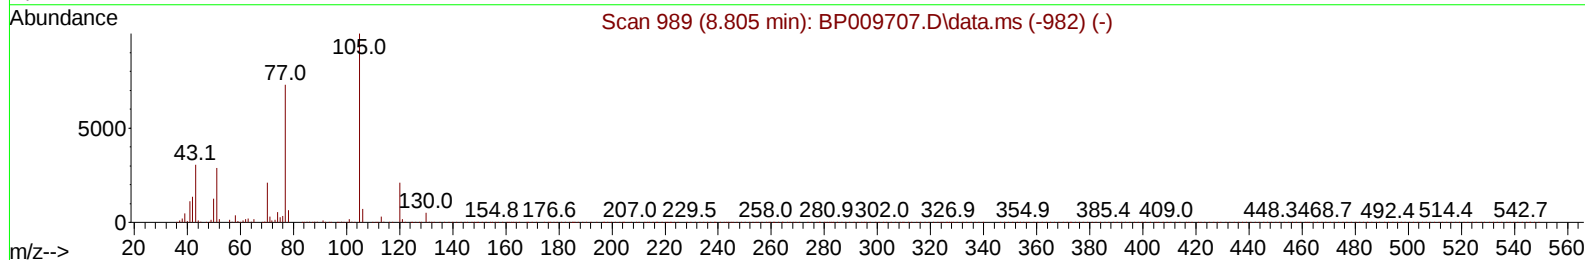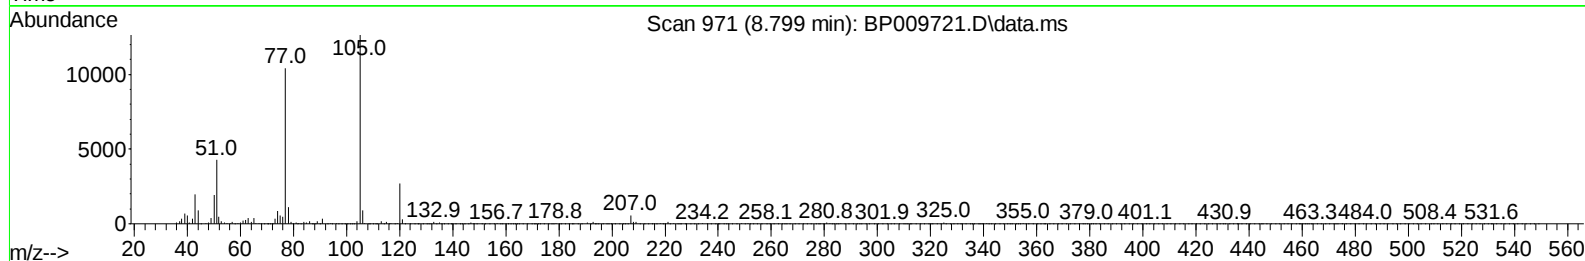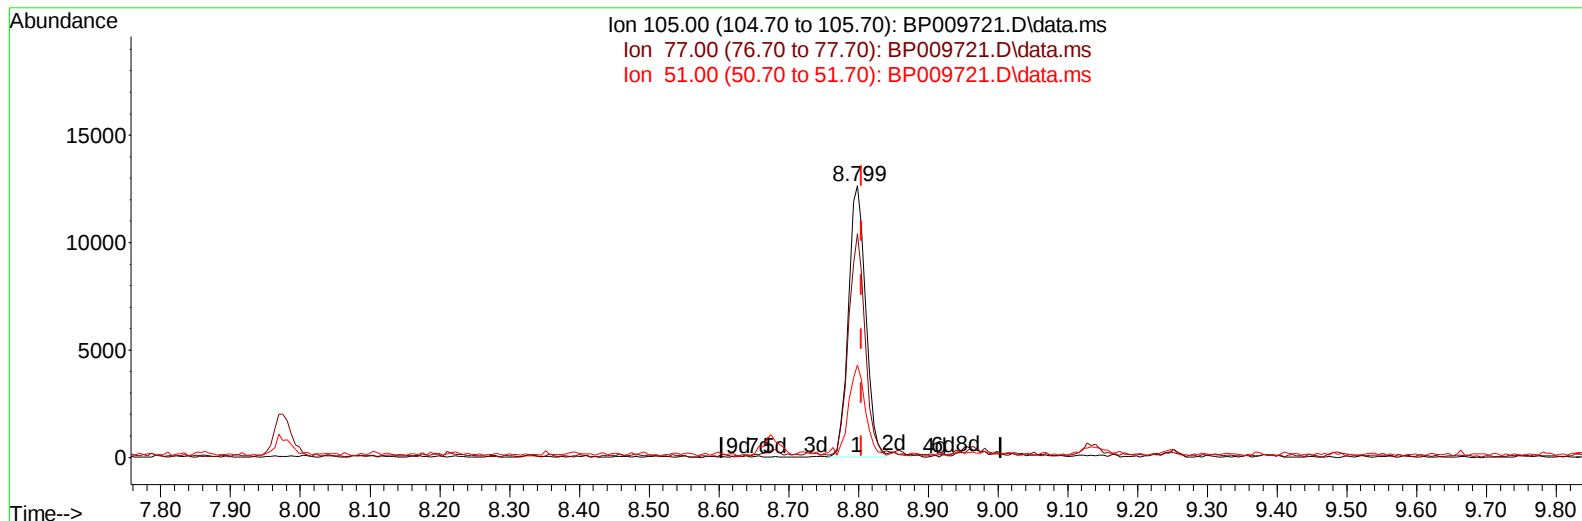

TIC: BP009721.D\data.ms

(16) Acetophenone

8.799min (-0.006) 2.16 ng/u1

response 21726

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	66.80	82.48#
51.00	17.30	34.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009721.D
 Acq On : 08 Apr 2022 17:04
 Operator : CG/JU
 Sample : N2182-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

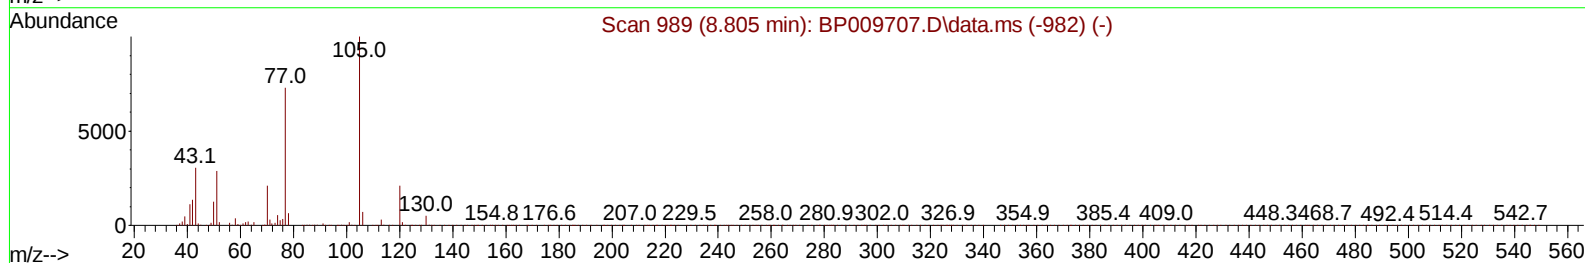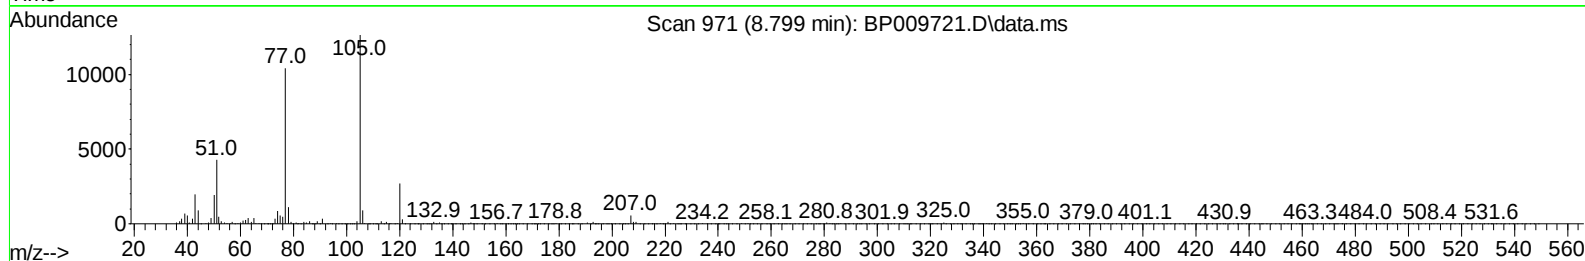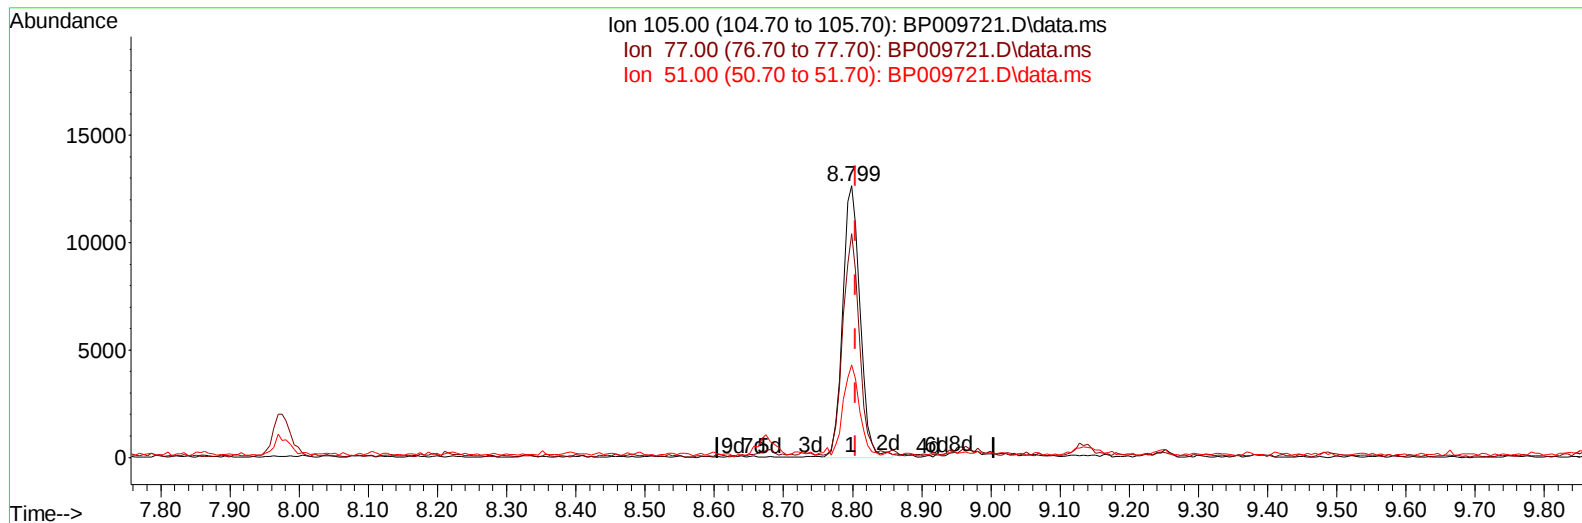

TIC: BP009721.D\data.ms

(16) Acetophenone

8.799min (-0.006) 2.20 ng/ul m

response 22075

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	66.80	82.48#
51.00	17.30	34.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009721.D
 Acq On : 08 Apr 2022 17:04
 Operator : CG/JU
 Sample : N2182-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

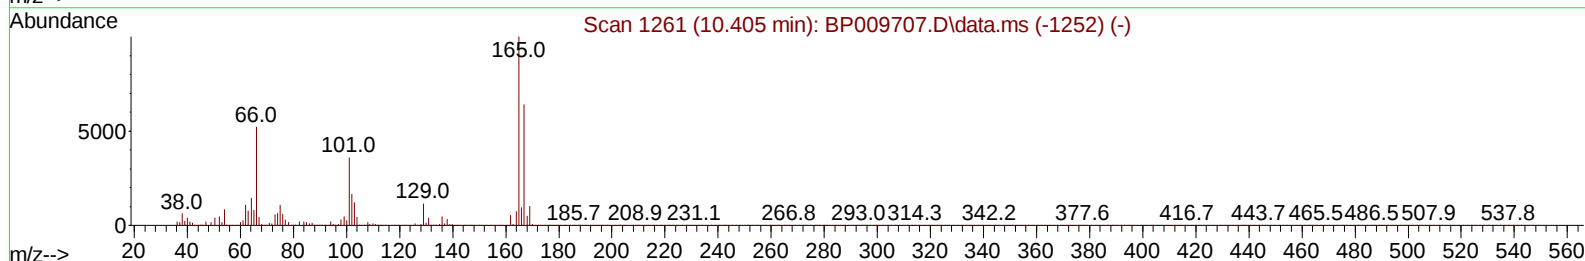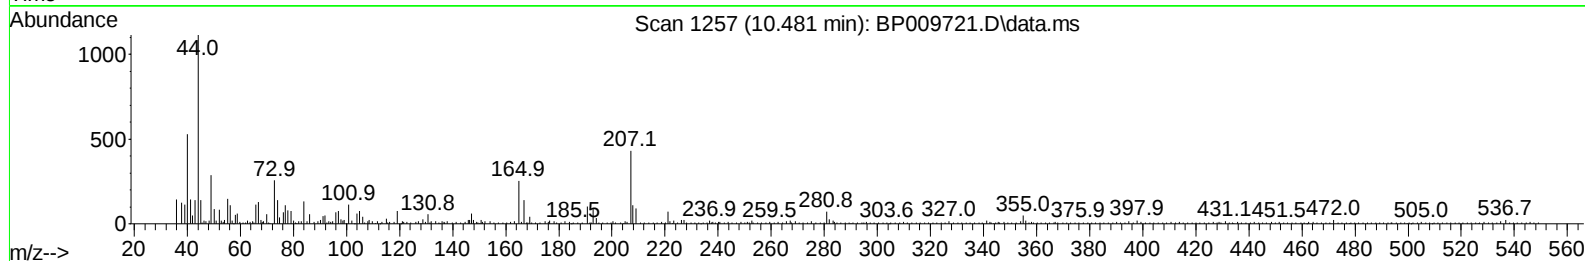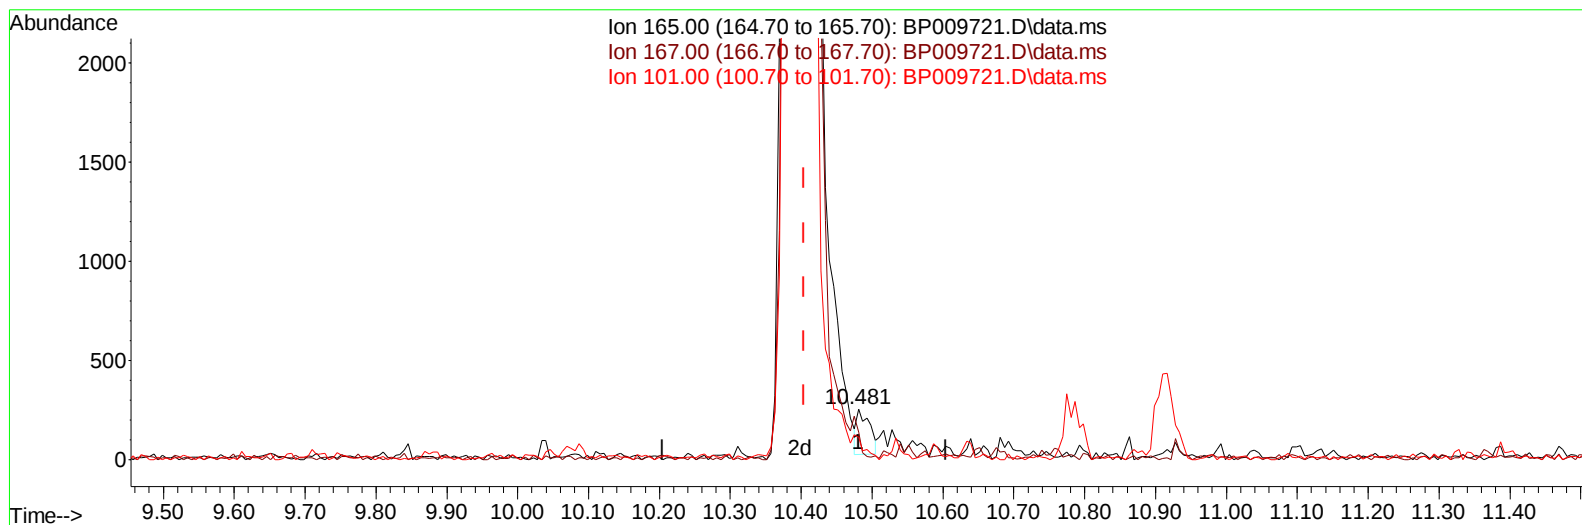

TIC: BP009721.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.481min (+ 0.076) 0.04 ng/u1

response 279

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	54.51
101.00	49.80	43.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009721.D
 Acq On : 08 Apr 2022 17:04
 Operator : CG/JU
 Sample : N2182-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

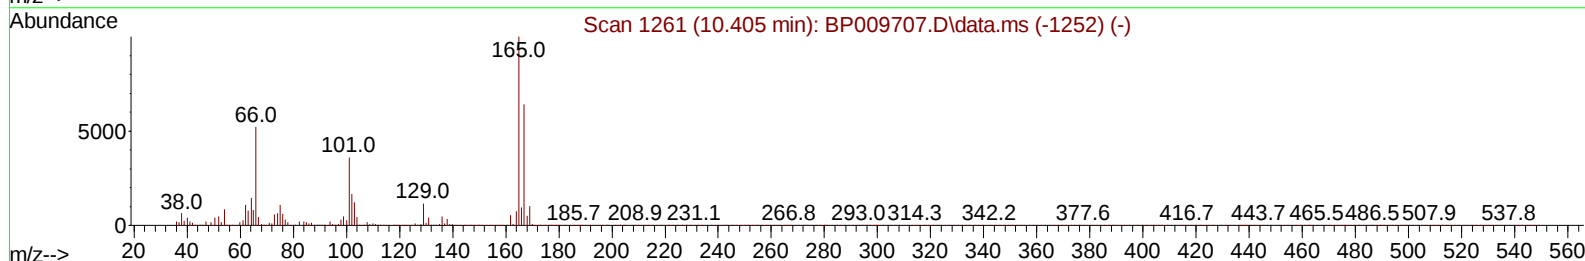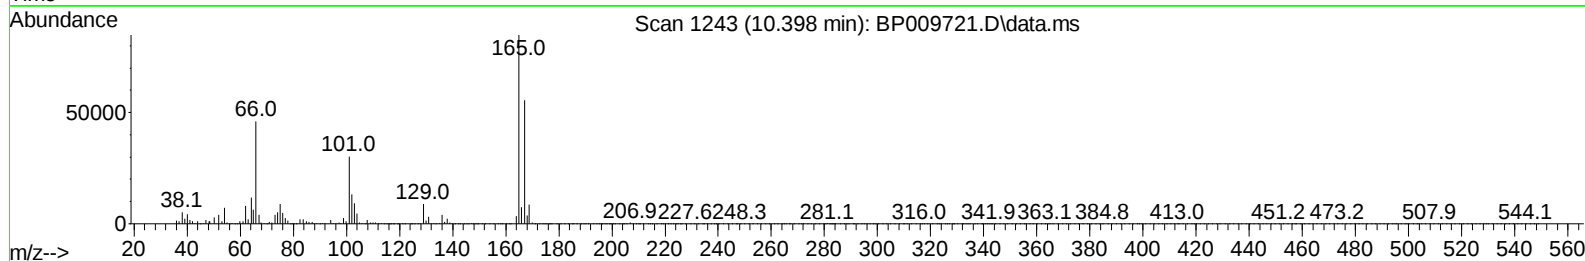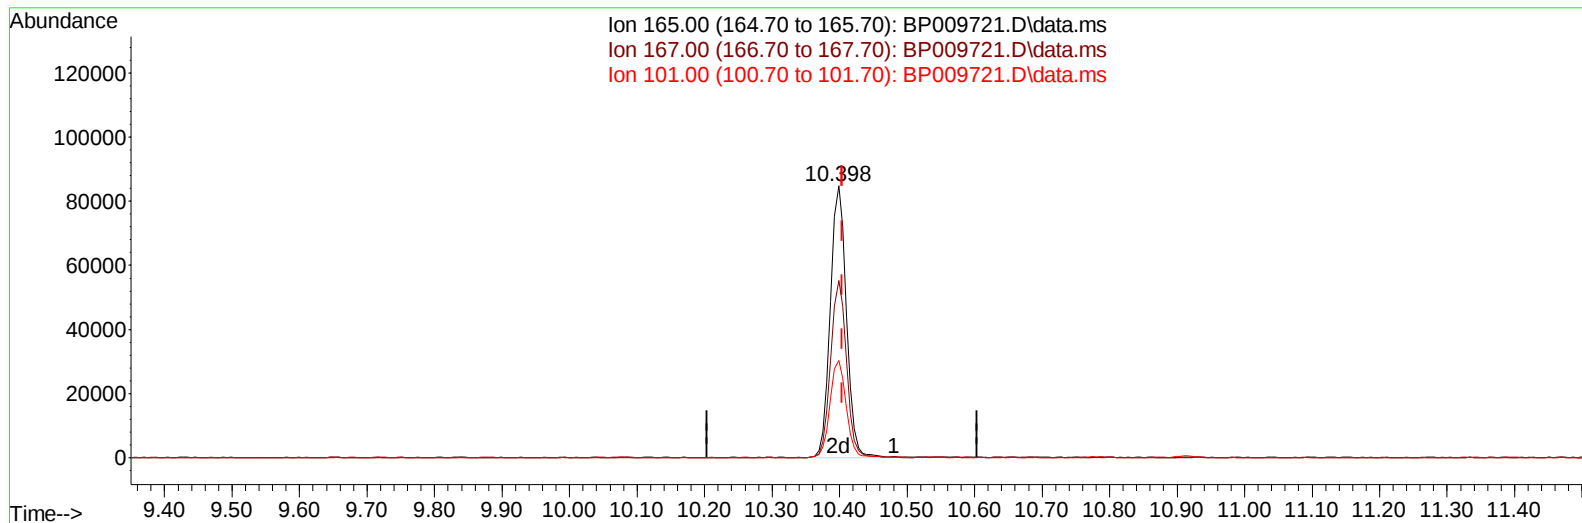

TIC: BP009721.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.398min (-0.006) 22.08 ng/ul m

response 140608

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	65.27
101.00	49.80	35.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009721.D
 Acq On : 08 Apr 2022 17:04
 Operator : CG/JU
 Sample : N2182-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

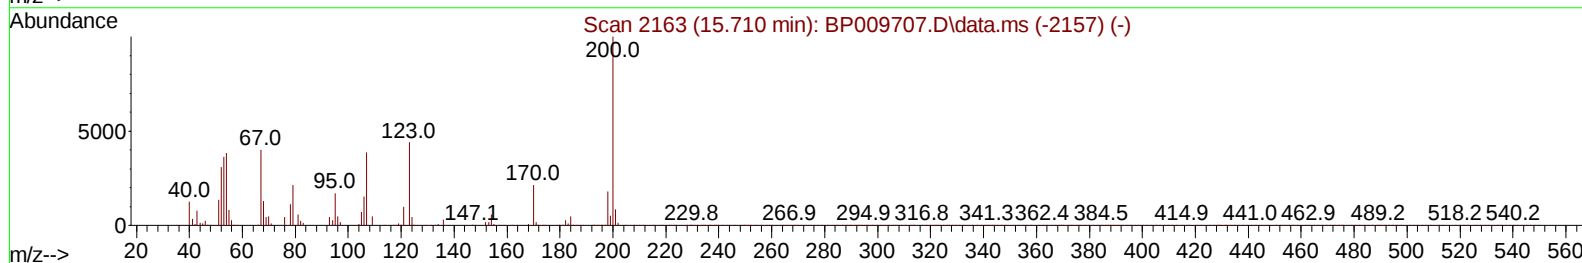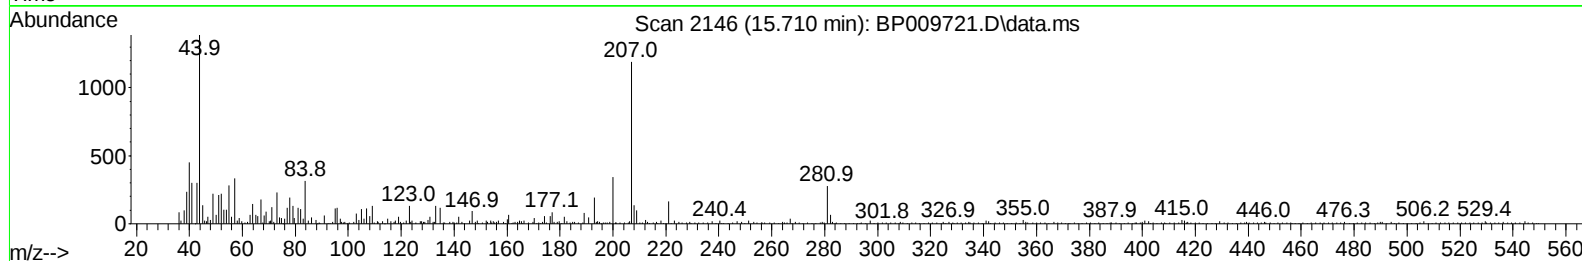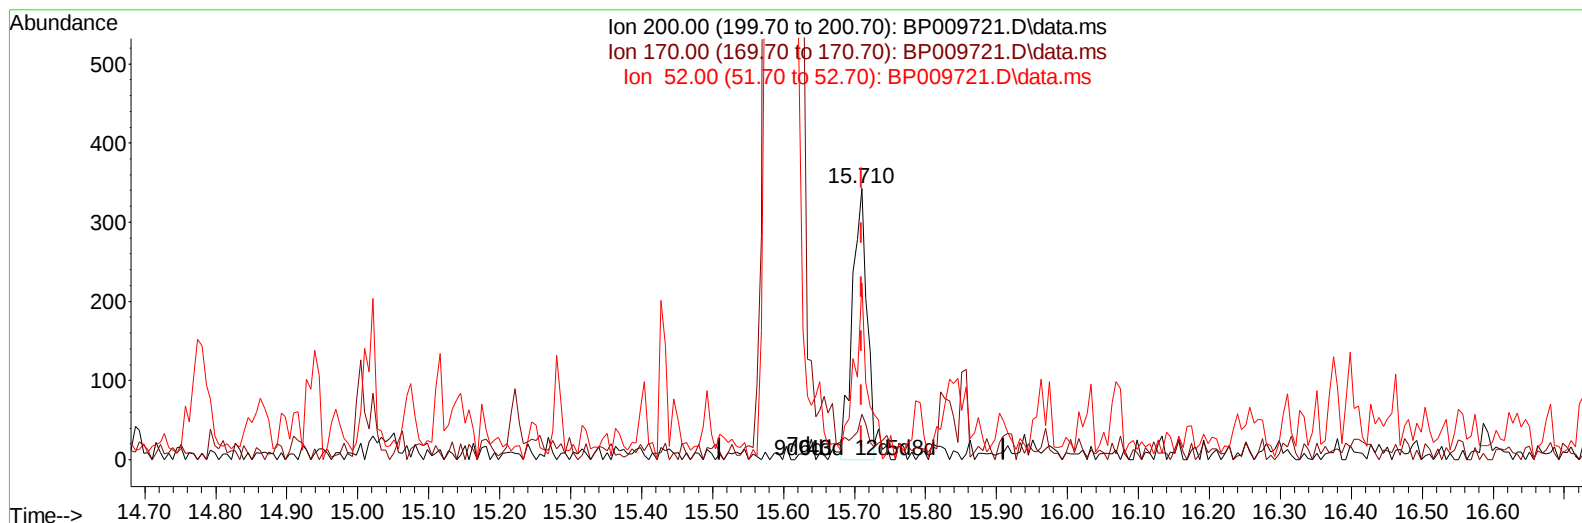

TIC: BP009721.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.710min (+ 0.000) 0.13 ng/u1

response 485

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.00	16.62#
52.00	21.20	65.01#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009721.D
Acq On : 08 Apr 2022 17:04
Operator : CG/JU
Sample : N2182-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 07 19:16:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

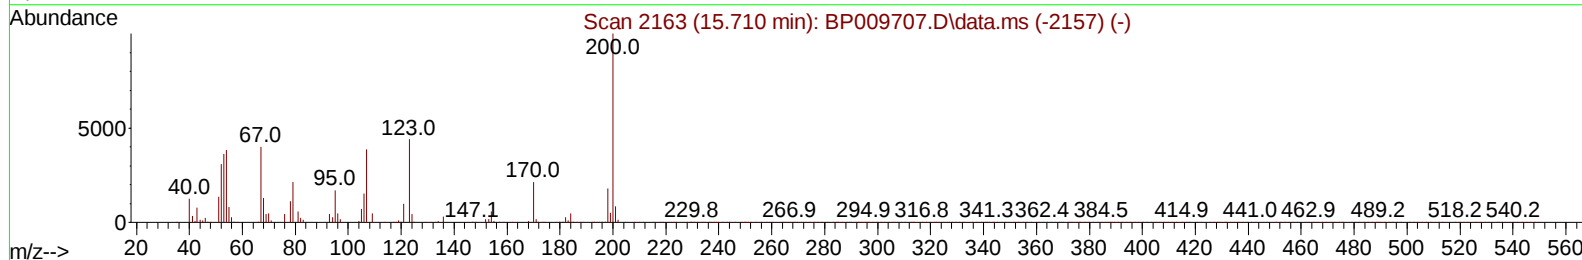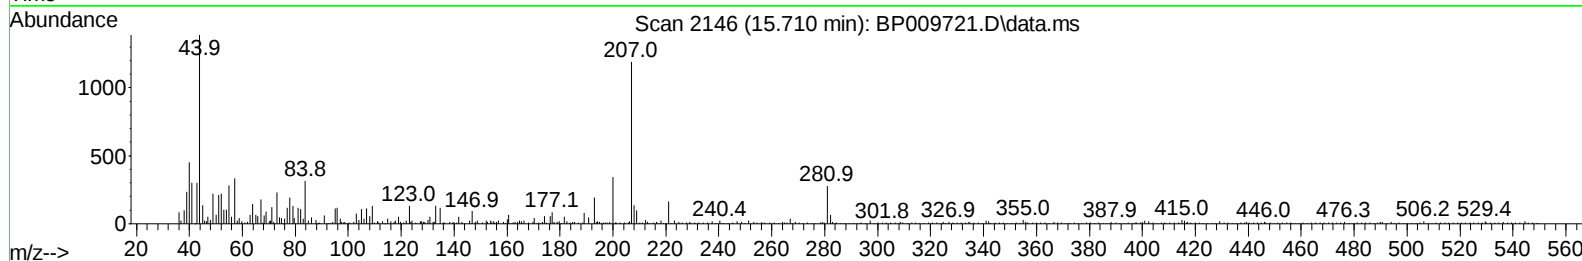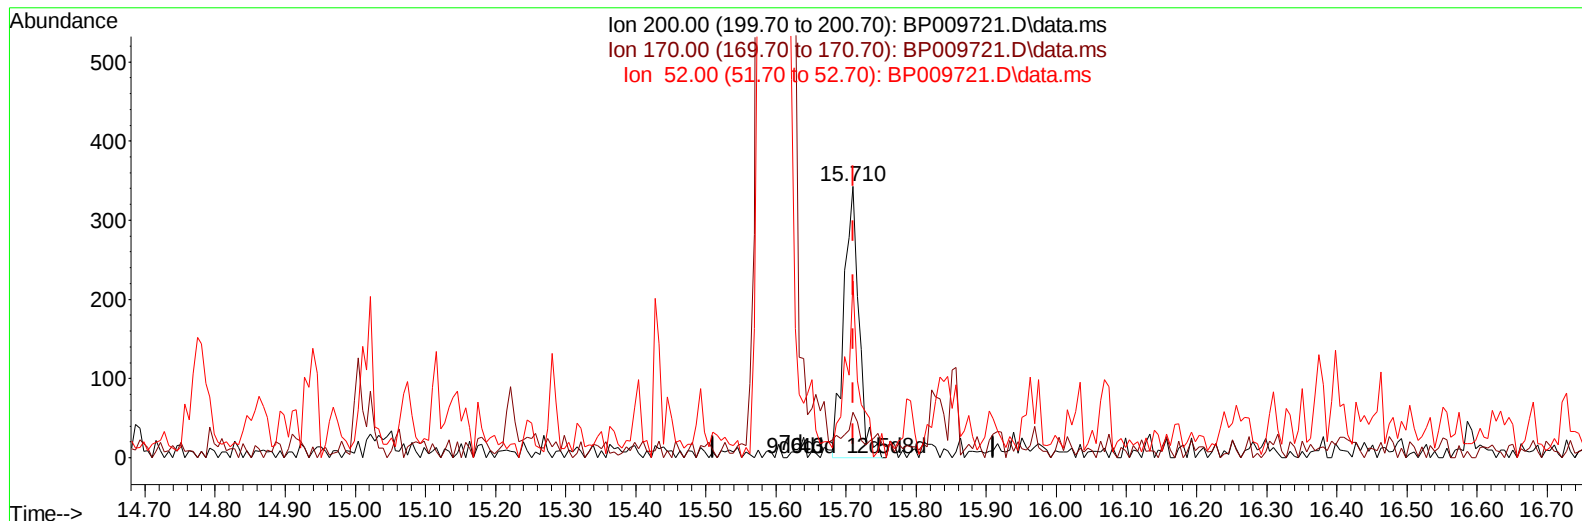

TIC: BP009721.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.710min (+ 0.000) 0.14 ng/ul m

response 510

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.00	12.24#
52.00	21.20	65.01#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009721.D
 Acq On : 08 Apr 2022 17:04
 Operator : CG/JU
 Sample : N2182-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	87048	20.000	ng/ul	0.00
20) Naphthalene-d8	10.787	136	384864	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.610	164	280633	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.357	188	633982	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.439	240	679236	20.000	ng/ul	# 0.00
88) Perylene-d12	23.915	264	685114	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	9854m	5.052	ng/uL	0.00
4) Pyridine-d5	3.811	84	61342	11.407	ng/ul	0.00
7) Phenol-d5	7.128	99	186605	24.417	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	136413	29.983	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	132353	22.959	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	183677	28.791	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	86870	31.300	ng/ul	0.00
24) 2-Nitrophenol-d4	9.857	143	44816	14.729	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.398	165	140608m	22.083	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	244826	26.997	ng/ul	0.00
46) Dimethylphthalate-d6	14.016	166	694808	31.519	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	787138	30.140	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143	749	0.187	ng/ul	0.00
60) Fluorene-d10	15.598	176	592741	31.964	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	510m	0.136	ng/ul	0.00
73) Anthracene-d10	17.457	188	963266	31.734	ng/ul	0.00
81) Pyrene-d10	19.686	212	1225811	33.044	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.757	264	1159995	32.513	ng/ul	0.00
Target Compounds						
						Qvalue
8) Phenol	7.152	94	17863m	2.335	ng/ul	
16) Acetophenone	8.799	105	22075m	2.196	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009721.D
Acq On : 08 Apr 2022 17:04
Operator : CG/JU
Sample : N2182-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R18

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:59:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 07 19:16:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

