

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP040822\  
 Data File : BP009718.D  
 Acq On : 08 Apr 2022 15:22  
 Operator : CG/JU  
 Sample : N2182-10  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 C0R17

Quant Time: Apr 08 22:27:57 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP040722.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Apr 07 19:16:52 2022  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	82469	20.000	ng/ul	0.00
20) Naphthalene-d8	10.786	136	363686	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.610	164	274087	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.357	188	628490	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.439	240	704210	20.000	ng/ul	# 0.00
88) Perylene-d12	23.915	264	726172	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	9185	4.971	ng/uL	0.00
4) Pyridine-d5	3.810	84	64421	12.644	ng/ul	0.00
7) Phenol-d5	7.128	99	181665	25.091	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.298	67	121482	28.184	ng/ul	0.00
11) 2-Chlorophenol-d4	7.504	132	144724	26.499	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	150460	24.894	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	77697	29.625	ng/ul	0.00
24) 2-Nitrophenol-d4	9.857	143	84772	29.482	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.398	165	152254	25.305	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	219418	25.604	ng/ul	0.00
46) Dimethylphthalate-d6	14.016	166	639440	29.700	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	690152	27.057	ng/ul	0.00
54) 4-Nitrophenol-d4	14.780	143	86969	22.274	ng/ul	0.00
60) Fluorene-d10	15.598	176	536616	29.628	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	70700	18.989	ng/ul	0.00
73) Anthracene-d10	17.457	188	930169	30.911	ng/ul	0.00
81) Pyrene-d10	19.686	212	1177073	30.605	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.762	264	1198650	31.697	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.798	105	15835	1.663	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP040822\  
 Data File : BP009718.D  
 Acq On : 08 Apr 2022 15:22  
 Operator : CG/JU  
 Sample : N2182-10  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 C0R17

Quant Time: Apr 08 22:27:57 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP040722.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Apr 07 19:16:52 2022  
 Response via : Initial Calibration

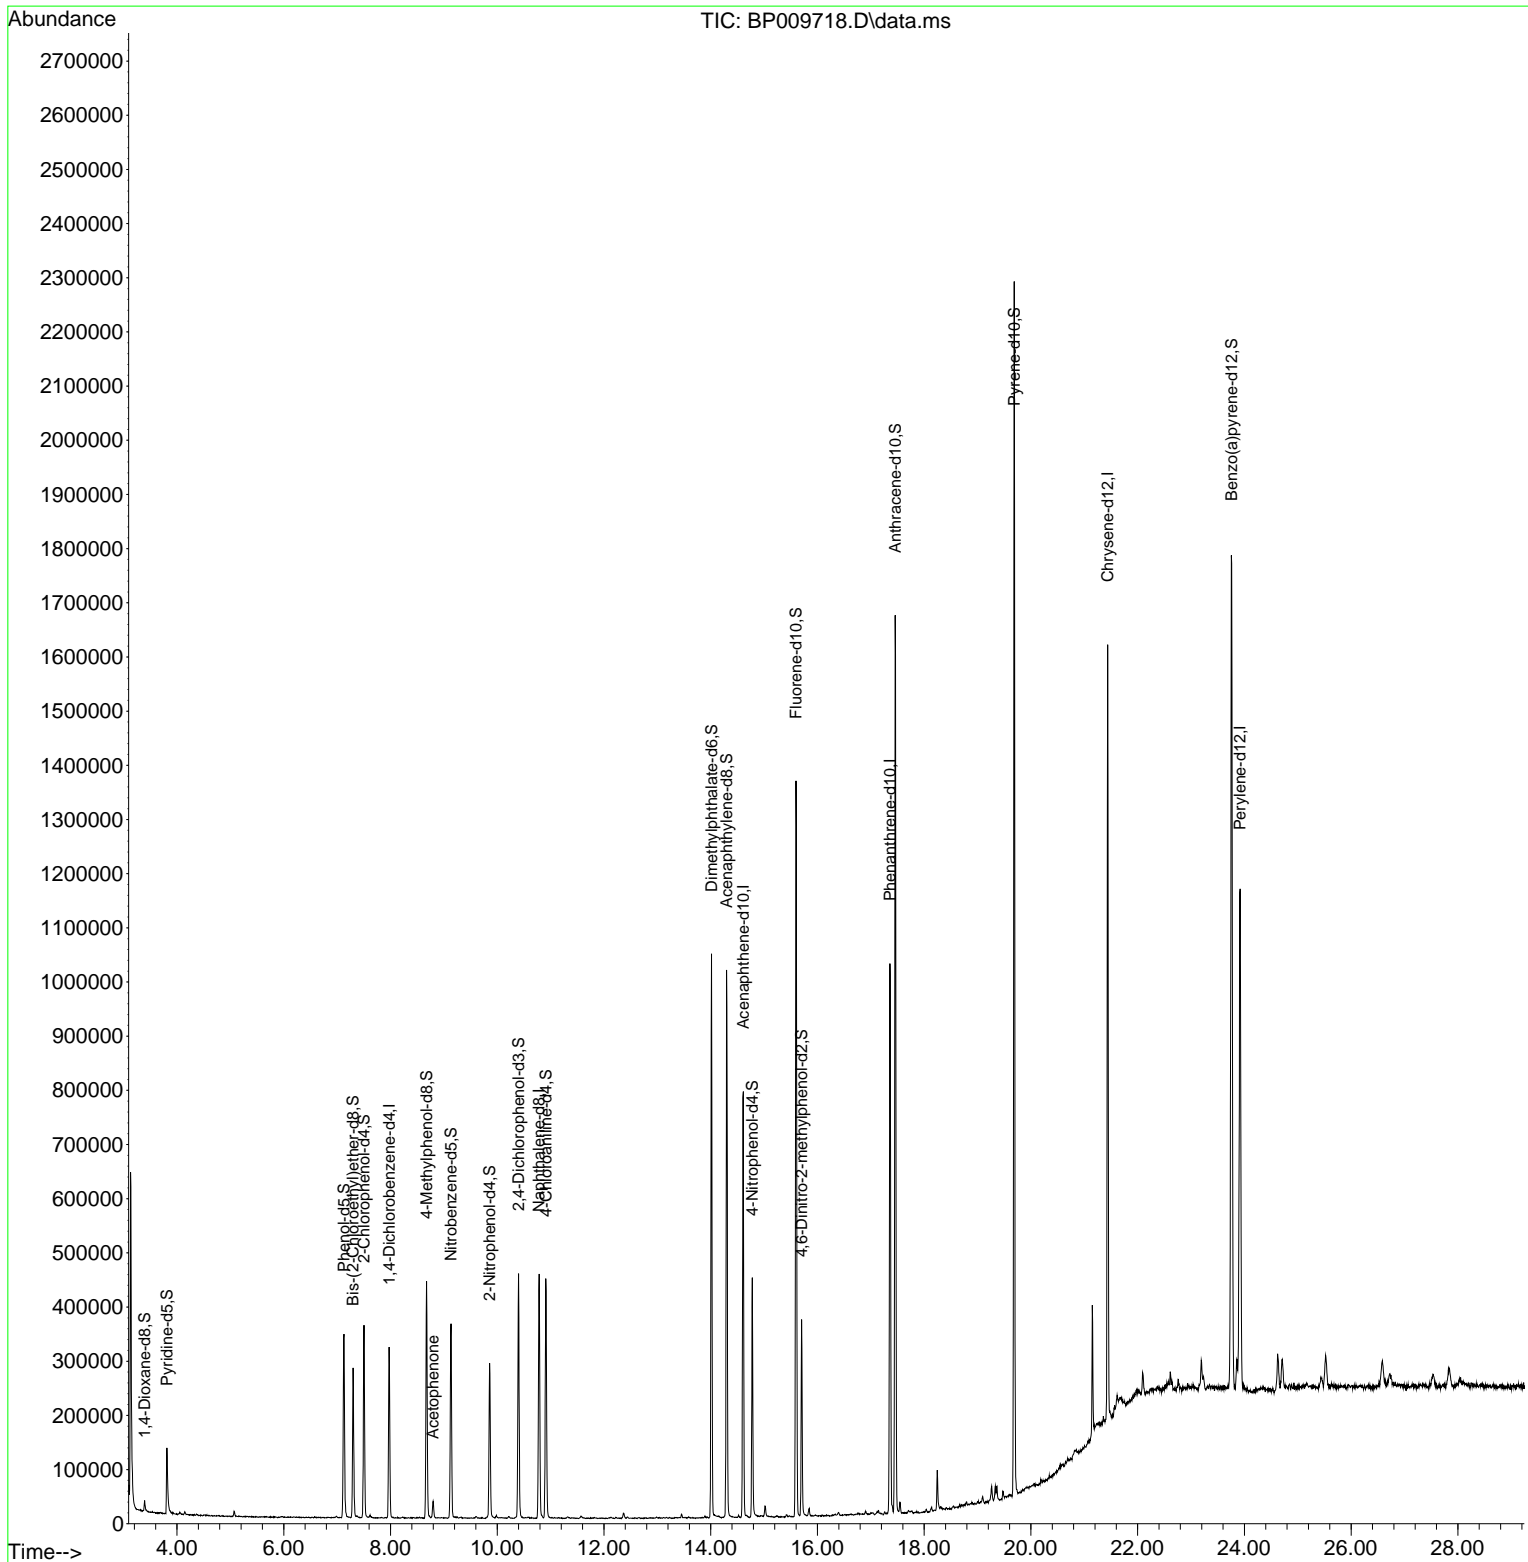

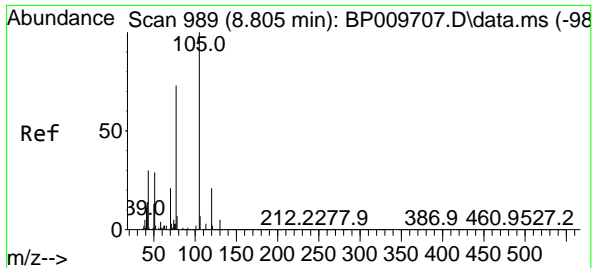

#16  
 Acetophenone  
 Concen: 1.663 ng/ul  
 RT: 8.798 min Scan# 91  
 Delta R.T. -0.006 min  
 Lab File: BP009718.D  
 Acq: 08 Apr 2022 15:22

Instrument :  
 BNA\_P  
 ClientSampleId :  
 C0R17

Tgt Ion:105 Resp: 15835

Ion	Ratio	Lower	Upper
105	100		
77	80.3	53.4	80.2#
51	30.0	13.8	20.8#

