

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009731.D
 Acq On : 08 Apr 2022 23:17
 Operator : CG/JU
 Sample : N2182-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R14

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
 Supervised By :Yogesh Patel 04/12/2022

Quant Time: Apr 09 01:16:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	42845	20.000	ng/u1	0.00
20) Naphthalene-d8	10.781	136	192168	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.604	164	144833	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.357	188	341924	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.433	240	411116	20.000	ng/u1	#-0.01
88) Perylene-d12	23.910	264	482153	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	2949m	3.072	ng/uL	0.00
4) Pyridine-d5	3.817	84	8313	3.141	ng/u1	0.00
7) Phenol-d5	7.122	99	57494	15.285	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	37704	16.837	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.499	132	45018	15.866	ng/u1	0.00
15) 4-Methylphenol-d8	8.669	113	38212	12.169	ng/u1	-0.01
21) Nitrobenzene-d5	9.128	128	23596	17.027	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.858	143	24947m	16.420	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	50956	16.028	ng/u1	0.00
31) 4-Chloroaniline-d4	10.910	131	57119	12.614	ng/u1	0.00
46) Dimethylphthalate-d6	14.010	166	212077	18.641	ng/u1	-0.01
49) Acenaphthylene-d8	14.299	160	221205	16.412	ng/u1	0.00
54) 4-Nitrophenol-d4	14.775	143	35156	17.039	ng/u1	-0.01
60) Fluorene-d10	15.593	176	183674	19.191	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.704	200	24735	12.211	ng/u1	0.00
73) Anthracene-d10	17.451	188	318645	19.464	ng/u1	-0.01
81) Pyrene-d10	19.681	212	450769	20.076	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.751	264	525960	20.947	ng/u1	-0.01
Target Compounds						
16) Acetophenone	8.799	105	13370m	2.702	ng/u1	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009731.D
Acq On : 08 Apr 2022 23:17
Operator : CG/JU
Sample : N2182-07
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0R14

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022


Quant Time: Apr 09 01:16:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 07 19:16:52 2022
Response via : Initial Calibration

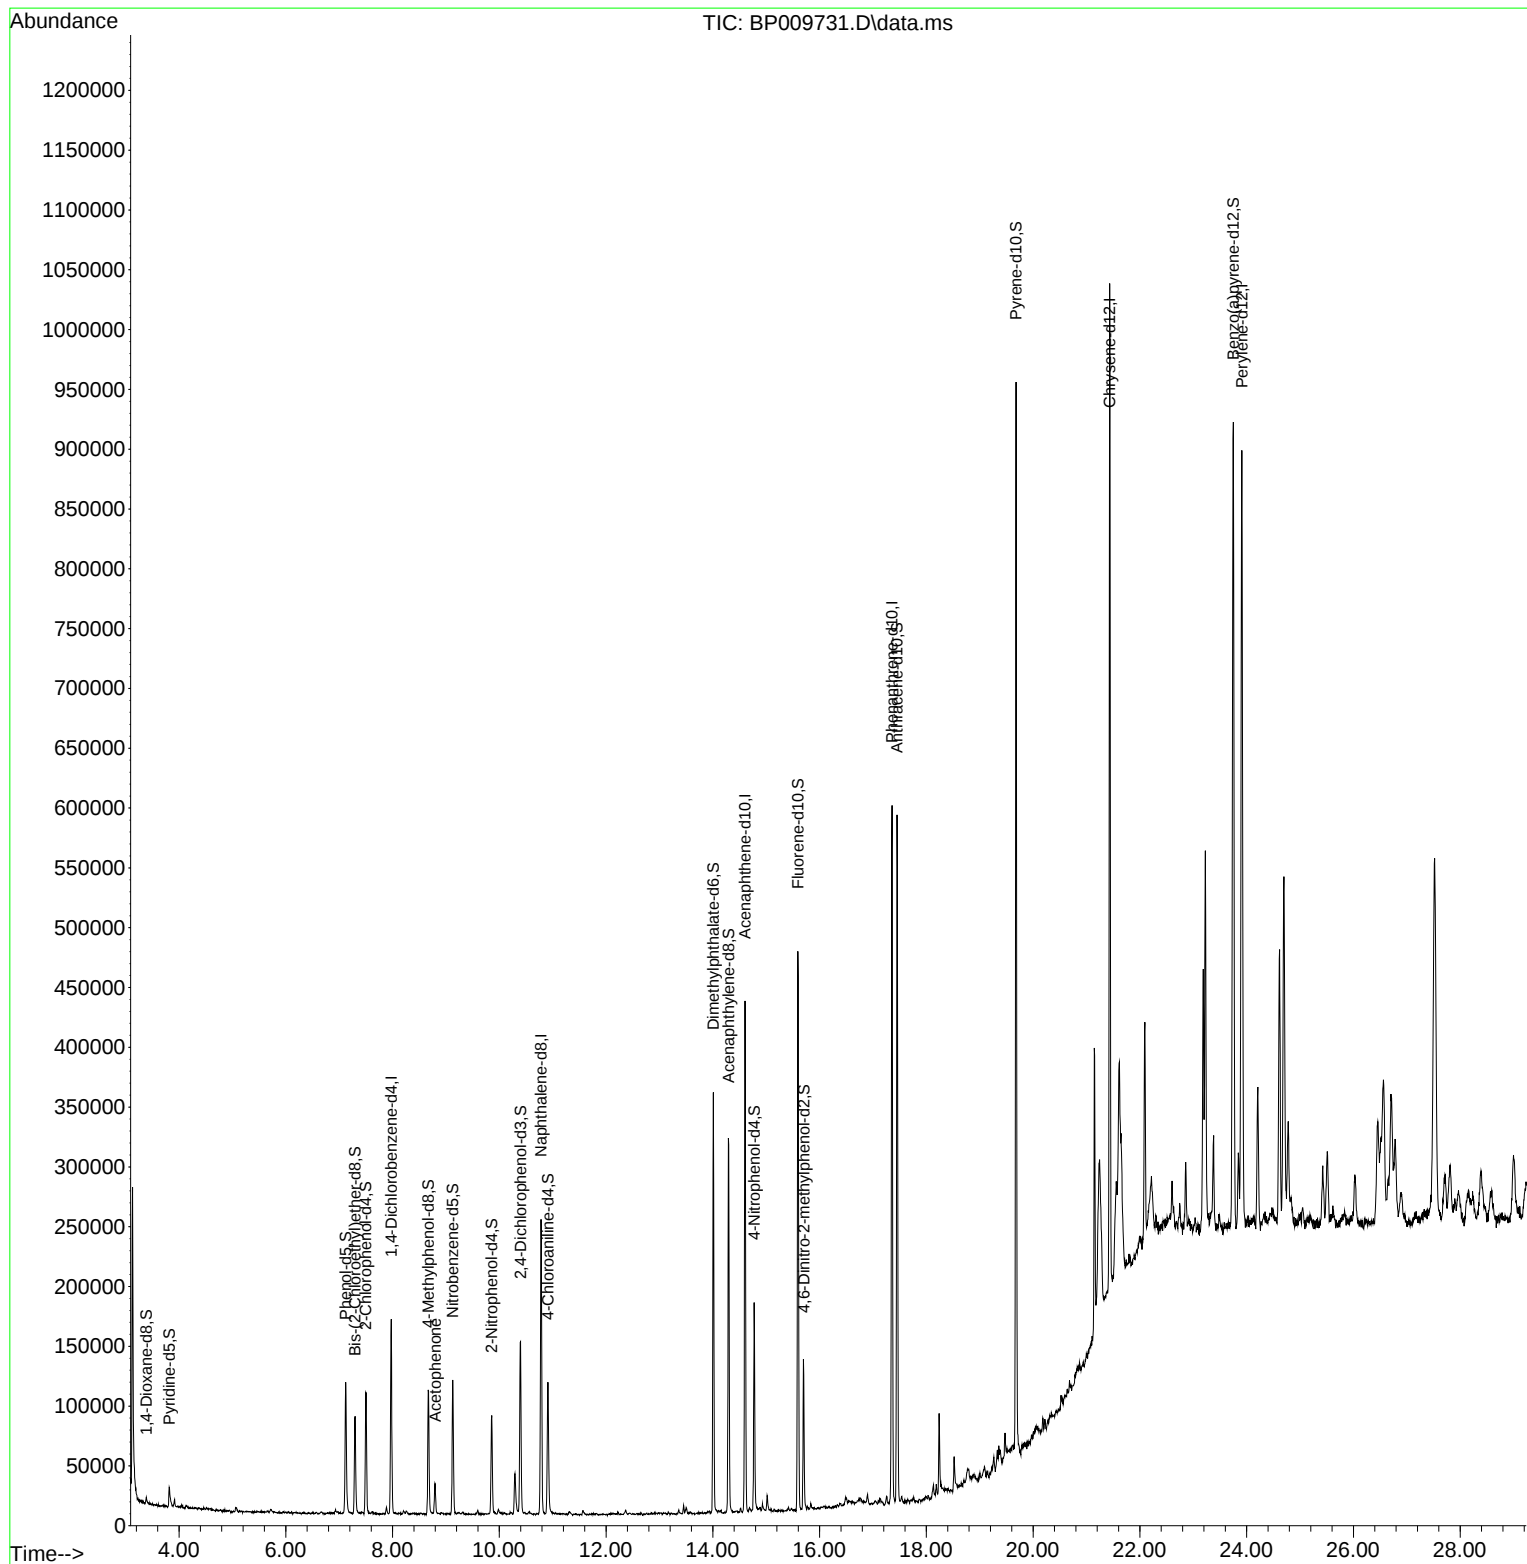

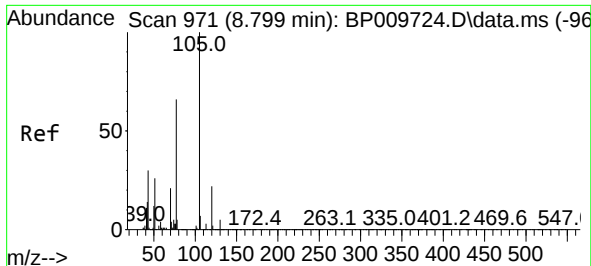

#16
Acetophenone
Concen: 2.702 ng/ul m
RT: 8.799 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP009731.D
Acq: 08 Apr 2022 23:17

Instrument :
BNA_P
ClientSampleId :
C0R14

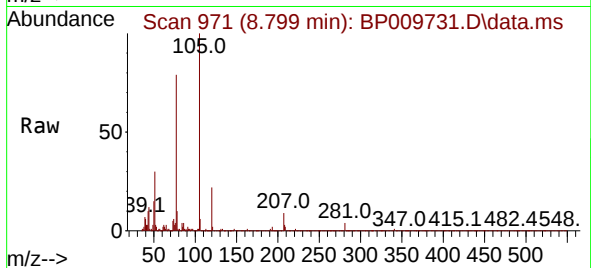

Tgt Ion:105 Resp: 13370
Ion Ratio Lower Upper
105 100
77 79.0 53.4 80.2
51 30.3 13.8 20.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/11/2022
Supervised By :Yogesh Patel 04/12/2022

