

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009712.D
 Acq On : 08 Apr 2022 11:59
 Operator : CG/JU
 Sample : N2183-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	25	rVB	584735	914501	50.08%	4.485%
2	3.393	48	52	58	rVB2	12729	16858	0.92%	0.083%
3	3.811	120	123	138	rBV	63431	110903	6.07%	0.544%
4	4.052	159	164	171	rVB8	3537	6984	0.38%	0.034%
5	4.152	176	181	185	rVB4	5397	7999	0.44%	0.039%
6	4.370	214	218	222	rBV7	4245	6304	0.35%	0.031%
7	4.475	233	236	239	rVV5	1851	2018	0.11%	0.010%
8	4.517	239	243	246	rVB6	1489	2415	0.13%	0.012%
9	4.717	273	277	279	rVB5	1956	2200	0.12%	0.011%
10	4.781	287	288	296	rVB8	3218	4309	0.24%	0.021%
11	4.964	315	319	321	rVB5	1488	2211	0.12%	0.011%
12	5.075	333	338	343	rVB3	10930	18172	1.00%	0.089%
13	5.534	412	416	417	rBV4	1595	1949	0.11%	0.010%
14	5.658	434	437	440	rBV5	1517	2489	0.14%	0.012%
15	6.840	635	638	643	rVB7	1783	2530	0.14%	0.012%
16	6.993	660	664	669	rVB5	2671	4666	0.26%	0.023%
17	7.128	678	687	700	rBV	198645	336665	18.43%	1.651%
18	7.299	710	716	726	rBV	152008	253797	13.90%	1.245%
19	7.369	726	728	734	rVB2	2982	5231	0.29%	0.026%
20	7.505	744	751	762	rBV	202023	324367	17.76%	1.591%
21	7.616	766	770	777	rVB8	4332	7071	0.39%	0.035%
22	7.975	824	831	840	rBV	304213	489107	26.78%	2.399%
23	8.046	840	843	848	rVB7	2535	3979	0.22%	0.020%
24	8.234	872	875	879	rVB6	2204	3224	0.18%	0.016%
25	8.675	942	950	960	rBV2	244818	398516	21.82%	1.954%
26	8.799	965	971	977	rVB2	21544	36398	1.99%	0.179%
27	9.134	1020	1028	1037	rBV	197438	336760	18.44%	1.652%
28	9.316	1053	1059	1063	rBV7	2463	5259	0.29%	0.026%
29	9.599	1104	1107	1113	rVV6	4822	8895	0.49%	0.044%
30	9.857	1142	1151	1158	rBV	144876	247529	13.55%	1.214%
31	9.981	1169	1172	1173	rBV3	2304	2055	0.11%	0.010%
32	10.222	1207	1213	1219	rVB9	2700	5589	0.31%	0.027%
33	10.399	1235	1243	1251	rBV	246171	418645	22.92%	2.053%
34	10.457	1251	1253	1259	rVB7	2611	2990	0.16%	0.015%
35	10.787	1297	1309	1323	rBV	432578	742792	40.67%	3.643%
36	10.910	1323	1330	1340	rBV	232186	412249	22.57%	2.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009712.D
 Acq On : 08 Apr 2022 11:59
 Operator : CG/JU
 Sample : N2183-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	11.316	1394	1399	1401	rBV6	1946	3259	0.18%	0.016%
38	11.575	1438	1443	1448	rBV6	3843	7415	0.41%	0.036%
39	11.687	1460	1462	1466	rBV5	1913	2800	0.15%	0.014%
40	12.222	1550	1553	1559	rVB7	3990	6359	0.35%	0.031%

41	12.375	1571	1579	1583	rVB4	6082	9353	0.51%	0.046%
42	12.904	1665	1669	1671	rVB4	1703	2276	0.12%	0.011%
43	13.034	1688	1691	1694	rVB4	1952	2010	0.11%	0.010%
44	13.116	1704	1705	1711	rVB6	2027	2675	0.15%	0.013%
45	13.175	1711	1715	1718	rBV5	2433	3828	0.21%	0.019%

46	13.240	1722	1726	1728	rVB5	1377	1906	0.10%	0.009%
47	13.346	1741	1744	1749	rVB7	1420	2269	0.12%	0.011%
48	13.457	1756	1763	1769	rBV	12130	19165	1.05%	0.094%
49	13.557	1777	1780	1782	rBV4	1361	1978	0.11%	0.010%
50	13.893	1833	1837	1840	rBV3	4032	4799	0.26%	0.024%

51	14.016	1852	1858	1865	rBV	577172	780653	42.75%	3.829%
52	14.151	1879	1881	1886	rVB6	2182	2704	0.15%	0.013%
53	14.298	1899	1906	1921	rBV	554682	831188	45.51%	4.076%
54	14.522	1939	1944	1949	rBV5	4035	6548	0.36%	0.032%
55	14.610	1951	1959	1970	rBV	742760	1125609	61.63%	5.520%

56	14.781	1980	1988	1999	rBV	233757	358621	19.64%	1.759%
57	14.940	2011	2015	2018	rBV6	2092	2809	0.15%	0.014%
58	15.022	2023	2029	2035	rBV4	22372	39270	2.15%	0.193%
59	15.069	2036	2037	2043	rVB6	2349	2763	0.15%	0.014%
60	15.345	2077	2084	2087	rBV8	1375	2676	0.15%	0.013%

61	15.428	2093	2098	2102	rBV7	3300	4859	0.27%	0.024%
62	15.475	2102	2106	2111	rVB8	2553	3647	0.20%	0.018%
63	15.522	2111	2114	2117	rVB5	1944	2032	0.11%	0.010%
64	15.598	2119	2127	2135	rBV	727871	1119422	61.30%	5.490%
65	15.704	2139	2145	2155	rBV	192264	268741	14.72%	1.318%

66	15.840	2164	2168	2174	rVB4	6973	11760	0.64%	0.058%
67	15.957	2184	2188	2191	rBV5	2755	4049	0.22%	0.020%
68	16.028	2197	2200	2201	rBV3	2018	2277	0.12%	0.011%
69	16.098	2209	2212	2218	rVB8	1596	2790	0.15%	0.014%
70	16.392	2258	2262	2266	rVB7	4091	6028	0.33%	0.030%

71	16.610	2297	2299	2302	rBV3	2988	2210	0.12%	0.011%
72	16.716	2313	2317	2320	rBV6	1407	2560	0.14%	0.013%
73	16.769	2323	2326	2331	rVB7	3448	4590	0.25%	0.023%
74	16.904	2345	2349	2352	rVB6	3355	5151	0.28%	0.025%
75	17.010	2364	2367	2370	rBV5	1857	2559	0.14%	0.013%

76	17.139	2387	2389	2393	rVB3	5067	5534	0.30%	0.027%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009712.D
 Acq On : 08 Apr 2022 11:59
 Operator : CG/JU
 Sample : N2183-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

77	17.263	2407	2410	2417	rBV9	3903	8295	0.45%	0.041%
78	17.357	2420	2426	2431	rVV	970607	1434854	78.57%	7.037%
79	17.404	2431	2434	2437	rVV	51188	69468	3.80%	0.341%
80	17.457	2437	2443	2454	rVV	890110	1301446	71.26%	6.383%
81	17.545	2454	2458	2466	rVB7	16309	25982	1.42%	0.127%
82	17.651	2474	2476	2480	rBV2	3829	4017	0.22%	0.020%
83	17.751	2490	2493	2504	rVB5	7775	15309	0.84%	0.075%
84	17.875	2512	2514	2515	rBV2	1966	1933	0.11%	0.009%
85	18.134	2552	2558	2565	rBV6	26900	46234	2.53%	0.227%
86	18.192	2565	2568	2569	rVV3	3641	4051	0.22%	0.020%
87	18.245	2573	2577	2586	rVV3	89135	134621	7.37%	0.660%
88	18.316	2587	2589	2592	rVB	7145	8047	0.44%	0.039%
89	18.416	2602	2606	2610	rBV5	7383	9728	0.53%	0.048%
90	18.545	2625	2628	2631	rBV4	5443	6571	0.36%	0.032%
91	18.669	2645	2649	2653	rBV4	16903	22364	1.22%	0.110%
92	18.704	2653	2655	2658	rVB3	5647	6058	0.33%	0.030%
93	19.263	2747	2750	2755	rVB5	15548	21292	1.17%	0.104%
94	19.363	2759	2767	2774	rVV	104374	159443	8.73%	0.782%
95	19.481	2784	2787	2790	rBV5	11181	15318	0.84%	0.075%
96	19.686	2816	2822	2834	rBV	1275228	1826258	100.00%	8.956%
97	21.151	3068	3071	3078	rBV	230839	286152	15.67%	1.403%
98	21.439	3114	3120	3125	rBV	1279162	1765280	96.66%	8.657%
99	23.757	3507	3514	3526	rVB2	835120	1717160	94.03%	8.421%
100	23.916	3535	3541	3549	rVB2	824999	1681664	92.08%	8.247%




Sum of corrected areas: 20390313

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009712.D
Acq On : 08 Apr 2022 11:59
Operator : CG/JU
Sample : N2183-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R46

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

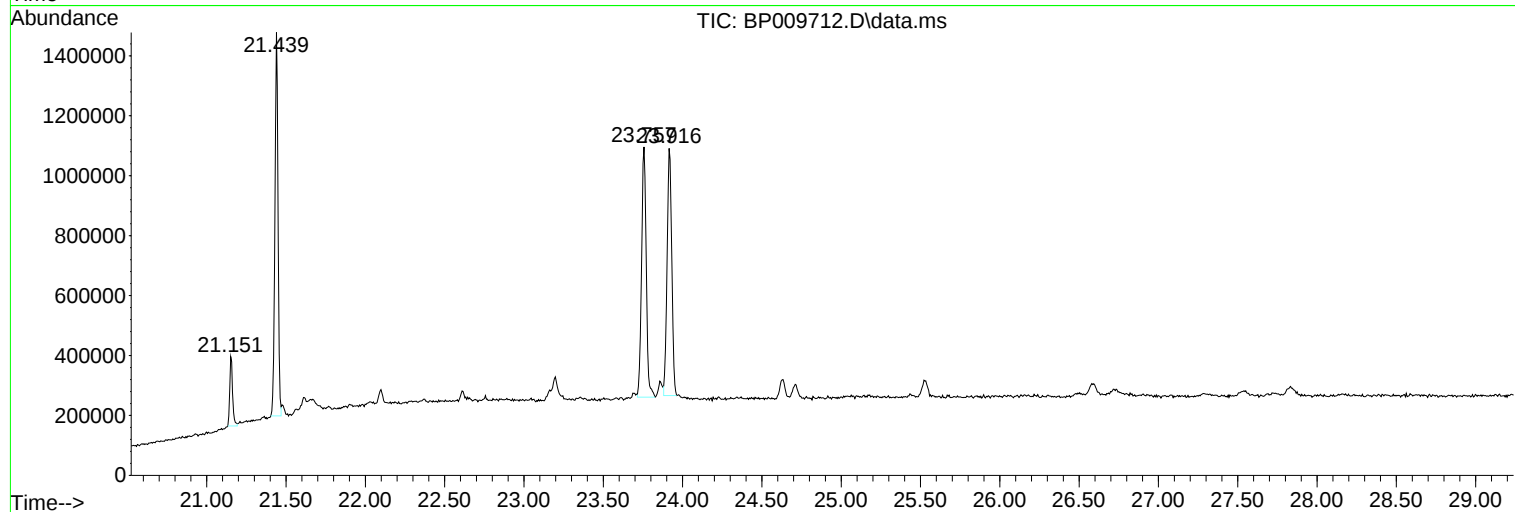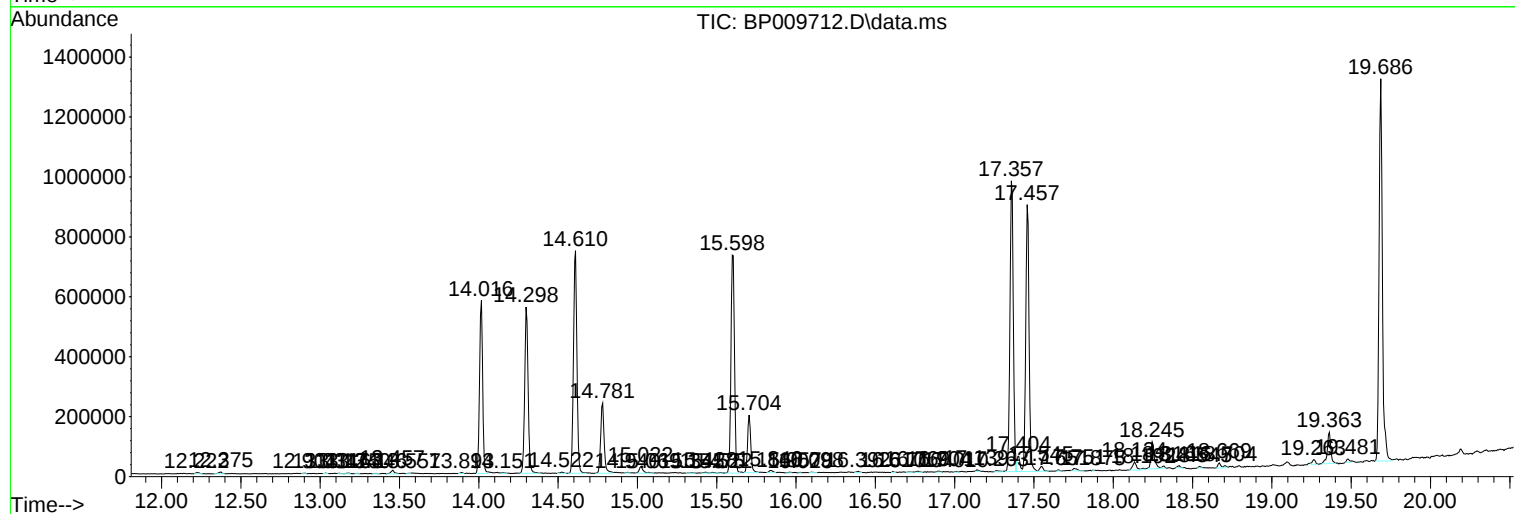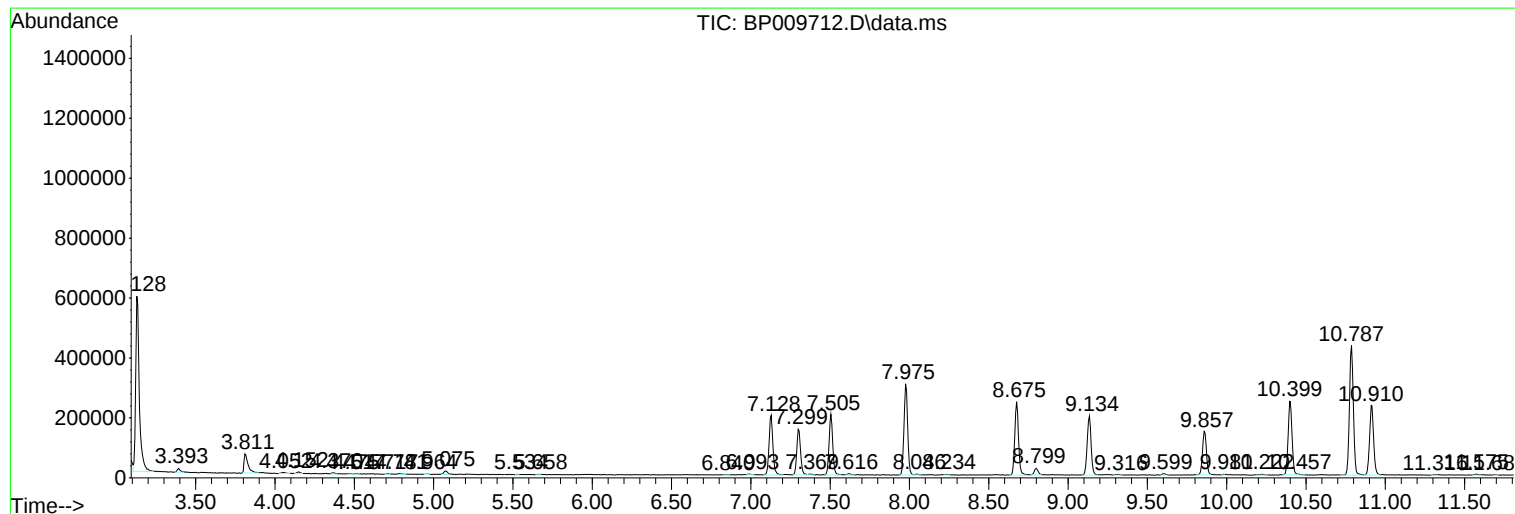

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009712.D
Acq On : 08 Apr 2022 11:59
Operator : CG/JU
Sample : N2183-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R46










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.128	37.39 ng/ul	914501	1,4-Dichlorobenzene-d4	7.975

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40		
4	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40		
5	1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23		

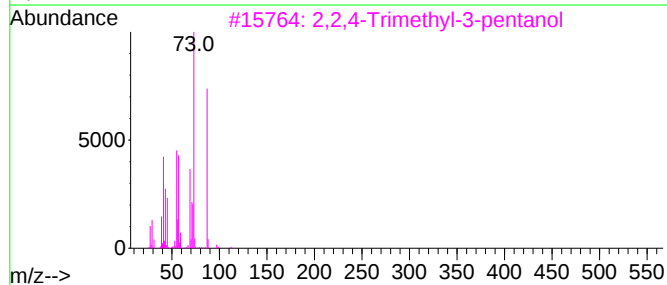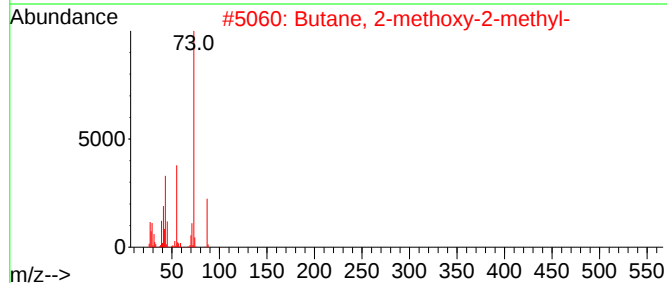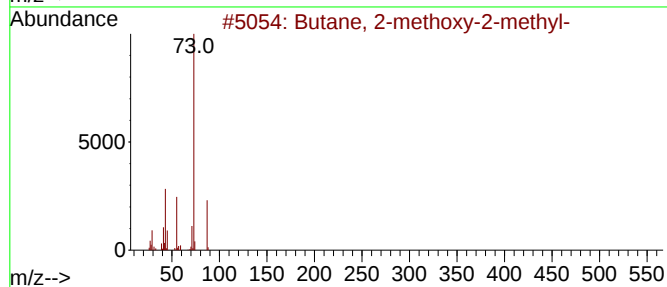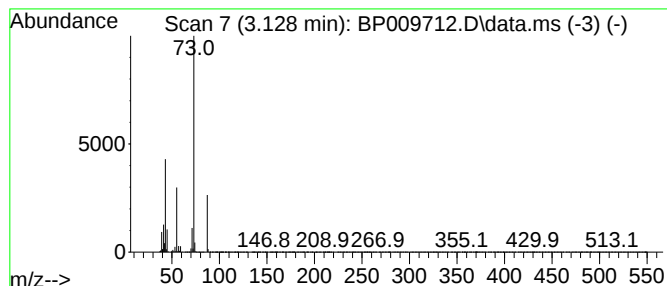

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009712.D
Acq On : 08 Apr 2022 11:59
Operator : CG/JU
Sample : N2183-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R46










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic21.151 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.151	3.24 ng/ul	286152	Chrysene-d12	21.439

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetradecane	196	C14H28	000295-17-0	95
2			1-Hexacosene	364	C26H52	018835-33-1	94
3			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	93
4			3-Eicosene, (E)-	280	C20H40	074685-33-9	91
5			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	91

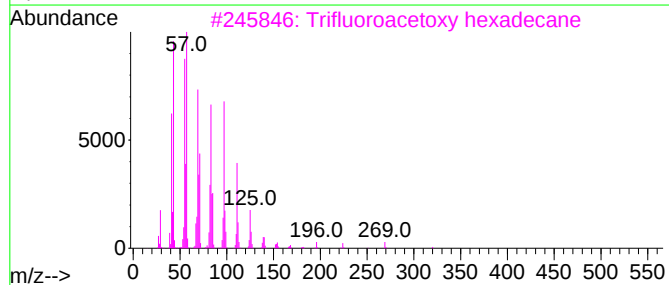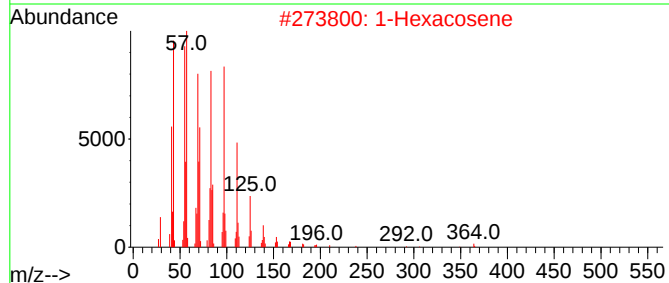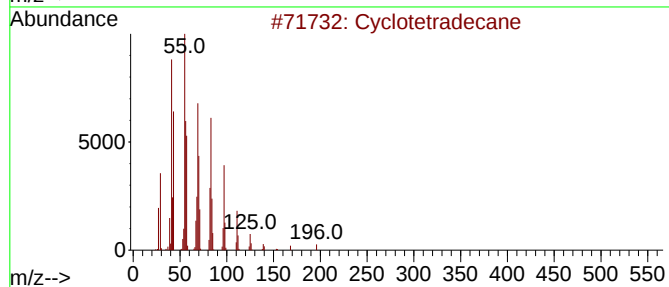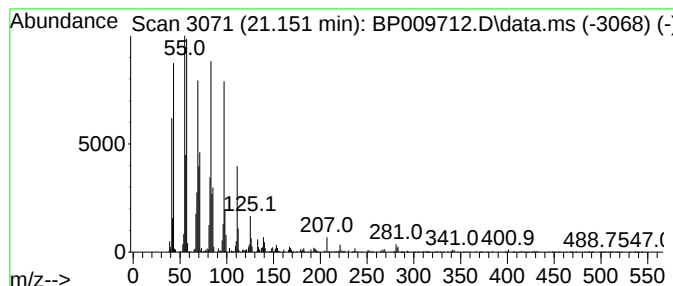

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009712.D
Acq On : 08 Apr 2022 11:59
Operator : CG/JU
Sample : N2183-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R46

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.128	37.4	ng/u1	914501	1	7.975	489107	20.0
(DEL) Alkane: C...	21.151	3.2	ng/u1	286152	5	21.439	1765280	20.0