

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009715.D
 Acq On : 08 Apr 2022 13:41
 Operator : CG/JU
 Sample : N2183-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	27	rVB	524236	806539	38.59%	3.813%
2	3.393	48	52	57	rVB	9593	15430	0.74%	0.073%
3	3.811	119	123	137	rBV	70197	126538	6.05%	0.598%
4	4.058	161	165	170	rVB7	4665	7989	0.38%	0.038%
5	4.146	175	180	183	rBV3	6234	9751	0.47%	0.046%
6	5.075	332	338	345	rVB2	7129	12625	0.60%	0.060%
7	5.216	359	362	365	rBV5	1291	2293	0.11%	0.011%
8	5.716	446	447	454	rVB7	1301	2355	0.11%	0.011%
9	7.128	678	687	698	rBV	173237	293917	14.06%	1.390%
10	7.299	710	716	727	rBV	135013	220808	10.57%	1.044%
11	7.369	727	728	733	rVB5	2348	2912	0.14%	0.014%
12	7.505	744	751	761	rBV	174003	280187	13.41%	1.325%
13	7.616	765	770	774	rVB6	2256	3828	0.18%	0.018%
14	7.975	824	831	840	rBV	343808	564831	27.03%	2.670%
15	8.052	840	844	850	rVB8	2729	5159	0.25%	0.024%
16	8.228	869	874	878	rBV8	2072	3580	0.17%	0.017%
17	8.675	941	950	960	rBV	234807	384267	18.39%	1.817%
18	8.799	966	971	978	rVB2	24381	37529	1.80%	0.177%
19	8.952	992	997	999	rVB5	1841	2508	0.12%	0.012%
20	9.134	1020	1028	1039	rBV	176238	302448	14.47%	1.430%
21	9.310	1056	1058	1064	rVB7	2719	3942	0.19%	0.019%
22	9.599	1102	1107	1117	rVB5	6281	12726	0.61%	0.060%
23	9.857	1141	1151	1160	rBV	133377	231206	11.06%	1.093%
24	9.987	1169	1173	1176	rBV6	2181	2947	0.14%	0.014%
25	10.228	1208	1214	1217	rVB6	1842	3031	0.15%	0.014%
26	10.398	1237	1243	1254	rVB	224164	373705	17.88%	1.767%
27	10.581	1270	1274	1279	rVB7	2434	3711	0.18%	0.018%
28	10.787	1300	1309	1320	rBV	504593	871101	41.68%	4.118%
29	10.910	1322	1330	1340	rVV	216666	381610	18.26%	1.804%
30	11.322	1394	1400	1406	rBV10	2739	6178	0.30%	0.029%
31	11.404	1410	1414	1417	rBV6	1957	2707	0.13%	0.013%
32	11.445	1417	1421	1425	rVB6	1917	3400	0.16%	0.016%
33	11.581	1438	1444	1450	rVB10	2594	5459	0.26%	0.026%
34	12.228	1548	1554	1559	rVB7	4183	7590	0.36%	0.036%
35	12.369	1573	1578	1583	rBV3	5822	8374	0.40%	0.040%
36	13.034	1688	1691	1694	rVB5	2459	2294	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009715.D
 Acq On : 08 Apr 2022 13:41
 Operator : CG/JU
 Sample : N2183-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	13.228	1720	1724	1727	rBV6	1945	2590	0.12%	0.012%
38	13.345	1740	1744	1748	rBV7	2246	3138	0.15%	0.015%
39	13.457	1758	1763	1768	rBV4	11760	19249	0.92%	0.091%
40	13.587	1782	1785	1789	rVB6	1679	2237	0.11%	0.011%

41	13.887	1833	1836	1841	rBV6	1600	2351	0.11%	0.011%
42	14.016	1849	1858	1865	rBV	539624	756810	36.21%	3.578%
43	14.298	1896	1906	1917	rBV	503209	774374	37.05%	3.661%
44	14.522	1940	1944	1947	rBV3	5366	7046	0.34%	0.033%
45	14.610	1951	1959	1970	rVV	880404	1327925	63.54%	6.278%

46	14.781	1981	1988	1995	rBV	242621	360481	17.25%	1.704%
47	15.022	2023	2029	2034	rBV7	16001	25357	1.21%	0.120%
48	15.251	2065	2068	2072	rVB6	1882	2668	0.13%	0.013%
49	15.422	2091	2097	2102	rBV8	5406	9830	0.47%	0.046%
50	15.475	2102	2106	2109	rBV6	3326	4838	0.23%	0.023%

51	15.598	2121	2127	2135	rBV	749319	1069459	51.17%	5.056%
52	15.704	2139	2145	2154	rBV	200745	285343	13.65%	1.349%
53	15.845	2164	2169	2173	rBV5	7673	10082	0.48%	0.048%
54	15.963	2187	2189	2194	rVB6	2750	4299	0.21%	0.020%
55	16.339	2249	2253	2256	rBV6	2064	2580	0.12%	0.012%

56	16.381	2258	2260	2263	rBV4	2259	2377	0.11%	0.011%
57	16.510	2280	2282	2287	rVB6	1608	2325	0.11%	0.011%
58	16.610	2296	2299	2300	rBV3	2038	2397	0.11%	0.011%
59	16.769	2321	2326	2330	rVB8	5128	8461	0.40%	0.040%
60	16.980	2359	2362	2365	rBV5	1773	2484	0.12%	0.012%

61	17.139	2383	2389	2395	rBV6	6528	14751	0.71%	0.070%
62	17.357	2420	2426	2437	rBV	1172090	1729267	82.75%	8.175%
63	17.457	2437	2443	2454	rVV	956599	1367210	65.42%	6.464%
64	17.545	2454	2458	2463	rVB5	20981	29066	1.39%	0.137%
65	17.651	2474	2476	2480	rVB5	3819	3567	0.17%	0.017%

66	18.039	2539	2542	2548	rVB7	9237	11825	0.57%	0.056%
67	18.133	2553	2558	2562	rBV7	7668	13945	0.67%	0.066%
68	18.245	2573	2577	2585	rBV2	48194	66455	3.18%	0.314%
69	18.316	2587	2589	2594	rVB4	6695	8162	0.39%	0.039%
70	18.604	2636	2638	2640	rBV3	3025	3353	0.16%	0.016%

71	18.669	2645	2649	2654	rBV5	17305	24786	1.19%	0.117%
72	19.263	2747	2750	2755	rVB5	17018	21656	1.04%	0.102%
73	19.333	2758	2762	2765	rBV4	18655	27563	1.32%	0.130%
74	19.474	2784	2786	2791	rVB6	10915	13538	0.65%	0.064%
75	19.686	2816	2822	2828	rBV	1403354	1835609	87.84%	8.678%

76	21.151	3068	3071	3077	rBV2	123378	163213	7.81%	0.772%
----	--------	------	------	------	------	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009715.D
Acq On : 08 Apr 2022 13:41
Operator : CG/JU
Sample : N2183-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R30

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION

77	21.439	3115	3120	3128	rBV	1591721	2089821	100.00%	9.880%
78	23.757	3507	3514	3525	rVB	964184	1947828	93.21%	9.209%
79	23.915	3535	3541	3552	rVB2	992304	2086471	99.84%	9.864%




Sum of corrected areas: 21152262

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009715.D
Acq On : 08 Apr 2022 13:41
Operator : CG/JU
Sample : N2183-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R30

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

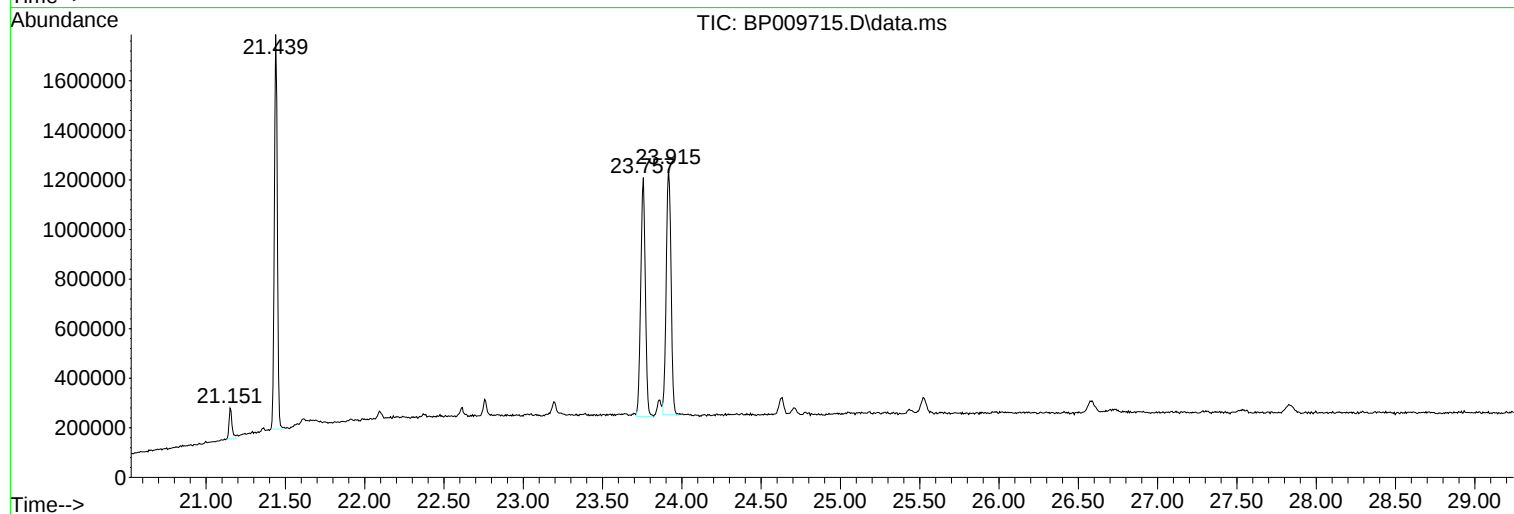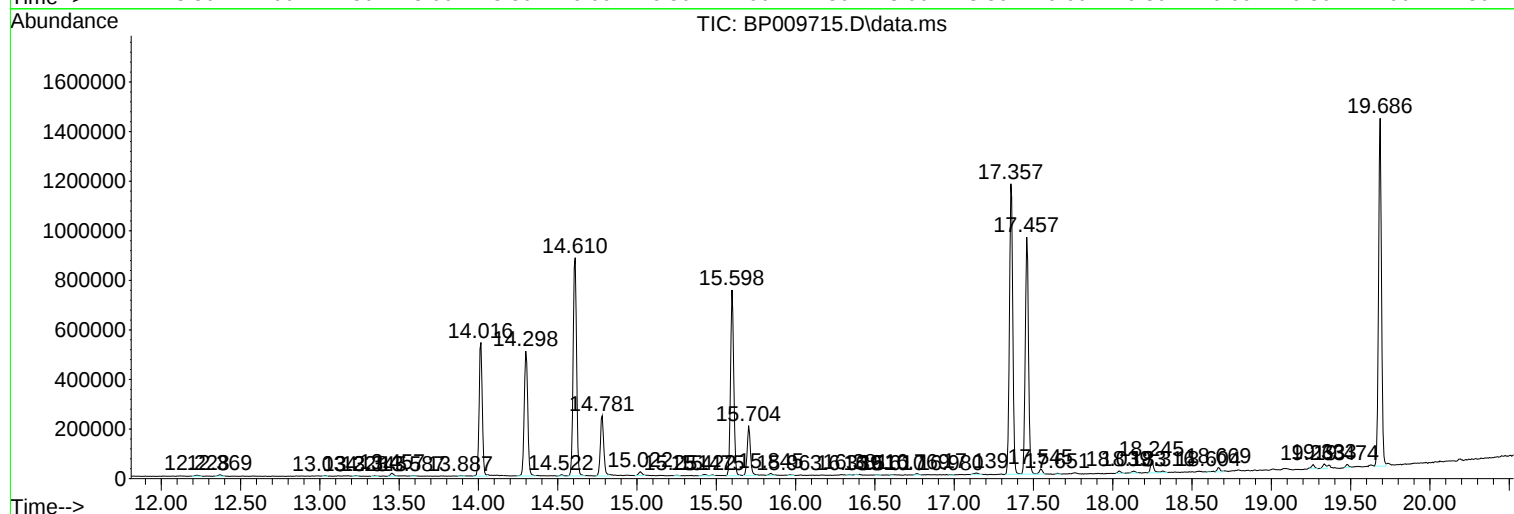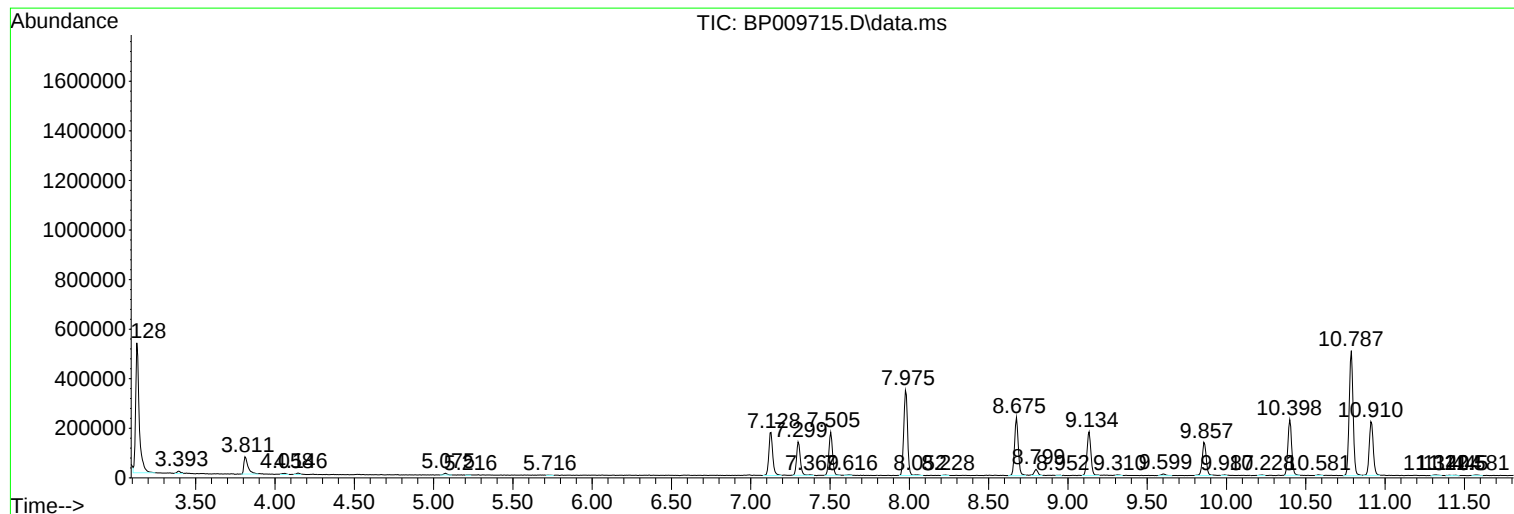

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009715.D
Acq On : 08 Apr 2022 13:41
Operator : CG/JU
Sample : N2183-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COR30










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.128	28.56 ng/ul	806539	1,4-Dichlorobenzene-d4	7.975

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	27
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

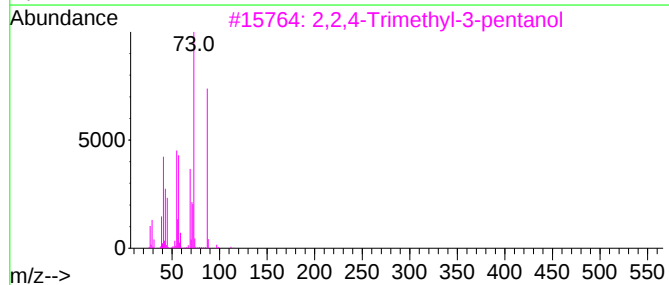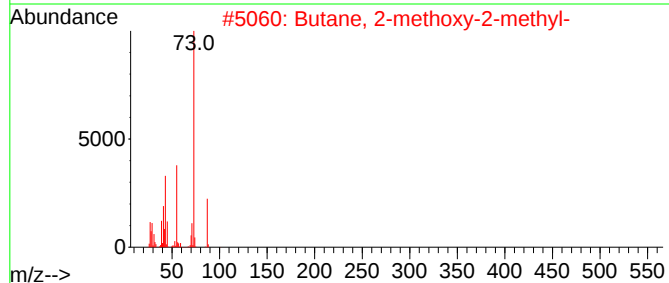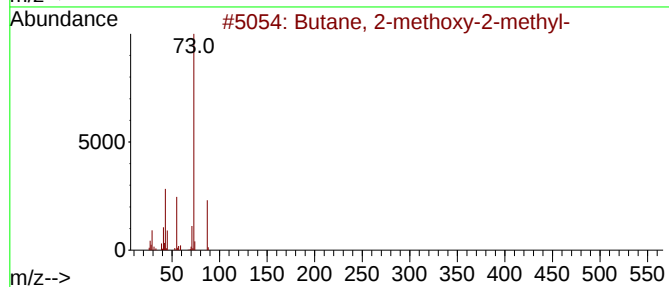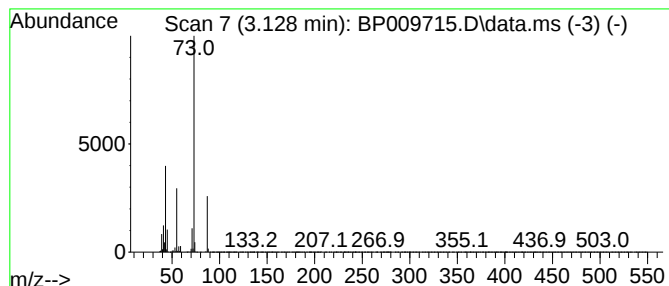

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009715.D
Acq On : 08 Apr 2022 13:41
Operator : CG/JU
Sample : N2183-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R30

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.128	28.6	ng/ul	806539	1	7.975	564831	20.0