

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
 Data File : BP009726.D
 Acq On : 08 Apr 2022 20:28
 Operator : CG/JU
 Sample : PB143934BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK934

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	12	rVB2	17342	23554	0.58%	0.058%
2	3.387	48	51	61	rVB	31416	48656	1.19%	0.120%
3	3.805	118	122	139	rBV	446561	714454	17.52%	1.756%
4	4.146	176	180	185	rBV	8618	11519	0.28%	0.028%
5	7.122	678	686	698	rBV	560338	915734	22.46%	2.250%
6	7.299	709	716	727	rBV	435494	690122	16.93%	1.696%
7	7.505	744	751	767	rVB	556071	908810	22.29%	2.233%
8	7.975	823	831	842	rBV	467032	746134	18.30%	1.834%
9	8.675	943	950	963	rBV	736105	1189703	29.18%	2.924%
10	9.134	1020	1028	1037	rBV	589255	992131	24.33%	2.438%
11	9.857	1140	1151	1166	rBV	504651	828785	20.33%	2.037%
12	10.399	1235	1243	1253	rBV	727166	1232735	30.23%	3.029%
13	10.781	1301	1308	1321	rVB	646052	1124445	27.58%	2.763%
14	10.910	1322	1330	1341	rVV	787970	1325089	32.50%	3.256%
15	12.369	1571	1578	1585	rBV	14657	26213	0.64%	0.064%
16	12.575	1609	1613	1619	rBV8	2080	4445	0.11%	0.011%
17	13.887	1832	1836	1843	rBV8	5241	8582	0.21%	0.021%
18	14.016	1851	1858	1871	rBV	1513510	2150132	52.73%	5.284%
19	14.298	1899	1906	1921	rBV	1574030	2305540	56.55%	5.666%
20	14.604	1951	1958	1968	rBV	1155907	1665708	40.85%	4.093%
21	14.781	1979	1988	2003	rBV	843802	1191001	29.21%	2.927%
22	15.016	2024	2028	2035	rVB9	1948	4201	0.10%	0.010%
23	15.598	2120	2127	2138	rBV	2104084	2965520	72.73%	7.288%
24	15.704	2138	2145	2160	rVV	744379	1048811	25.72%	2.577%
25	15.839	2163	2168	2174	rVB	21762	32508	0.80%	0.080%
26	16.387	2256	2261	2267	rVB6	6658	10346	0.25%	0.025%
27	17.034	2367	2371	2374	rBV6	5092	5866	0.14%	0.014%
28	17.139	2385	2389	2395	rBV2	7214	10674	0.26%	0.026%
29	17.357	2419	2426	2435	rBV	1480463	2110070	51.75%	5.186%
30	17.457	2436	2443	2454	rVV	2354678	3364468	82.52%	8.268%
31	17.728	2484	2489	2492	rBV7	2719	4111	0.10%	0.010%
32	19.263	2745	2750	2755	rBV3	31451	45598	1.12%	0.112%
33	19.328	2756	2761	2766	rBV	33756	46178	1.13%	0.113%
34	19.686	2815	2822	2828	rBV	2928339	4062792	99.65%	9.984%
35	21.439	3114	3120	3125	rBV	1777239	2431249	59.63%	5.975%
36	23.757	3506	3514	3524	rVB	2056190	4077248	100.00%	10.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009726.D
Acq On : 08 Apr 2022 20:28
Operator : CG/JU
Sample : PB143934BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK934

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION

37	23.916	3534	3541	3550	rVB2	1130829	2368553	58.09%	5.821%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 40691685

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009726.D
Acq On : 08 Apr 2022 20:28
Operator : CG/JU
Sample : PB143934BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK934

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

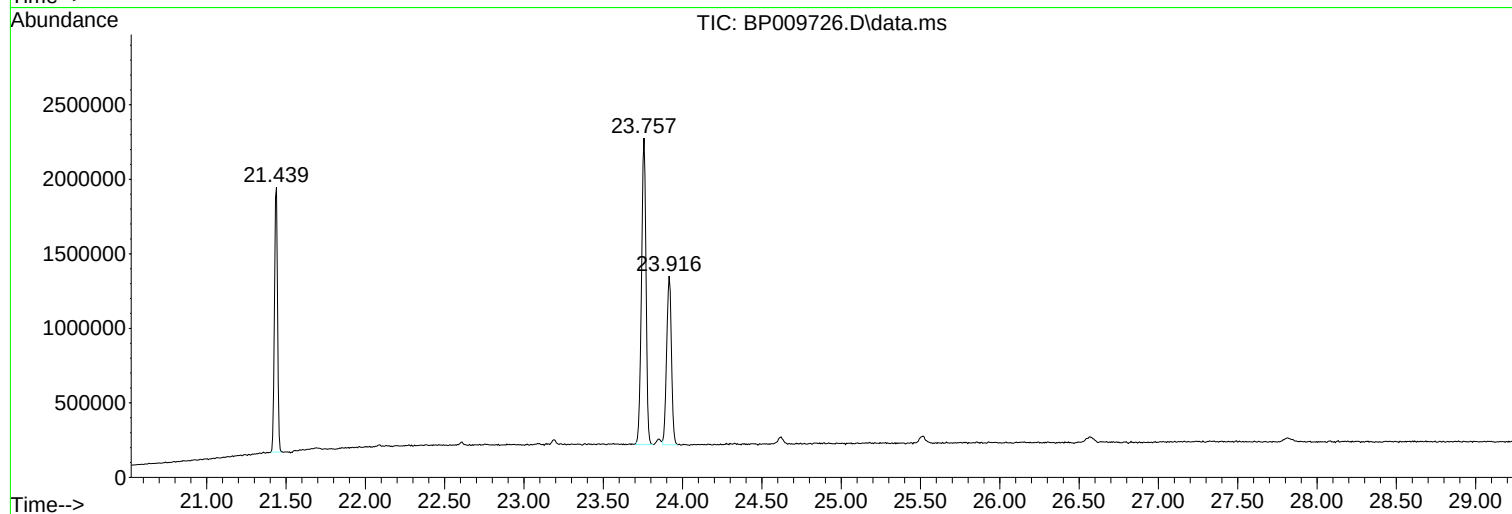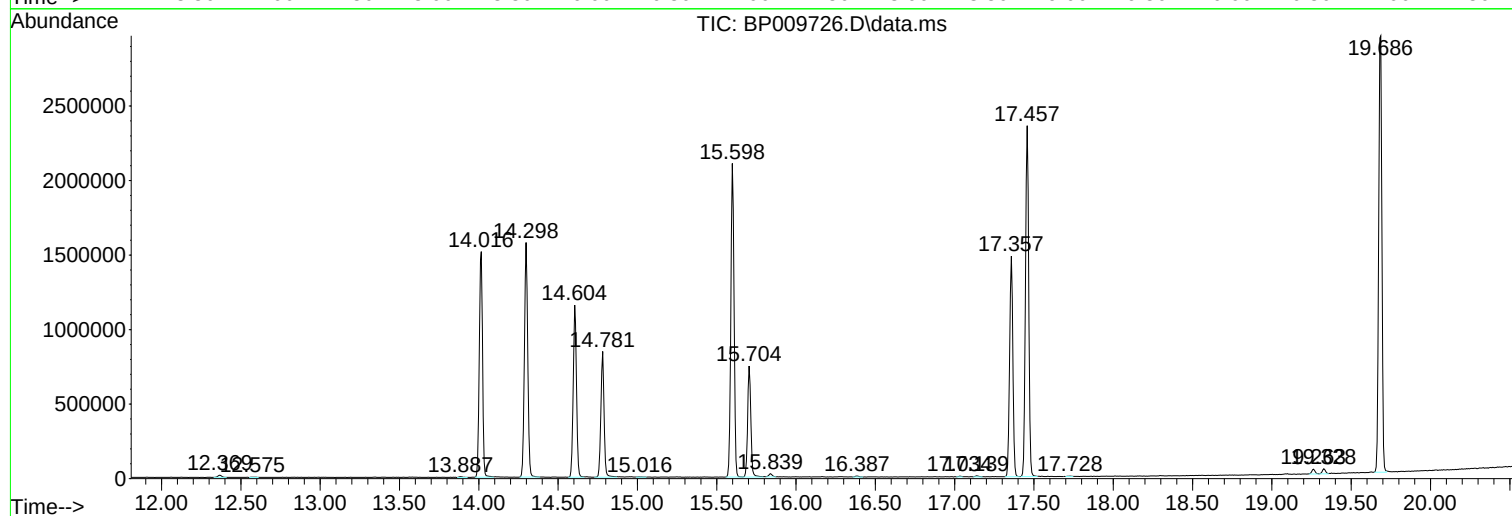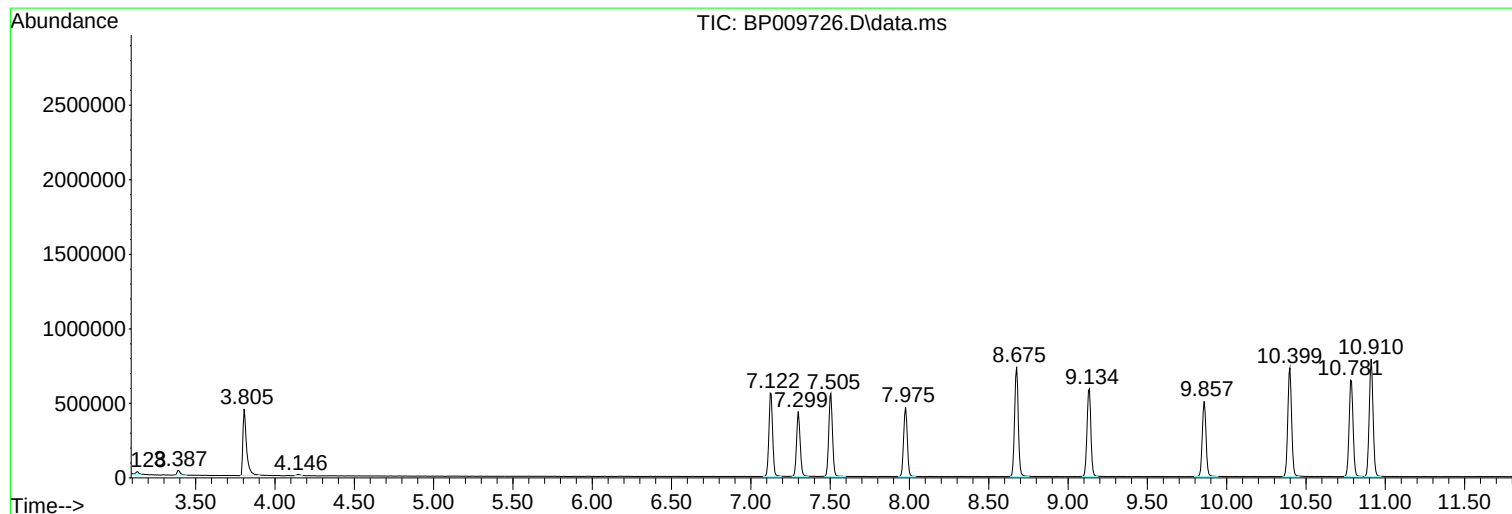

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009726.D
Acq On : 08 Apr 2022 20:28
Operator : CG/JU
Sample : PB143934BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK934

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040822\
Data File : BP009726.D
Acq On : 08 Apr 2022 20:28
Operator : CG/JU
Sample : PB143934BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK934

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
