

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041025\
 Data File : BP024249.D
 Acq On : 10 Apr 2025 12:35
 Operator : RC/JU
 Sample : Q1745-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 IB-6.5-WC

Quant Time: Apr 10 13:02:32 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 10 11:43:37 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.740	152	285331	20.000	ng	0.00
21) Naphthalene-d8	10.516	136	1116410	20.000	ng	-0.01
39) Acenaphthene-d10	14.375	164	652208	20.000	ng	-0.02
64) Phenanthrene-d10	17.180	188	1289734	20.000	ng	-0.01
76) Chrysene-d12	21.616	240	1454072	20.000	ng	-0.03
86) Perylene-d12	24.968	264	1698482	20.000	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.358	112	2355292	131.767	ng	0.00
7) Phenol-d6	6.922	99	2717762	113.699	ng	0.00
23) Nitrobenzene-d5	8.887	82	1899504	95.997	ng	0.00
42) 2,4,6-Tribromophenol	15.898	330	1366931	166.387	ng	0.00
45) 2-Fluorobiphenyl	12.987	172	4046305	91.480	ng	-0.01
79) Terphenyl-d14	19.892	244	6875553	97.606	ng	-0.02


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041025\
Data File : BP024249.D
Acq On : 10 Apr 2025 12:35
Operator : RC/JU
Sample : Q1745-12
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
IB-6.5-WC

Quant Time: Apr 10 13:02:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 10 11:43:37 2025
Response via : Initial Calibration




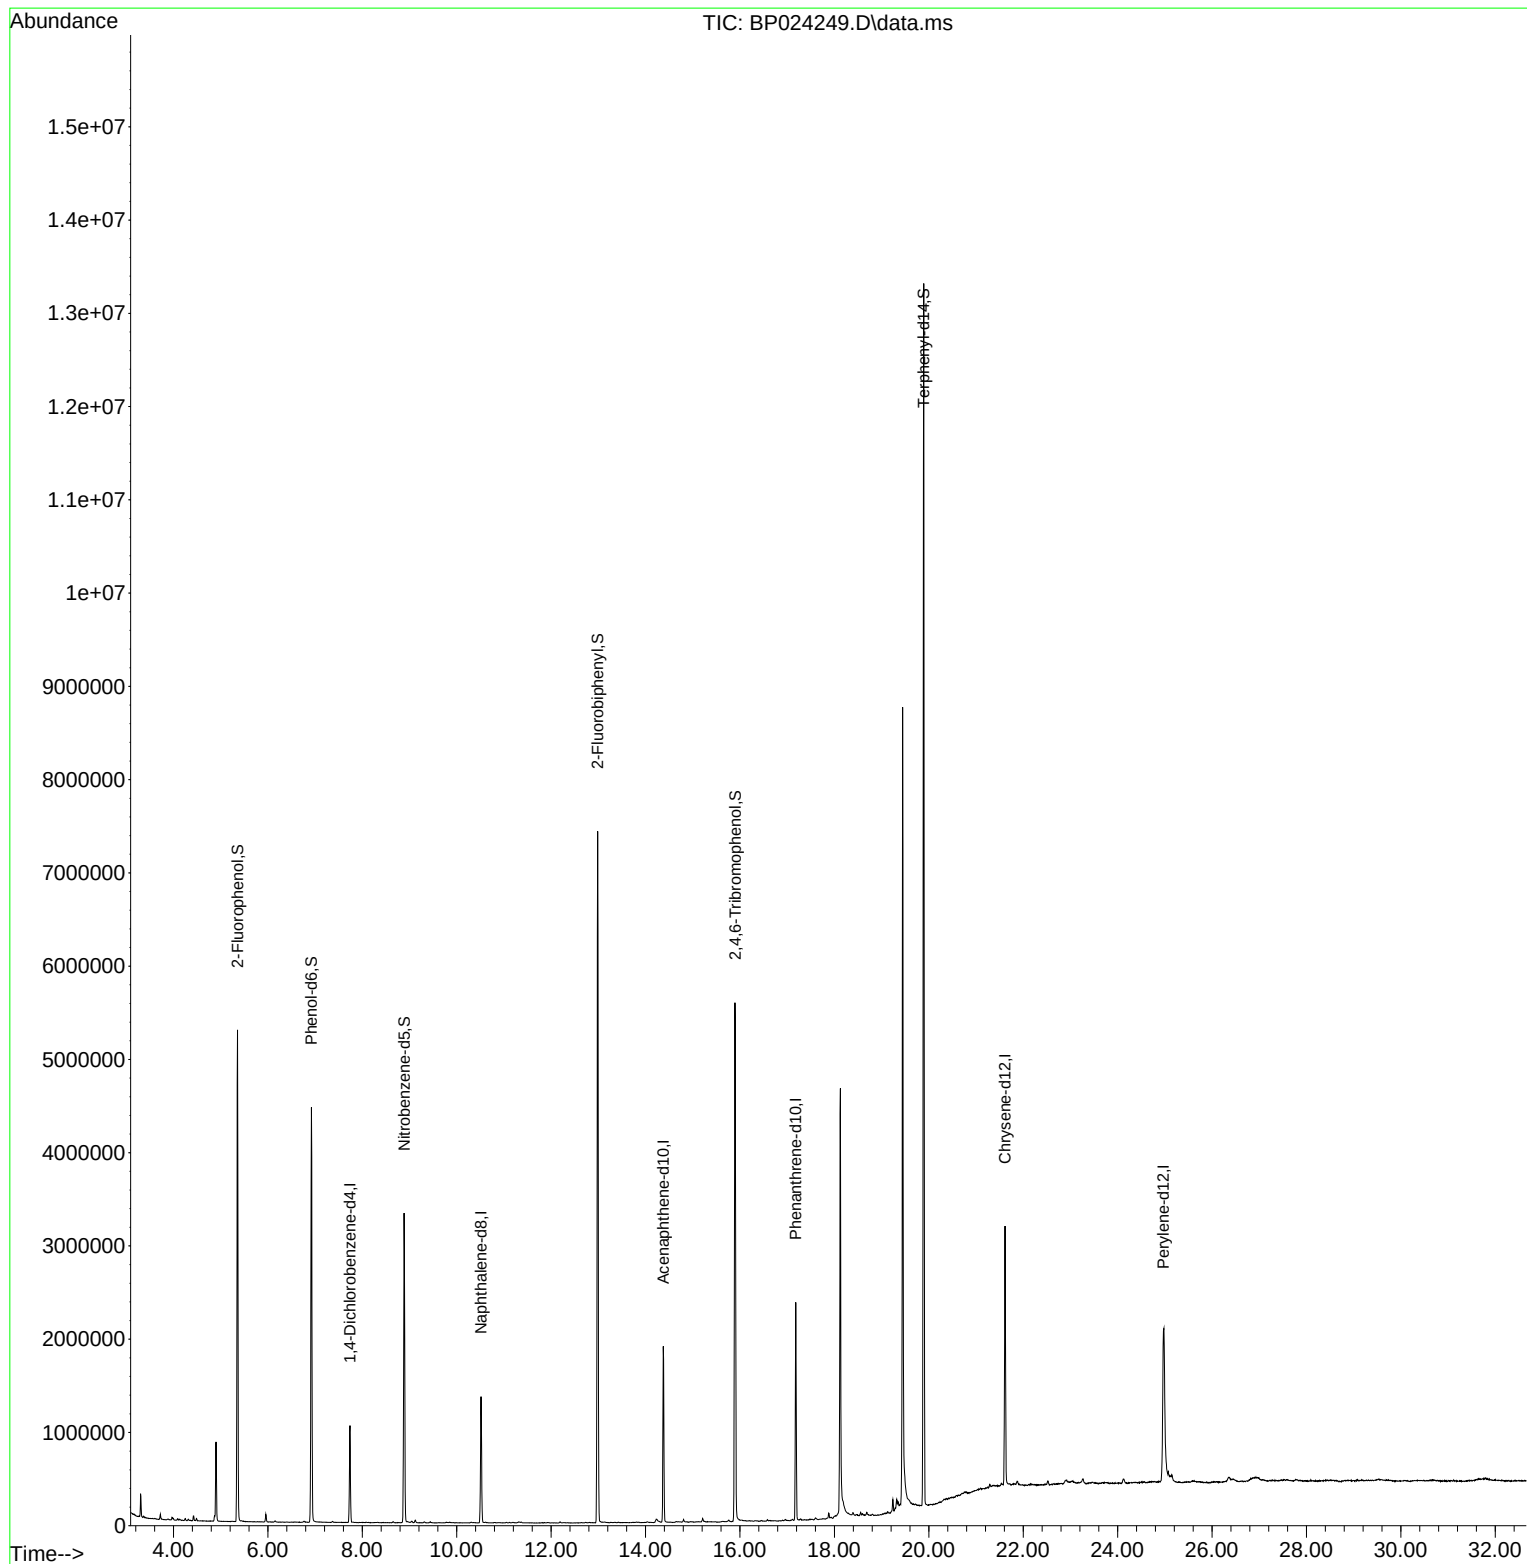




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.740 min Scan# 796
Delta R.T. -0.006 min
Lab File: BP024249.D
Acq: 10 Apr 2025 12:35




Instrument :
BNA_P
ClientSampleId :
IB-6.5-WC


Tgt Ion:152 Resp: 285331
Ion Ratio Lower Upper
152 100
150 156.3 125.5 188.3
115 60.1 46.3 69.5

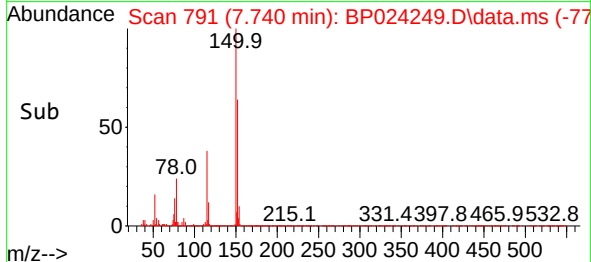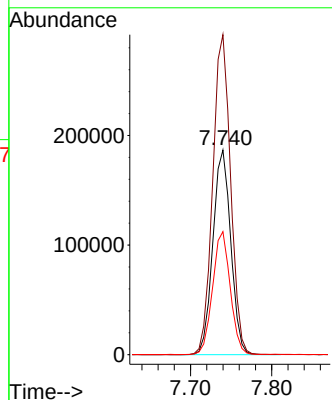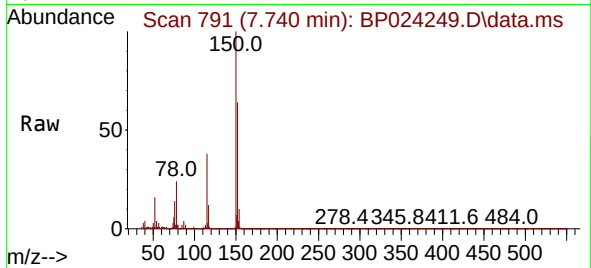

#5
2-Fluorophenol
Concen: 131.767 ng
RT: 5.358 min Scan# 386
Delta R.T. 0.000 min
Lab File: BP024249.D
Acq: 10 Apr 2025 12:35

Tgt Ion:112 Resp: 2355292
Ion Ratio Lower Upper
112 100
64 51.9 41.3 61.9
63 25.8 20.6 31.0

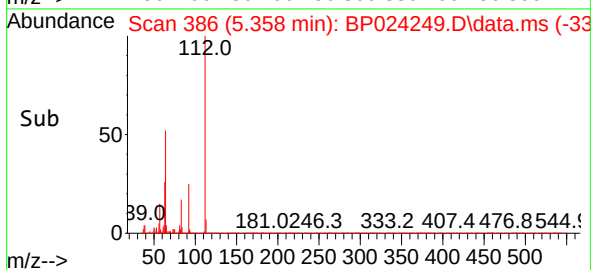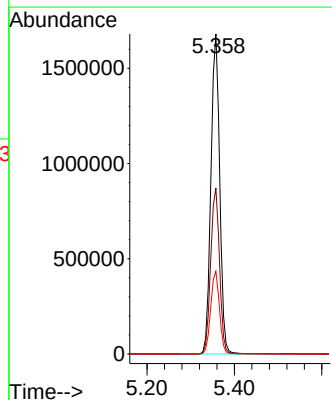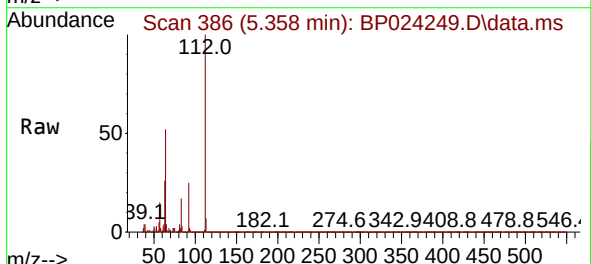







#7
Phenol-d6
Concen: 113.699 ng
RT: 6.922 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP024249.D
Acq: 10 Apr 2025 12:35

Instrument :
BNA_P
ClientSampleId :
IB-6.5-WC

Tgt Ion: 99 Resp: 2717762




Ion	Ratio	Lower	Upper
99	100		
42	13.6	10.6	16.0
71	30.4	23.3	34.9

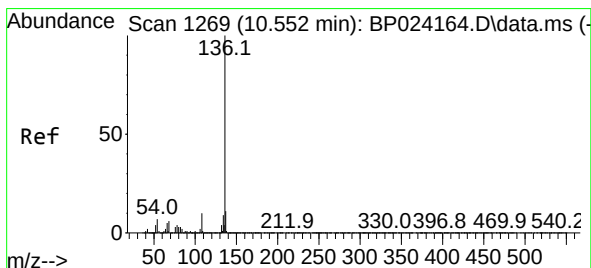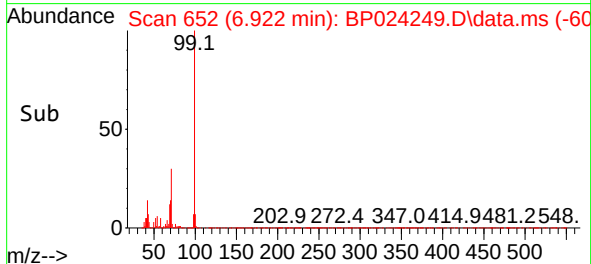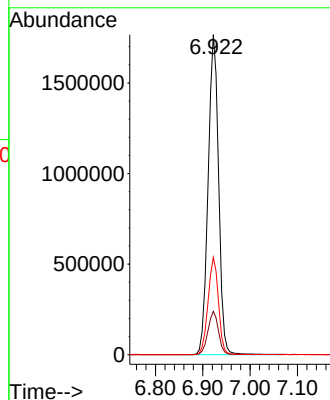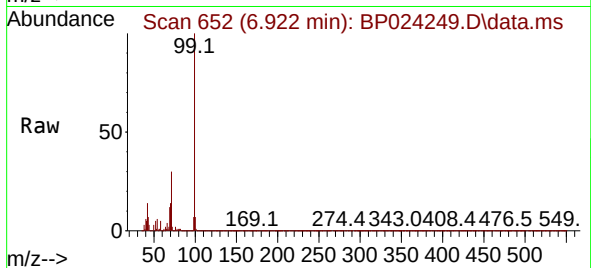


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.516 min Scan# 1263
Delta R.T. -0.012 min
Lab File: BP024249.D
Acq: 10 Apr 2025 12:35

Tgt Ion:136 Resp: 1116410

Ion	Ratio	Lower	Upper
136	100		
137	10.8	9.0	13.4
54	6.9	5.3	7.9
68	6.7	5.0	7.4


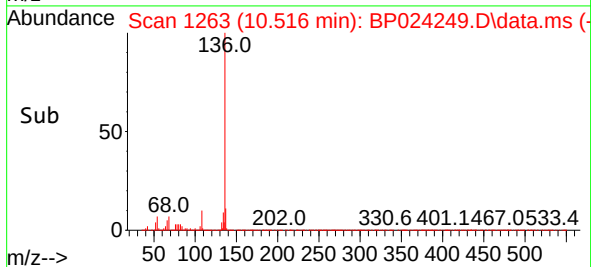
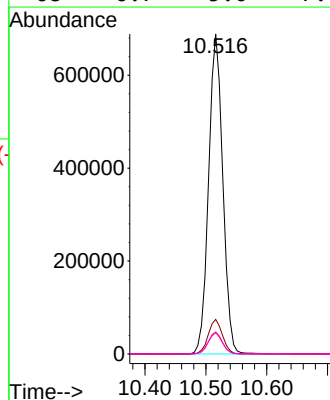
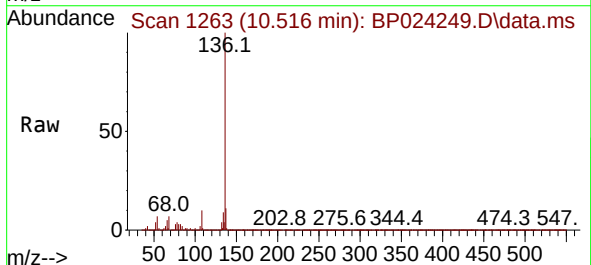




#23
Nitrobenzene-d5
Concen: 95.997 ng
RT: 8.887 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP024249.D
Acq: 10 Apr 2025 12:35




Instrument :
BNA_P
ClientSampleId :
IB-6.5-WC


Tgt Ion: 82 Resp: 1899504
Ion Ratio Lower Upper
82 100
128 46.8 37.4 56.0
54 41.1 32.5 48.7

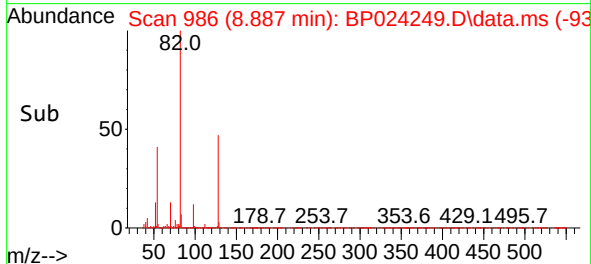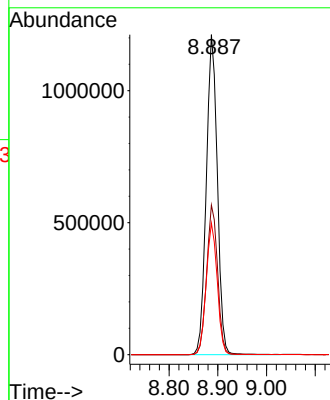

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.375 min Scan# 1919
Delta R.T. -0.018 min
Lab File: BP024249.D
Acq: 10 Apr 2025 12:35

Tgt Ion: 164 Resp: 652208
Ion Ratio Lower Upper
164 100
162 100.2 80.6 121.0
160 44.6 35.4 53.2


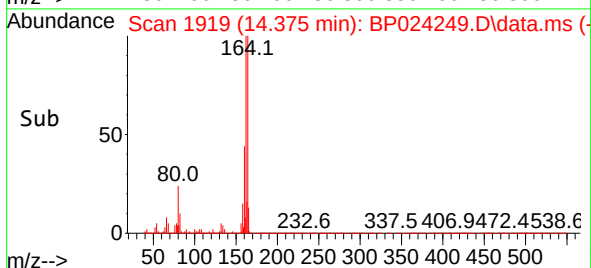
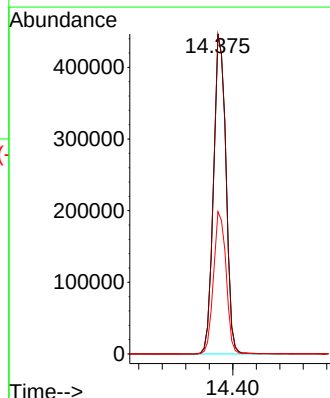
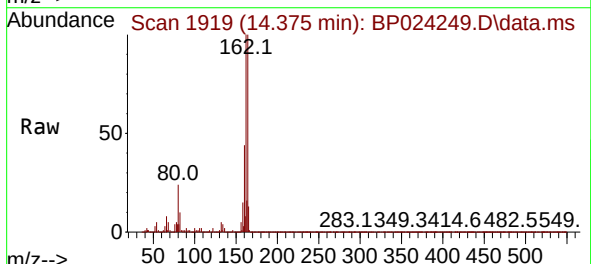




#42
2,4,6-Tribromophenol
Concen: 166.387 ng
RT: 15.898 min Scan# 2181
Delta R.T. 0.000 min
Lab File: BP024249.D
Acq: 10 Apr 2025 12:35




Instrument :
BNA_P
ClientSampleId :
IB-6.5-WC


Tgt Ion:330 Resp: 1366931
Ion Ratio Lower Upper
330 100
332 97.0 77.6 116.4
141 29.8 25.0 37.6

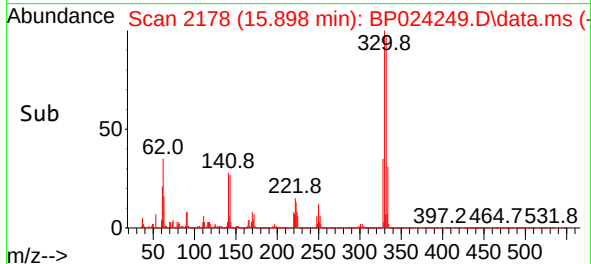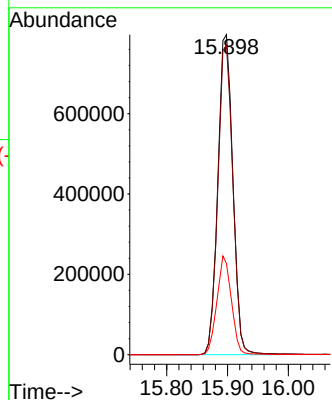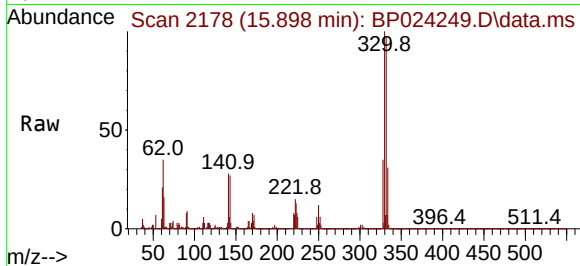

#45
2-Fluorobiphenyl
Concen: 91.480 ng
RT: 12.987 min Scan# 1683
Delta R.T. -0.012 min
Lab File: BP024249.D
Acq: 10 Apr 2025 12:35

Tgt Ion:172 Resp: 4046305
Ion Ratio Lower Upper
172 100
171 35.7 28.3 42.5
170 23.7 19.0 28.4

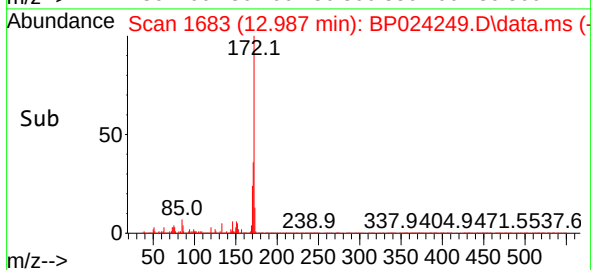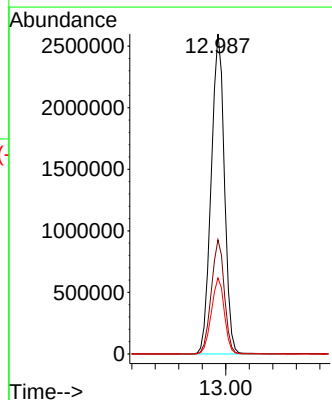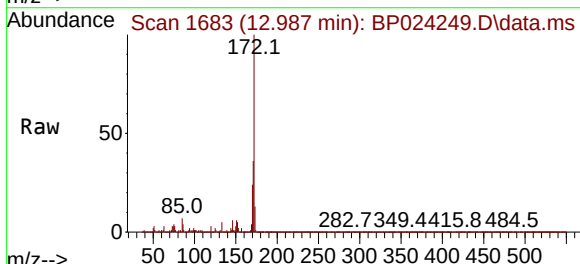




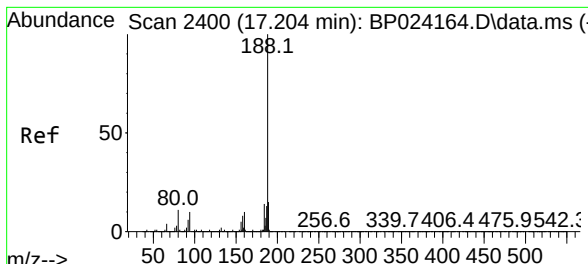


#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.180 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP024249.D
 Acq: 10 Apr 2025 12:35

Instrument :
 BNA_P
 ClientSampleId :
 IB-6.5-WC

Tgt Ion:188 Resp: 1289734




Ion	Ratio	Lower	Upper
188	100		
94	10.9	8.1	12.1
80	11.9	8.9	13.3

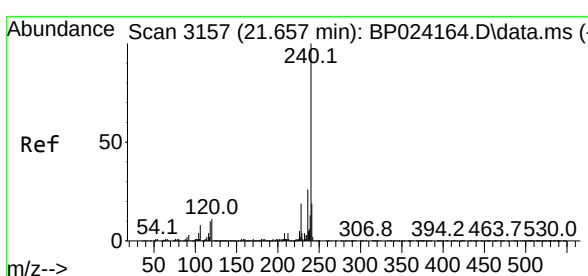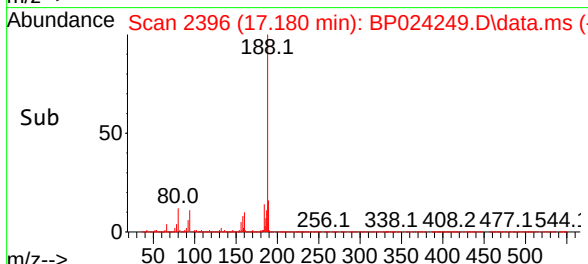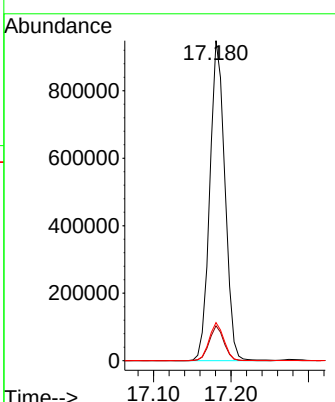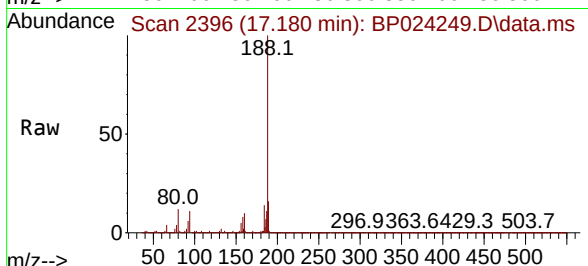


#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.616 min Scan# 3150
 Delta R.T. -0.029 min
 Lab File: BP024249.D
 Acq: 10 Apr 2025 12:35

Tgt Ion:240 Resp: 1454072

Ion	Ratio	Lower	Upper
240	100		
120	11.7	9.2	13.8
236	25.4	20.4	30.6


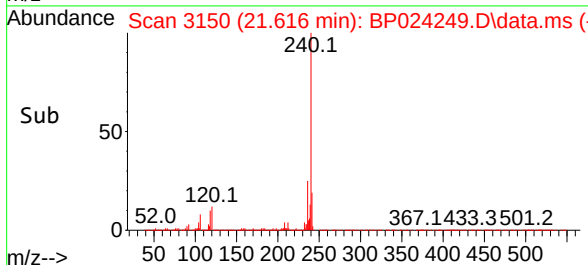
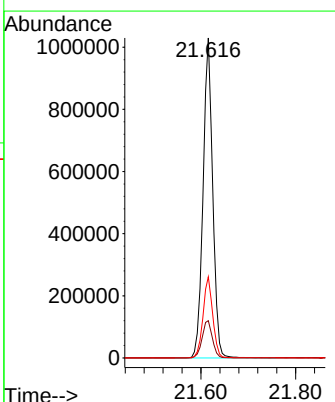
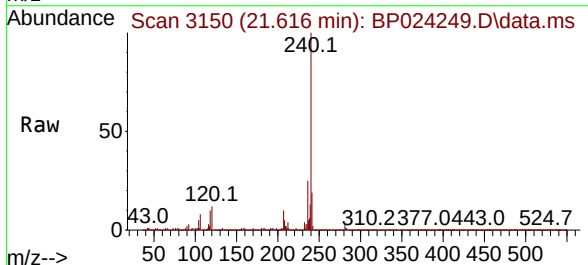




#79
 Terphenyl-d14
 Concen: 97.606 ng
 RT: 19.892 min Scan# 21
 Delta R.T. -0.023 min
 Lab File: BP024249.D
 Acq: 10 Apr 2025 12:35

Instrument :
 BNA_P
 ClientSampleId :
 IB-6.5-WC

Tgt Ion:244 Resp: 6875553
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.7 8.5
 122 11.6 9.6 14.4

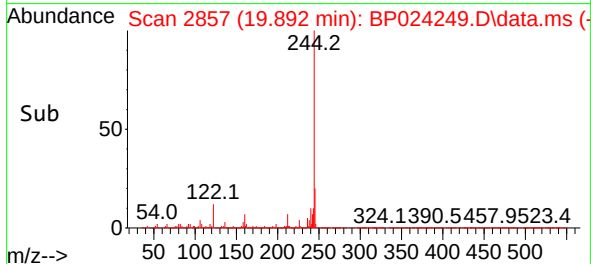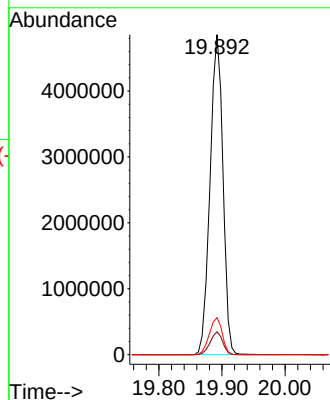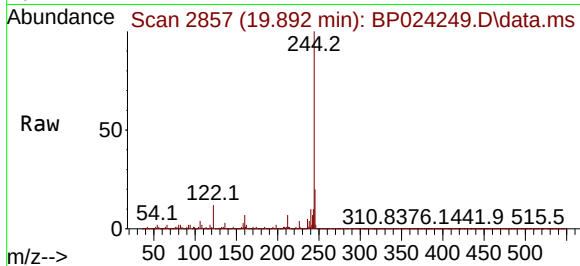

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.968 min Scan# 3720
 Delta R.T. -0.041 min
 Lab File: BP024249.D
 Acq: 10 Apr 2025 12:35

Tgt Ion:264 Resp: 1698482
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.5 27.7
 265 22.5 17.7 26.5

