
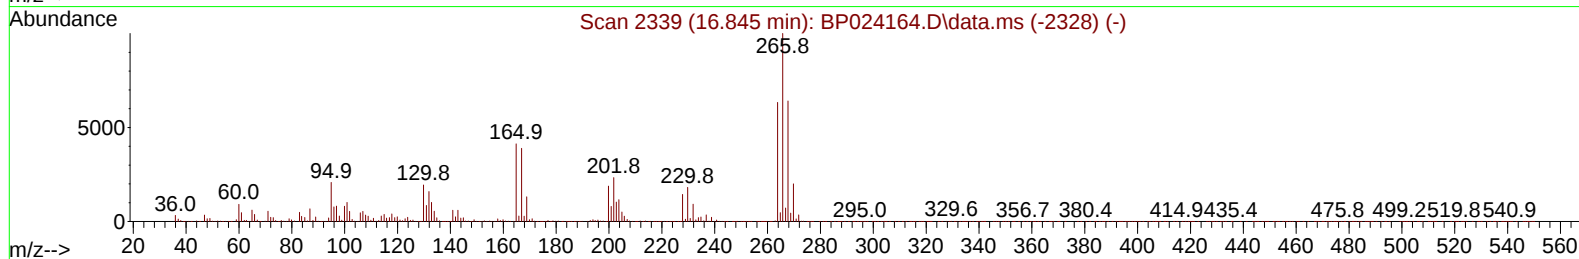
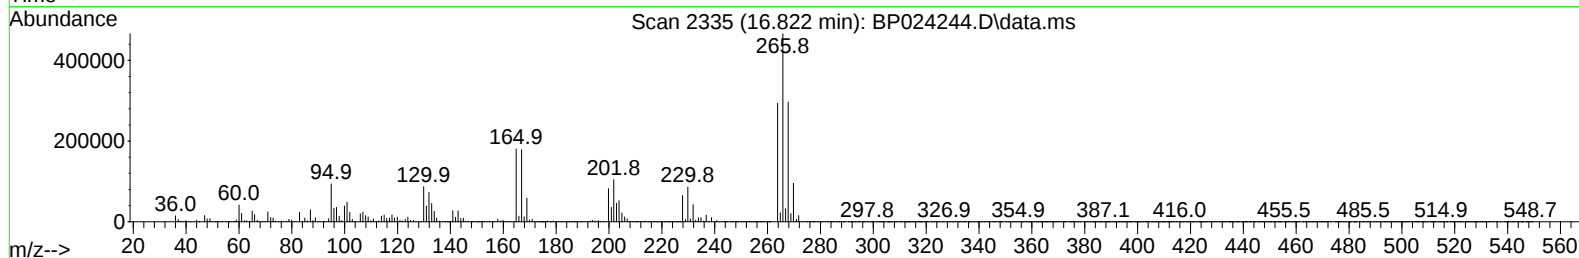


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP041025\  
Data File : BP024244.D  
Acq On : 10 Apr 2025 09:05  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 14:43:14 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 10 11:43:37 2025  
Response via : Initial Calibration

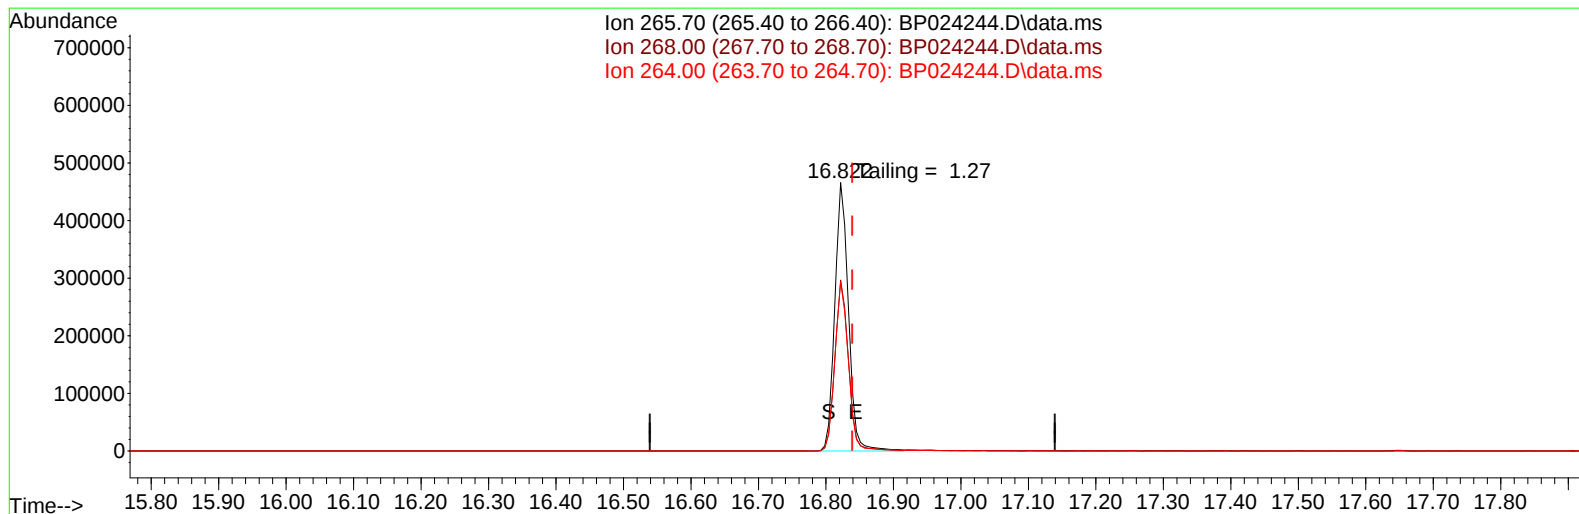

TIC: BP024244.D\data.ms

**(70) Pentachlorophenol (C)**




**16.822min (-0.018) 2689216.60 ng**

**response 655373**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.10  | 63.70  |
| 264.00 | 63.30  | 63.06  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP041025\  
Data File : BP024244.D  
Acq On : 10 Apr 2025 09:05  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 14:43:14 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 10 11:43:37 2025  
Response via : Initial Calibration

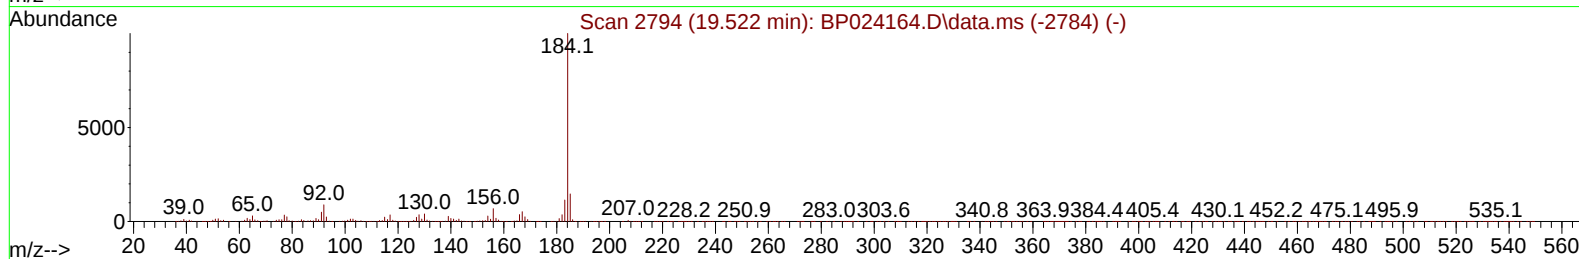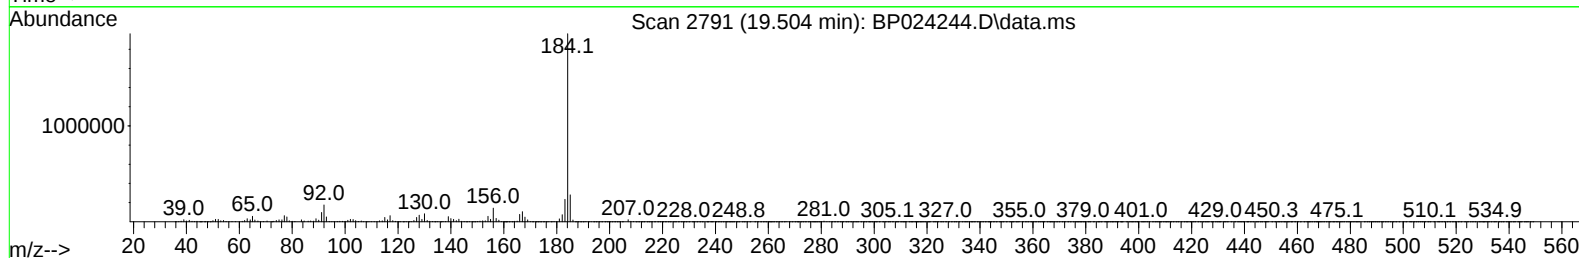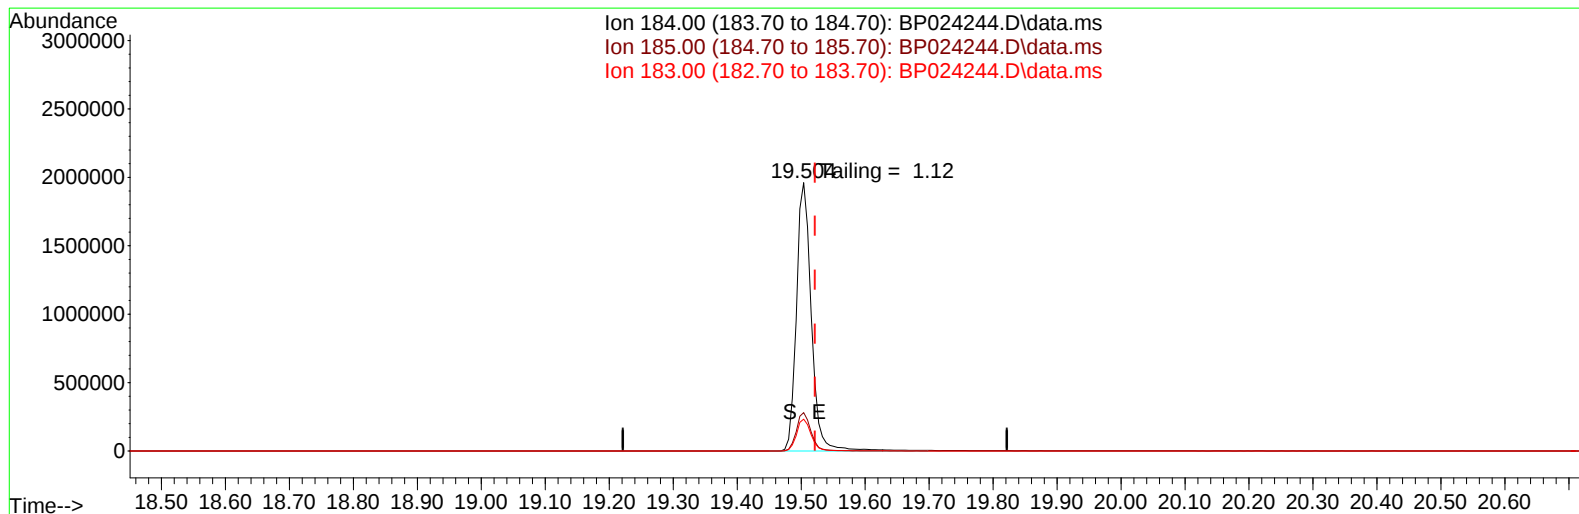

TIC: BP024244.D\data.ms

**(77) Benzidine****19.504min (-0.018) 3933451.82 ng****response 3182452**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 14.33  |
| 183.00 | 11.40  | 11.89  |
| 0.00   | 0.00   | 0.00   |