
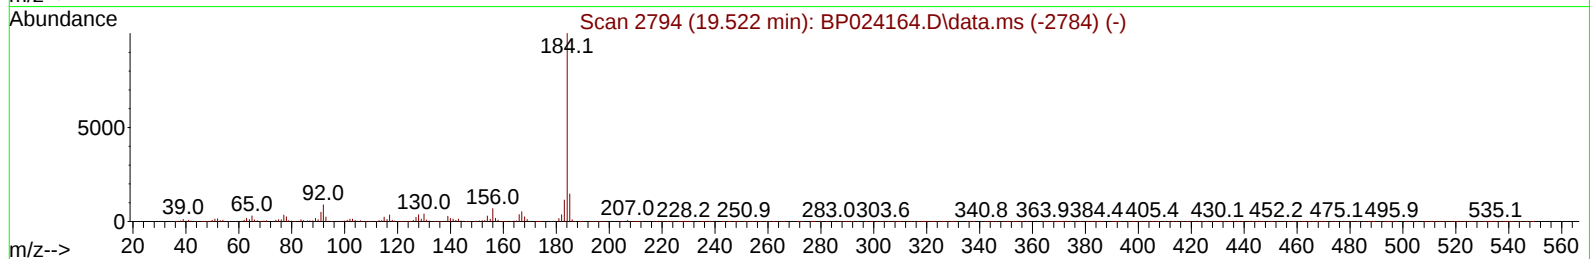
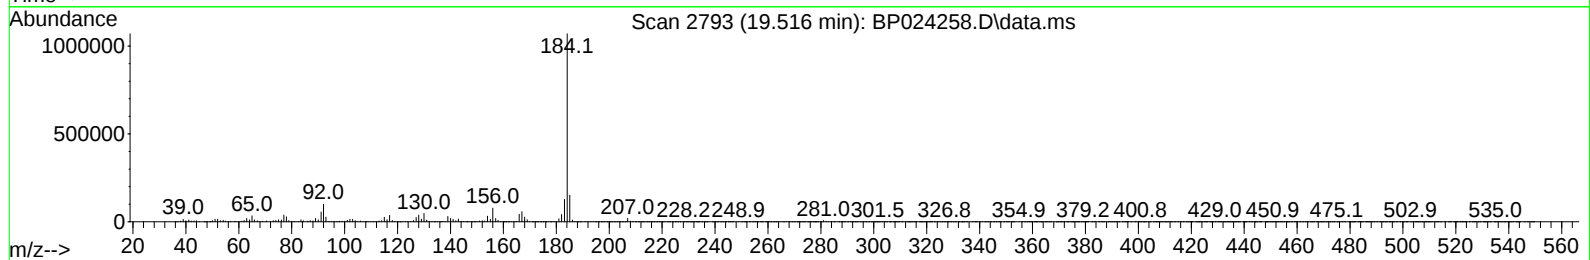


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041125\
Data File : BP024258.D
Acq On : 11 Apr 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 11:43:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 10 11:43:37 2025
Response via : Initial Calibration

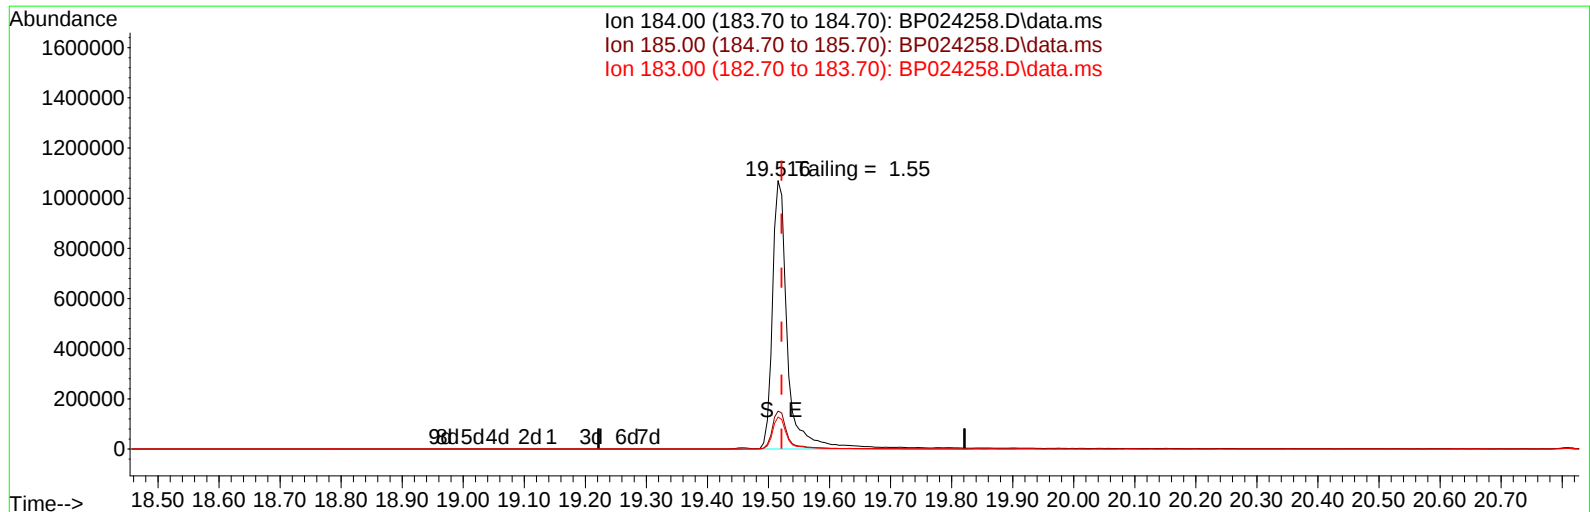

TIC: BP024258.D\data.ms

(77) Benzidine

19.516min (-0.006) 993482.96 ng m

response 1879156

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.14
183.00	11.40	11.94
0.00	0.00	0.00