

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041125\
 Data File : BP024260.D
 Acq On : 11 Apr 2025 10:23
 Operator : RC/JU
 Sample : PB167537BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB167537BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.916	306	311	322	rBV	1431560	1891634	10.71%	2.339%
2	5.375	382	389	401	rBV	6036190	8515868	48.20%	10.529%
3	5.975	486	491	498	rBV	215185	302701	1.71%	0.374%
4	6.946	647	656	674	rBV	5137685	8496720	48.09%	10.505%
5	7.757	787	794	803	rVB	1035374	1564325	8.85%	1.934%
6	8.910	980	990	1008	rBV	3299246	5504207	31.16%	6.805%
7	10.540	1258	1267	1281	rBV	1250680	2162531	12.24%	2.674%
8	13.004	1678	1686	1699	rBV	8780491	12445605	70.45%	15.388%
9	14.386	1912	1921	1934	rBV	1858083	2722915	15.41%	3.367%
10	15.904	2170	2179	2198	rBV	5713887	9338377	52.86%	11.546%
11	17.192	2390	2398	2412	rBV2	2008239	3079397	17.43%	3.807%
12	19.916	2854	2861	2875	rBV	12399590	17666801	100.00%	21.843%
13	21.639	3148	3154	3168	rBV2	2125280	3510961	19.87%	4.341%
14	25.003	3718	3726	3745	rVB	1236860	3678416	20.82%	4.548%




Sum of corrected areas: 80880458

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041125\
Data File : BP024260.D
Acq On : 11 Apr 2025 10:23
Operator : RC/JU
Sample : PB167537BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167537BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

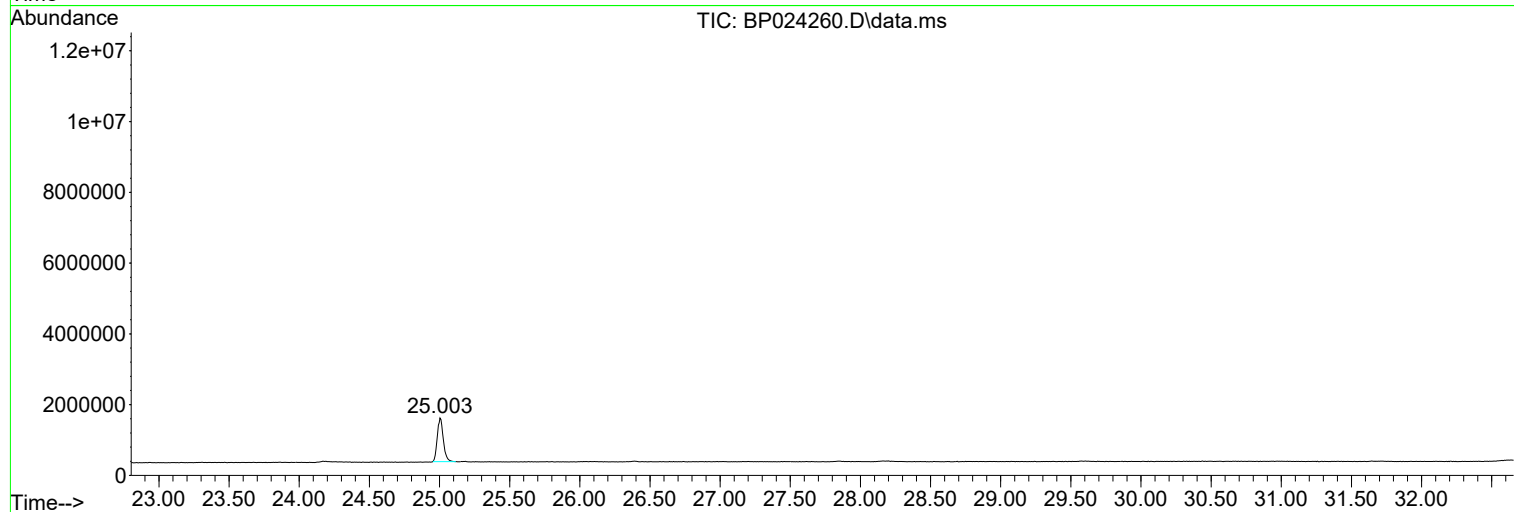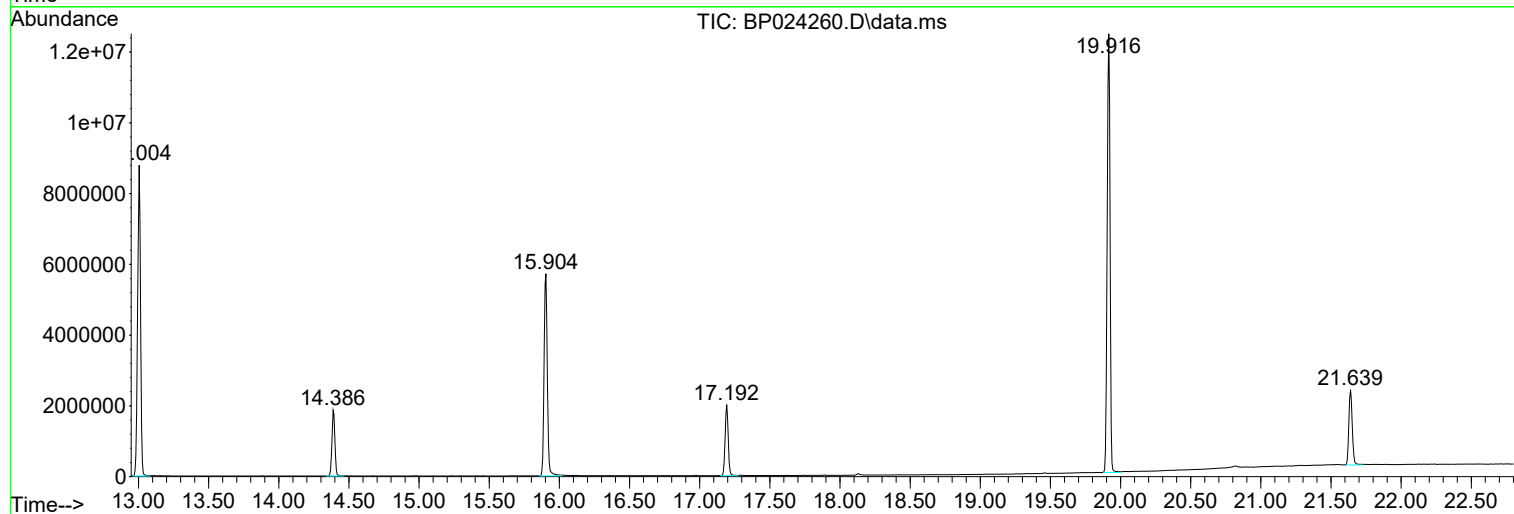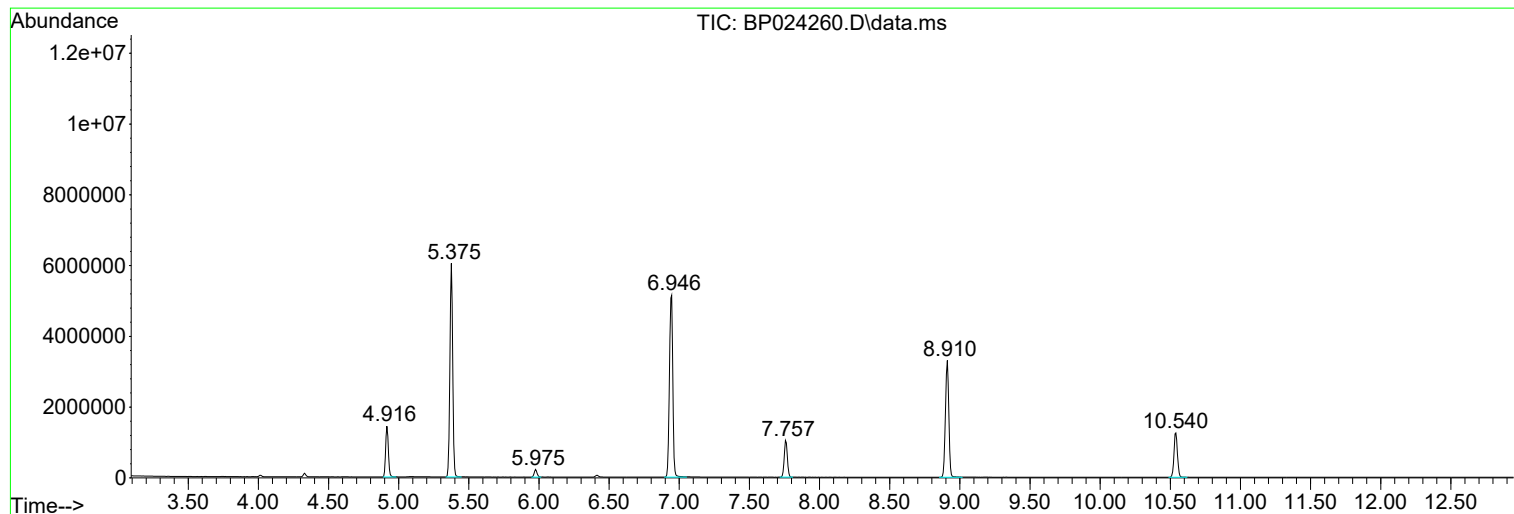

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041125\
Data File : BP024260.D
Acq On : 11 Apr 2025 10:23
Operator : RC/JU
Sample : PB167537BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167537BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041125\
Data File : BP024260.D
Acq On : 11 Apr 2025 10:23
Operator : RC/JU
Sample : PB167537BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167537BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------