




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041322\
 Data File : BP009810.D
 Acq On : 13 Apr 2022 10:34
 Operator : CG/JU
 Sample : PB144053BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK053

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:04:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

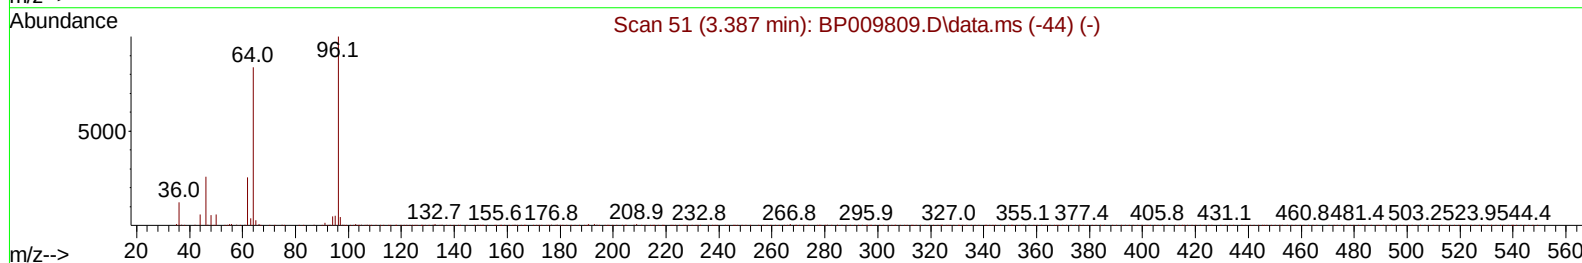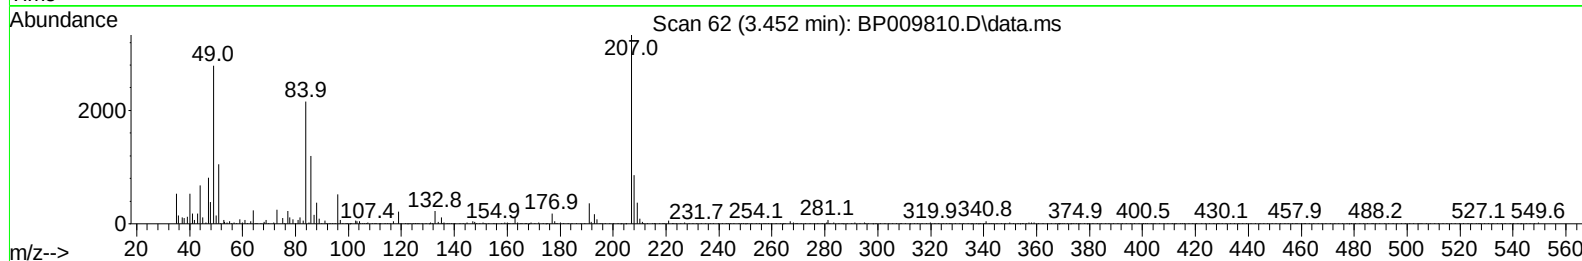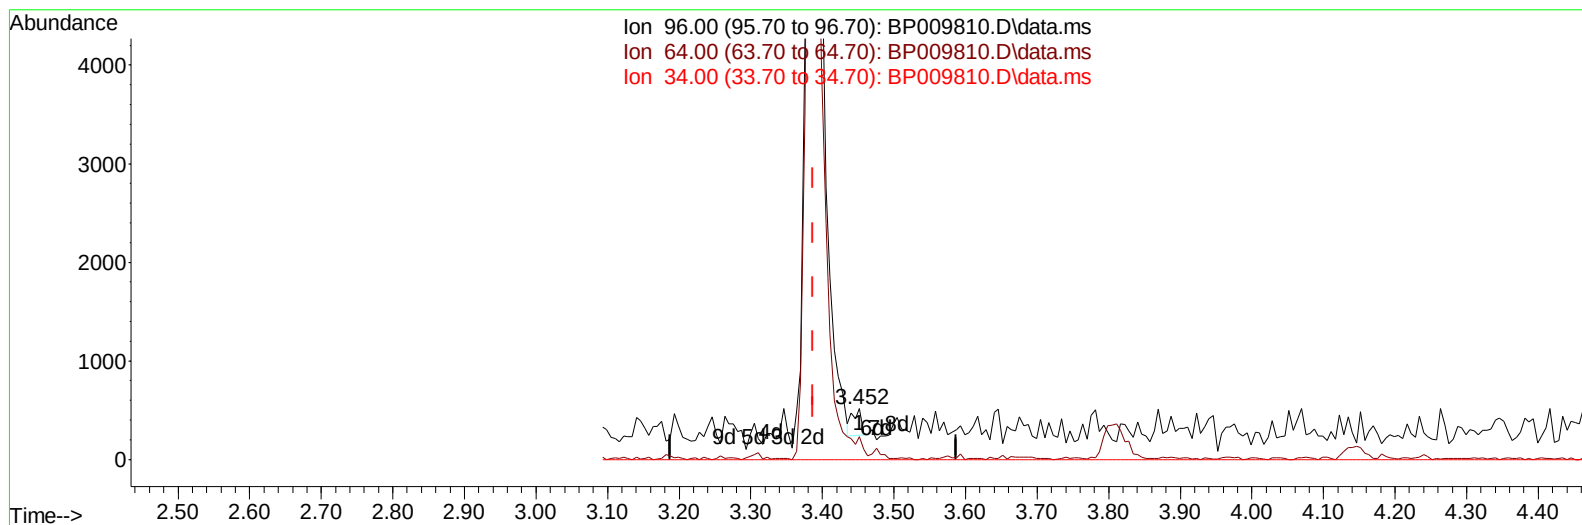

TIC: BP009810.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.452min (+ 0.065) 0.09 ng/uL

response 245

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	45.35
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041322\
 Data File : BP009810.D
 Acq On : 13 Apr 2022 10:34
 Operator : CG/JU
 Sample : PB144053BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK053

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:04:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

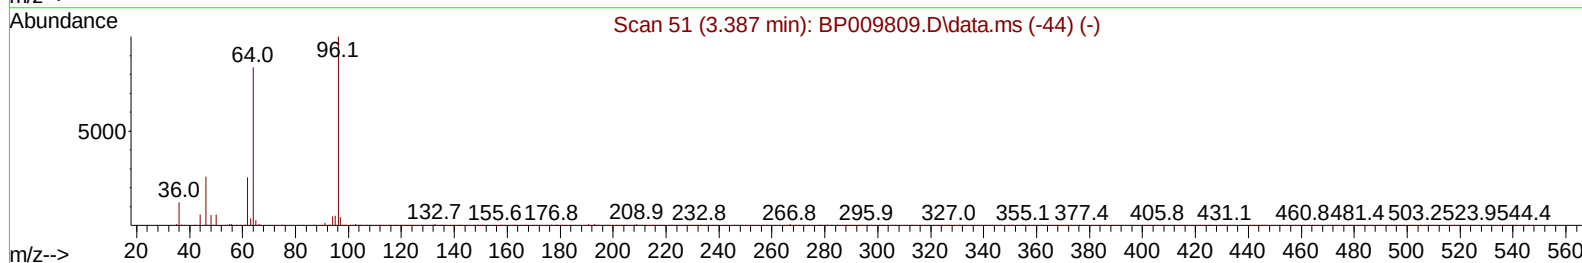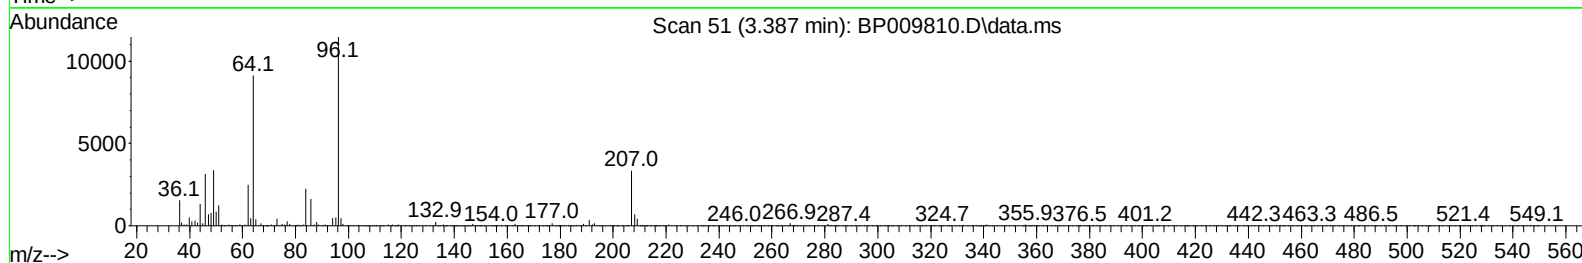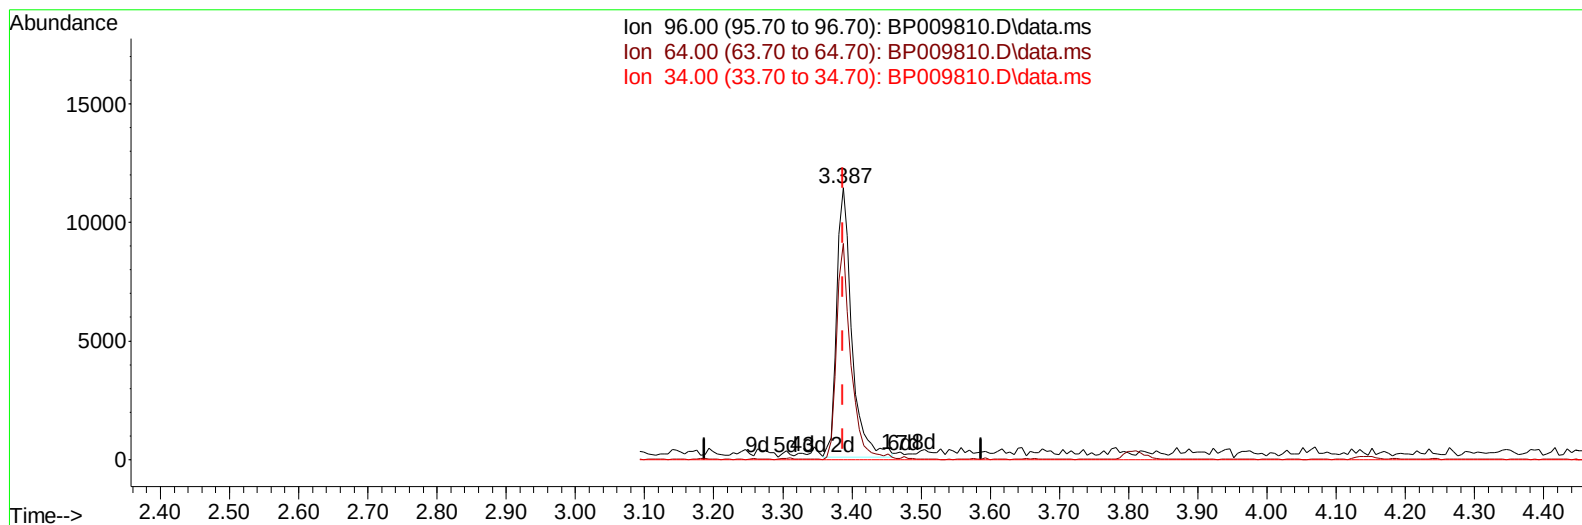

TIC: BP009810.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.387min (+ 0.000) 6.22 ng/uL m

response 17419

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.66#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041322\
 Data File : BP009810.D
 Acq On : 13 Apr 2022 10:34
 Operator : CG/JU
 Sample : PB144053BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK053

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:04:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.969	152		124934	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136		560377	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164		396689	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188		871152	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.427	240		867710	20.000	ng/ul	# 0.00
88) Perylene-d12	23.892	264		751630	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.387	96		17419m	6.223	ng/uL	0.00
4) Pyridine-d5	3.805	84		226231	29.311	ng/ul	0.00
7) Phenol-d5	7.116	99		279726	25.503	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67		188620	28.886	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132		230452	27.854	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113		241694	26.396	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128		119443	29.557	ng/ul	0.00
24) 2-Nitrophenol-d4	9.852	143		128717	29.053	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165		228331	24.629	ng/ul	0.00
31) 4-Chloroaniline-d4	10.904	131		349967	26.504	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166		871974	27.983	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160		951522	25.775	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143		136920	24.229	ng/ul	0.00
60) Fluorene-d10	15.587	176		728357	27.786	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200		115166	22.316	ng/ul	0.00
73) Anthracene-d10	17.445	188		1182072	28.340	ng/ul	0.00
81) Pyrene-d10	19.675	212		1417178	29.904	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264		1155037	29.509	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041322\
Data File : BP009810.D
Acq On : 13 Apr 2022 10:34
Operator : CG/JU
Sample : PB144053BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK053

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/14/2022
Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 14 01:04:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

