

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041322\
 Data File : BP009812.D
 Acq On : 13 Apr 2022 11:41
 Operator : CG/JU
 Sample : PB144076BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK076

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	11	rVB3	11115	15261	0.30%	0.030%
2	3.387	47	51	62	rVB	39539	63312	1.26%	0.123%
3	3.799	117	121	145	rBV	527694	897878	17.82%	1.746%
4	4.134	175	178	187	rVB2	13992	25907	0.51%	0.050%
5	7.116	674	685	699	rVB	723983	1155677	22.94%	2.247%
6	7.287	707	714	724	rBV	554699	887616	17.62%	1.726%
7	7.493	741	749	758	rBV	733914	1166995	23.17%	2.269%
8	7.963	819	829	839	rBV	596289	958488	19.03%	1.864%
9	8.663	938	948	960	rBV	946066	1520414	30.18%	2.956%
10	9.122	1016	1026	1041	rBV	780736	1281145	25.43%	2.491%
11	9.846	1141	1149	1162	rBV	653545	1061812	21.08%	2.065%
12	10.387	1231	1241	1256	rBV	942270	1562626	31.02%	3.039%
13	10.769	1297	1306	1320	rBV	885867	1484330	29.47%	2.886%
14	10.899	1320	1328	1342	rBV	1006960	1703209	33.81%	3.312%
15	12.357	1570	1576	1582	rVB2	18930	30583	0.61%	0.059%
16	13.569	1778	1782	1790	rVB9	2572	5461	0.11%	0.011%
17	13.875	1827	1834	1841	rBV10	3214	6405	0.13%	0.012%
18	14.004	1848	1856	1864	rBV	1882388	2667885	52.96%	5.188%
19	14.287	1897	1904	1919	rBV	1924414	2871210	57.00%	5.583%
20	14.593	1949	1956	1966	rBV	1465241	2144675	42.57%	4.170%
21	14.769	1979	1986	2002	rBV	1008305	1506457	29.90%	2.929%
22	15.234	2059	2065	2070	rBV8	2519	5583	0.11%	0.011%
23	15.587	2117	2125	2137	rBV	2663451	3735767	74.16%	7.264%
24	15.692	2137	2143	2154	rBV	925061	1286048	25.53%	2.501%
25	15.828	2162	2166	2175	rVB2	28648	44978	0.89%	0.087%
26	16.375	2253	2259	2264	rBV5	9125	14080	0.28%	0.027%
27	17.028	2364	2370	2376	rVB10	4733	8502	0.17%	0.017%
28	17.134	2381	2388	2391	rBV3	8390	16094	0.32%	0.031%
29	17.345	2417	2424	2433	rBV	1885615	2704147	53.68%	5.258%
30	17.445	2434	2441	2459	rVB	2961436	4178284	82.94%	8.125%
31	19.081	2716	2719	2724	rBV7	5177	9537	0.19%	0.019%
32	19.251	2743	2748	2753	rVB3	37977	53065	1.05%	0.103%
33	19.316	2755	2759	2765	rVB	40306	52623	1.04%	0.102%
34	19.675	2813	2820	2826	rBV	3653854	5037498	100.00%	9.795%
35	21.422	3112	3117	3124	rBV	2338754	3133229	62.20%	6.093%
36	23.733	3502	3510	3518	rBV2	2401700	4793297	95.15%	9.320%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041322\
Data File : BP009812.D
Acq On : 13 Apr 2022 11:41
Operator : CG/JU
Sample : PB144076BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION

37	23.804	3519	3522	3527	rVV	104326	168483	3.34%	0.328%
38	23.892	3529	3537	3547	rVB2	1405313	2935076	58.26%	5.707%
39	24.568	3648	3652	3660	rVB2	117883	233841	4.64%	0.455%




Sum of corrected areas: 51427478

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041322\
Data File : BP009812.D
Acq On : 13 Apr 2022 11:41
Operator : CG/JU
Sample : PB144076BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

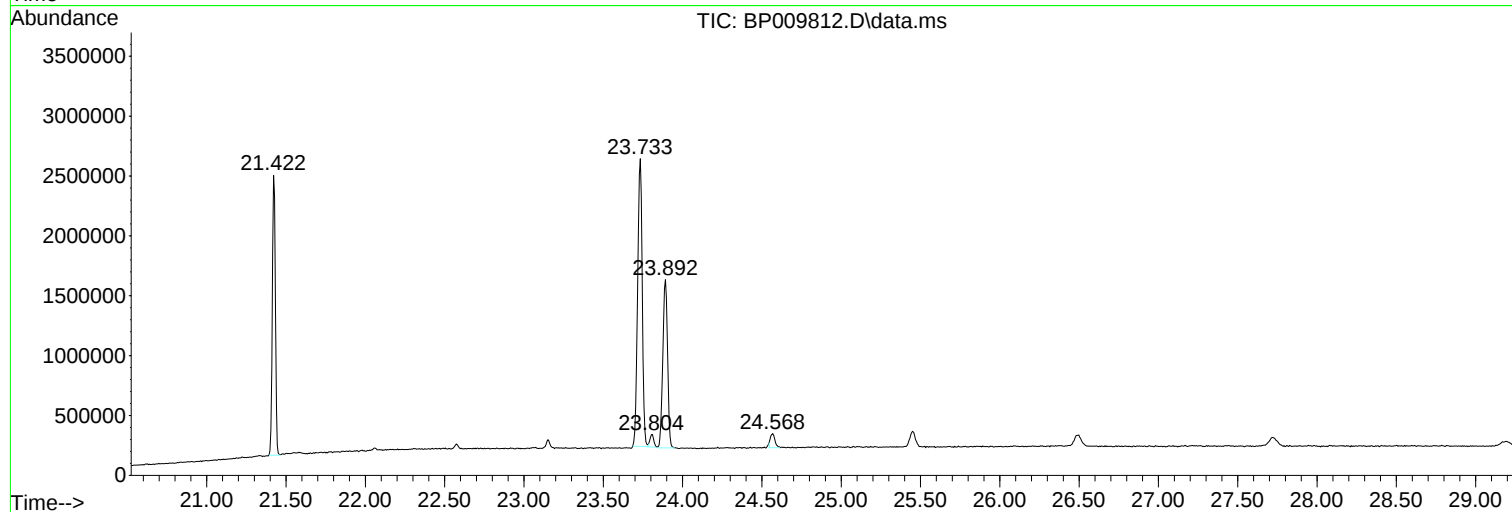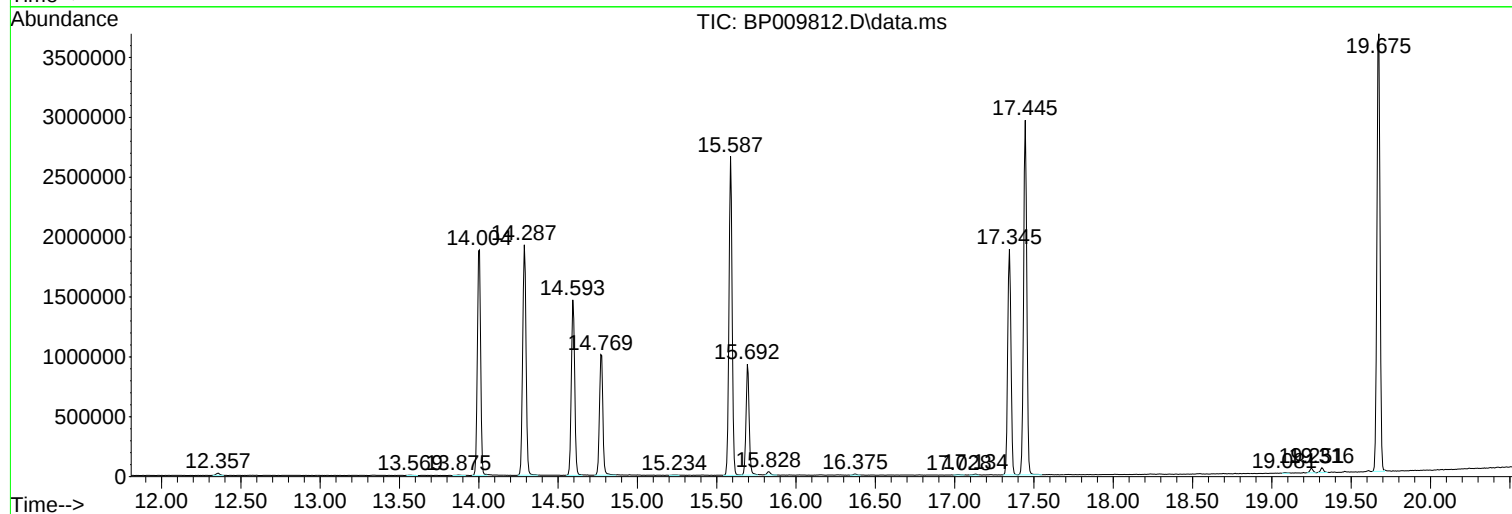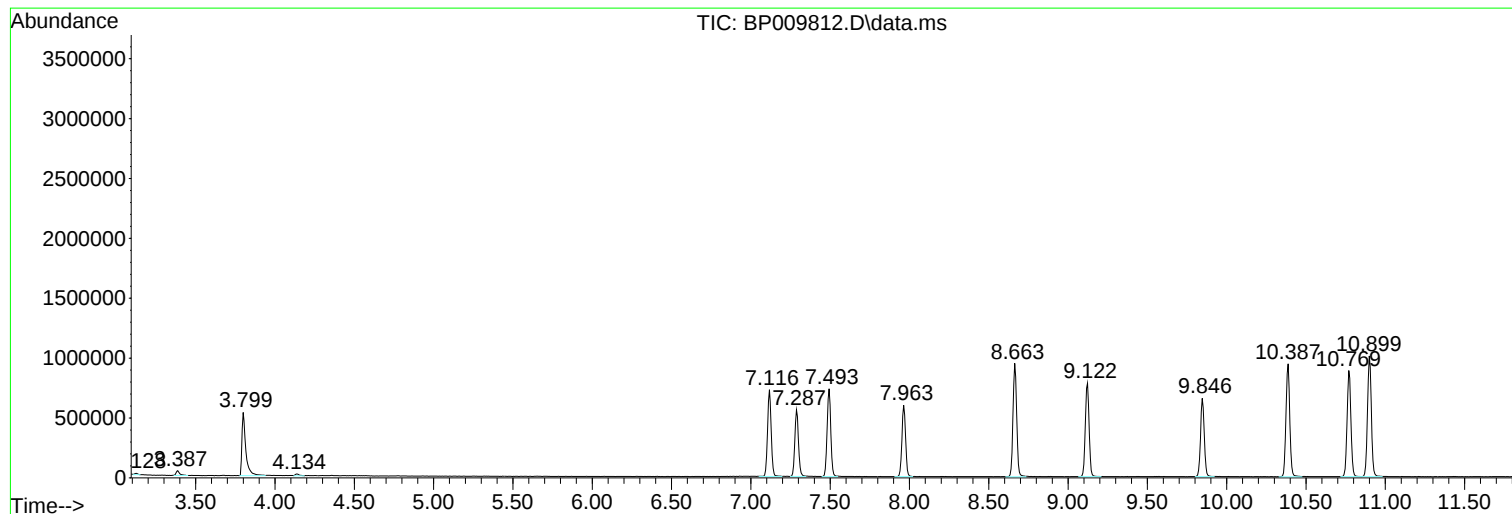

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041322\
Data File : BP009812.D
Acq On : 13 Apr 2022 11:41
Operator : CG/JU
Sample : PB144076BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041322\
Data File : BP009812.D
Acq On : 13 Apr 2022 11:41
Operator : CG/JU
Sample : PB144076BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc