




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009864.D
Acq On : 15 Apr 2022 16:44
Operator : CG/JU
Sample : N2422-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J11

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:02:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

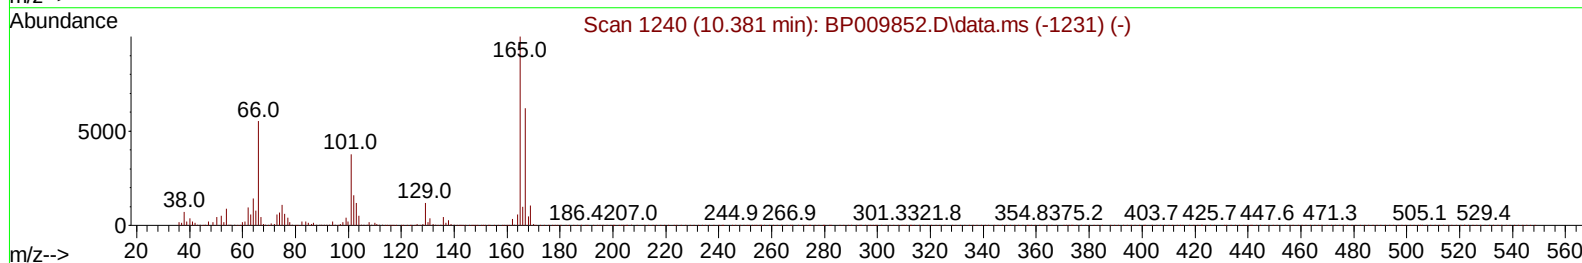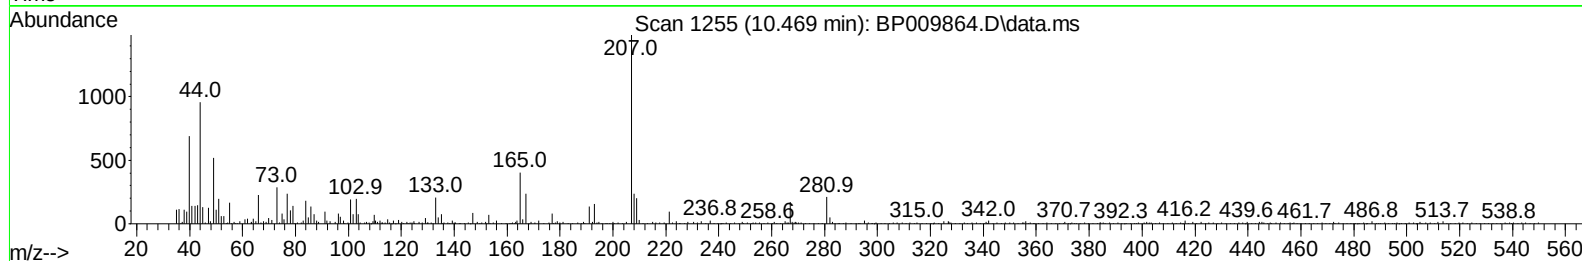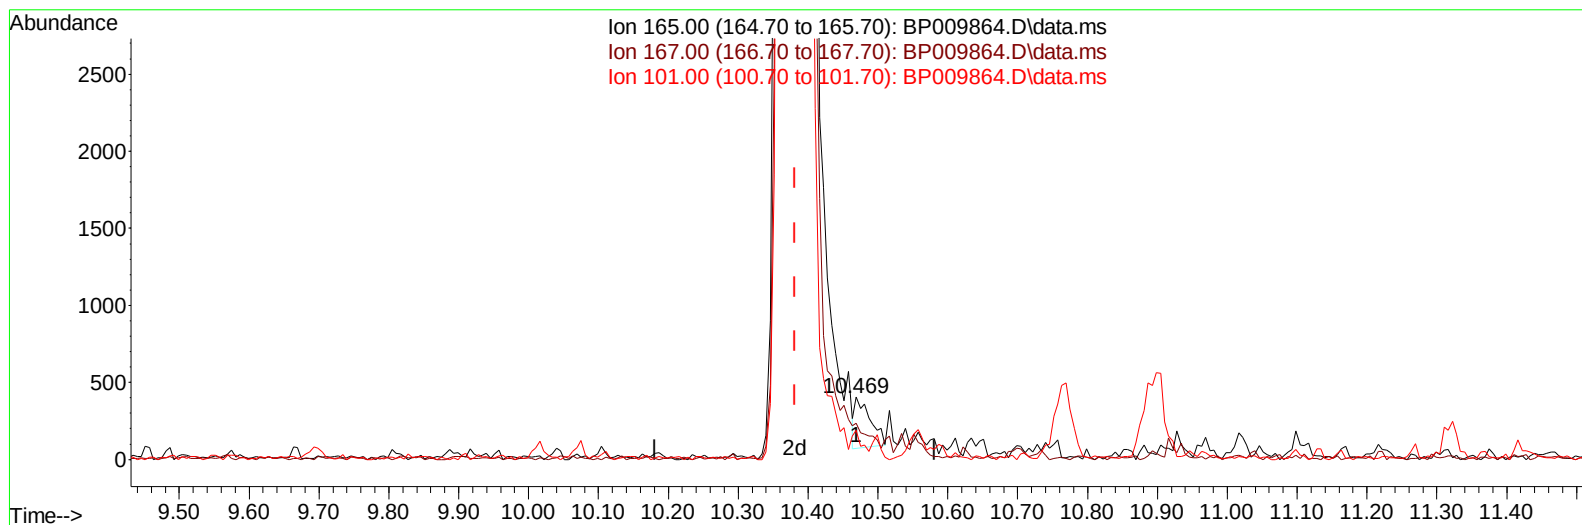

TIC: BP009864.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.469min (+ 0.088) 0.05 ng/ul

response 505

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	58.17
101.00	49.80	47.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009864.D
 Acq On : 15 Apr 2022 16:44
 Operator : CG/JU
 Sample : N2422-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J11

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:02:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

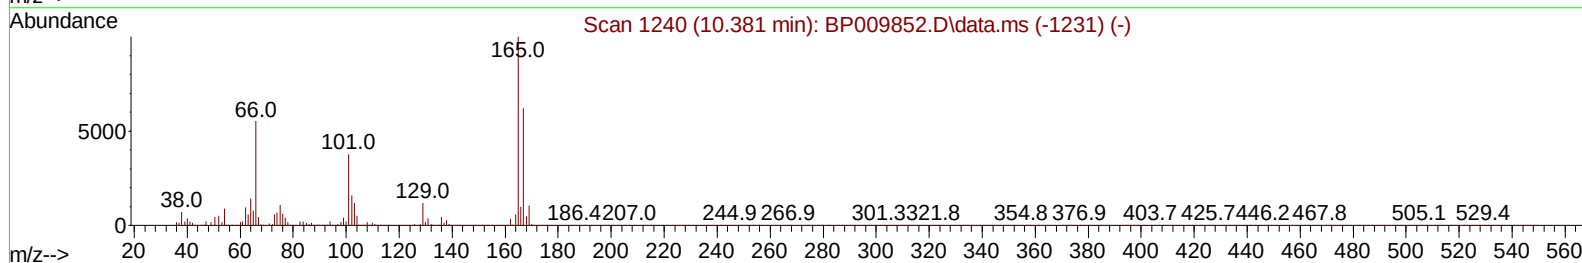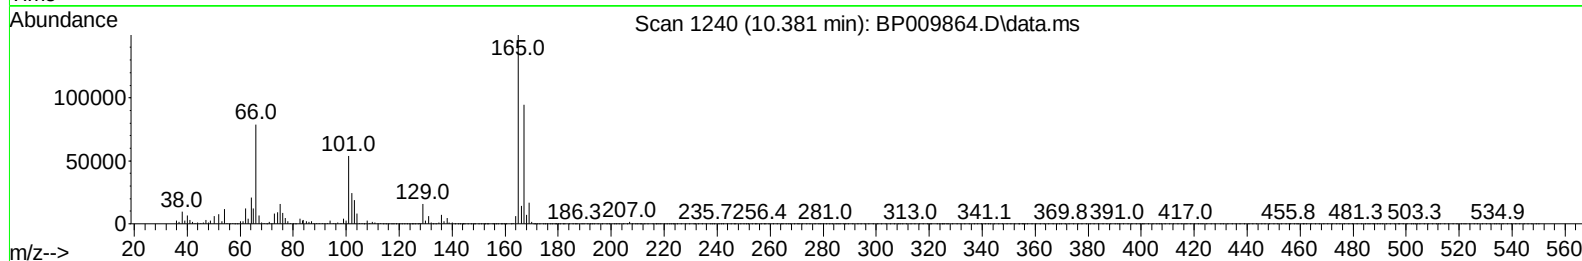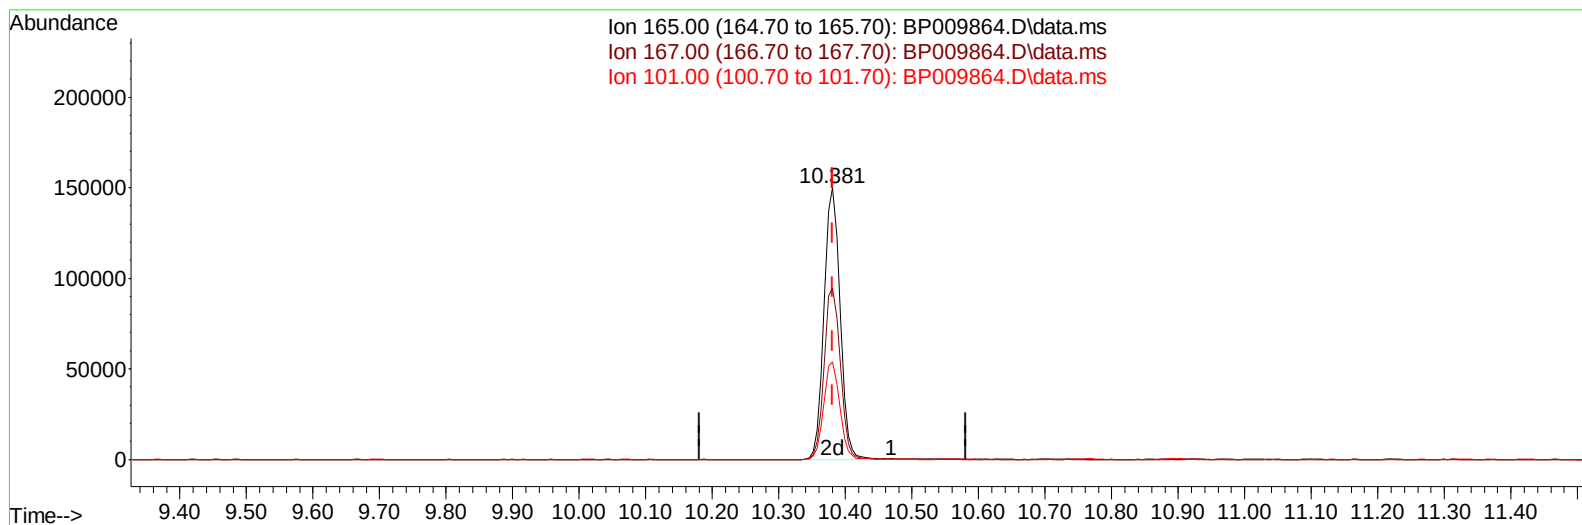

TIC: BP009864.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.381min (-0.000) 22.36 ng/ul m

response 250551

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	63.17
101.00	49.80	36.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009864.D
 Acq On : 15 Apr 2022 16:44
 Operator : CG/JU
 Sample : N2422-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J11

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:02:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	155568	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	677257	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	476757	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1054313	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.421	240	1003475	20.000	ng/ul	# 0.00
88) Perylene-d12	23.886	264	870358	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	13410	3.847	ng/uL	0.00
4) Pyridine-d5	3.805	84	58709	6.109	ng/ul	0.00
7) Phenol-d5	7.110	99	72020	5.273	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	218051	26.817	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	206141	20.009	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	145048	12.722	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	138342	28.326	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	144657	27.016	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	250551m	22.362	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	312014	19.552	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	1040301	27.779	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1142382	25.748	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	32799	4.829	ng/ul	0.00
60) Fluorene-d10	15.581	176	903695	28.685	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	162017	25.940	ng/ul	0.00
73) Anthracene-d10	17.439	188	1555500	30.814	ng/ul	0.00
81) Pyrene-d10	19.669	212	1915218	34.946	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	1538570	33.945	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009864.D
Acq On : 15 Apr 2022 16:44
Operator : CG/JU
Sample : N2422-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J11

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

Quant Time: Apr 18 01:02:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

