




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009874.D
 Acq On : 15 Apr 2022 22:55
 Operator : CG/JU
 Sample : N2422-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J03

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:06:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

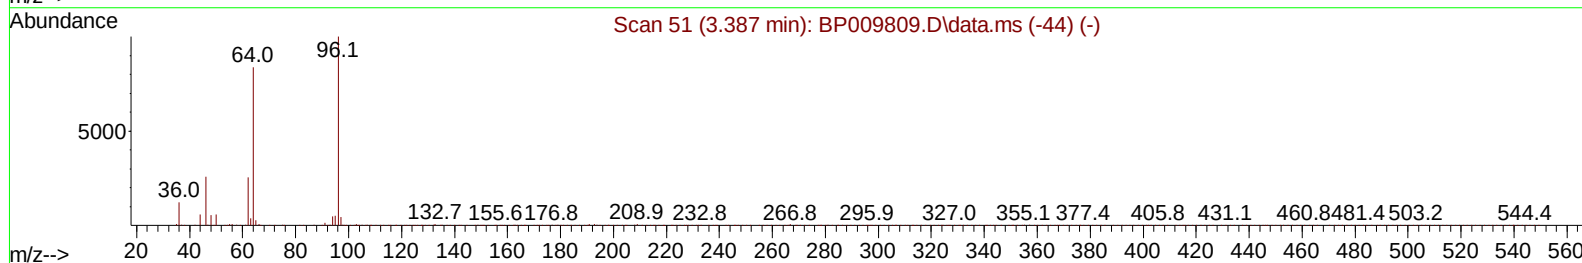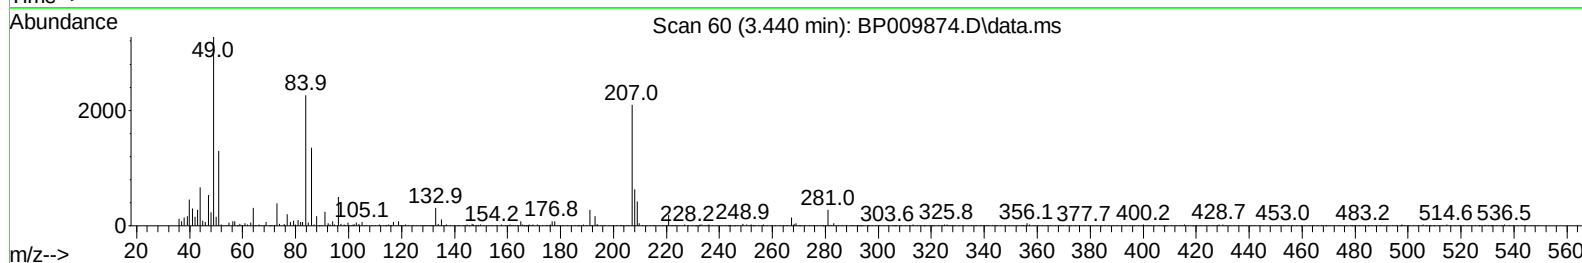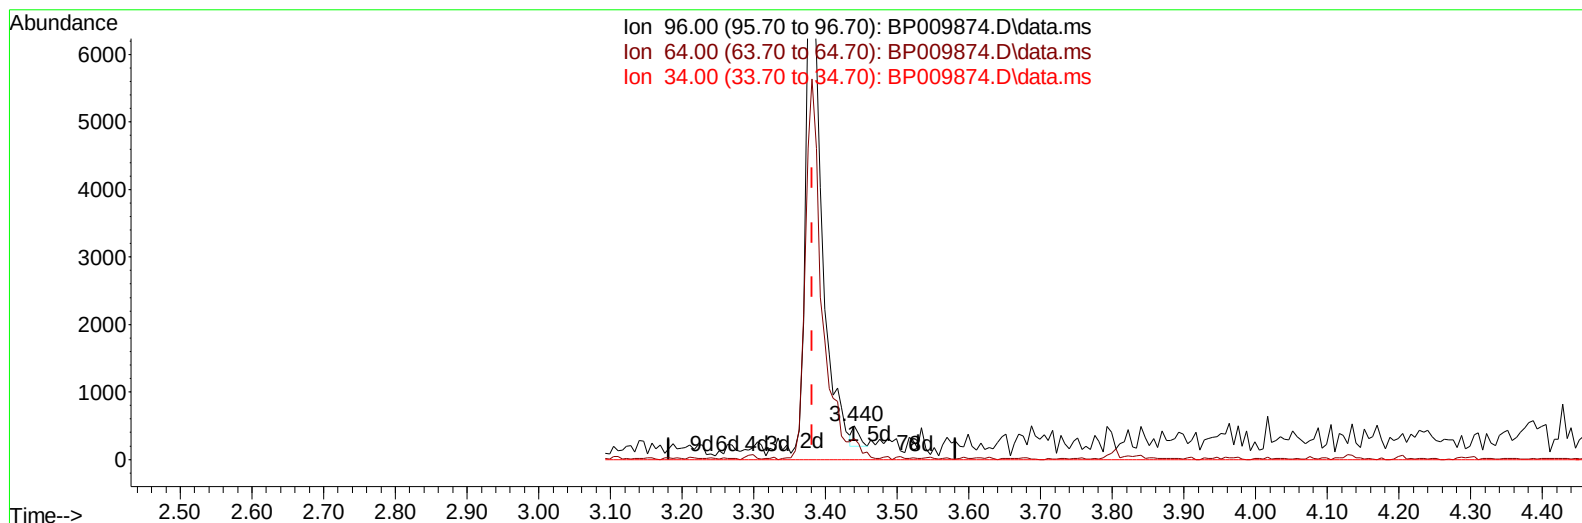

TIC: BP009874.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.440min (+ 0.059) 0.06 ng/uL

response 189

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	61.40
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009874.D
 Acq On : 15 Apr 2022 22:55
 Operator : CG/JU
 Sample : N2422-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J03

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:06:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

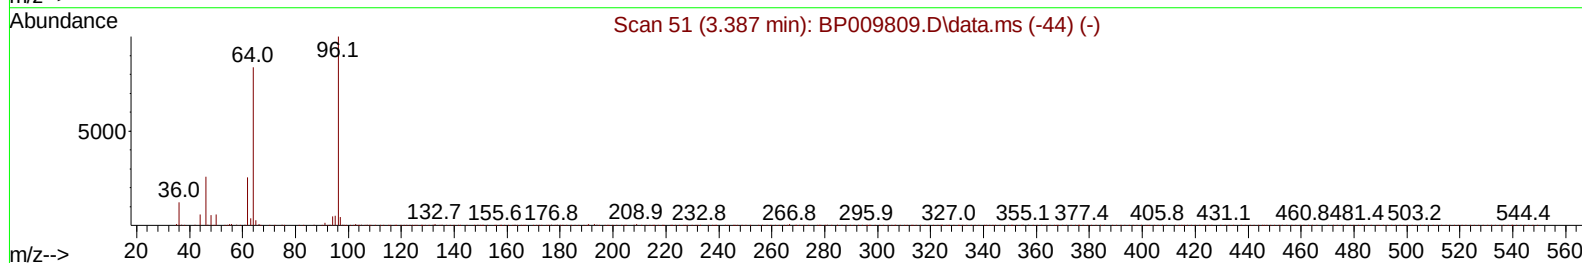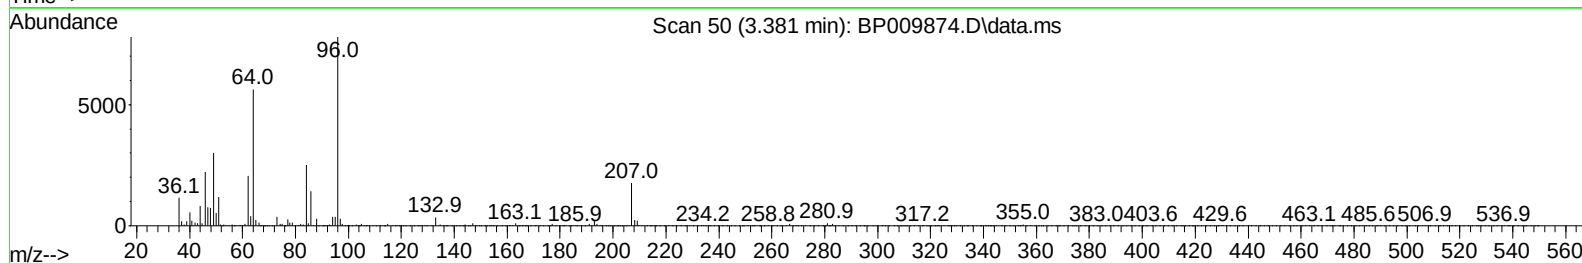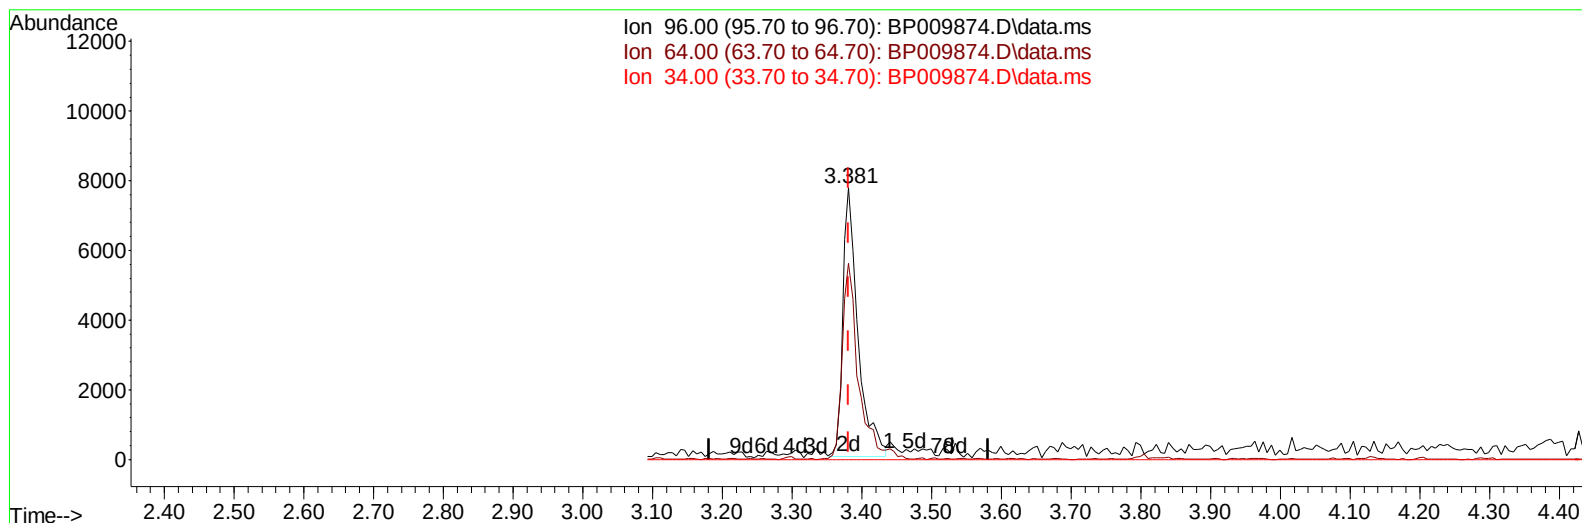

TIC: BP009874.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.000) 3.95 ng/uL m

response 11619

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	72.34#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009874.D
 Acq On : 15 Apr 2022 22:55
 Operator : CG/JU
 Sample : N2422-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J03

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:06:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

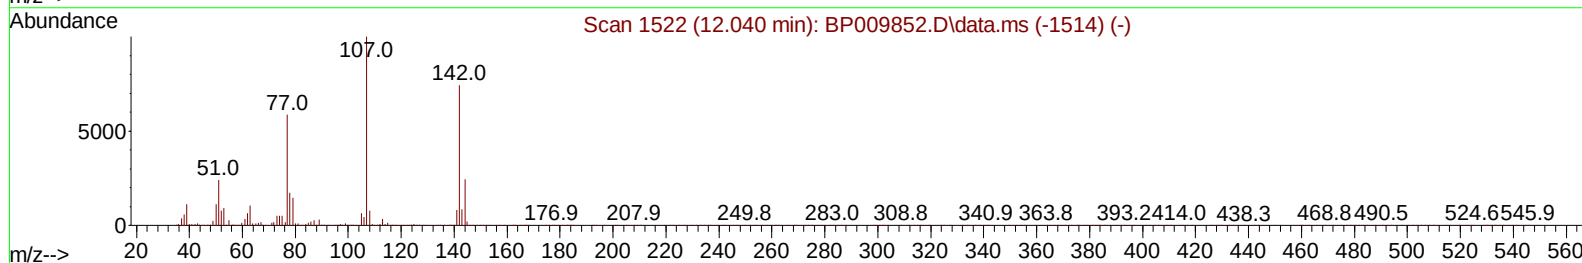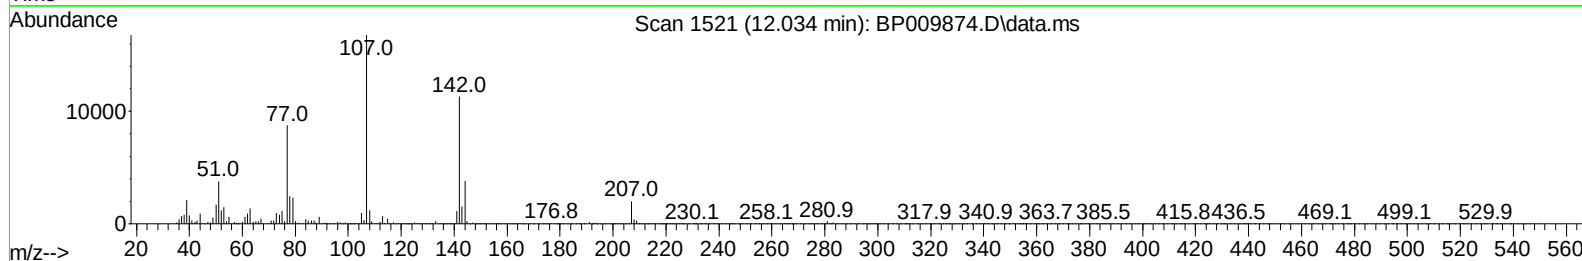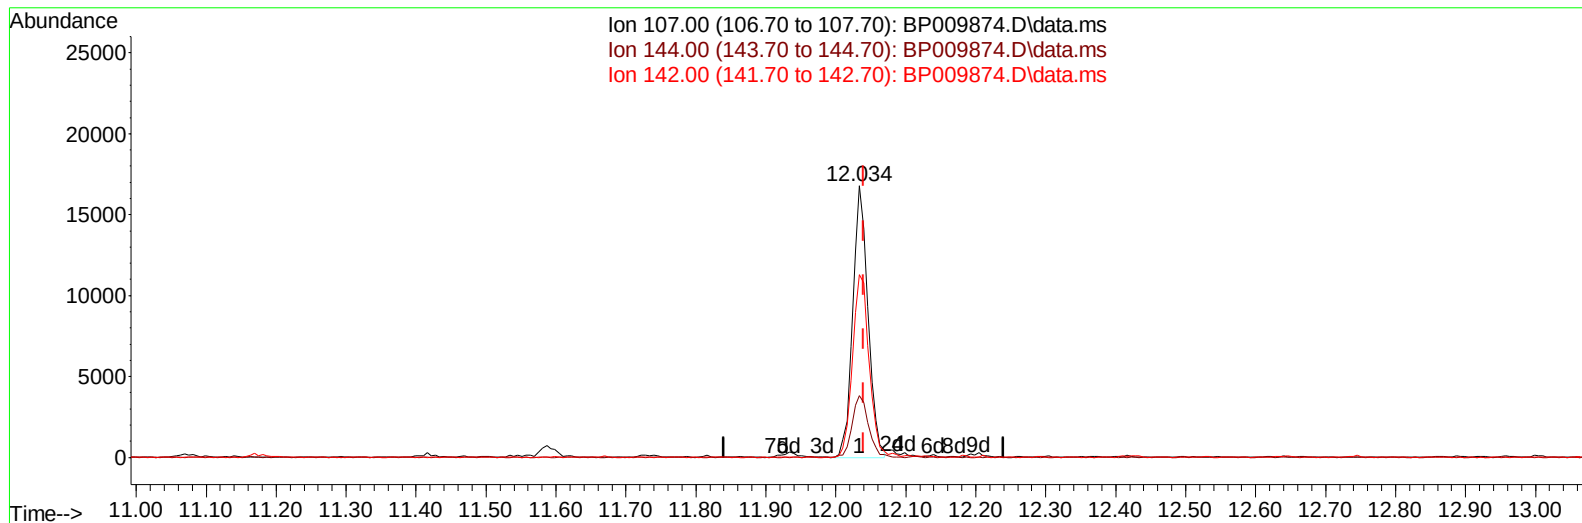

TIC: BP009874.D\data.ms

(35) 4-Chloro-3-methylphenol (C)

12.034min (-0.006) 2.20 ng/ul

response 25232

Ion	Exp%	Act%
107.00	100.00	100.00
144.00	19.80	22.68
142.00	48.60	67.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009874.D
 Acq On : 15 Apr 2022 22:55
 Operator : CG/JU
 Sample : N2422-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J03

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:06:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

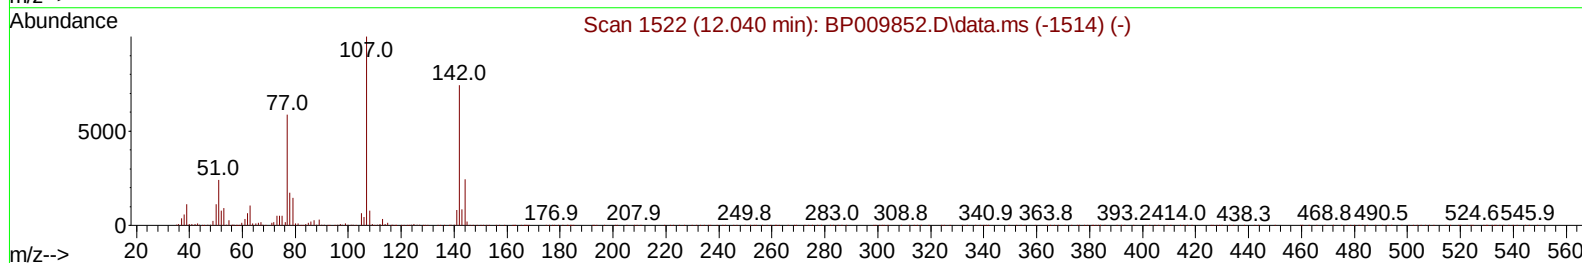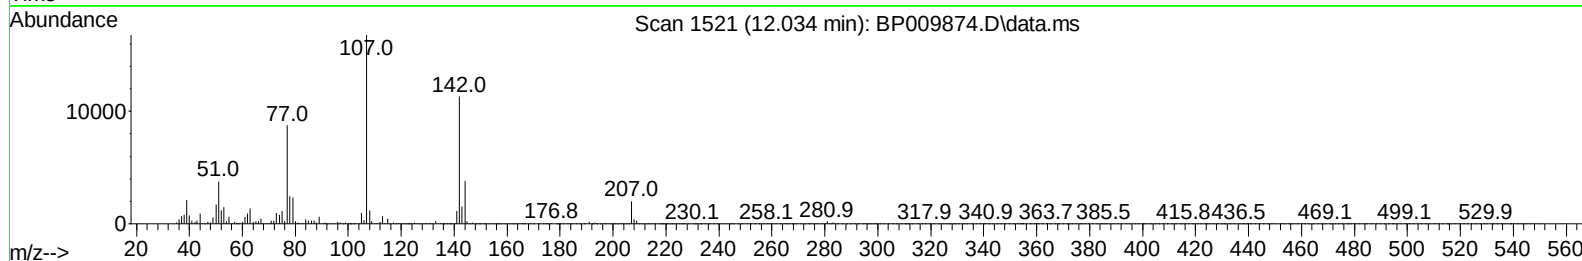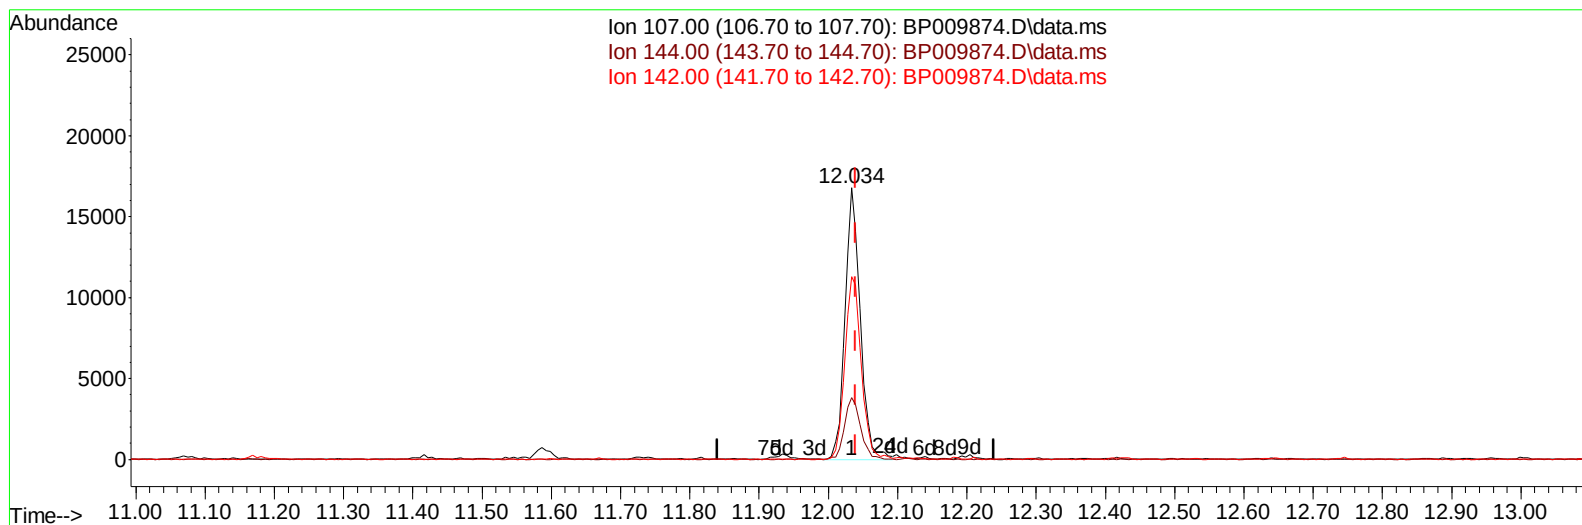

TIC: BP009874.D\data.ms

(35) 4-Chloro-3-methylphenol (C)

12.034min (-0.006) 2.24 ng/ul m

response 25693

Ion	Exp%	Act%
107.00	100.00	100.00
144.00	19.80	22.68
142.00	48.60	67.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009874.D
 Acq On : 15 Apr 2022 22:55
 Operator : CG/JU
 Sample : N2422-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J03

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:06:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

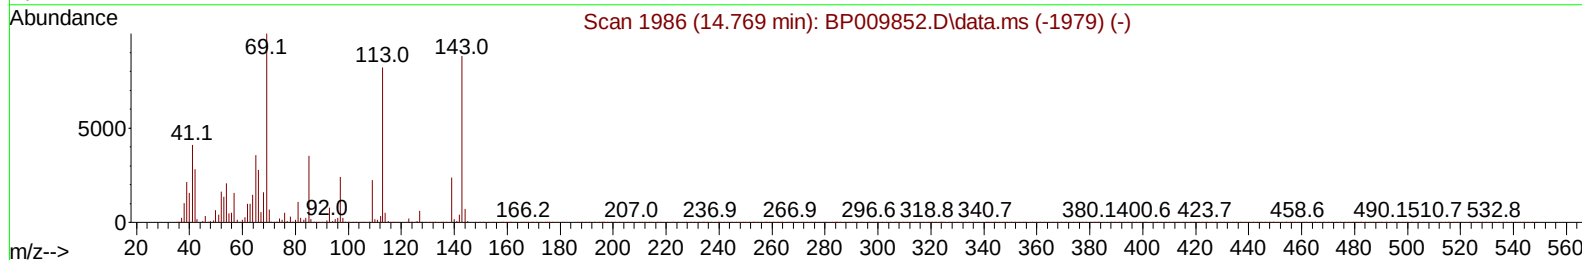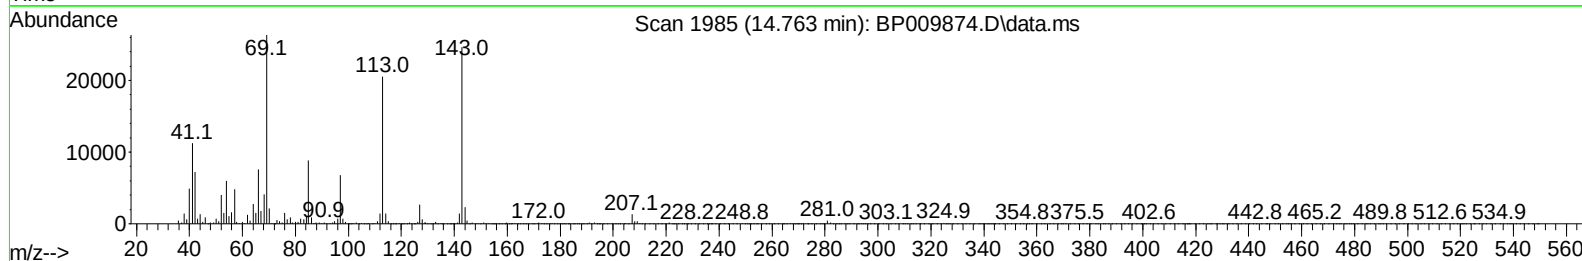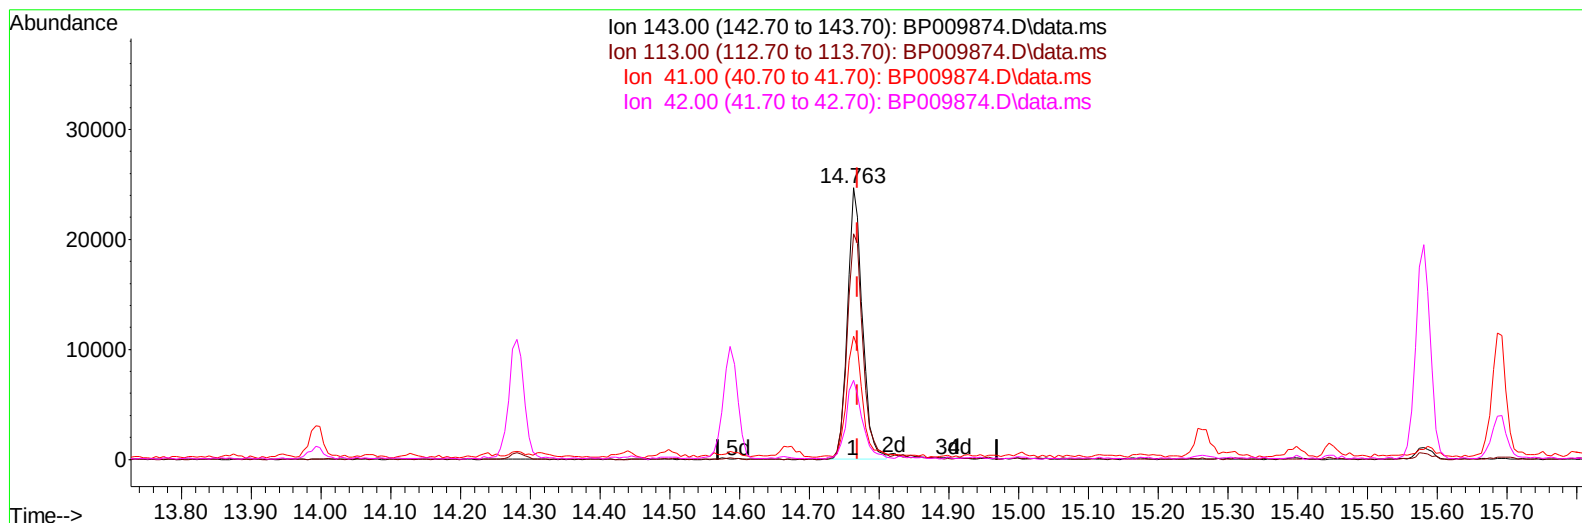

TIC: BP009874.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 5.83 ng/ul

response 36551

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.14#
41.00	23.20	45.51#
42.00	18.00	29.15#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009874.D
Acq On : 15 Apr 2022 22:55
Operator : CG/JU
Sample : N2422-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J03

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:06:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

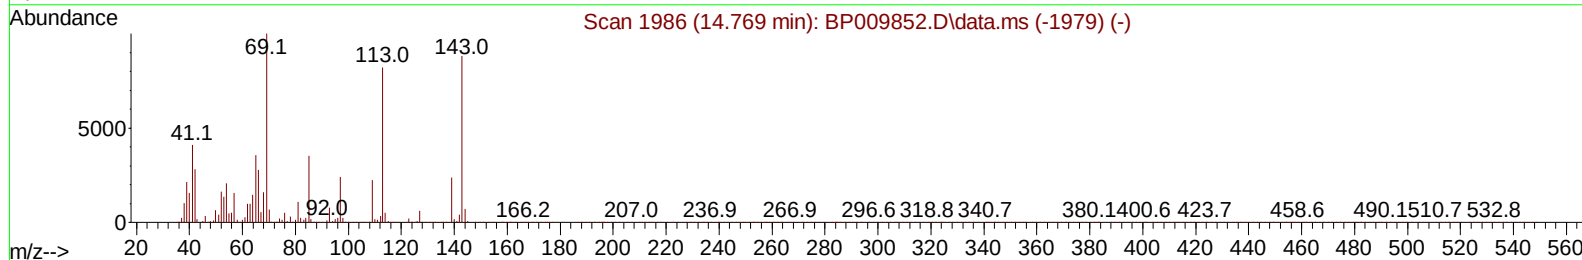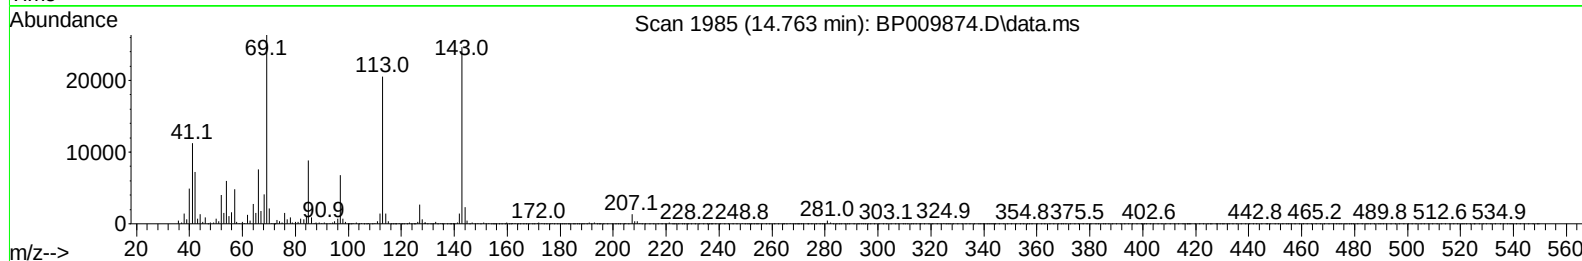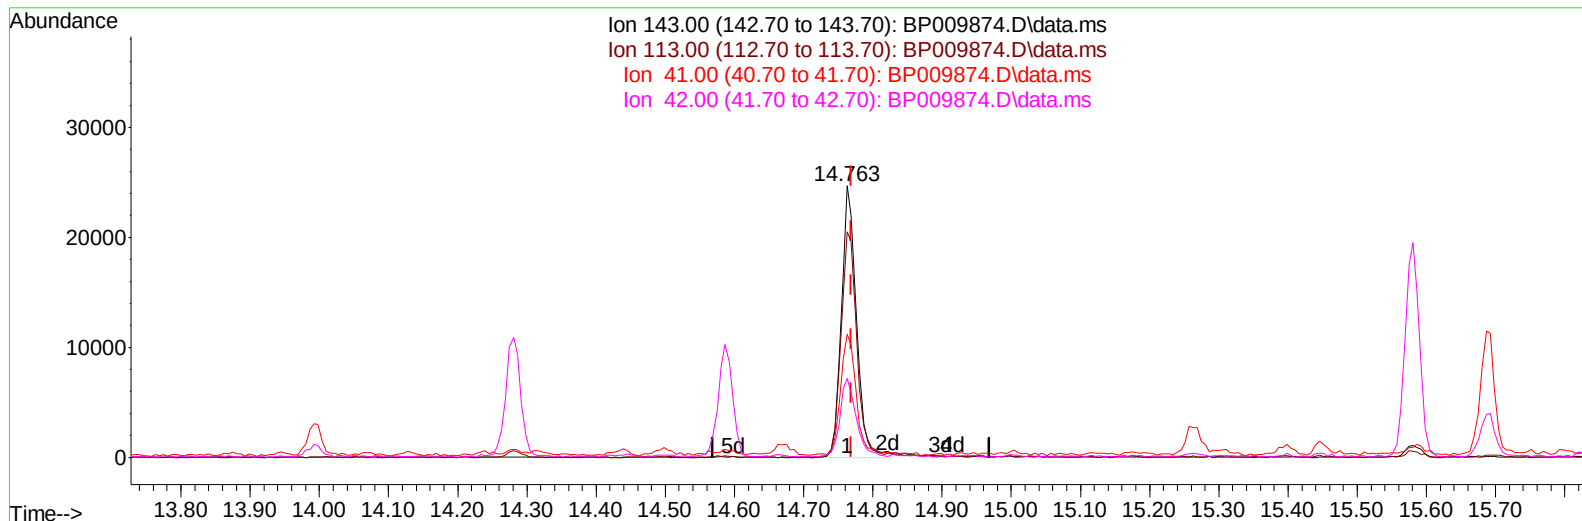

TIC: BP009874.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 5.91 ng/ul m

response 37077

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.14#
41.00	23.20	45.51#
42.00	18.00	29.15#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009874.D
 Acq On : 15 Apr 2022 22:55
 Operator : CG/JU
 Sample : N2422-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J03

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:06:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	131389	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.763	136	591139	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	440151	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1002196	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.421	240	1097049	20.000	ng/ul	# 0.00
88) Perylene-d12	23.886	264	1073573	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	11619m	3.947	ng/uL	0.00
4) Pyridine-d5	3.805	84	45704	5.631	ng/ul	0.00
7) Phenol-d5	7.110	99	65136	5.647	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	215497	31.380	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	201415	23.148	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	142903	14.840	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	140218	32.893	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	148443	31.762	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	257610	26.341	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	354071	25.419	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	1143644	33.078	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1220692	29.801	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	37077m	5.913	ng/ul	0.00
60) Fluorene-d10	15.581	176	994354	34.188	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	182345	30.713	ng/ul	0.00
73) Anthracene-d10	17.439	188	1755066	36.576	ng/ul	0.00
81) Pyrene-d10	19.669	212	2181252	36.405	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	2162183	38.674	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.034	107	25693m	2.236	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009874.D
Acq On : 15 Apr 2022 22:55
Operator : CG/JU
Sample : N2422-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J03

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

Quant Time: Apr 18 01:06:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

