




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009879.D
Acq On : 16 Apr 2022 01:43
Operator : CG/JU
Sample : N2422-14
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:07:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

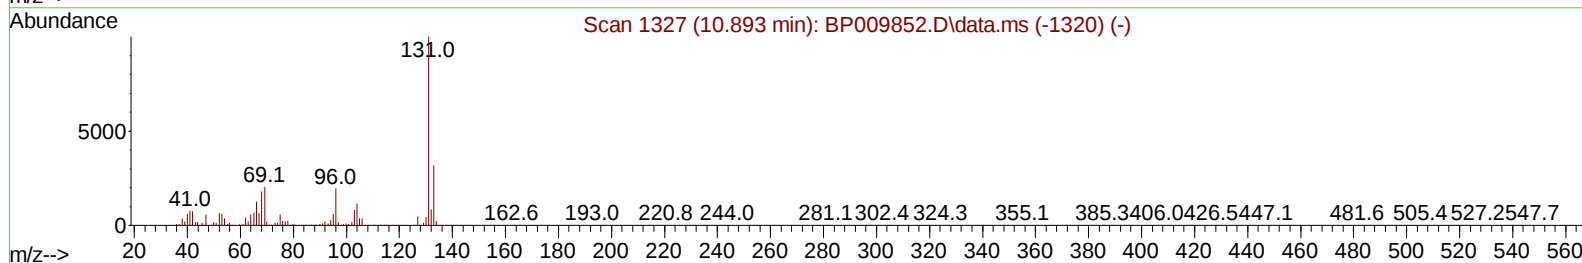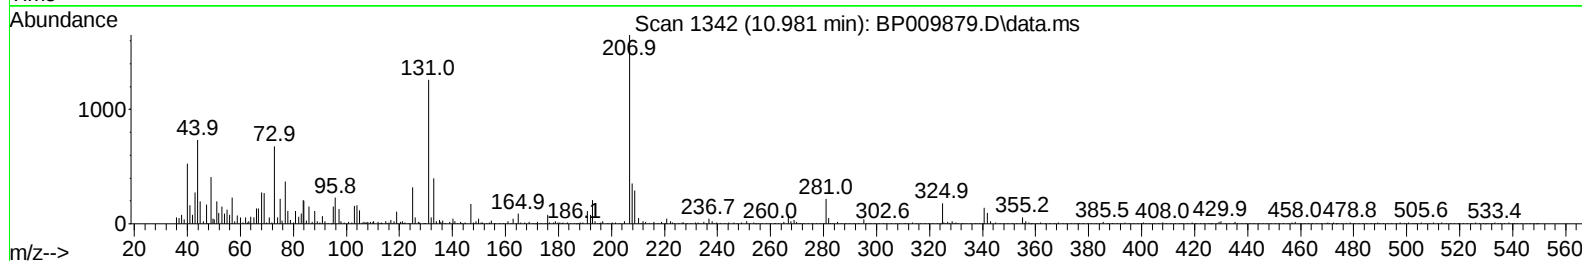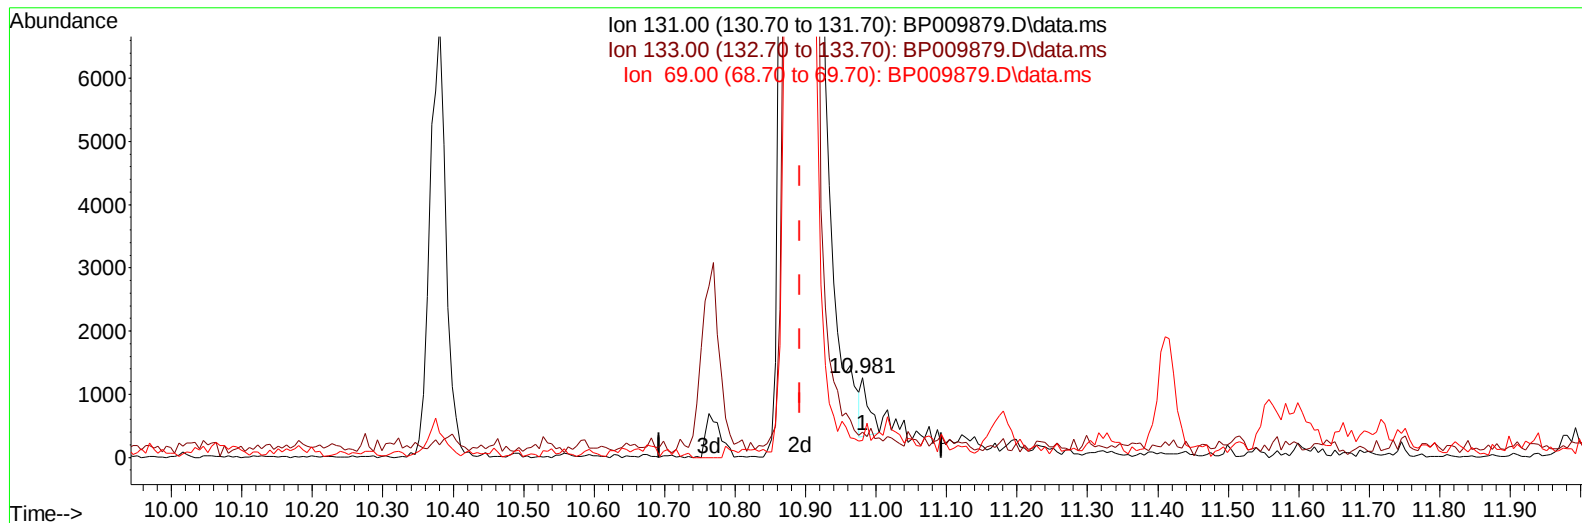

TIC: BP009879.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.981min (+ 0.088) 0.05 ng/u1

response 738

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	31.67
69.00	26.10	21.43
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009879.D
Acq On : 16 Apr 2022 01:43
Operator : CG/JU
Sample : N2422-14
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:07:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

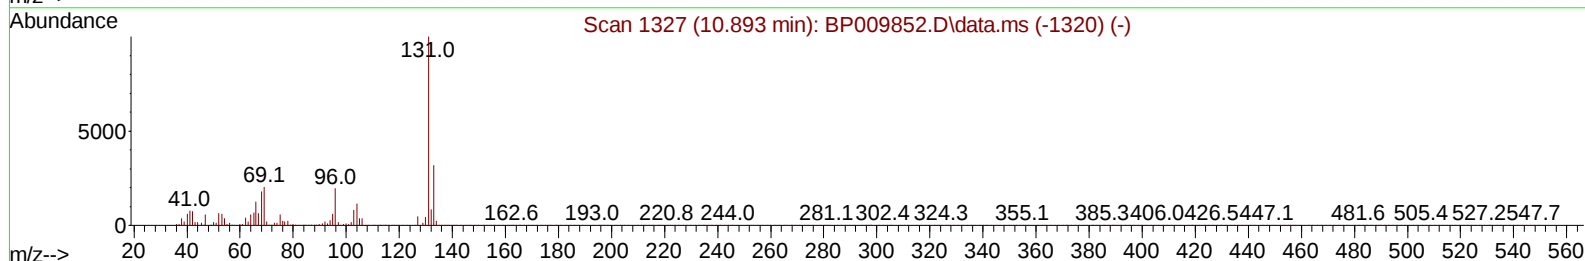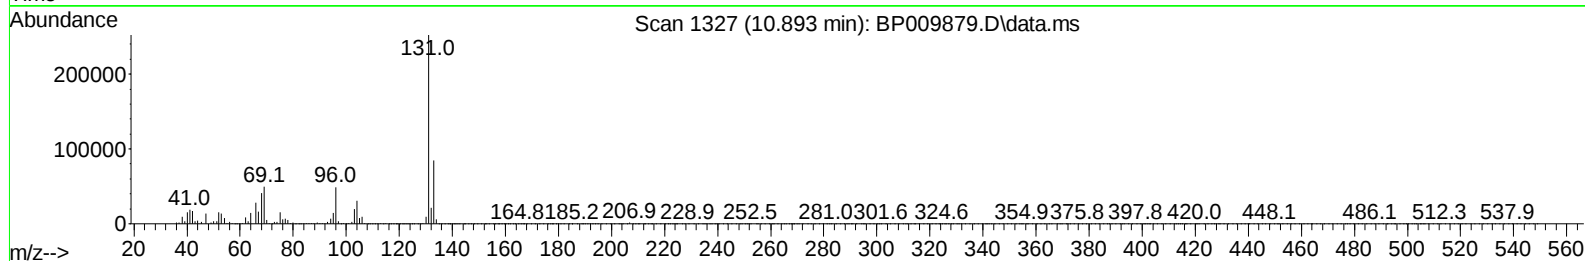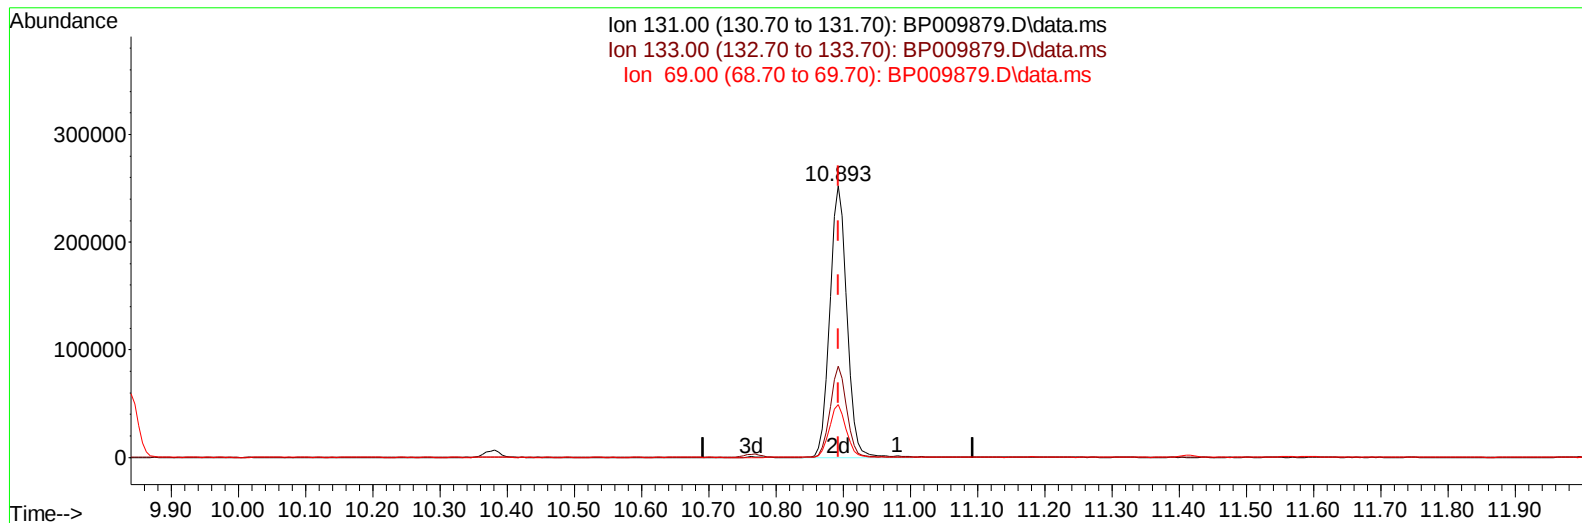

TIC: BP009879.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.893min (-0.000) 28.71 ng/ul m

response 444931

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	33.58
69.00	26.10	19.52#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009879.D
 Acq On : 16 Apr 2022 01:43
 Operator : CG/JU
 Sample : N2422-14
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

Quant Time: Apr 18 01:07:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	145801	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	657759	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	468258	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1051474	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.416	240	1045113	20.000	ng/ul	# 0.00
88) Perylene-d12	23.880	264	906604	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	13530	4.142	ng/uL	0.00
4) Pyridine-d5	3.805	84	75183	8.347	ng/ul	0.00
7) Phenol-d5	7.110	99	86364	6.747	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	250494	32.871	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	239622	24.817	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	174748	16.354	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	165535	34.899	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	171651	33.008	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	296365	27.235	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	444931m	28.707	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	1279317	34.781	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1371588	31.475	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	43230	6.481	ng/ul	0.00
60) Fluorene-d10	15.581	176	1102022	35.615	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	199687	32.058	ng/ul	0.00
73) Anthracene-d10	17.439	188	1997534	39.678	ng/ul	0.00
81) Pyrene-d10	19.669	212	2375805	41.623	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	1957383	41.459	ng/ul	0.00
Target Compounds						
					Qvalue	
35) 4-Chloro-3-methylphenol	12.034	107	27326	2.138	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009879.D
Acq On : 16 Apr 2022 01:43
Operator : CG/JU
Sample : N2422-14
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:07:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

