




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009882.D
Acq On : 16 Apr 2022 03:24
Operator : CG/JU
Sample : N2421-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J55

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:08:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

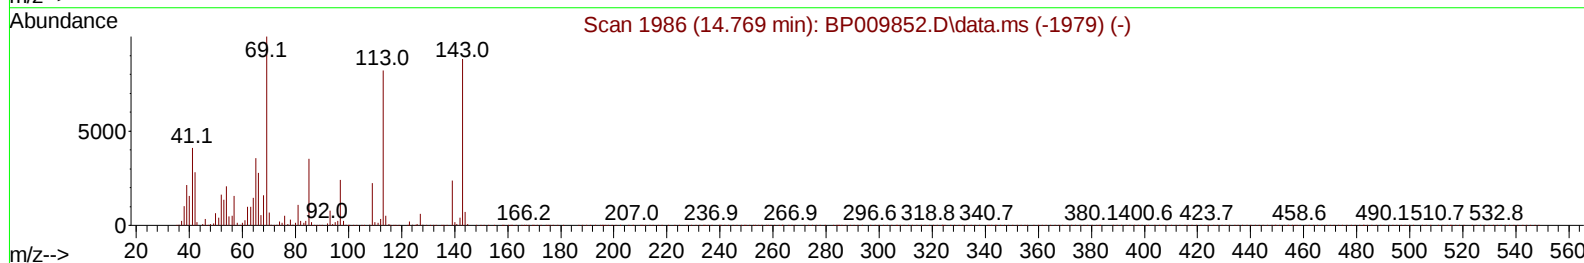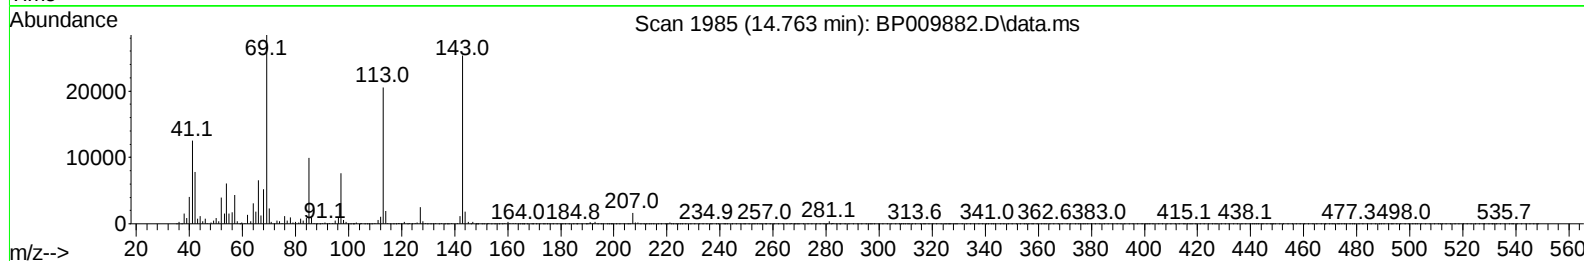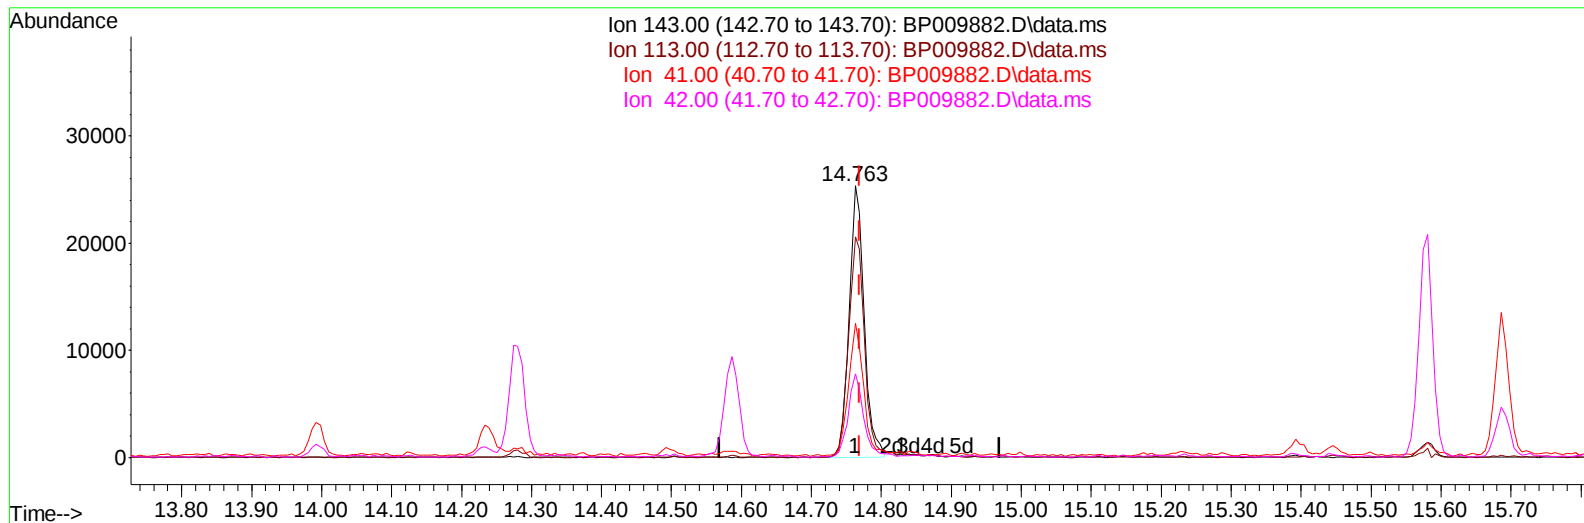

TIC: BP009882.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 6.41 ng/u1

response 37385

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	81.24#
41.00	23.20	49.46#
42.00	18.00	30.89#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009882.D
Acq On : 16 Apr 2022 03:24
Operator : CG/JU
Sample : N2421-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J55

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

Quant Time: Apr 18 01:08:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

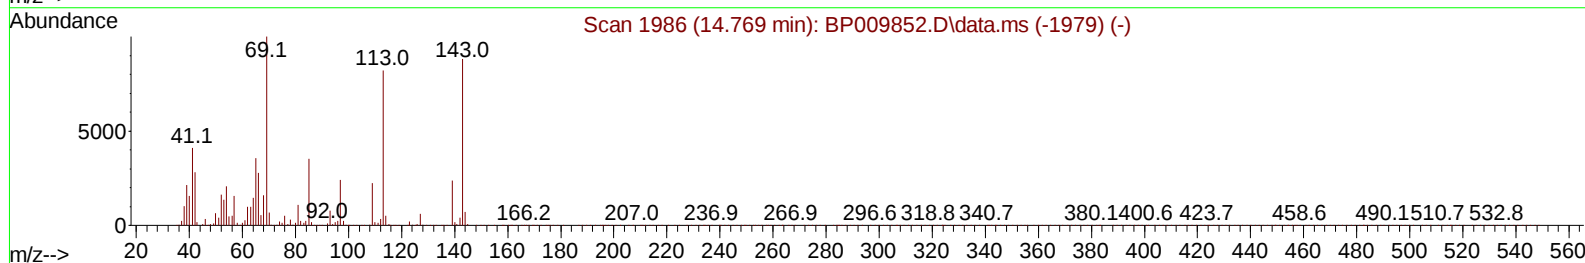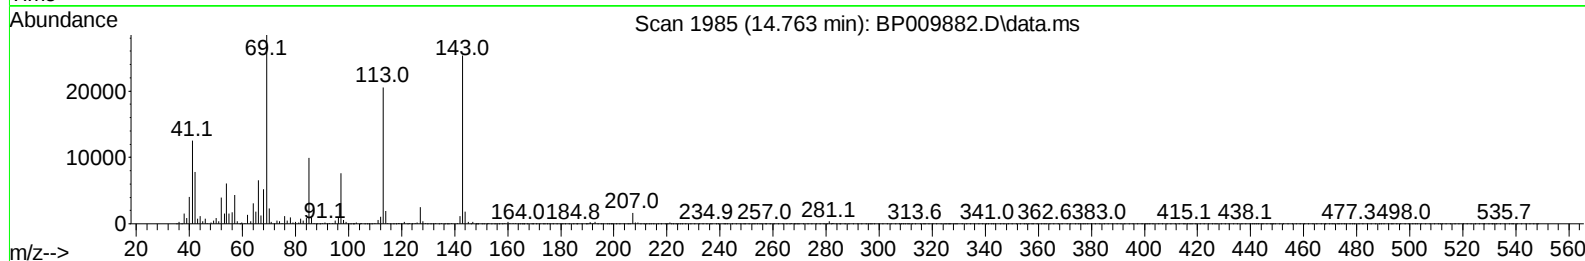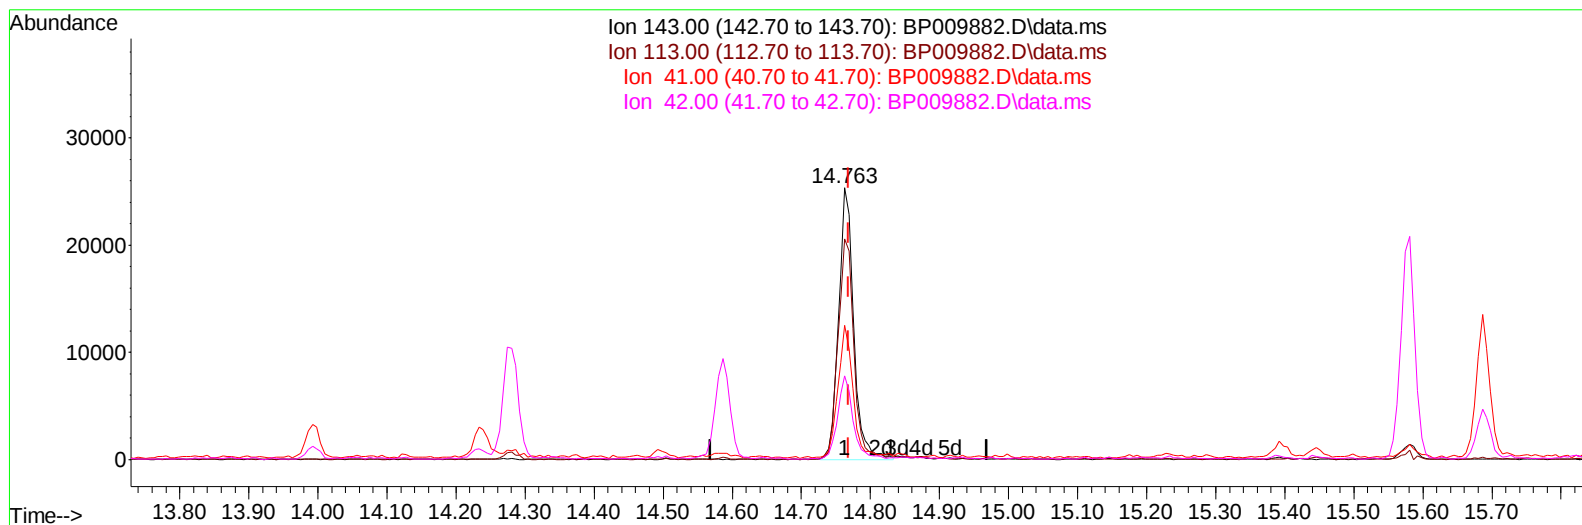

TIC: BP009882.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 6.52 ng/u1 m

response 38040

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	81.24#
41.00	23.20	49.46#
42.00	18.00	30.89#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009882.D
 Acq On : 16 Apr 2022 03:24
 Operator : CG/JU
 Sample : N2421-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J55

Manual IntegrationsAPPROVED

Quant Time: Apr 18 01:08:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	131302	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	575546	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	409565	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	915243	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.415	240	917109	20.000	ng/ul	# 0.00
88) Perylene-d12	23.880	264	809720	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	15523	5.276	ng/uL	0.00
4) Pyridine-d5	3.799	84	81341	10.028	ng/ul	0.00
7) Phenol-d5	7.110	99	82169	7.128	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	237049	34.542	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	230374	26.494	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	163777	17.019	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	159290	38.379	ng/ul	0.00
24) 2-Nitrophenol-d4	9.839	143	165726	36.421	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	276040	28.990	ng/ul	0.00
31) 4-Chloroaniline-d4	10.892	131	377593	27.842	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	1184647	36.822	ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	1289987	33.845	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	38040m	6.520	ng/ul	0.00
60) Fluorene-d10	15.580	176	1061568	39.224	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	194893	35.945	ng/ul	0.00
73) Anthracene-d10	17.439	188	1870647	42.688	ng/ul	0.00
81) Pyrene-d10	19.668	212	2261275	45.146	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	1899567	45.048	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009882.D
Acq On : 16 Apr 2022 03:24
Operator : CG/JU
Sample : N2421-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J55

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

Quant Time: Apr 18 01:08:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

