

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009861.D
 Acq On : 15 Apr 2022 15:03
 Operator : CG/JU
 Sample : N2422-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J96

Quant Time: Apr 18 01:01:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	132380	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	590149	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	428820	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	958508	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.421	240	931107	20.000	ng/ul	# 0.00
88) Perylene-d12	23.886	264	791465	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	15131	5.101	ng/uL	0.00
4) Pyridine-d5	3.805	84	62207	7.606	ng/ul	0.00
7) Phenol-d5	7.110	99	81024	6.972	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	239194	34.570	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	220856	25.192	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	161673	16.664	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	154868	36.390	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	161695	34.656	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	275092	28.176	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	388309	27.924	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	1198248	35.573	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1317224	33.008	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	37338	6.112	ng/ul	0.00
60) Fluorene-d10	15.581	176	1048621	37.006	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	186693	32.879	ng/ul	0.00
73) Anthracene-d10	17.439	188	1801623	39.257	ng/ul	0.00
81) Pyrene-d10	19.669	212	2174060	42.752	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	1727379	41.910	ng/ul	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.157	77	60893	5.574	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009861.D
Acq On : 15 Apr 2022 15:03
Operator : CG/JU
Sample : N2422-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J96

Quant Time: Apr 18 01:01:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

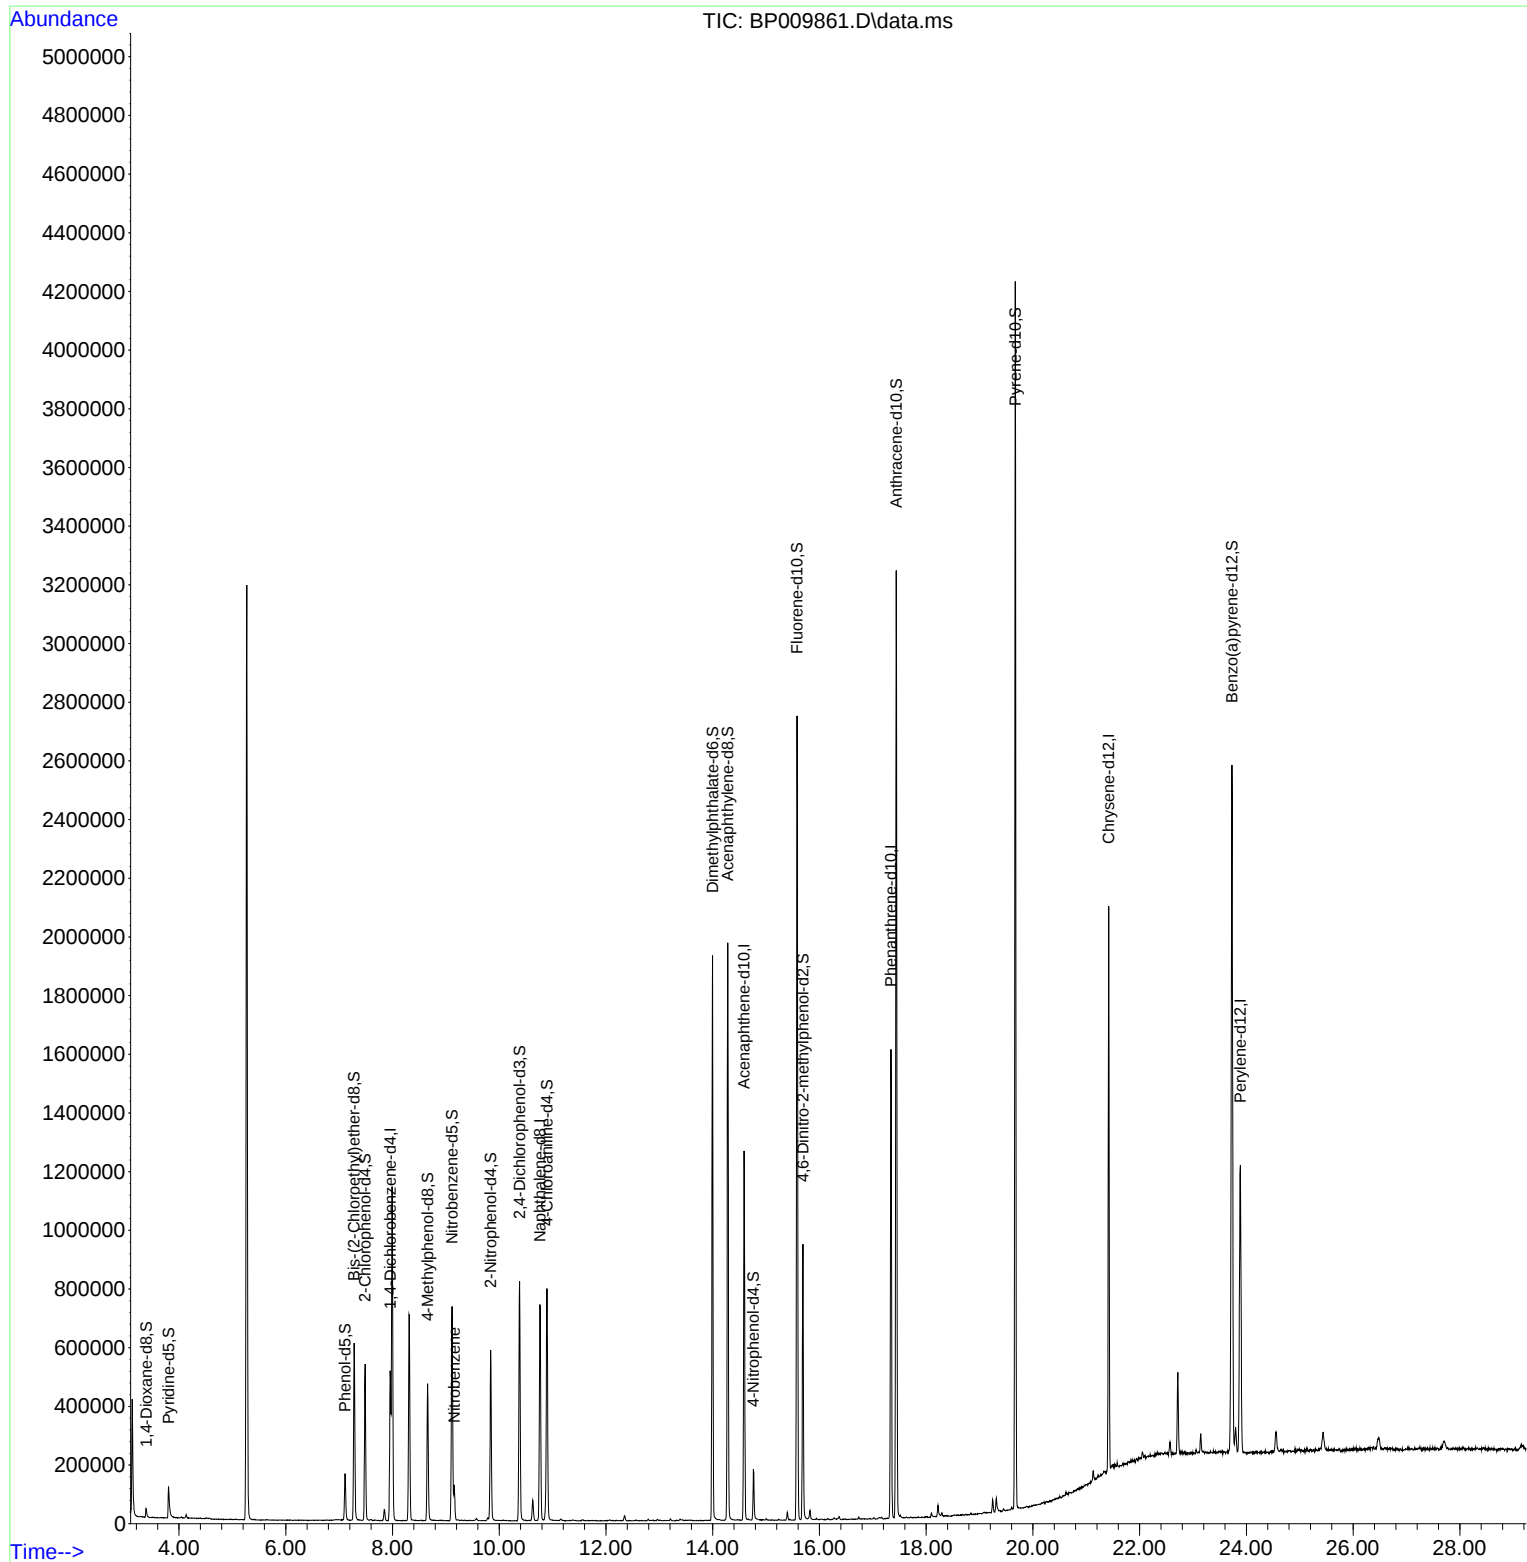

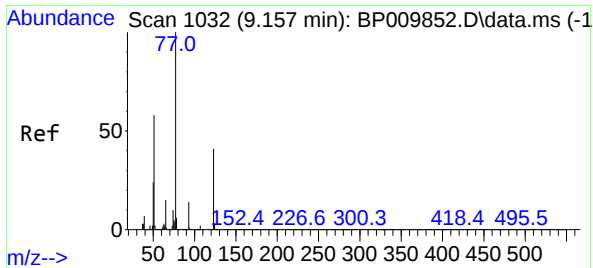

#22
 Nitrobenzene
 Concen: 5.574 ng/ul
 RT: 9.157 min Scan# 10
 Delta R.T. -0.000 min
 Lab File: BP009861.D
 Acq: 15 Apr 2022 15:03

Instrument :
 BNA_P
 ClientSampleId :
 C0J96

Tgt Ion: 77 Resp: 60893

Ion	Ratio	Lower	Upper
77	100		
123	40.8	42.3	63.5#
65	16.8	5.8	8.8#

