

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009873.D
 Acq On : 15 Apr 2022 22:21
 Operator : CG/JU
 Sample : N2421-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J56

Quant Time: Apr 18 01:05:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	147489	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.763	136	663757	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	488896	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.340	188	1098854	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.422	240	1137567	20.000	ng/ul	# 0.00
88) Perylene-d12	23.886	264	1028844	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	13197	3.993	ng/uL	0.00
4) Pyridine-d5	3.799	84	69431	7.620	ng/ul	0.00
7) Phenol-d5	7.111	99	80932	6.250	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	232934	30.217	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	225277	23.064	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	158127	14.629	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	155636	32.515	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	161194	30.717	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	281981	25.679	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	356739	22.809	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	1195561	31.132	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1307981	28.749	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	39536	5.677	ng/ul	0.00
60) Fluorene-d10	15.581	176	1074226	33.251	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.693	200	202755	31.147	ng/ul	0.00
73) Anthracene-d10	17.439	188	1916328	36.424	ng/ul	0.00
81) Pyrene-d10	19.669	212	2365428	38.073	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	2044847	38.165	ng/ul	0.00


Target Compounds					Qvalue
8) Phenol	7.140	94	15300	1.180 ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009873.D
Acq On : 15 Apr 2022 22:21
Operator : CG/JU
Sample : N2421-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J56

Quant Time: Apr 18 01:05:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

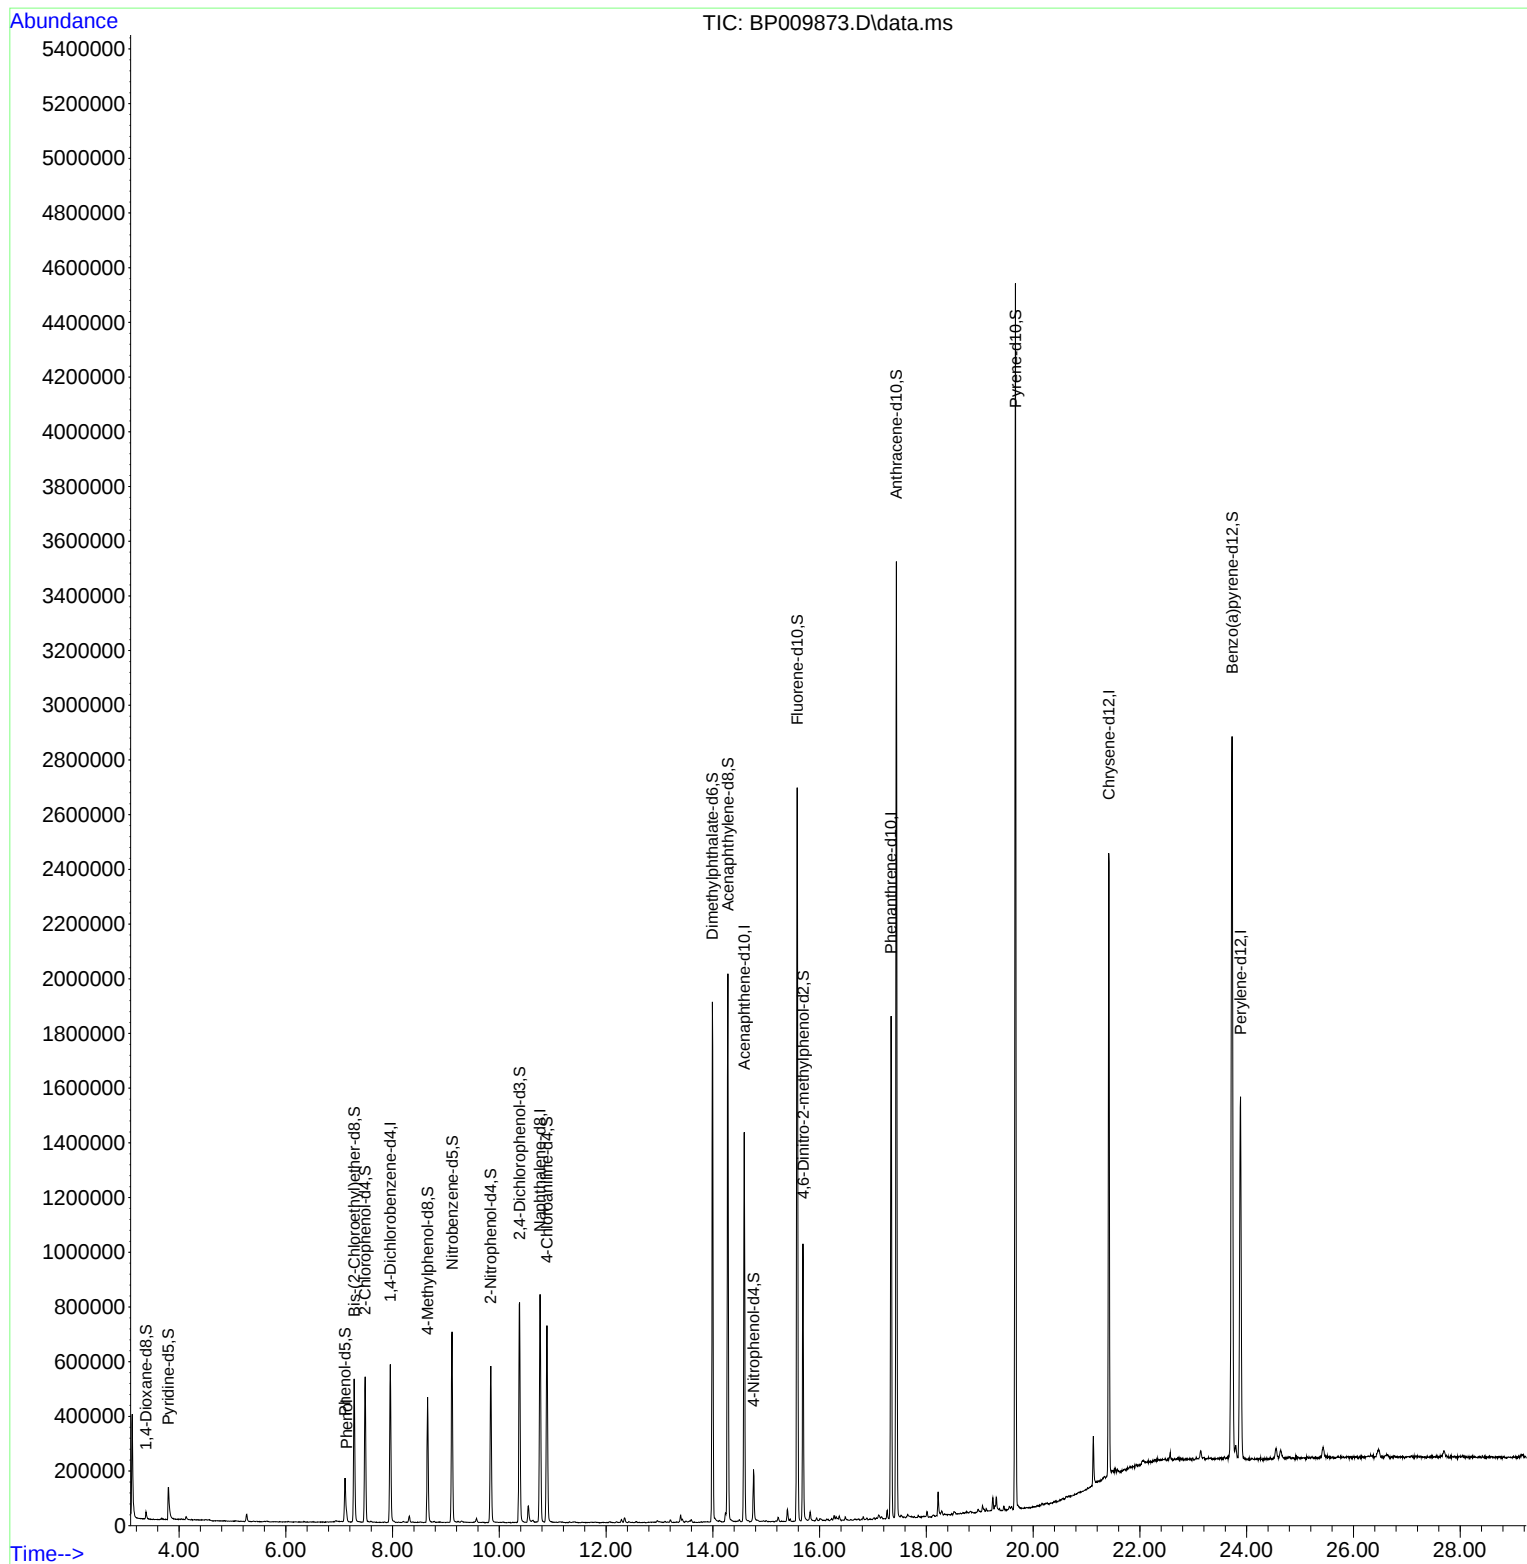

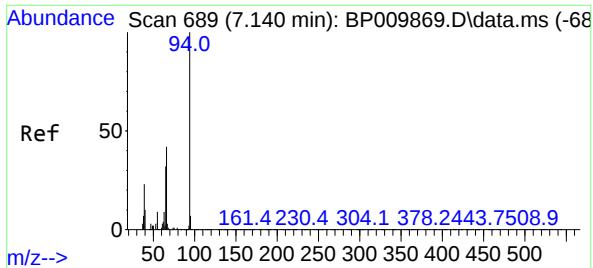

#8
Phenol
Concen: 1.180 ng/ul
RT: 7.140 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP009873.D
Acq: 15 Apr 2022 22:21

Instrument :
BNA_P
ClientSampleId :
C0J56

Tgt Ion: 94 Resp: 15300
Ion Ratio Lower Upper
94 100
65 31.6 19.0 28.6#
66 47.0 34.6 51.8

