

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009880.D
 Acq On : 16 Apr 2022 02:17
 Operator : CG/JU
 Sample : N2421-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HY5

Quant Time: Apr 18 01:07:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	134458	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	589769	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	430110	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	974696	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.416	240	1046395	20.000	ng/ul	# 0.00
88) Perylene-d12	23.880	264	966679	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	13288	4.411	ng/uL	0.00
4) Pyridine-d5	3.799	84	93262	11.227	ng/ul	0.00
7) Phenol-d5	7.111	99	87244	7.391	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	242094	34.449	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	231586	26.008	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	170867	17.339	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	160471	37.731	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	169959	36.450	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	295063	30.241	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	318627	22.928	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	1243256	36.798	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1344536	33.591	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	46391	7.571	ng/ul	0.00
60) Fluorene-d10	15.581	176	1083129	38.109	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	205614	35.610	ng/ul	0.00
73) Anthracene-d10	17.439	188	1883844	40.367	ng/ul	0.00
81) Pyrene-d10	19.669	212	2313128	40.475	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	2122313	42.159	ng/ul	0.00


Target Compounds					Qvalue	
8) Phenol	7.134	94	16130	1.365	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009880.D
Acq On : 16 Apr 2022 02:17
Operator : CG/JU
Sample : N2421-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY5


Quant Time: Apr 18 01:07:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

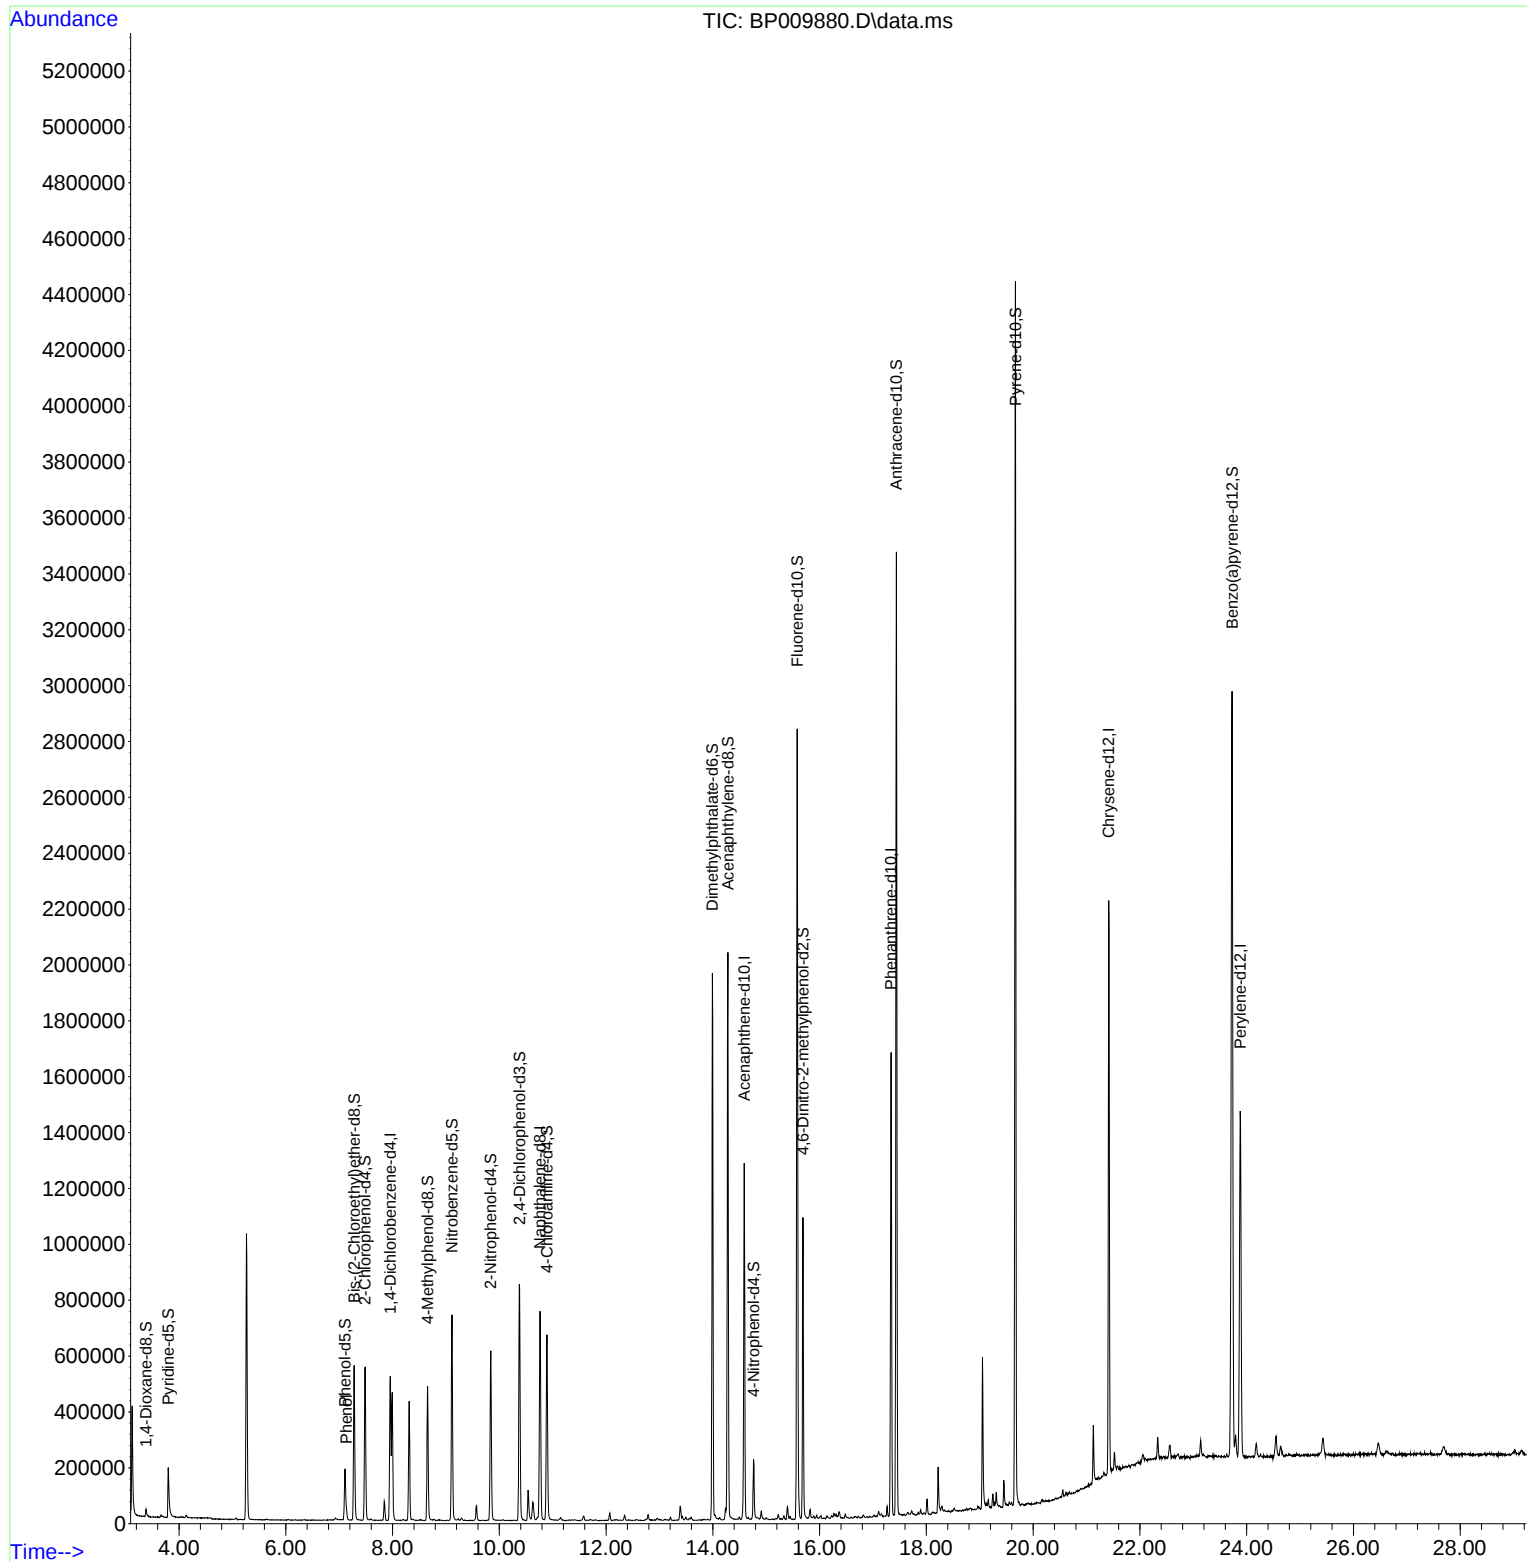

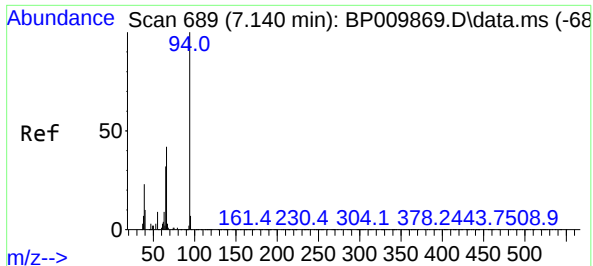

#8
Phenol
Concen: 1.365 ng/ul
RT: 7.134 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP009880.D
Acq: 16 Apr 2022 02:17

Instrument :
BNA_P
ClientSampleId :
C0HY5

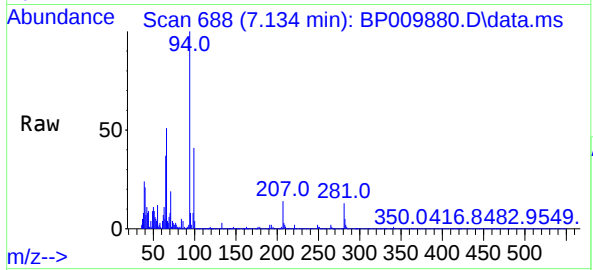

Tgt Ion: 94 Resp: 16130
Ion Ratio Lower Upper
94 100
65 37.1 19.0 28.6#
66 51.1 34.6 51.8

