

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009881.D
 Acq On : 16 Apr 2022 02:50
 Operator : CG/JU
 Sample : N2422-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J42

Quant Time: Apr 18 01:07:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	119266	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	546073	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	395364	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	903566	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.416	240	941663	20.000	ng/ul	# 0.00
88) Perylene-d12	23.880	264	869895	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	11842	4.431	ng/uL	0.00
4) Pyridine-d5	3.805	84	69513	9.434	ng/ul	0.00
7) Phenol-d5	7.111	99	54613	5.216	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	141929	22.768	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	135417	17.145	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	101880	11.656	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	89092	22.624	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	90901	21.055	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	166783	18.461	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	342060	26.584	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	728545	23.459	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	773510	21.023	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	27858	4.946	ng/ul	0.00
60) Fluorene-d10	15.581	176	626783	23.991	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	101675	18.995	ng/ul	0.00
73) Anthracene-d10	17.434	188	1083008	25.034	ng/ul	0.00
81) Pyrene-d10	19.669	212	1420223	27.615	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	1264069	27.904	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.140	94	19558	1.866	ng/ul#	86
78) Di-n-butylphthalate	18.292	149	203296	3.741	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009881.D
Acq On : 16 Apr 2022 02:50
Operator : CG/JU
Sample : N2422-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J42

Quant Time: Apr 18 01:07:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration




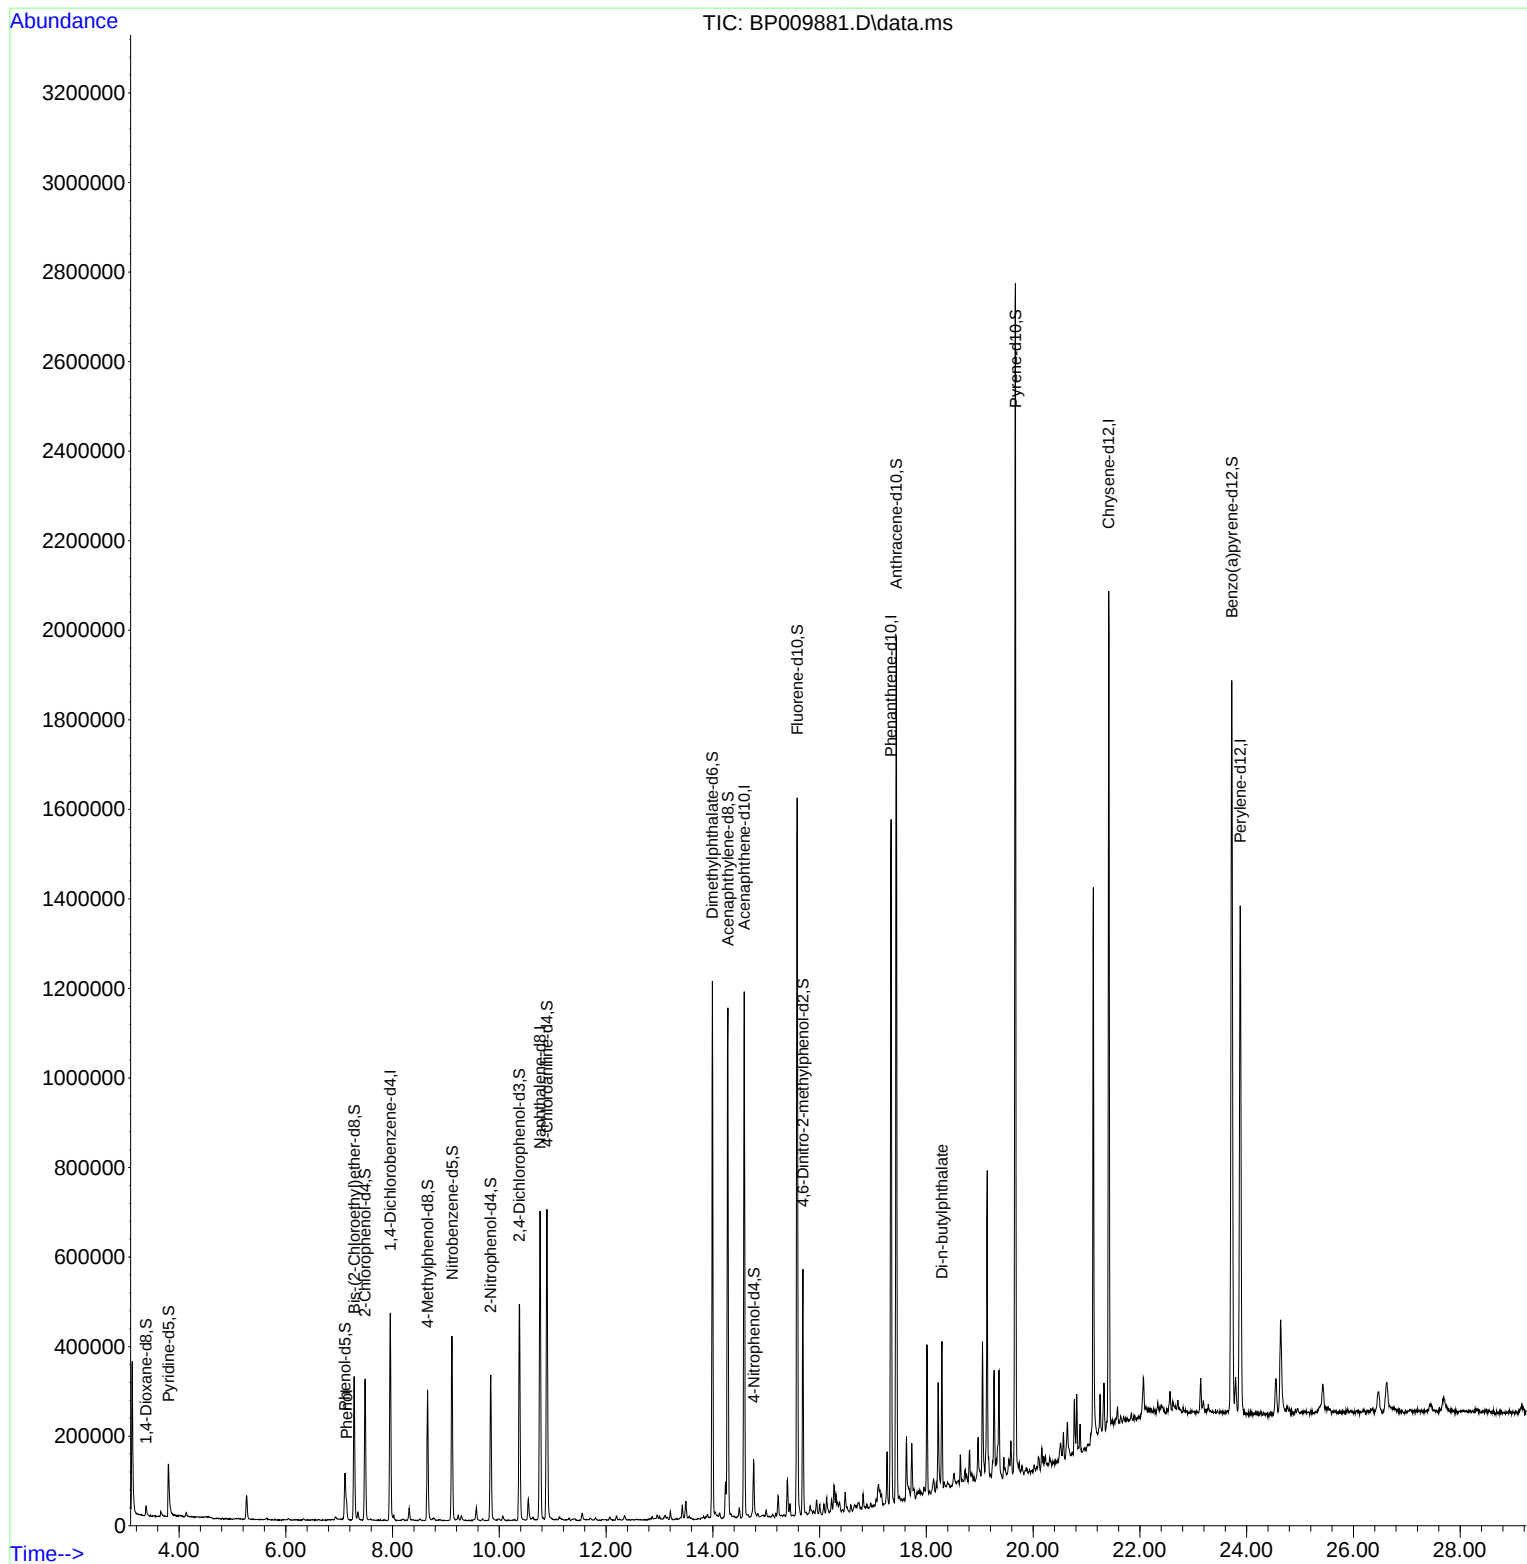


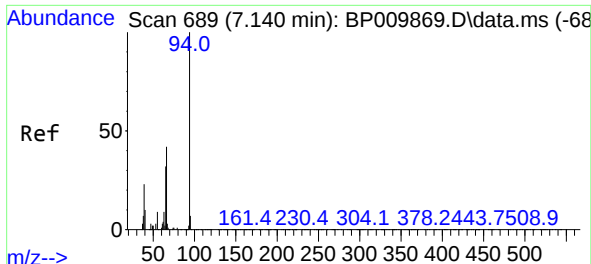

#8
Phenol
Concen: 1.866 ng/ul
RT: 7.140 min Scan# 689
Delta R.T. 0.000 min
Lab File: BP009881.D
Acq: 16 Apr 2022 02:50

Instrument :
BNA_P
ClientSampleId :
C0J42

Tgt Ion: 94 Resp: 19558
Ion Ratio Lower Upper
94 100
65 35.2 19.0 28.6#
66 37.8 34.6 51.8

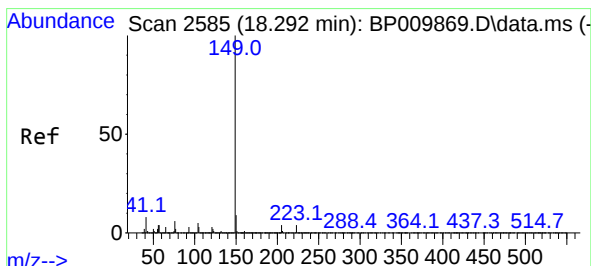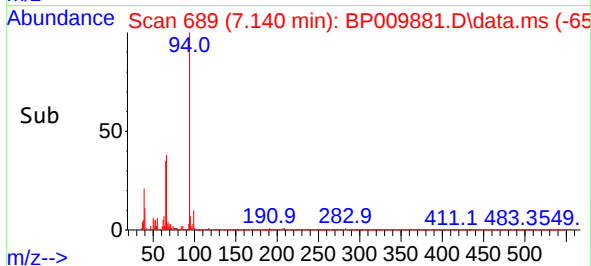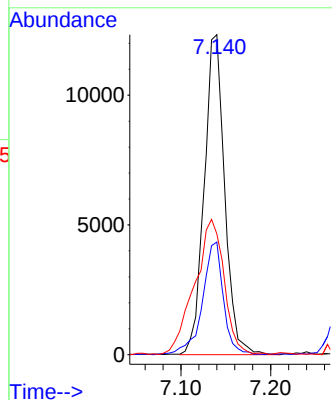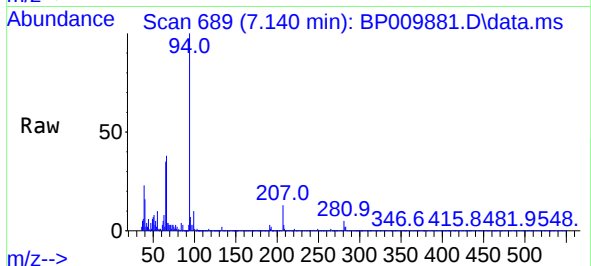

#78
Di-n-butylphthalate
Concen: 3.741 ng/ul
RT: 18.292 min Scan# 2585
Delta R.T. -0.006 min
Lab File: BP009881.D
Acq: 16 Apr 2022 02:50

Tgt Ion: 149 Resp: 203296
Ion Ratio Lower Upper
149 100
150 9.3 9.6 14.4#
104 5.8 6.2 9.4#

