

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009896.D
 Acq On : 16 Apr 2022 11:48
 Operator : CG/JU
 Sample : N2421-14
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J45

Quant Time: Apr 18 01:12:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	139888	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	623570	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	461332	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1056688	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.416	240	1088432	20.000	ng/ul	# 0.00
88) Perylene-d12	23.880	264	994969	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	13211	4.215	ng/uL	0.00
4) Pyridine-d5	3.805	84	52153	6.035	ng/ul	0.00
7) Phenol-d5	7.111	99	73719	6.003	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	209810	28.696	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	199906	21.579	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	145932	14.234	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	135633	30.162	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	143352	29.077	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	249498	24.185	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	364481	24.806	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	1084804	29.935	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1177780	27.434	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	38818	5.907	ng/ul	0.00
60) Fluorene-d10	15.581	176	943080	30.936	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	170427	27.225	ng/ul	0.00
73) Anthracene-d10	17.439	188	1636889	32.354	ng/ul	0.00
81) Pyrene-d10	19.669	212	2021774	34.011	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	1775841	34.273	ng/ul	0.00
Target Compounds						
					Qvalue	
39) 1,2,4,5-Tetrachloroben...	12.787	216	442262	31.334	ng/ul	93
75) 1,2,3,4-Tetrachloroben...	13.387	216	310159	20.302	ng/uL#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009896.D
Acq On : 16 Apr 2022 11:48
Operator : CG/JU
Sample : N2421-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J45

Quant Time: Apr 18 01:12:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration




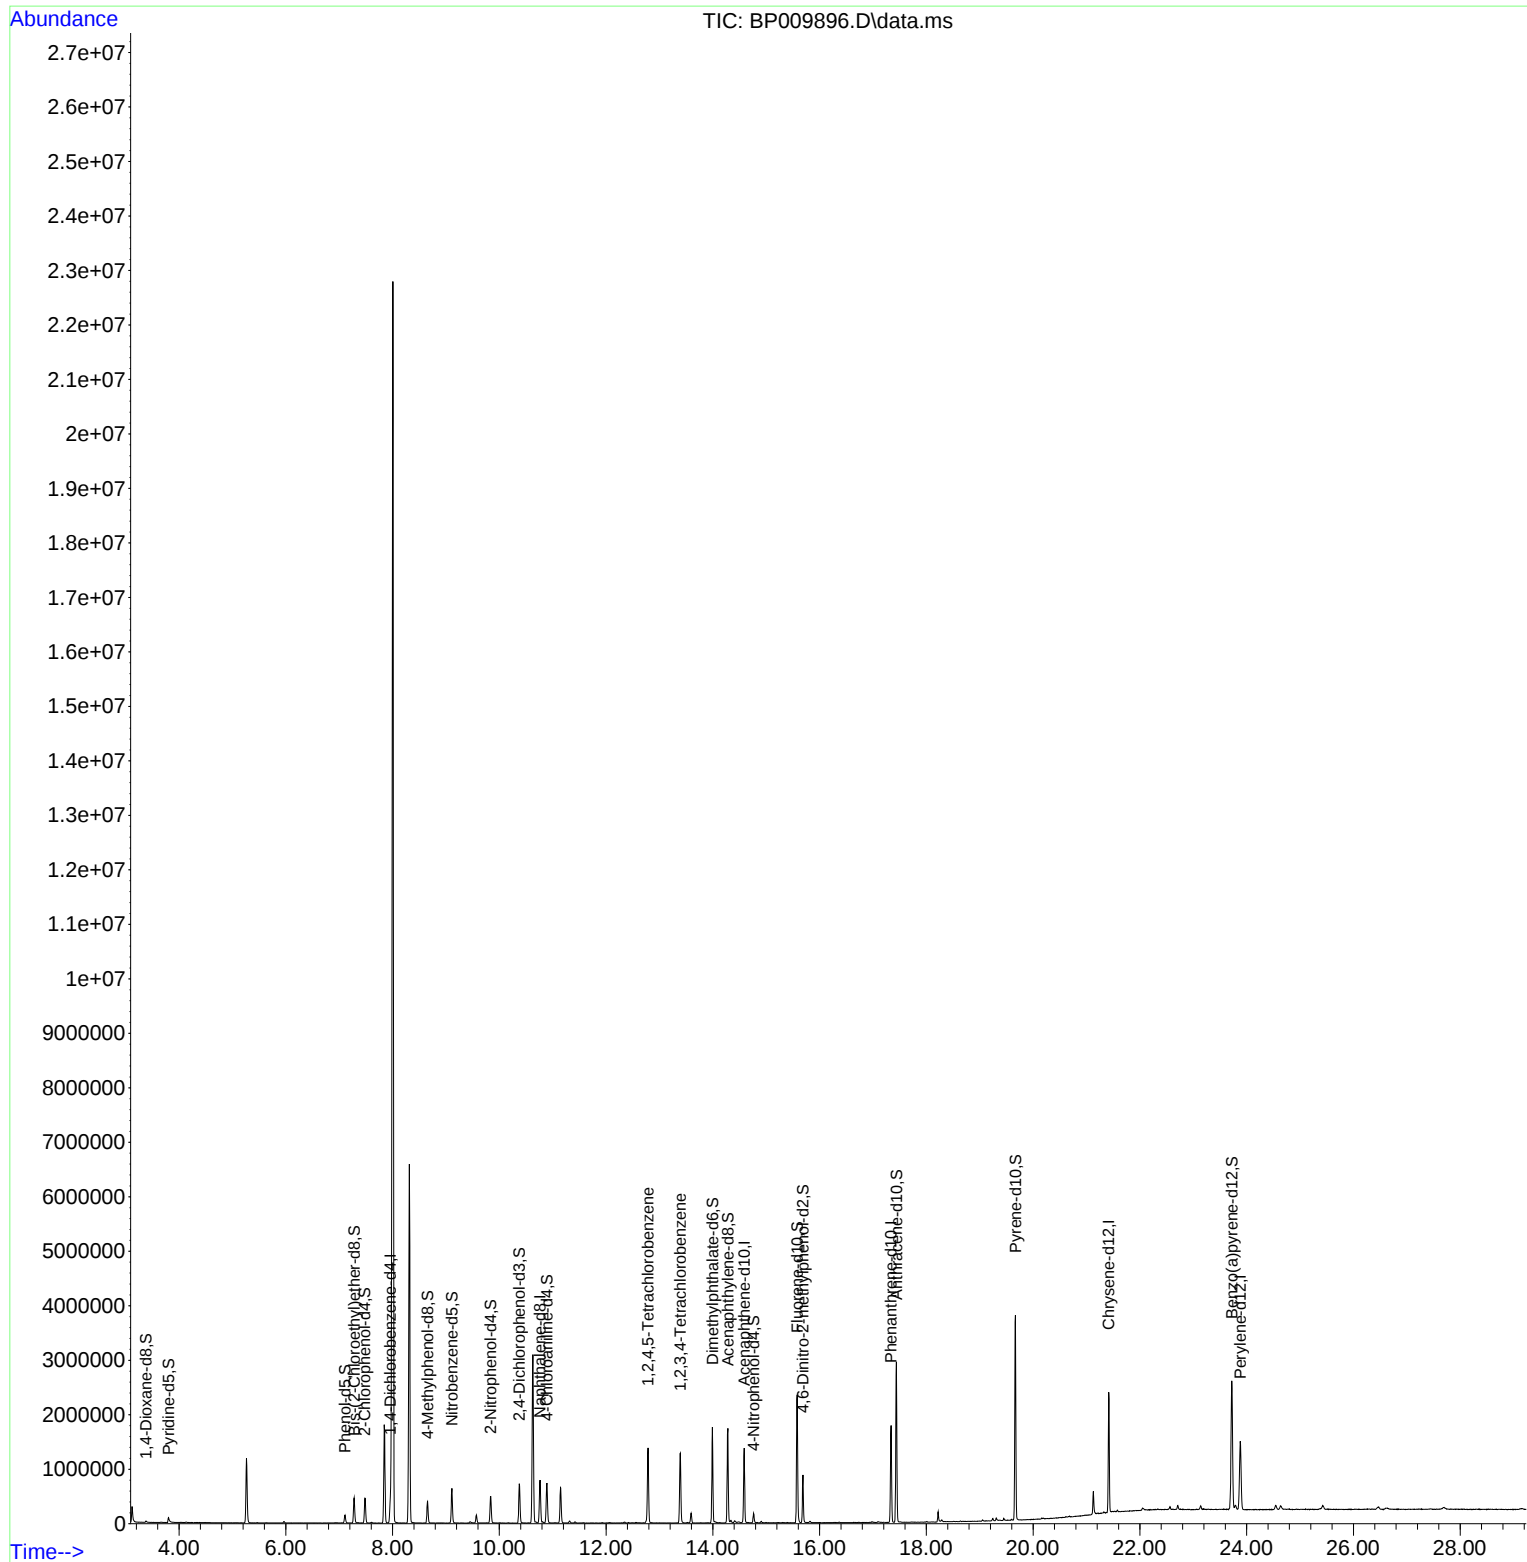


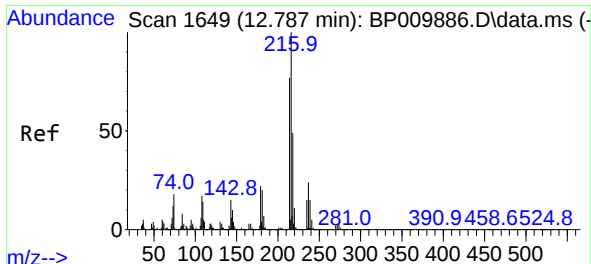

#39
1,2,4,5-Tetrachlorobenzene
Concen: 31.334 ng/ul
RT: 12.787 min Scan# 1649
Delta R.T. -0.006 min
Lab File: BP009896.D
Acq: 16 Apr 2022 11:48

Instrument :
BNA_P
ClientSampleId :
C0J45

Tgt Ion:216 Resp: 442262
Ion Ratio Lower Upper
216 100
214 78.0 58.2 87.2
179 20.8 14.2 21.2
108 15.9 15.3 22.9

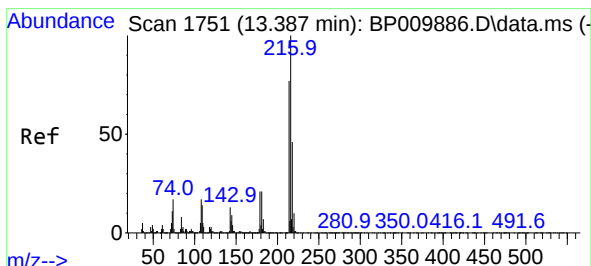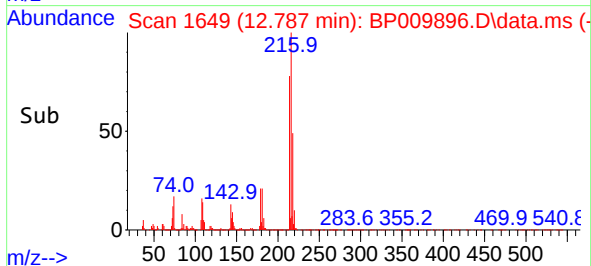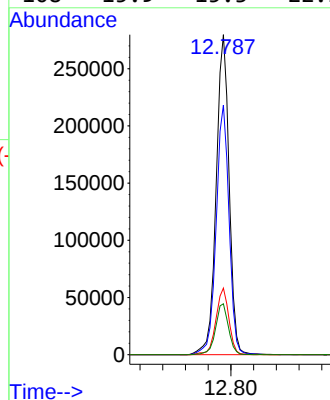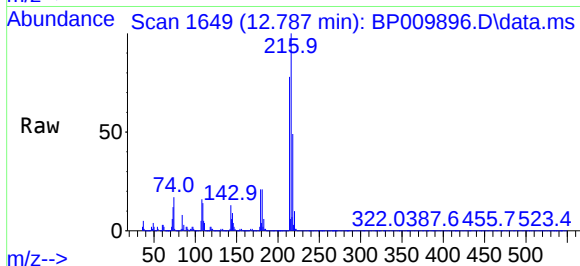

#75
1,2,3,4-Tetrachlorobenzene
Concen: 20.302 ng/ul
RT: 13.387 min Scan# 1751
Delta R.T. -0.006 min
Lab File: BP009896.D
Acq: 16 Apr 2022 11:48

Tgt Ion:216 Resp: 310159
Ion Ratio Lower Upper
216 100
214 76.7 50.4 75.6#
218 48.3 35.2 52.8

