

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009899.D
 Acq On : 16 Apr 2022 13:29
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Quant Time: Apr 18 01:13:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	140483	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	640657	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	472358	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1067252	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.421	240	1080917	20.000	ng/ul	# 0.00
88) Perylene-d12	23.886	264	966131	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	13327	4.234	ng/uL	0.00
4) Pyridine-d5	3.799	84	97822	11.271	ng/ul	0.00
7) Phenol-d5	7.110	99	80925	6.561	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	254304	34.634	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	235640	25.328	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	171108	16.619	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	171441	37.109	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	179508	35.440	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	303843	28.667	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	448710	29.724	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	1361505	36.694	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1465986	33.350	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	41123	6.111	ng/ul	0.00
60) Fluorene-d10	15.581	176	1190276	38.133	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	207399	32.804	ng/ul	0.00
73) Anthracene-d10	17.439	188	2059493	40.304	ng/ul	0.00
81) Pyrene-d10	19.669	212	2462368	41.711	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	2187135	43.471	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.134	94	14780	1.197	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009899.D
Acq On : 16 Apr 2022 13:29
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COHX0


Quant Time: Apr 18 01:13:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

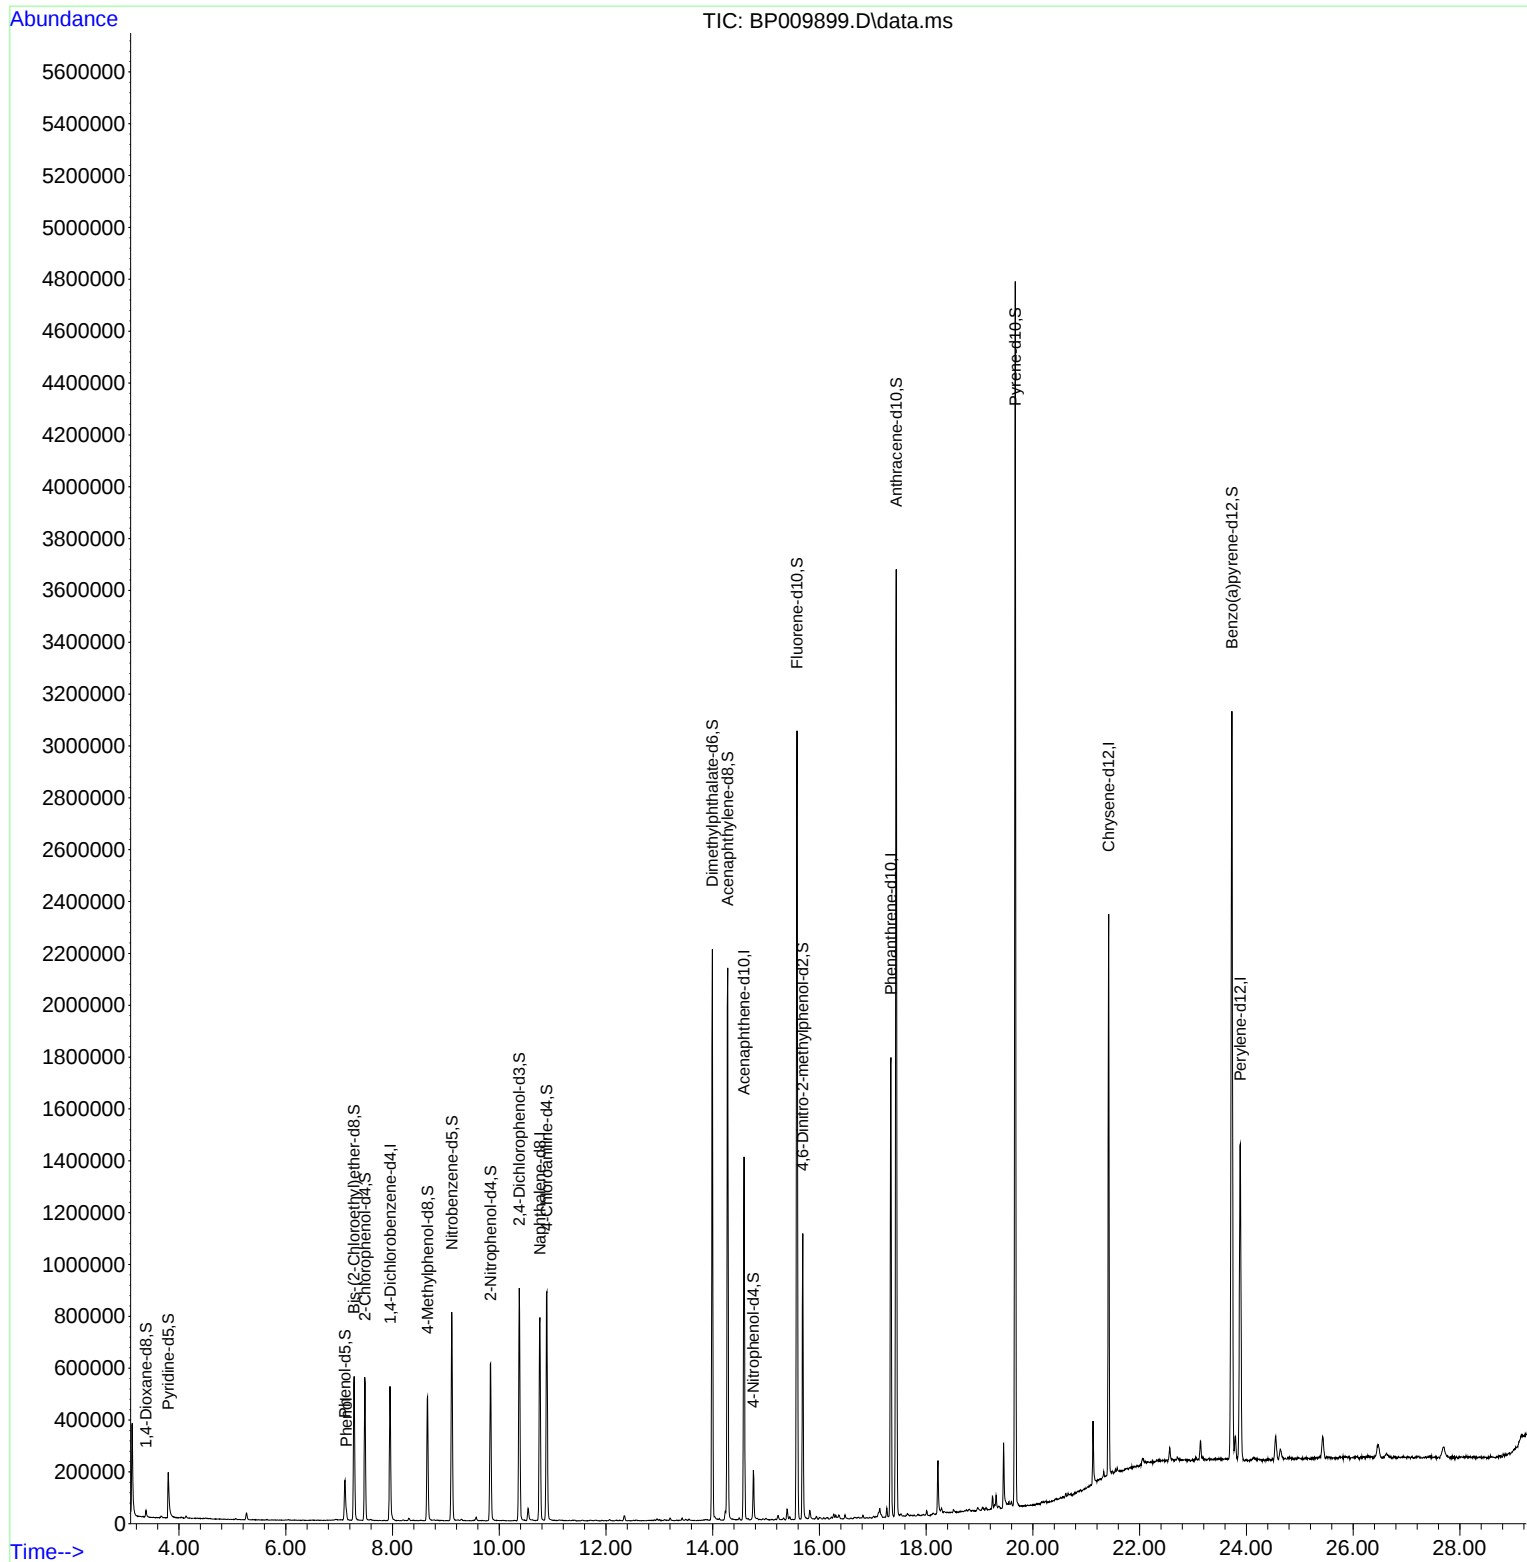

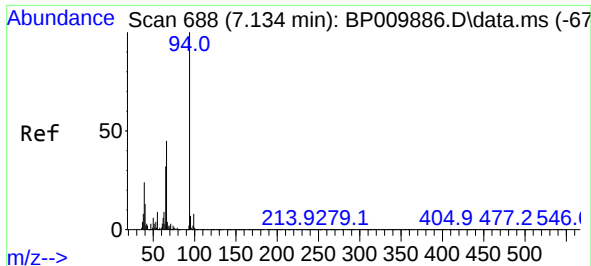

#8
Phenol
Concen: 1.197 ng/ul
RT: 7.134 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP009899.D
Acq: 16 Apr 2022 13:29

Instrument :
BNA_P
ClientSampleId :
COHX0

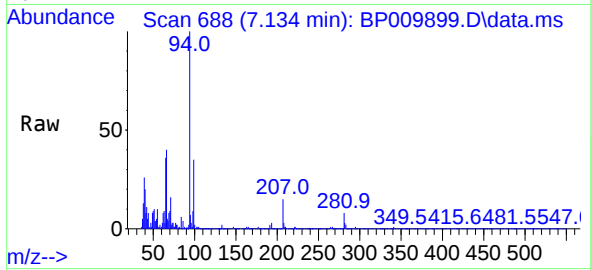

Tgt Ion: 94 Resp: 14780
Ion Ratio Lower Upper
94 100
65 36.3 19.0 28.6#
66 40.5 34.6 51.8

