

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009853.D
 Acq On : 15 Apr 2022 10:31
 Operator : CG/JU
 Sample : PB144122BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	19	rVB2	21350	39822	0.89%	0.086%
2	3.381	46	50	61	rVB	36257	56838	1.27%	0.123%
3	3.799	117	121	139	rBV	487736	816448	18.31%	1.772%
4	4.134	175	178	185	rVB3	8851	12646	0.28%	0.027%
5	7.111	677	684	695	rBV	632107	1018535	22.84%	2.211%
6	7.281	706	713	728	rVB	500724	816567	18.31%	1.772%
7	7.487	741	748	759	rBV	662001	1035610	23.23%	2.248%
8	7.958	821	828	837	rBV	596020	970888	21.78%	2.107%
9	8.658	938	947	960	rBV	847240	1377341	30.89%	2.989%
10	9.116	1015	1025	1038	rBV	695502	1146664	25.72%	2.489%
11	9.840	1141	1148	1159	rBV	550493	932889	20.92%	2.025%
12	10.381	1229	1240	1251	rBV	820702	1398311	31.36%	3.035%
13	10.763	1298	1305	1318	rBV	913796	1586193	35.58%	3.443%
14	10.893	1319	1327	1342	rBV	879106	1522966	34.16%	3.305%
15	12.346	1569	1574	1583	rVB2	17275	29003	0.65%	0.063%
16	13.999	1845	1855	1865	rBV	1707950	2383186	53.45%	5.172%
17	14.281	1896	1903	1921	rBV	1808859	2628186	58.95%	5.704%
18	14.593	1948	1956	1966	rBV	1516705	2342626	52.54%	5.084%
19	14.769	1976	1986	2001	rBV	781787	1160114	26.02%	2.518%
20	15.410	2091	2095	2098	rBV6	2776	4734	0.11%	0.010%
21	15.581	2117	2124	2136	rBV	2399029	3396054	76.17%	7.370%
22	15.693	2136	2143	2154	rBV	732634	1061981	23.82%	2.305%
23	15.822	2161	2165	2170	rVB	26541	38430	0.86%	0.083%
24	16.269	2236	2241	2243	rBV5	3757	6139	0.14%	0.013%
25	16.369	2252	2258	2264	rBV4	8517	15784	0.35%	0.034%
26	17.022	2365	2369	2373	rVB7	5683	8596	0.19%	0.019%
27	17.128	2382	2387	2395	rVB3	8264	12972	0.29%	0.028%
28	17.340	2416	2423	2433	rBV	2064009	2910195	65.27%	6.316%
29	17.440	2433	2440	2454	rVV	2743515	3784803	84.89%	8.214%
30	18.228	2570	2574	2577	rBV5	4494	6729	0.15%	0.015%
31	19.245	2742	2747	2751	rBV3	34641	50317	1.13%	0.109%
32	19.316	2754	2759	2764	rVV	34572	49427	1.11%	0.107%
33	19.669	2813	2819	2829	rBV	3438465	4458631	100.00%	9.677%
34	21.422	3111	3117	3123	rBV	2251513	3047374	68.35%	6.614%
35	23.722	3501	3508	3517	rVB2	1709412	3463948	77.69%	7.518%
36	23.886	3528	3536	3545	rVB2	1203846	2485658	55.75%	5.395%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009853.D
Acq On : 15 Apr 2022 10:31
Operator : CG/JU
Sample : PB144122BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK122

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION


Sum of corrected areas: 46076605

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009853.D
Acq On : 15 Apr 2022 10:31
Operator : CG/JU
Sample : PB144122BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

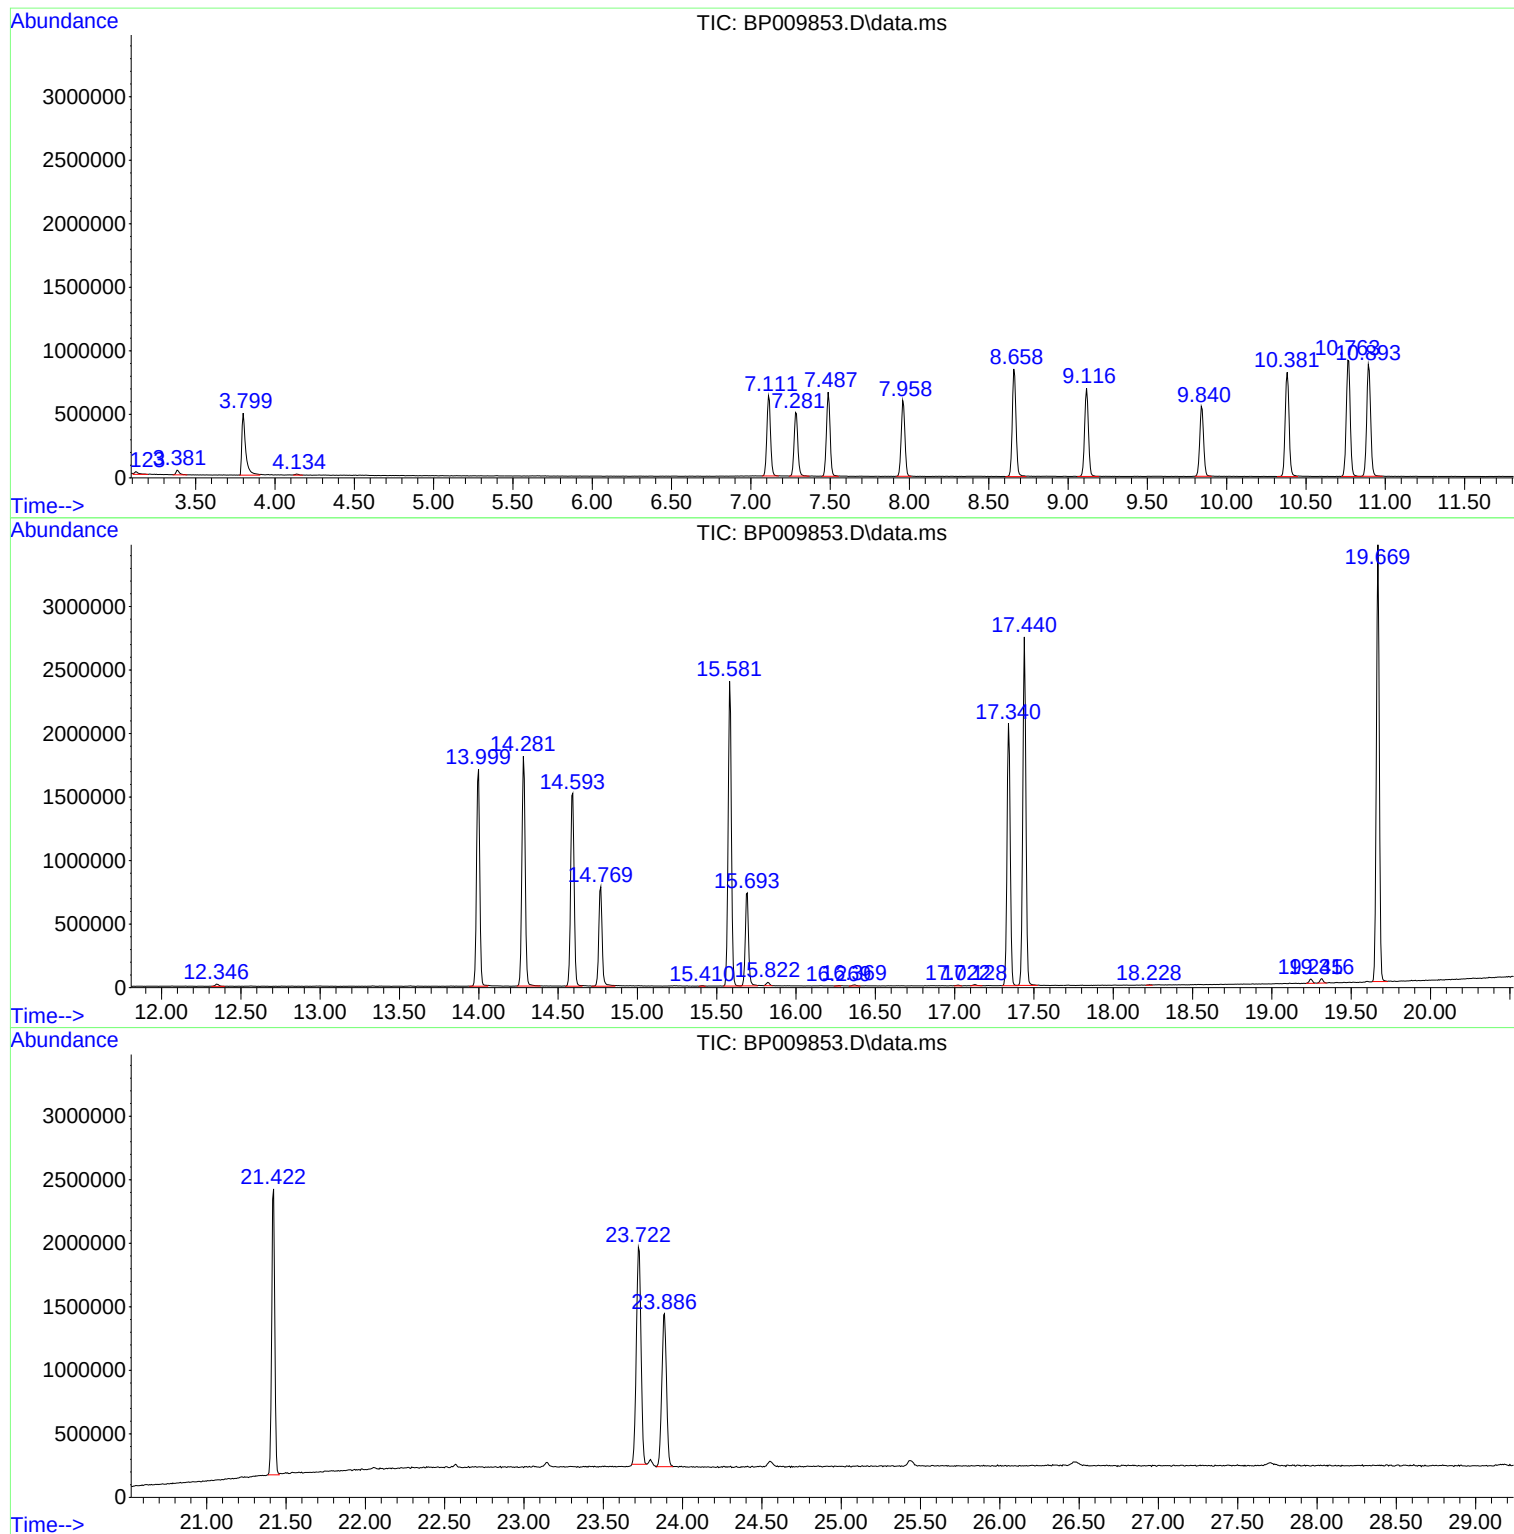

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009853.D
Acq On : 15 Apr 2022 10:31
Operator : CG/JU
Sample : PB144122BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009853.D
Acq On : 15 Apr 2022 10:31
Operator : CG/JU
Sample : PB144122BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc