

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009858.D
 Acq On : 15 Apr 2022 13:22
 Operator : CG/JU
 Sample : N2422-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	22	rVB	287333	433864	8.99%	1.071%
2	3.381	46	50	59	rVB	21904	34378	0.71%	0.085%
3	3.805	118	122	134	rBV	115135	214815	4.45%	0.530%
4	4.134	174	178	183	rVB3	7399	11563	0.24%	0.029%
5	4.670	265	269	275	rBV8	3124	5204	0.11%	0.013%
6	6.934	650	654	659	rBV7	3350	5572	0.12%	0.014%
7	7.111	676	684	693	rBV	114468	195658	4.05%	0.483%
8	7.281	706	713	725	rBV	413195	679443	14.08%	1.677%
9	7.487	741	748	761	rBV	420973	669073	13.87%	1.651%
10	7.958	820	828	838	rBV	419882	693040	14.36%	1.710%
11	8.658	940	947	961	rBV	354827	580097	12.02%	1.431%
12	9.116	1018	1025	1037	rBV	578451	970368	20.11%	2.394%
13	9.234	1039	1045	1051	rVV3	13913	22664	0.47%	0.056%
14	9.293	1051	1055	1061	rVB8	2813	5730	0.12%	0.014%
15	9.569	1097	1102	1108	rVB4	9625	16381	0.34%	0.040%
16	9.840	1139	1148	1163	rBV	449879	756202	15.67%	1.866%
17	10.381	1232	1240	1255	rBV	641298	1104853	22.90%	2.726%
18	10.563	1264	1271	1276	rBV7	6289	12687	0.26%	0.031%
19	10.763	1298	1305	1319	rVB	621237	1085760	22.50%	2.679%
20	10.893	1319	1327	1337	rBV	646652	1133090	23.48%	2.796%
21	11.557	1435	1440	1444	rBV6	4447	8171	0.17%	0.020%
22	12.069	1521	1527	1535	rBV9	5151	10242	0.21%	0.025%
23	12.163	1538	1543	1546	rBV5	4326	5840	0.12%	0.014%
24	12.351	1565	1575	1581	rBV2	14072	25596	0.53%	0.063%
25	12.963	1674	1679	1684	rVV7	5459	9129	0.19%	0.023%
26	13.210	1715	1721	1728	rBV6	7800	11302	0.23%	0.028%
27	13.434	1756	1759	1765	rVB7	5587	7071	0.15%	0.017%
28	13.563	1777	1781	1787	rBV8	3475	6800	0.14%	0.017%
29	13.869	1829	1833	1836	rBV6	4244	7079	0.15%	0.017%
30	13.993	1848	1854	1861	rBV	1564105	2176810	45.11%	5.371%
31	14.122	1872	1876	1885	rVB	4623	11032	0.23%	0.027%
32	14.281	1891	1903	1916	rBV	1570196	2338762	48.47%	5.771%
33	14.498	1936	1940	1944	rBV5	5557	7060	0.15%	0.017%
34	14.587	1947	1955	1965	rBV	1029938	1610085	33.37%	3.973%
35	14.669	1967	1969	1973	rVB5	5292	5853	0.12%	0.014%
36	14.763	1979	1985	1993	rBV	141956	225016	4.66%	0.555%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009858.D
 Acq On : 15 Apr 2022 13:22
 Operator : CG/JU
 Sample : N2422-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	14.851	1996	2000	2011	rVB	18073	32762	0.68%	0.081%
38	14.998	2021	2025	2033	rBV	6008	10272	0.21%	0.025%
39	15.222	2059	2063	2069	rVB	10314	17100	0.35%	0.042%
40	15.398	2088	2093	2098	rBV3	33571	49476	1.03%	0.122%
41	15.445	2098	2101	2105	rVB5	5177	8390	0.17%	0.021%
42	15.581	2117	2124	2136	rBV	2225206	3207811	66.48%	7.915%
43	15.687	2136	2142	2155	rBV	785344	1136007	23.54%	2.803%
44	15.822	2159	2165	2170	rVV4	24355	40114	0.83%	0.099%
45	15.945	2182	2186	2192	rVB6	10734	16394	0.34%	0.040%
46	16.004	2192	2196	2202	rBV8	5236	8116	0.17%	0.020%
47	16.087	2205	2210	2215	rVB9	3516	5642	0.12%	0.014%
48	16.134	2215	2218	2226	rBV10	7003	14775	0.31%	0.036%
49	16.228	2230	2234	2237	rBV6	5325	6874	0.14%	0.017%
50	16.269	2237	2241	2245	rBV7	12149	19826	0.41%	0.049%
51	16.369	2255	2258	2263	rVB5	9712	14211	0.29%	0.035%
52	16.481	2274	2277	2282	rVV6	8049	11472	0.24%	0.028%
53	16.816	2332	2334	2339	rVB5	7130	8864	0.18%	0.022%
54	17.022	2365	2369	2373	rBV7	4019	5869	0.12%	0.014%
55	17.110	2378	2384	2388	rBV8	7302	16982	0.35%	0.042%
56	17.269	2406	2411	2415	rBV3	19335	26117	0.54%	0.064%
57	17.339	2417	2423	2432	rVV	1440232	2031257	42.10%	5.012%
58	17.439	2433	2440	2452	rBV	2836311	3971425	82.30%	9.800%
59	17.628	2468	2472	2476	rBV	22321	32954	0.68%	0.081%
60	18.010	2535	2537	2541	rVB5	10845	12009	0.25%	0.030%
61	18.222	2569	2573	2580	rBV2	41250	51788	1.07%	0.128%
62	18.292	2581	2585	2590	rVB	61738	71710	1.49%	0.177%
63	18.639	2642	2644	2648	rVB4	10956	8085	0.17%	0.020%
64	18.969	2698	2700	2706	rVB4	12240	14903	0.31%	0.037%
65	19.057	2712	2715	2720	rBV3	19206	22879	0.47%	0.056%
66	19.245	2743	2747	2752	rBV2	37652	52331	1.08%	0.129%
67	19.310	2755	2758	2762	rVV	32054	40054	0.83%	0.099%
68	19.451	2779	2782	2785	rBV5	17327	21989	0.46%	0.054%
69	19.669	2813	2819	2829	rBV	3583929	4794542	99.36%	11.831%
70	21.127	3064	3067	3072	rVB2	82509	105776	2.19%	0.261%
71	21.422	3111	3117	3123	rBV	1747974	2384839	49.42%	5.885%
72	23.727	3501	3509	3517	rBV2	2433358	4825386	100.00%	11.907%
73	23.886	3529	3536	3551	rVB2	1107501	2331472	48.32%	5.753%


Sum of corrected areas: 40526763

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009858.D
Acq On : 15 Apr 2022 13:22
Operator : CG/JU
Sample : N2422-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

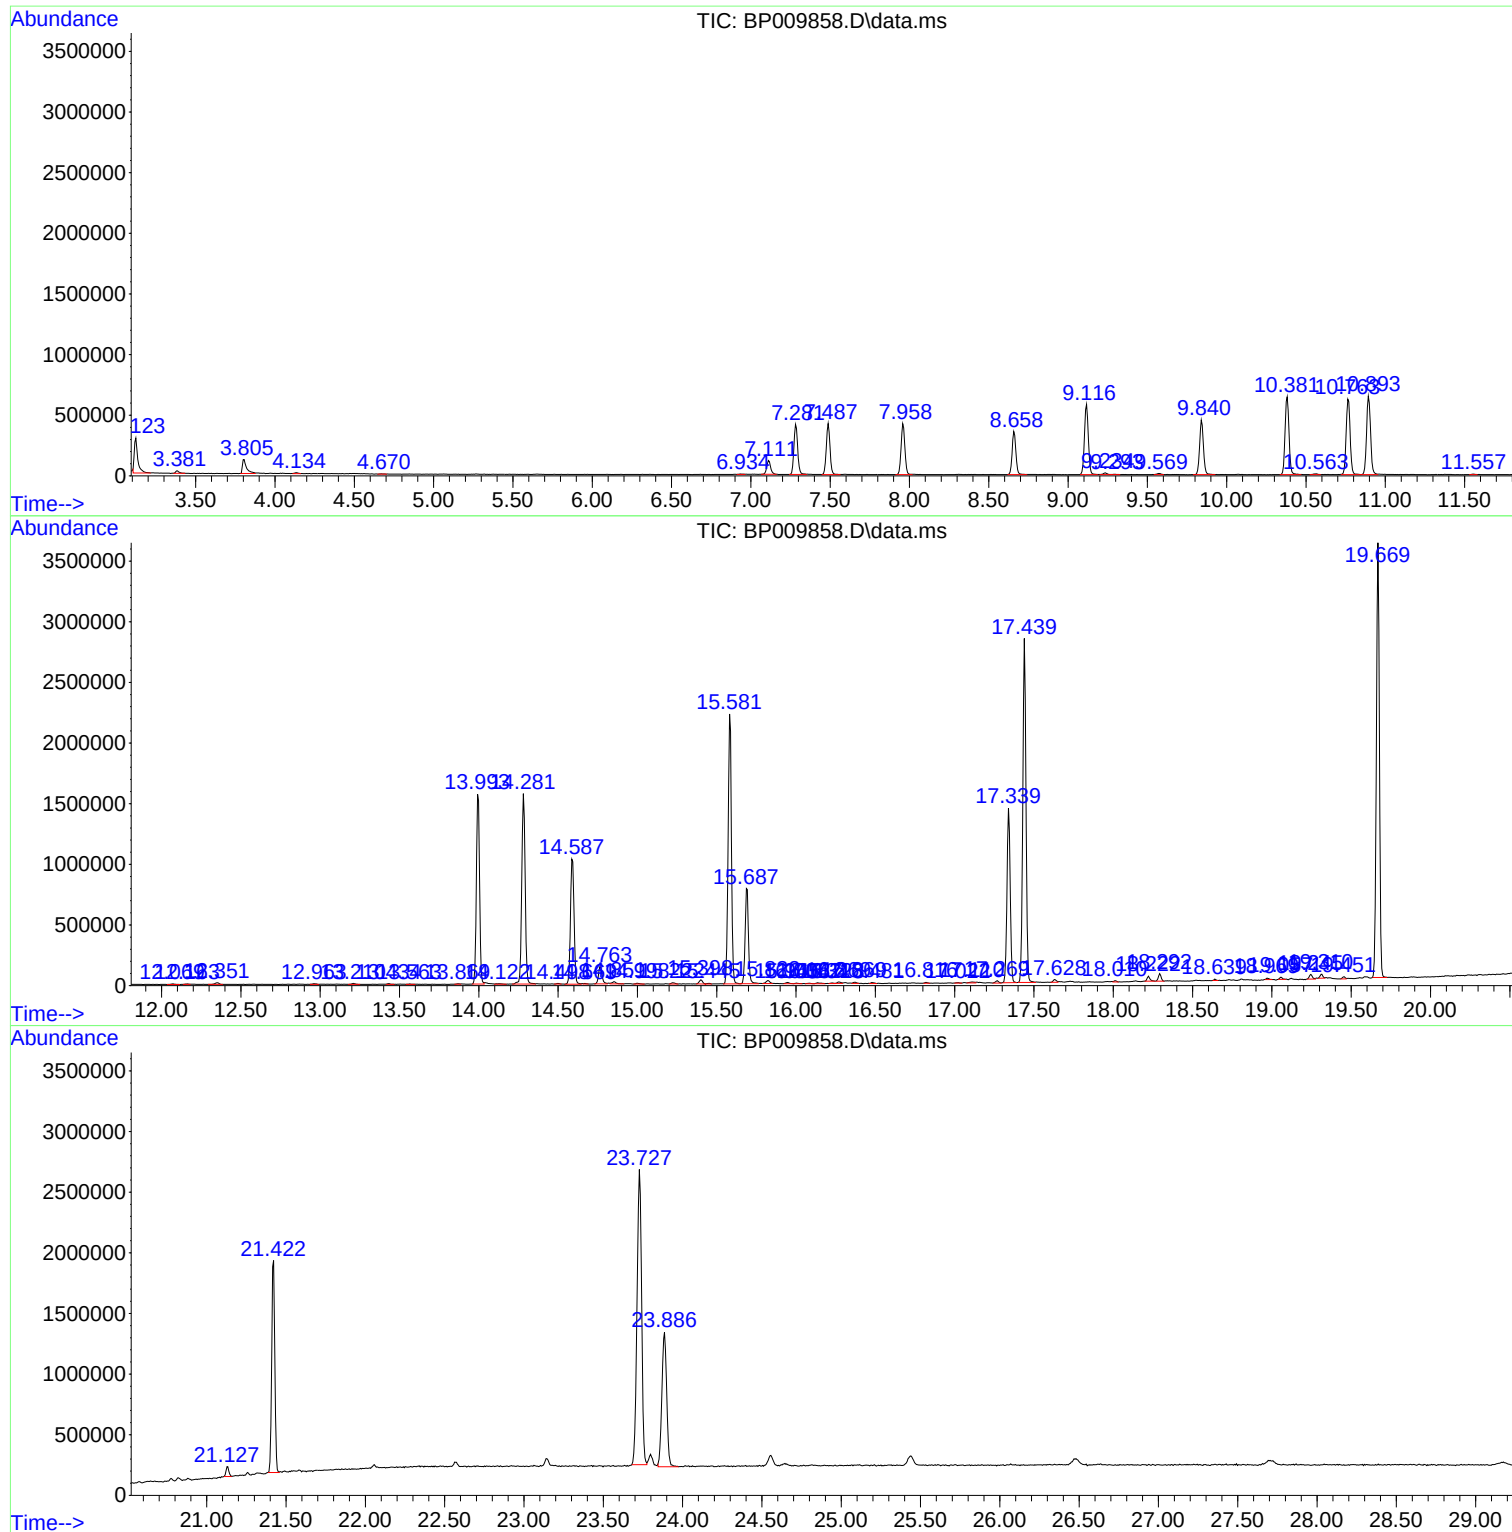

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009858.D
Acq On : 15 Apr 2022 13:22
Operator : CG/JU
Sample : N2422-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J33










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.123	12.52 ng/ul	433864	1,4-Dichlorobenzene-d4	7.958

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	45
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	38
5			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9

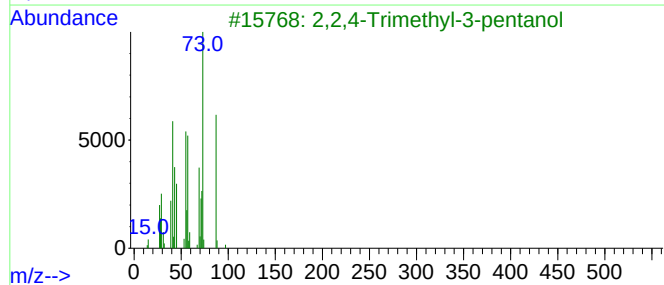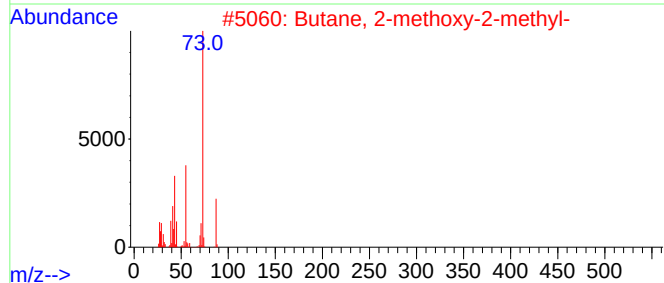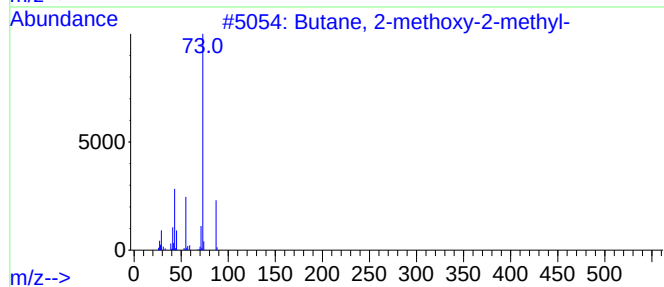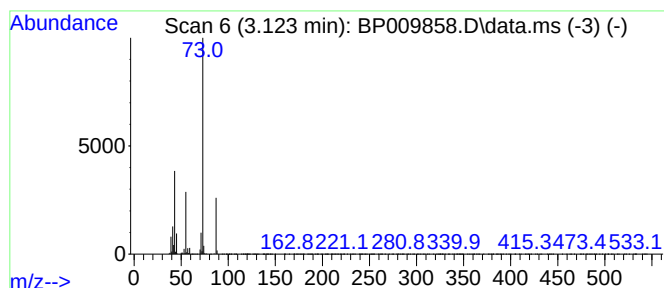

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009858.D
Acq On : 15 Apr 2022 13:22
Operator : CG/JU
Sample : N2422-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.123	12.5	ng/u1	433864	1	7.958	693040	20.0