

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009870.D
 Acq On : 15 Apr 2022 20:40
 Operator : CG/JU
 Sample : PB144126BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	18	rVB2	21507	39699	0.71%	0.077%
2	3.381	46	50	64	rVB	40275	63588	1.14%	0.124%
3	3.799	117	121	137	rBV	511478	892790	15.99%	1.735%
4	4.134	173	178	184	rBV3	11159	18734	0.34%	0.036%
5	5.264	365	370	376	rVB5	5785	11759	0.21%	0.023%
6	7.110	676	684	699	rBV	747442	1163559	20.84%	2.261%
7	7.281	706	713	724	rBV	576724	926676	16.59%	1.801%
8	7.487	741	748	760	rBV	735435	1174485	21.03%	2.282%
9	7.957	821	828	839	rBV	522542	834505	14.94%	1.622%
10	8.657	938	947	963	rBV	959108	1564053	28.01%	3.040%
11	9.116	1016	1025	1038	rBV	782395	1315676	23.56%	2.557%
12	9.840	1141	1148	1163	rBV	634960	1074788	19.25%	2.089%
13	10.381	1233	1240	1254	rBV	944236	1604091	28.73%	3.117%
14	10.763	1297	1305	1317	rBV	759883	1298304	23.25%	2.523%
15	10.893	1319	1327	1343	rBV	1026404	1768806	31.67%	3.437%
16	12.351	1568	1575	1580	rBV2	18966	33098	0.59%	0.064%
17	12.563	1608	1611	1620	rVB7	3110	5587	0.10%	0.011%
18	13.992	1846	1854	1866	rBV	1984759	2837473	50.81%	5.514%
19	14.281	1894	1903	1919	rBV	2104988	3049580	54.61%	5.927%
20	14.587	1947	1955	1965	rBV	1329311	1956324	35.03%	3.802%
21	14.769	1978	1986	1998	rBV	1005004	1486032	26.61%	2.888%
22	15.581	2116	2124	2136	rBV	2735299	3993170	71.51%	7.760%
23	15.692	2136	2143	2159	rVV	938588	1399216	25.06%	2.719%
24	15.822	2159	2165	2172	rVB2	32353	51036	0.91%	0.099%
25	16.269	2239	2241	2248	rVB6	3283	6108	0.11%	0.012%
26	16.363	2251	2257	2263	rBV5	11495	18899	0.34%	0.037%
27	17.016	2365	2368	2374	rVB7	6162	9400	0.17%	0.018%
28	17.116	2379	2385	2391	rBV7	5320	13689	0.25%	0.027%
29	17.339	2416	2423	2431	rBV	1652194	2467123	44.18%	4.795%
30	17.439	2433	2440	2451	rVV	3206003	4579010	82.00%	8.899%
31	19.245	2743	2747	2753	rVB3	44939	63169	1.13%	0.123%
32	19.310	2753	2758	2764	rBV	45736	71857	1.29%	0.140%
33	19.669	2812	2819	2834	rBV	4383399	5584241	100.00%	10.852%
34	21.421	3111	3117	3123	rBV	2045402	2781542	49.81%	5.406%
35	23.727	3501	3509	3516	rBV2	2437956	4898239	87.72%	9.519%
36	23.886	3528	3536	3547	rVB2	1143812	2400076	42.98%	4.664%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009870.D
Acq On : 15 Apr 2022 20:40
Operator : CG/JU
Sample : PB144126BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 51456382

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009870.D
Acq On : 15 Apr 2022 20:40
Operator : CG/JU
Sample : PB144126BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

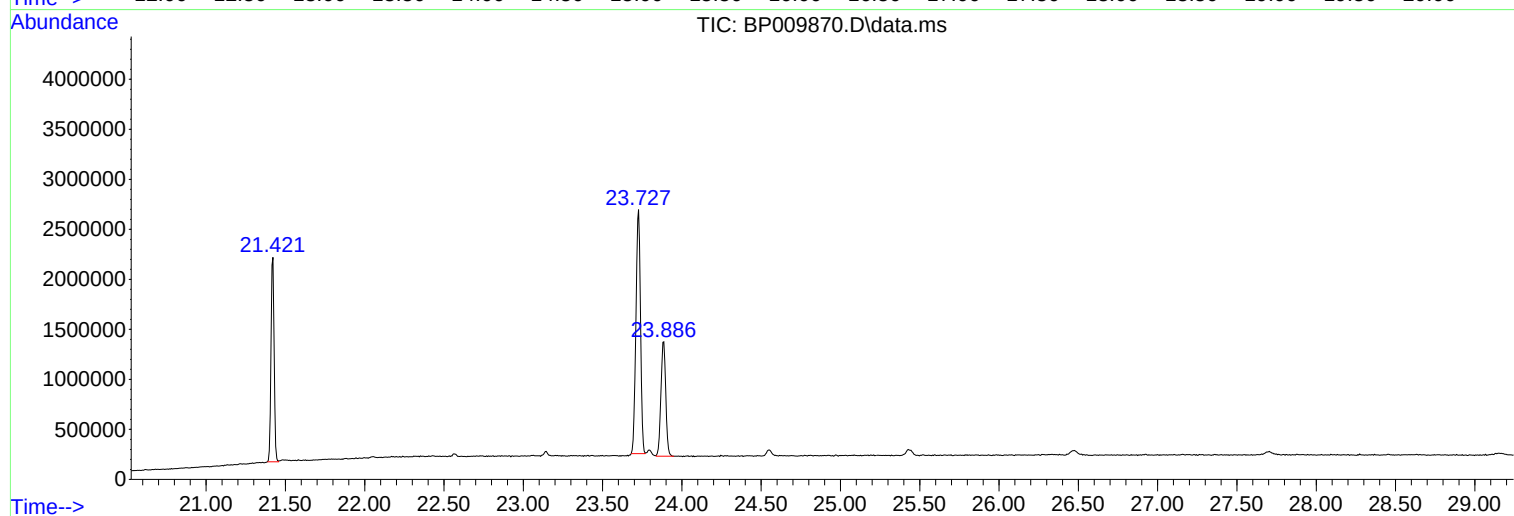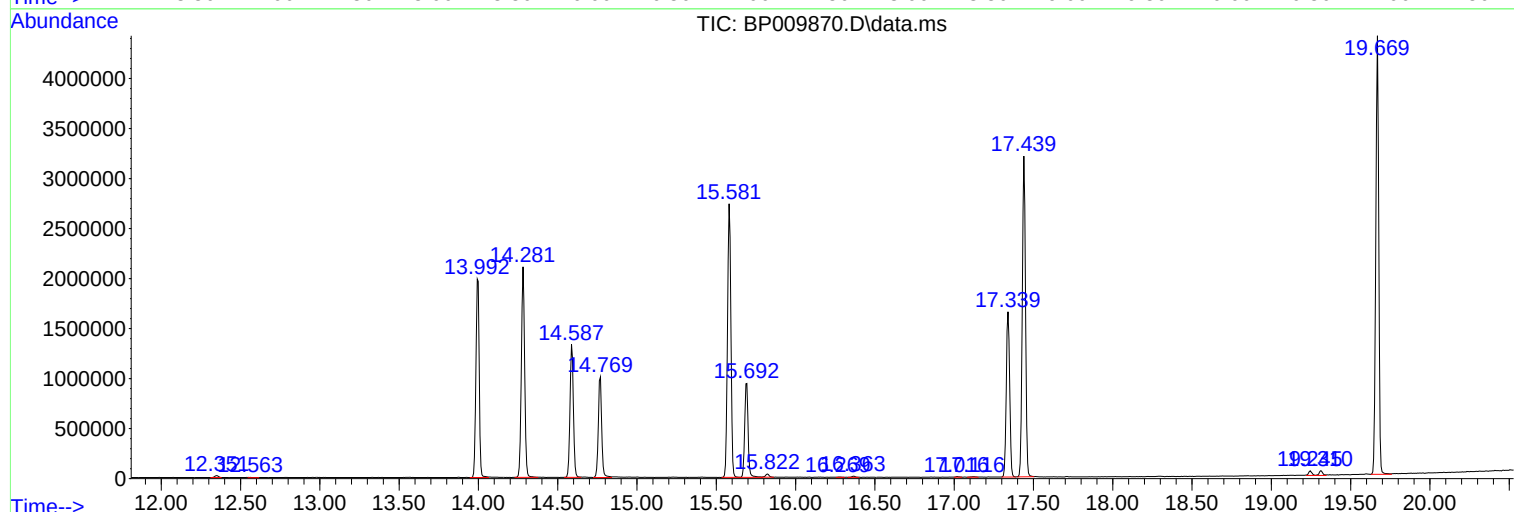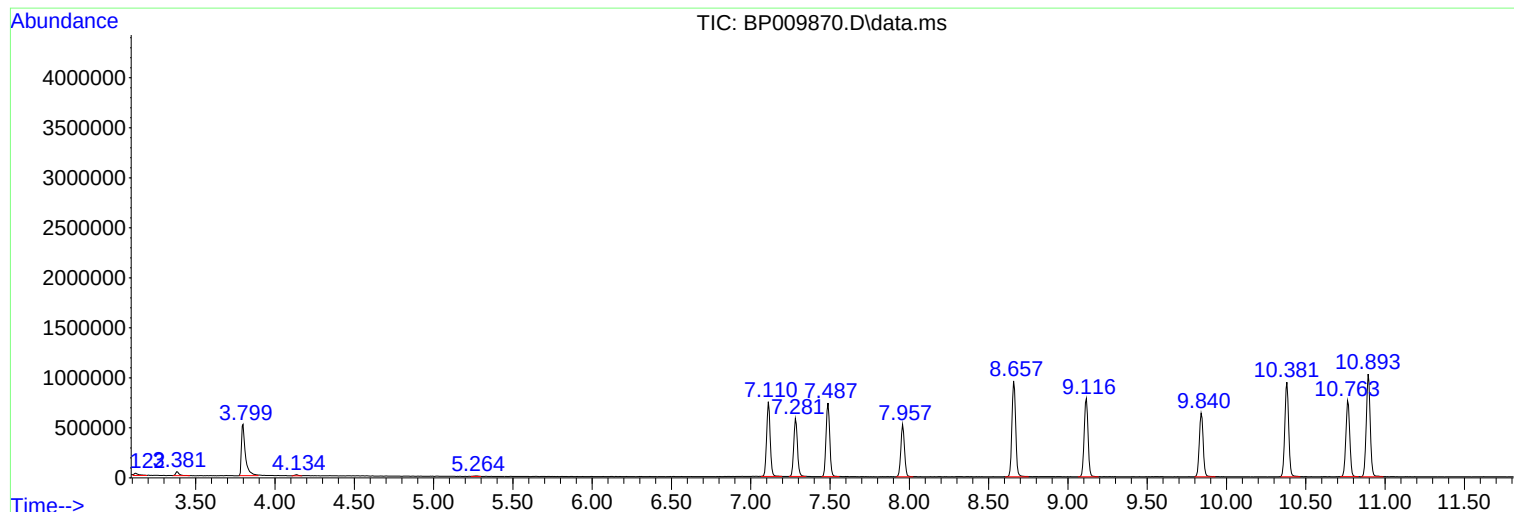

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009870.D
Acq On : 15 Apr 2022 20:40
Operator : CG/JU
Sample : PB144126BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009870.D
Acq On : 15 Apr 2022 20:40
Operator : CG/JU
Sample : PB144126BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------