

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009873.D
 Acq On : 15 Apr 2022 22:21
 Operator : CG/JU
 Sample : N2421-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	20	rVB	379723	554910	9.27%	1.097%
2	3.381	46	50	57	rVB	26759	37299	0.62%	0.074%
3	3.805	118	122	135	rBV	118035	225065	3.76%	0.445%
4	4.134	174	178	185	rBV2	11308	16998	0.28%	0.034%
5	5.270	364	371	378	rBV	27385	46057	0.77%	0.091%
6	6.934	651	654	659	rBV7	3981	8132	0.14%	0.016%
7	7.111	678	684	700	rVB2	160780	303431	5.07%	0.600%
8	7.281	702	713	726	rBV	524214	844987	14.12%	1.671%
9	7.487	740	748	756	rBV	532009	859409	14.36%	1.699%
10	7.958	820	828	838	rBV	577404	925965	15.47%	1.831%
11	8.205	863	870	873	rBV8	4021	7347	0.12%	0.015%
12	8.316	883	889	895	rBV2	23691	41345	0.69%	0.082%
13	8.658	940	947	958	rBV	458134	745061	12.45%	1.473%
14	8.781	963	968	973	rVB8	4041	7894	0.13%	0.016%
15	9.116	1017	1025	1036	rBV	696031	1189759	19.88%	2.352%
16	9.293	1050	1055	1060	rBV7	4638	8876	0.15%	0.018%
17	9.575	1095	1103	1110	rVB3	15508	29828	0.50%	0.059%
18	9.840	1139	1148	1158	rBV	572702	945854	15.81%	1.870%
19	10.381	1232	1240	1256	rVB	803536	1380224	23.07%	2.729%
20	10.546	1261	1268	1276	rBV2	60672	115543	1.93%	0.228%
21	10.634	1278	1283	1287	rVB6	6248	11274	0.19%	0.022%
22	10.763	1297	1305	1318	rVB	833347	1421339	23.75%	2.810%
23	10.893	1319	1327	1345	rVV	718684	1252778	20.94%	2.477%
24	11.128	1361	1367	1371	rBV9	2530	6128	0.10%	0.012%
25	11.316	1394	1399	1403	rBV8	3997	6705	0.11%	0.013%
26	12.193	1543	1548	1553	rBV8	3636	6708	0.11%	0.013%
27	12.287	1560	1564	1569	rBV4	10993	16132	0.27%	0.032%
28	12.346	1569	1574	1580	rVV2	16898	29590	0.49%	0.059%
29	12.428	1583	1588	1594	rBV10	3892	6562	0.11%	0.013%
30	12.569	1605	1612	1617	rBV9	4170	8194	0.14%	0.016%
31	12.957	1674	1678	1683	rBV6	6038	10137	0.17%	0.020%
32	13.204	1715	1720	1726	rVB5	9440	15570	0.26%	0.031%
33	13.399	1745	1753	1756	rBV3	26441	43361	0.72%	0.086%
34	13.428	1756	1758	1763	rVV4	12571	17424	0.29%	0.034%
35	13.499	1766	1770	1776	rVV9	5469	11949	0.20%	0.024%
36	13.563	1776	1781	1783	rVV6	5528	10267	0.17%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009873.D
 Acq On : 15 Apr 2022 22:21
 Operator : CG/JU
 Sample : N2421-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	13.599	1783	1787	1793	rVB	10152	16980	0.28%	0.034%
38	13.993	1847	1854	1861	rBV	1901212	2645246	44.21%	5.230%
39	14.240	1890	1896	1897	rBV	32891	45013	0.75%	0.089%
40	14.281	1897	1903	1922	rVB	2003803	2898949	48.45%	5.731%
41	14.498	1936	1940	1946	rVB4	7496	10698	0.18%	0.021%
42	14.587	1946	1955	1967	rBV	1423854	2121617	35.45%	4.195%
43	14.763	1975	1985	1996	rBV	190851	307825	5.14%	0.609%
44	15.222	2059	2063	2070	rVB2	16864	28420	0.47%	0.056%
45	15.398	2086	2093	2098	rBV2	45185	72215	1.21%	0.143%
46	15.451	2098	2102	2106	rVB2	9271	12200	0.20%	0.024%
47	15.581	2117	2124	2136	rBV	2681851	3996056	66.78%	7.900%
48	15.687	2136	2142	2157	rBV	1013221	1426941	23.85%	2.821%
49	15.822	2160	2165	2172	rVB2	32189	50540	0.84%	0.100%
50	15.945	2180	2186	2190	rBV7	11644	18571	0.31%	0.037%
51	16.004	2192	2196	2199	rBV5	6951	11543	0.19%	0.023%
52	16.128	2214	2217	2221	rBV5	6002	10589	0.18%	0.021%
53	16.228	2227	2234	2237	rBV9	8538	14511	0.24%	0.029%
54	16.269	2237	2241	2245	rVV4	18757	31400	0.52%	0.062%
55	16.310	2245	2248	2251	rVV3	15270	23330	0.39%	0.046%
56	16.369	2255	2258	2264	rVB6	17024	25451	0.43%	0.050%
57	16.481	2274	2277	2282	rBV5	11726	15713	0.26%	0.031%
58	16.816	2330	2334	2339	rVV8	10749	14791	0.25%	0.029%
59	16.887	2343	2346	2349	rVB5	6934	9596	0.16%	0.019%
60	17.022	2364	2369	2372	rBV7	7118	11358	0.19%	0.022%
61	17.063	2372	2376	2378	rVV5	6628	8109	0.14%	0.016%
62	17.104	2379	2383	2389	rVV4	15456	34691	0.58%	0.069%
63	17.157	2389	2392	2398	rVB6	8747	15139	0.25%	0.030%
64	17.269	2404	2411	2416	rBV4	32595	48448	0.81%	0.096%
65	17.340	2416	2423	2432	rVV	1837610	2671186	44.64%	5.281%
66	17.440	2433	2440	2452	rVV	3496340	4955755	82.82%	9.798%
67	17.528	2452	2455	2459	rVB5	7031	11182	0.19%	0.022%
68	17.651	2470	2476	2484	rBV9	12306	32228	0.54%	0.064%
69	17.845	2506	2509	2512	rBV4	7999	8971	0.15%	0.018%
70	18.010	2534	2537	2543	rVB3	22021	29382	0.49%	0.058%
71	18.128	2553	2557	2561	rBV7	7058	15006	0.25%	0.030%
72	18.222	2569	2573	2580	rBV2	88151	126465	2.11%	0.250%
73	18.287	2582	2584	2589	rVB4	15945	22214	0.37%	0.044%
74	18.516	2621	2623	2627	rBV5	8039	13787	0.23%	0.027%
75	18.969	2697	2700	2704	rBV4	10150	14689	0.25%	0.029%
76	19.051	2711	2714	2718	rBV4	21113	29922	0.50%	0.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009873.D
 Acq On : 15 Apr 2022 22:21
 Operator : CG/JU
 Sample : N2421-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

77	19.122	2724	2726	2730	rVB5	9497	10587	0.18%	0.021%
78	19.245	2743	2747	2751	rBV2	47095	63116	1.05%	0.125%
79	19.281	2751	2753	2755	rVV3	14074	17129	0.29%	0.034%
80	19.310	2755	2758	2763	rVB	42682	56852	0.95%	0.112%
81	19.451	2779	2782	2785	rBV4	15681	21478	0.36%	0.042%
82	19.669	2812	2819	2826	rBV	4482846	5983999	100.00%	11.831%
83	21.128	3063	3067	3074	rBV2	182745	254400	4.25%	0.503%
84	21.416	3111	3116	3124	rBV	2275770	3053827	51.03%	6.038%
85	23.727	3500	3509	3517	rBV	2628163	5375630	89.83%	10.628%
86	23.886	3528	3536	3547	rVB2	1323625	2718639	45.43%	5.375%




Sum of corrected areas: 50580486

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009873.D
Acq On : 15 Apr 2022 22:21
Operator : CG/JU
Sample : N2421-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

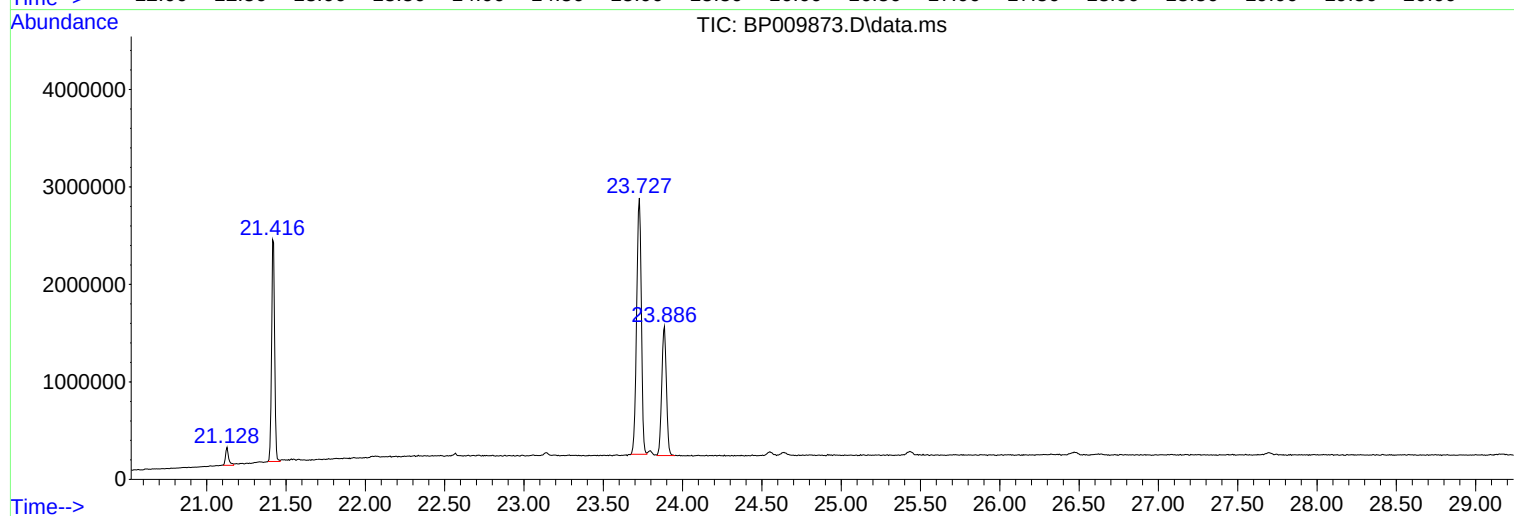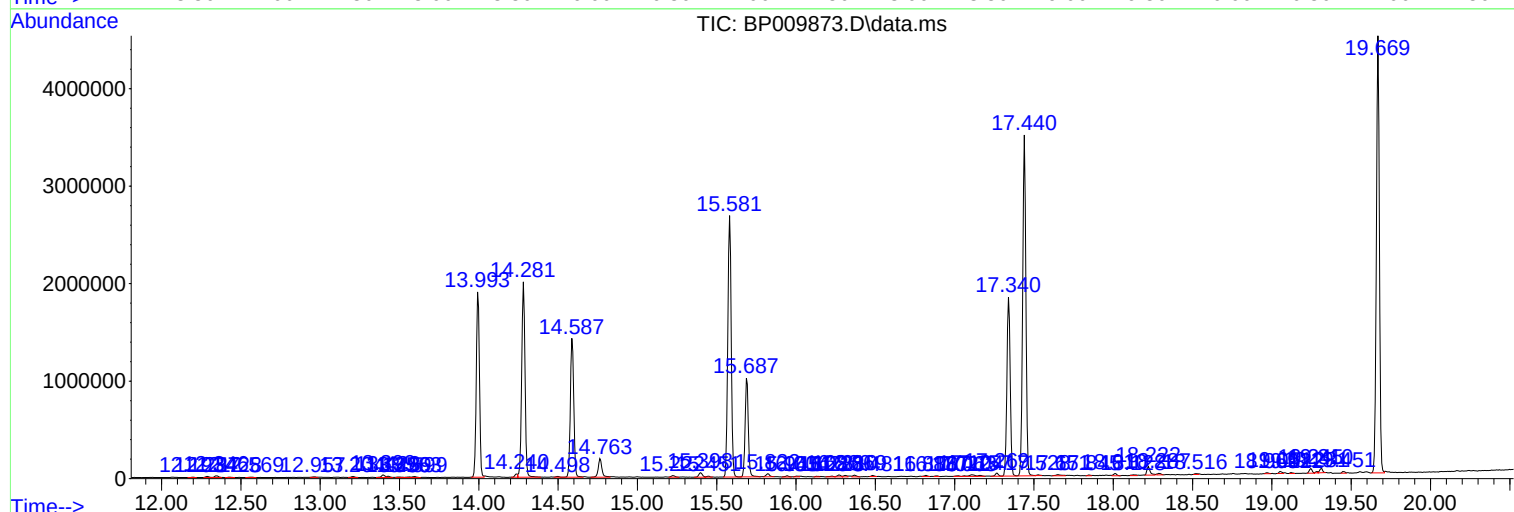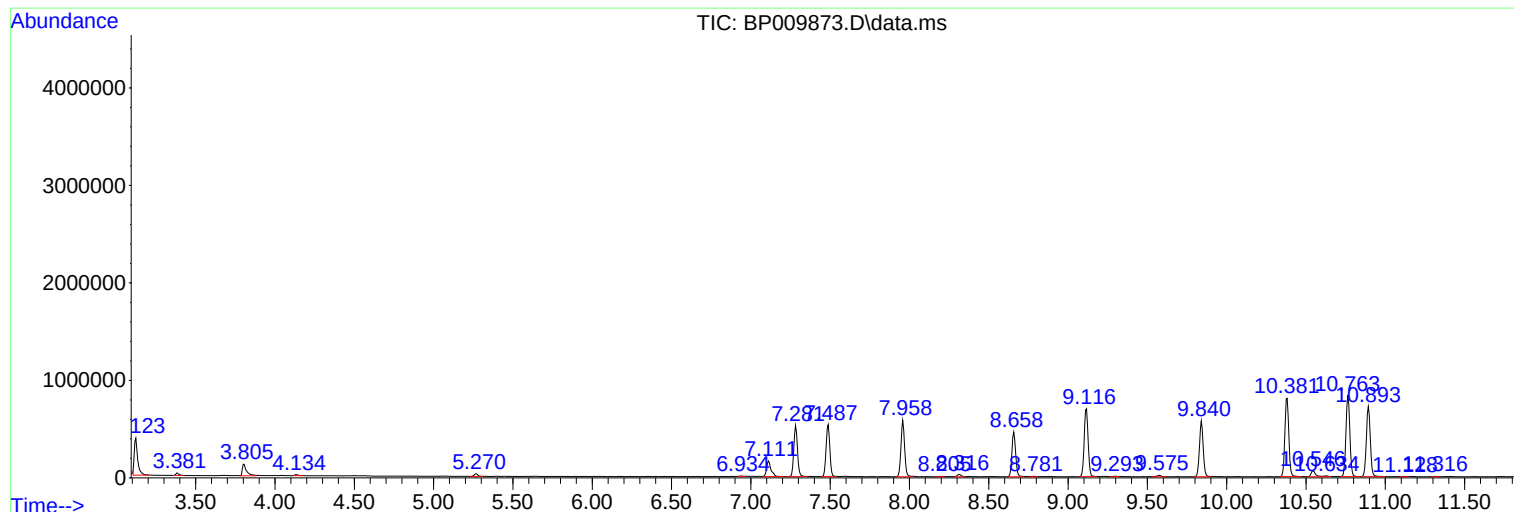

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009873.D
Acq On : 15 Apr 2022 22:21
Operator : CG/JU
Sample : N2421-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J56










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.123	11.99 ng/ul	554910	1,4-Dichlorobenzene-d4	7.958

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	56
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	38
4			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	38
5			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25

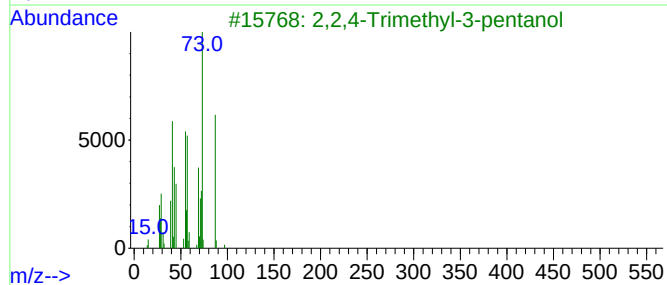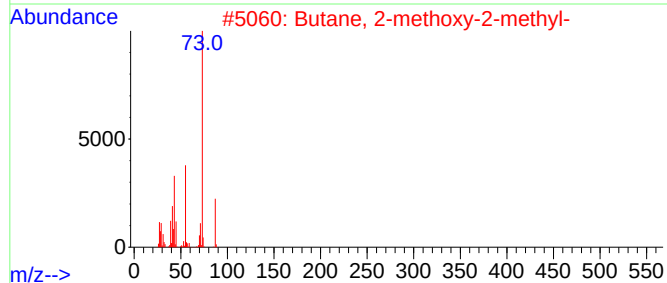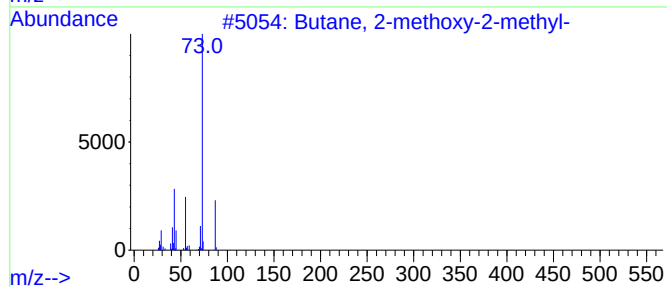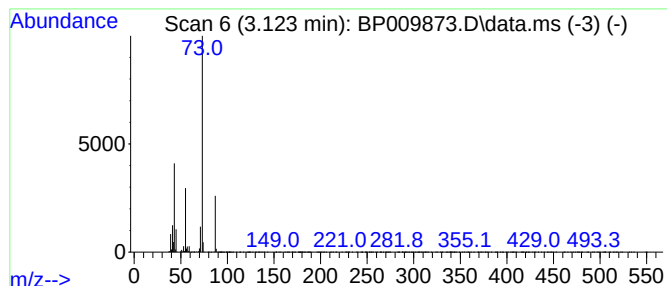

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009873.D
Acq On : 15 Apr 2022 22:21
Operator : CG/JU
Sample : N2421-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.123	12.0	ng/ul	554910	1	7.958	925965	20.0