

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009876.D
 Acq On : 16 Apr 2022 00:02
 Operator : CG/JU
 Sample : N2421-06DL 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HY6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	16	rVB	50489	74311	2.39%	0.434%
2	3.817	121	124	132	rBV3	13915	24753	0.79%	0.145%
3	4.134	174	178	185	rVB3	10488	18126	0.58%	0.106%
4	5.264	366	370	376	rBV2	14246	22226	0.71%	0.130%
5	7.111	679	684	693	rVB2	22787	42408	1.36%	0.248%
6	7.281	707	713	722	rBV	46816	80465	2.58%	0.470%
7	7.487	743	748	756	rVB	53355	85099	2.73%	0.497%
8	7.846	808	809	816	rVB7	3885	4917	0.16%	0.029%
9	7.958	820	828	843	rVV	577619	964645	30.97%	5.634%
10	8.316	883	889	893	rVB8	4324	7788	0.25%	0.045%
11	8.658	941	947	959	rVB	50383	84488	2.71%	0.493%
12	9.116	1017	1025	1032	rBV	62231	107334	3.45%	0.627%
13	9.569	1098	1102	1106	rVB7	3457	5325	0.17%	0.031%
14	9.840	1142	1148	1155	rBV	42896	74646	2.40%	0.436%
15	10.381	1233	1240	1248	rBV	72027	127508	4.09%	0.745%
16	10.557	1265	1270	1276	rBV4	8238	18968	0.61%	0.111%
17	10.763	1297	1305	1320	rVB	862161	1459889	46.86%	8.527%
18	10.893	1320	1327	1337	rBV2	72684	126814	4.07%	0.741%
19	12.787	1644	1649	1651	rBV6	2379	3129	0.10%	0.018%
20	12.910	1665	1670	1675	rBV8	1711	3603	0.12%	0.021%
21	12.969	1675	1680	1682	rBV6	2067	3130	0.10%	0.018%
22	13.204	1717	1720	1724	rVB6	3183	4358	0.14%	0.025%
23	13.428	1755	1758	1764	rBV8	2272	3448	0.11%	0.020%
24	13.869	1829	1833	1836	rBV6	5708	7636	0.25%	0.045%
25	13.993	1848	1854	1860	rBV	186166	259493	8.33%	1.516%
26	14.040	1860	1862	1866	rVB5	4932	7079	0.23%	0.041%
27	14.128	1874	1877	1880	rVB5	3188	3944	0.13%	0.023%
28	14.240	1890	1896	1897	rBV6	8090	10755	0.35%	0.063%
29	14.281	1897	1903	1914	rVB	165867	257521	8.27%	1.504%
30	14.587	1948	1955	1966	rBV	1493761	2229895	71.58%	13.024%
31	14.769	1981	1986	1992	rBV3	14285	24385	0.78%	0.142%
32	15.222	2058	2063	2068	rBV9	2893	6131	0.20%	0.036%
33	15.398	2090	2093	2098	rVB6	6294	9521	0.31%	0.056%
34	15.581	2117	2124	2133	rBV	267818	393528	12.63%	2.299%
35	15.687	2137	2142	2151	rBV2	53406	86842	2.79%	0.507%
36	15.945	2182	2186	2191	rVB8	2745	5461	0.18%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009876.D
 Acq On : 16 Apr 2022 00:02
 Operator : CG/JU
 Sample : N2421-06DL 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HY6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	16.004	2191	2196	2198	rBV6	3247	5907	0.19%	0.035%
38	16.140	2214	2219	2220	rBV5	3385	5145	0.17%	0.030%
39	16.222	2229	2233	2236	rBV6	2855	4117	0.13%	0.024%
40	16.316	2244	2249	2250	rBV5	4359	5832	0.19%	0.034%
41	16.487	2271	2278	2280	rBV8	4512	8546	0.27%	0.050%
42	16.657	2304	2307	2310	rBV4	3083	4628	0.15%	0.027%
43	17.110	2380	2384	2391	rBV4	5275	11303	0.36%	0.066%
44	17.269	2407	2411	2414	rVB6	8457	11624	0.37%	0.068%
45	17.339	2415	2423	2431	rBV	1986266	2856538	91.70%	16.684%
46	17.439	2434	2440	2453	rVB	312562	485100	15.57%	2.833%
47	17.722	2485	2488	2490	rBV4	3467	3451	0.11%	0.020%
48	17.951	2525	2527	2533	rVB7	2610	3348	0.11%	0.020%
49	18.016	2533	2538	2542	rVB8	7806	12706	0.41%	0.074%
50	18.163	2561	2563	2566	rBV4	2869	3650	0.12%	0.021%
51	18.222	2569	2573	2577	rBV5	18267	24992	0.80%	0.146%
52	19.051	2710	2714	2722	rBV7	19268	37096	1.19%	0.217%
53	19.445	2779	2781	2786	rBV6	6929	10032	0.32%	0.059%
54	19.663	2813	2818	2830	rBV2	442987	621824	19.96%	3.632%
55	21.128	3064	3067	3071	rBV4	47323	60914	1.96%	0.356%
56	21.416	3111	3116	3123	rBV	2254205	3115155	100.00%	18.195%
57	23.721	3502	3508	3515	rVB	236524	473245	15.19%	2.764%
58	23.880	3528	3535	3548	rVB2	1298123	2706193	86.87%	15.806%




Sum of corrected areas: 17120915

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009876.D
Acq On : 16 Apr 2022 00:02
Operator : CG/JU
Sample : N2421-06DL 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

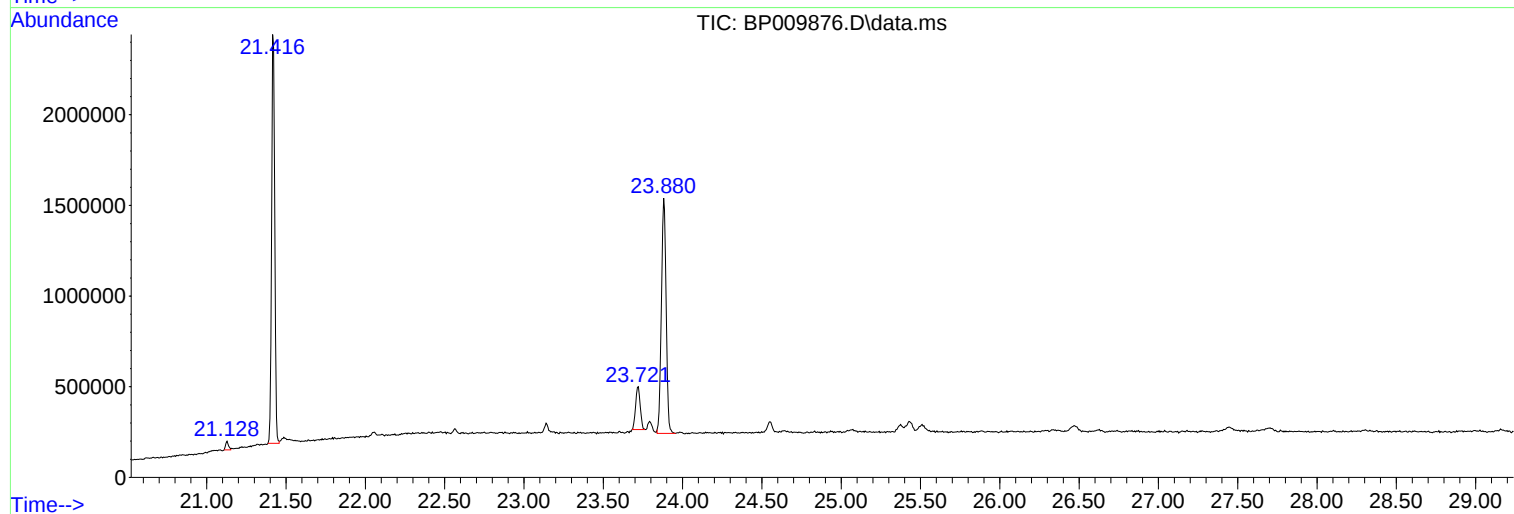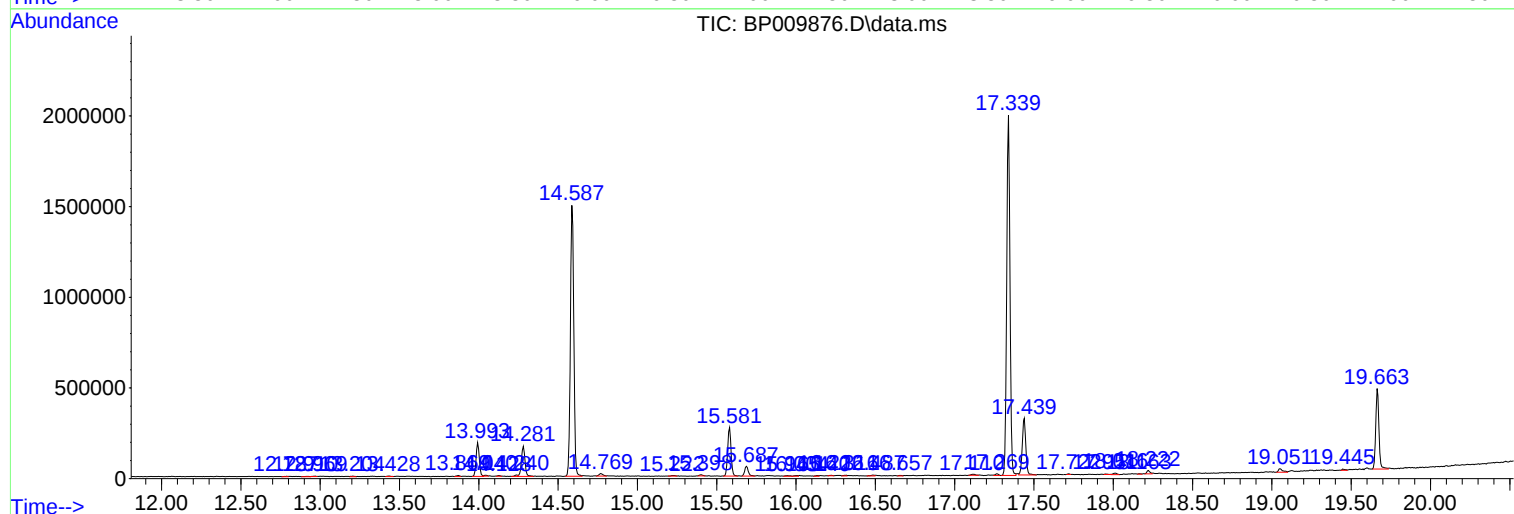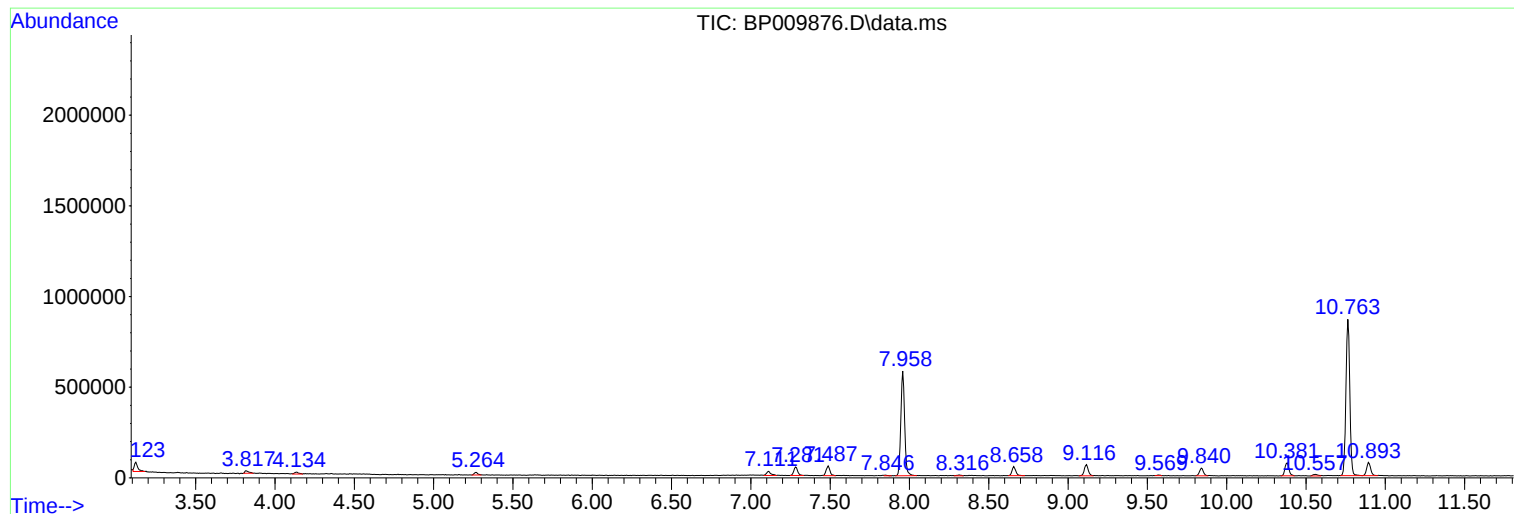

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009876.D
Acq On : 16 Apr 2022 00:02
Operator : CG/JU
Sample : N2421-06DL 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009876.D
Acq On : 16 Apr 2022 00:02
Operator : CG/JU
Sample : N2421-06DL 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
