

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
 Data File : BP009888.D
 Acq On : 16 Apr 2022 07:19
 Operator : CG/JU
 Sample : PB144146BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK146

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	14	rVB2	14370	22579	0.47%	0.049%
2	3.381	46	50	56	rVB	38357	50852	1.05%	0.110%
3	3.793	117	120	143	rBV	476887	852535	17.59%	1.837%
4	4.134	172	178	185	rBV5	8460	17150	0.35%	0.037%
5	7.111	675	684	694	rBV	677748	1083931	22.37%	2.336%
6	7.281	704	713	726	rBV	525604	854696	17.64%	1.842%
7	7.481	740	747	758	rBV	675059	1104316	22.79%	2.380%
8	7.958	819	828	839	rBV	487385	800943	16.53%	1.726%
9	8.658	939	947	962	rBV	893868	1439980	29.71%	3.103%
10	9.110	1016	1024	1036	rBV	714633	1210072	24.97%	2.608%
11	9.840	1139	1148	1161	rBV	600124	1002904	20.69%	2.161%
12	10.375	1231	1239	1252	rBV	863125	1486072	30.66%	3.203%
13	10.763	1296	1305	1317	rBV	722505	1236517	25.52%	2.665%
14	10.893	1317	1327	1348	rVB	935280	1603270	33.08%	3.455%
15	12.346	1568	1574	1583	rVB2	18528	31617	0.65%	0.068%
16	13.993	1845	1854	1871	rBV	1848199	2547637	52.57%	5.490%
17	14.281	1895	1903	1917	rBV	1877588	2756334	56.88%	5.940%
18	14.587	1948	1955	1964	rBV	1227252	1808239	37.31%	3.897%
19	14.763	1976	1985	2001	rBV	863611	1299535	26.82%	2.801%
20	14.992	2022	2024	2029	rVB6	3044	4962	0.10%	0.011%
21	15.240	2062	2066	2071	rVB8	3245	6334	0.13%	0.014%
22	15.581	2115	2124	2133	rBV	2545742	3572684	73.72%	7.699%
23	15.687	2136	2142	2155	rVV	818932	1172225	24.19%	2.526%
24	15.822	2159	2165	2172	rVB2	27604	45240	0.93%	0.097%
25	16.363	2253	2257	2265	rVB5	9292	14189	0.29%	0.031%
26	17.016	2364	2368	2374	rVB9	5435	10249	0.21%	0.022%
27	17.339	2416	2423	2431	rBV	1602342	2297415	47.41%	4.951%
28	17.439	2433	2440	2453	rBV	2770080	4032887	83.22%	8.691%
29	19.245	2743	2747	2753	rVB	39246	51407	1.06%	0.111%
30	19.310	2753	2758	2765	rBV	38325	57440	1.19%	0.124%
31	19.669	2812	2819	2829	rBV	3601215	4846213	100.00%	10.444%
32	21.416	3111	3116	3124	rBV	1903591	2591827	53.48%	5.586%
33	23.721	3500	3508	3516	rBV2	2165980	4267600	88.06%	9.197%
34	23.880	3528	3535	3545	rVB2	1077318	2221861	45.85%	4.788%

Sum of corrected areas: 46401712

Instrument :

BNA_P

ClientSampleId :




SBLK146

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009888.D
Acq On : 16 Apr 2022 07:19
Operator : CG/JU
Sample : PB144146BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK146

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

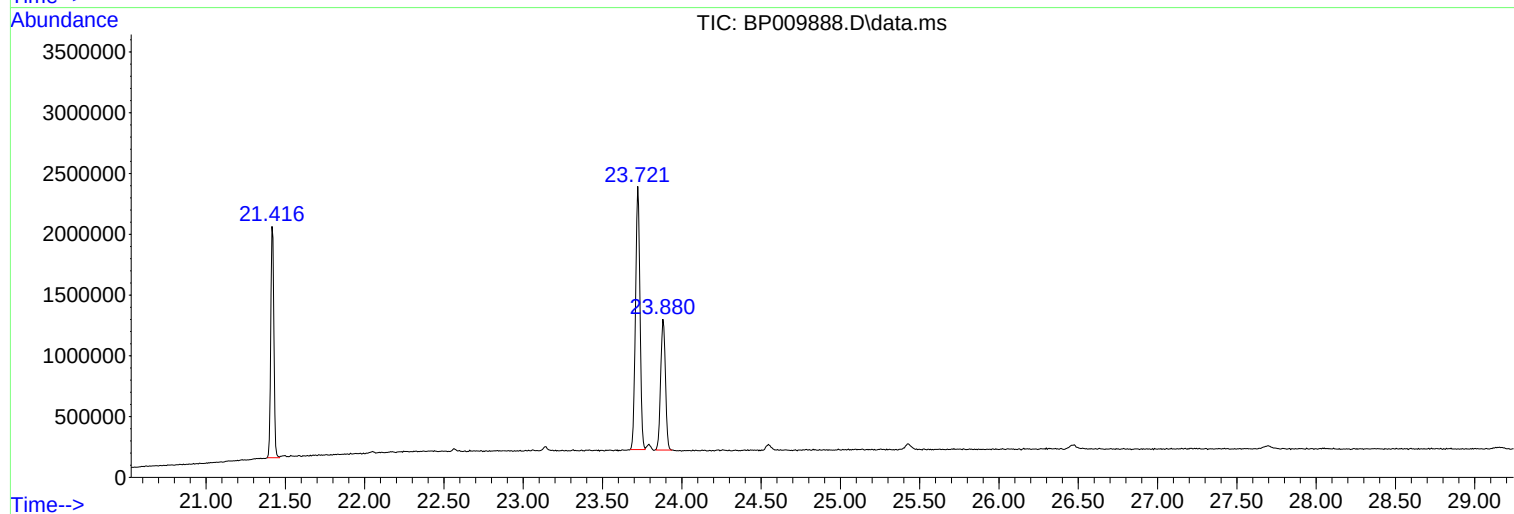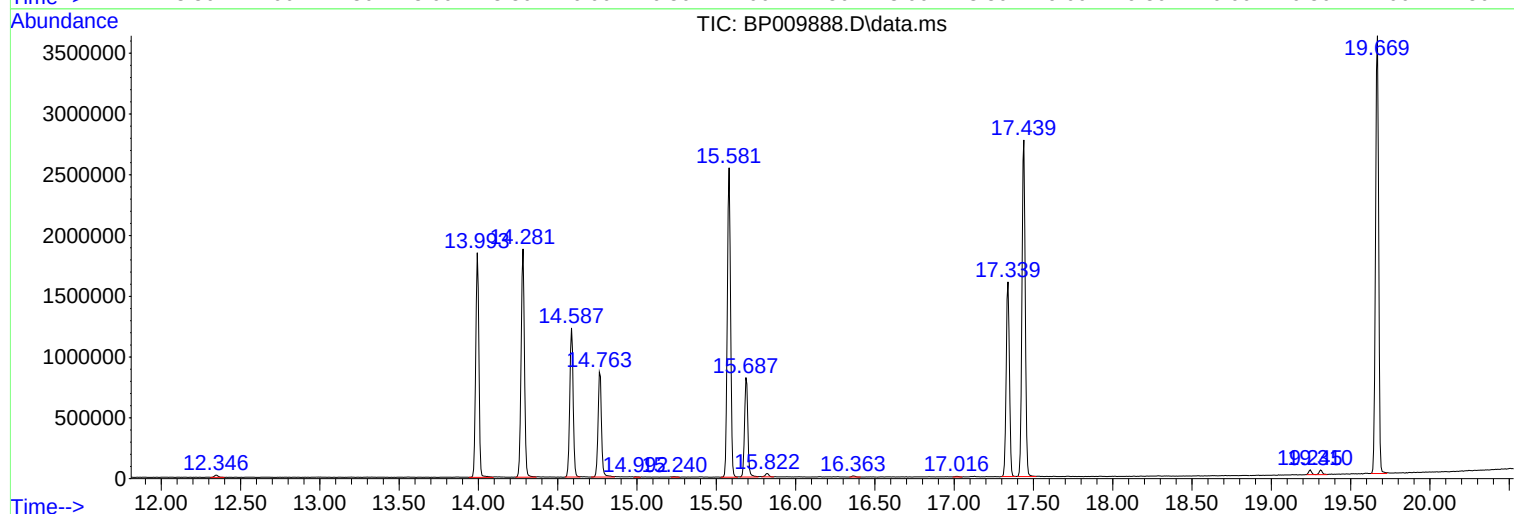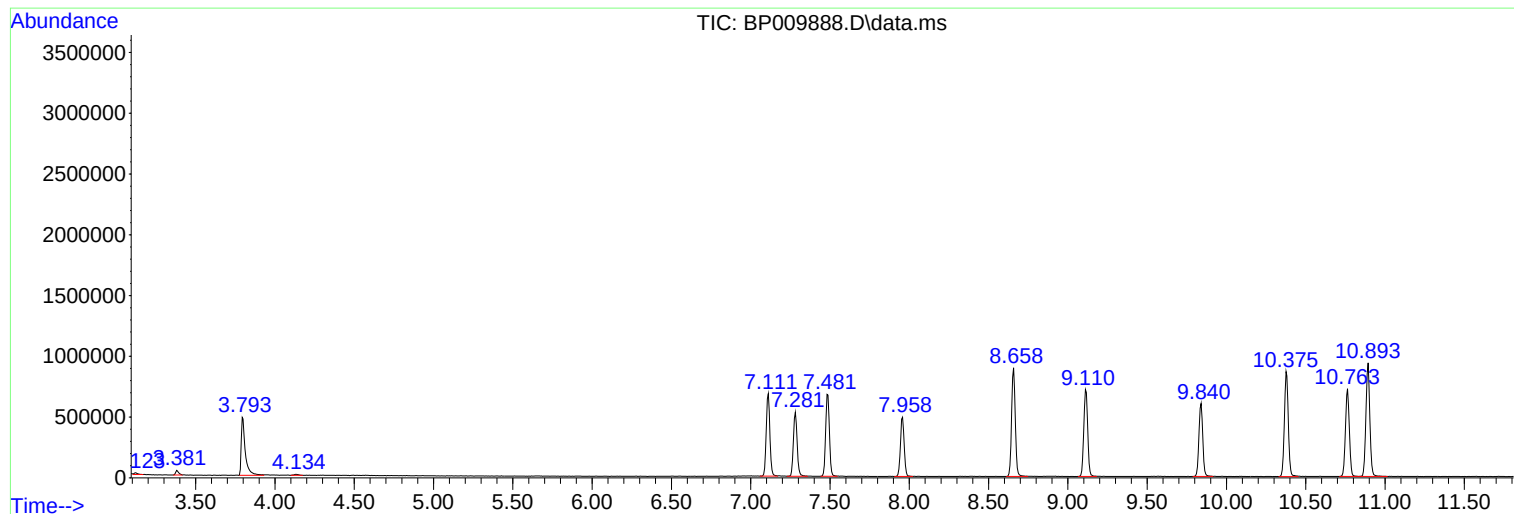

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009888.D
Acq On : 16 Apr 2022 07:19
Operator : CG/JU
Sample : PB144146BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK146

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041522\
Data File : BP009888.D
Acq On : 16 Apr 2022 07:19
Operator : CG/JU
Sample : PB144146BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK146

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc