
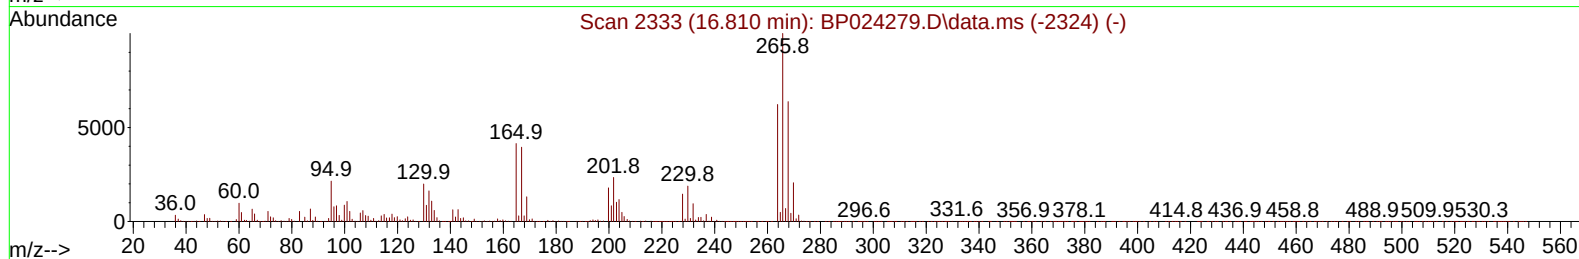
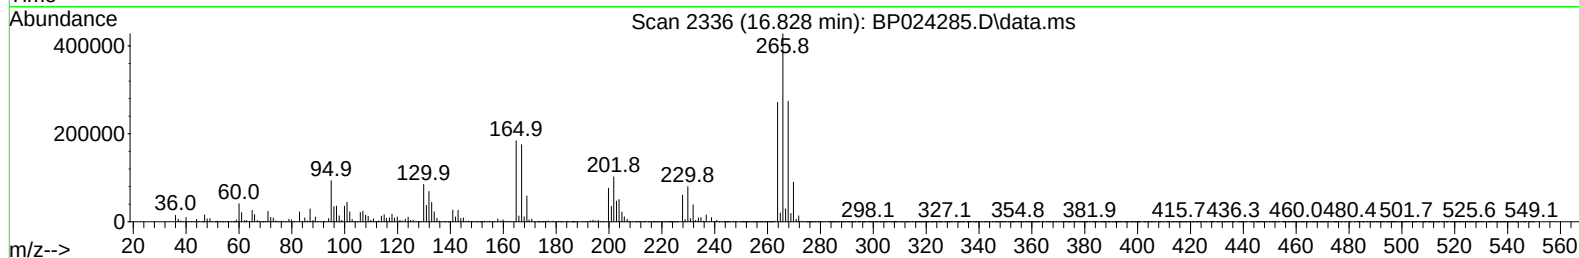


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041525\
Data File : BP024285.D
Acq On : 15 Apr 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 12:53:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

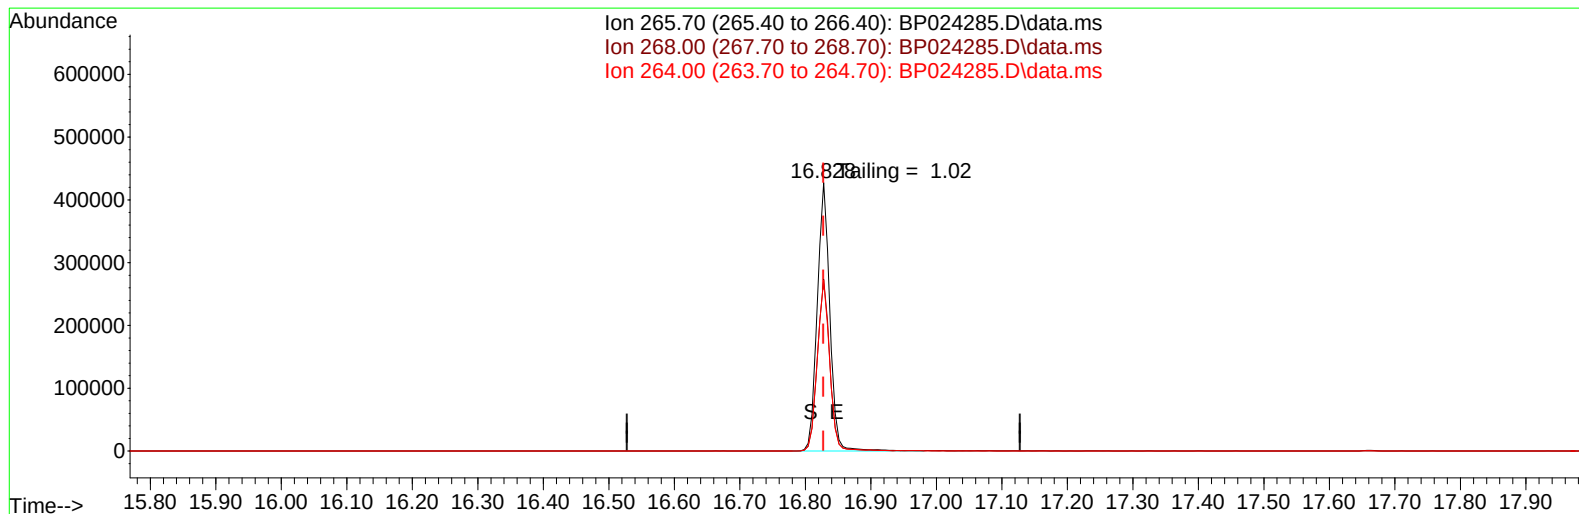

TIC: BP024285.D\data.ms

(70) Pentachlorophenol (C)




16.828min (+ 0.000) 207154.57 ng

response 569074

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.97
264.00	62.20	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041525\
Data File : BP024285.D
Acq On : 15 Apr 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 12:53:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

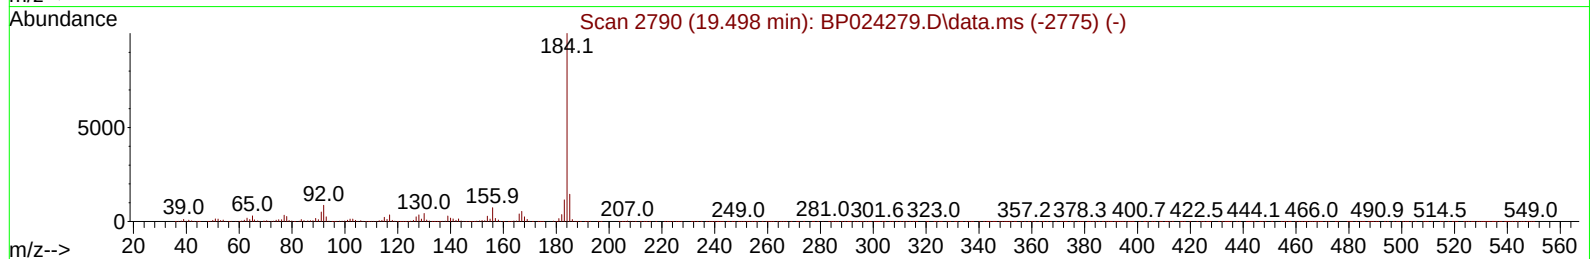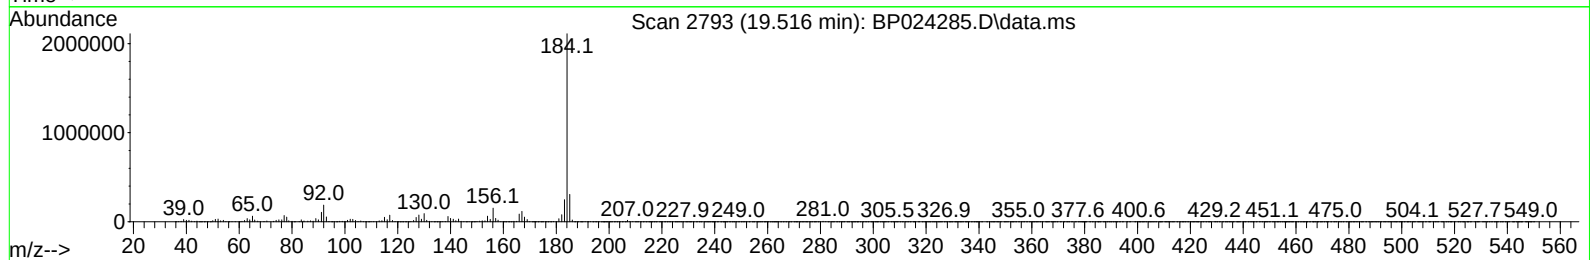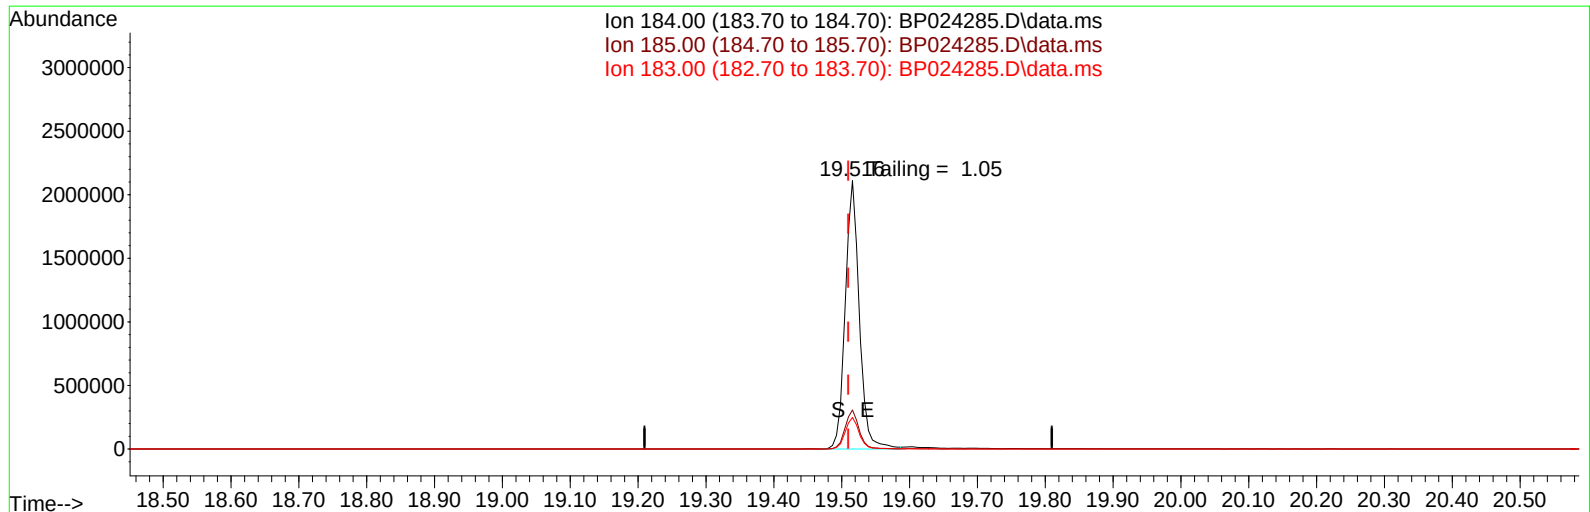

TIC: BP024285.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 25118.03 ng

response 3032050

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.58
183.00	11.50	11.75
0.00	0.00	0.00