

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041525\
 Data File : BP024291.D
 Acq On : 15 Apr 2025 12:43
 Operator : RC/JU
 Sample : Q1771-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-7C

Quant Time: Apr 15 13:11:01 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 15 04:48:42 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	329036	20.000	ng	0.00
21) Naphthalene-d8	10.504	136	1266138	20.000	ng	0.00
39) Acenaphthene-d10	14.357	164	701826	20.000	ng	-0.01
64) Phenanthrene-d10	17.163	188	1267211	20.000	ng	-0.02
76) Chrysene-d12	21.616	240	1201894	20.000	ng	0.00
86) Perylene-d12	24.986	264	1296224	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.352	112	2425826	121.901	ng	0.00
7) Phenol-d6	6.916	99	2757596	101.202	ng	0.00
23) Nitrobenzene-d5	8.875	82	2070069	93.227	ng	0.00
42) 2,4,6-Tribromophenol	15.875	330	1209901	124.602	ng	-0.02
45) 2-Fluorobiphenyl	12.969	172	4007272	87.423	ng	-0.01
79) Terphenyl-d14	19.892	244	5341472	89.579	ng	-0.03


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041525\
Data File : BP024291.D
Acq On : 15 Apr 2025 12:43
Operator : RC/JU
Sample : Q1771-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-7C

Quant Time: Apr 15 13:11:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration




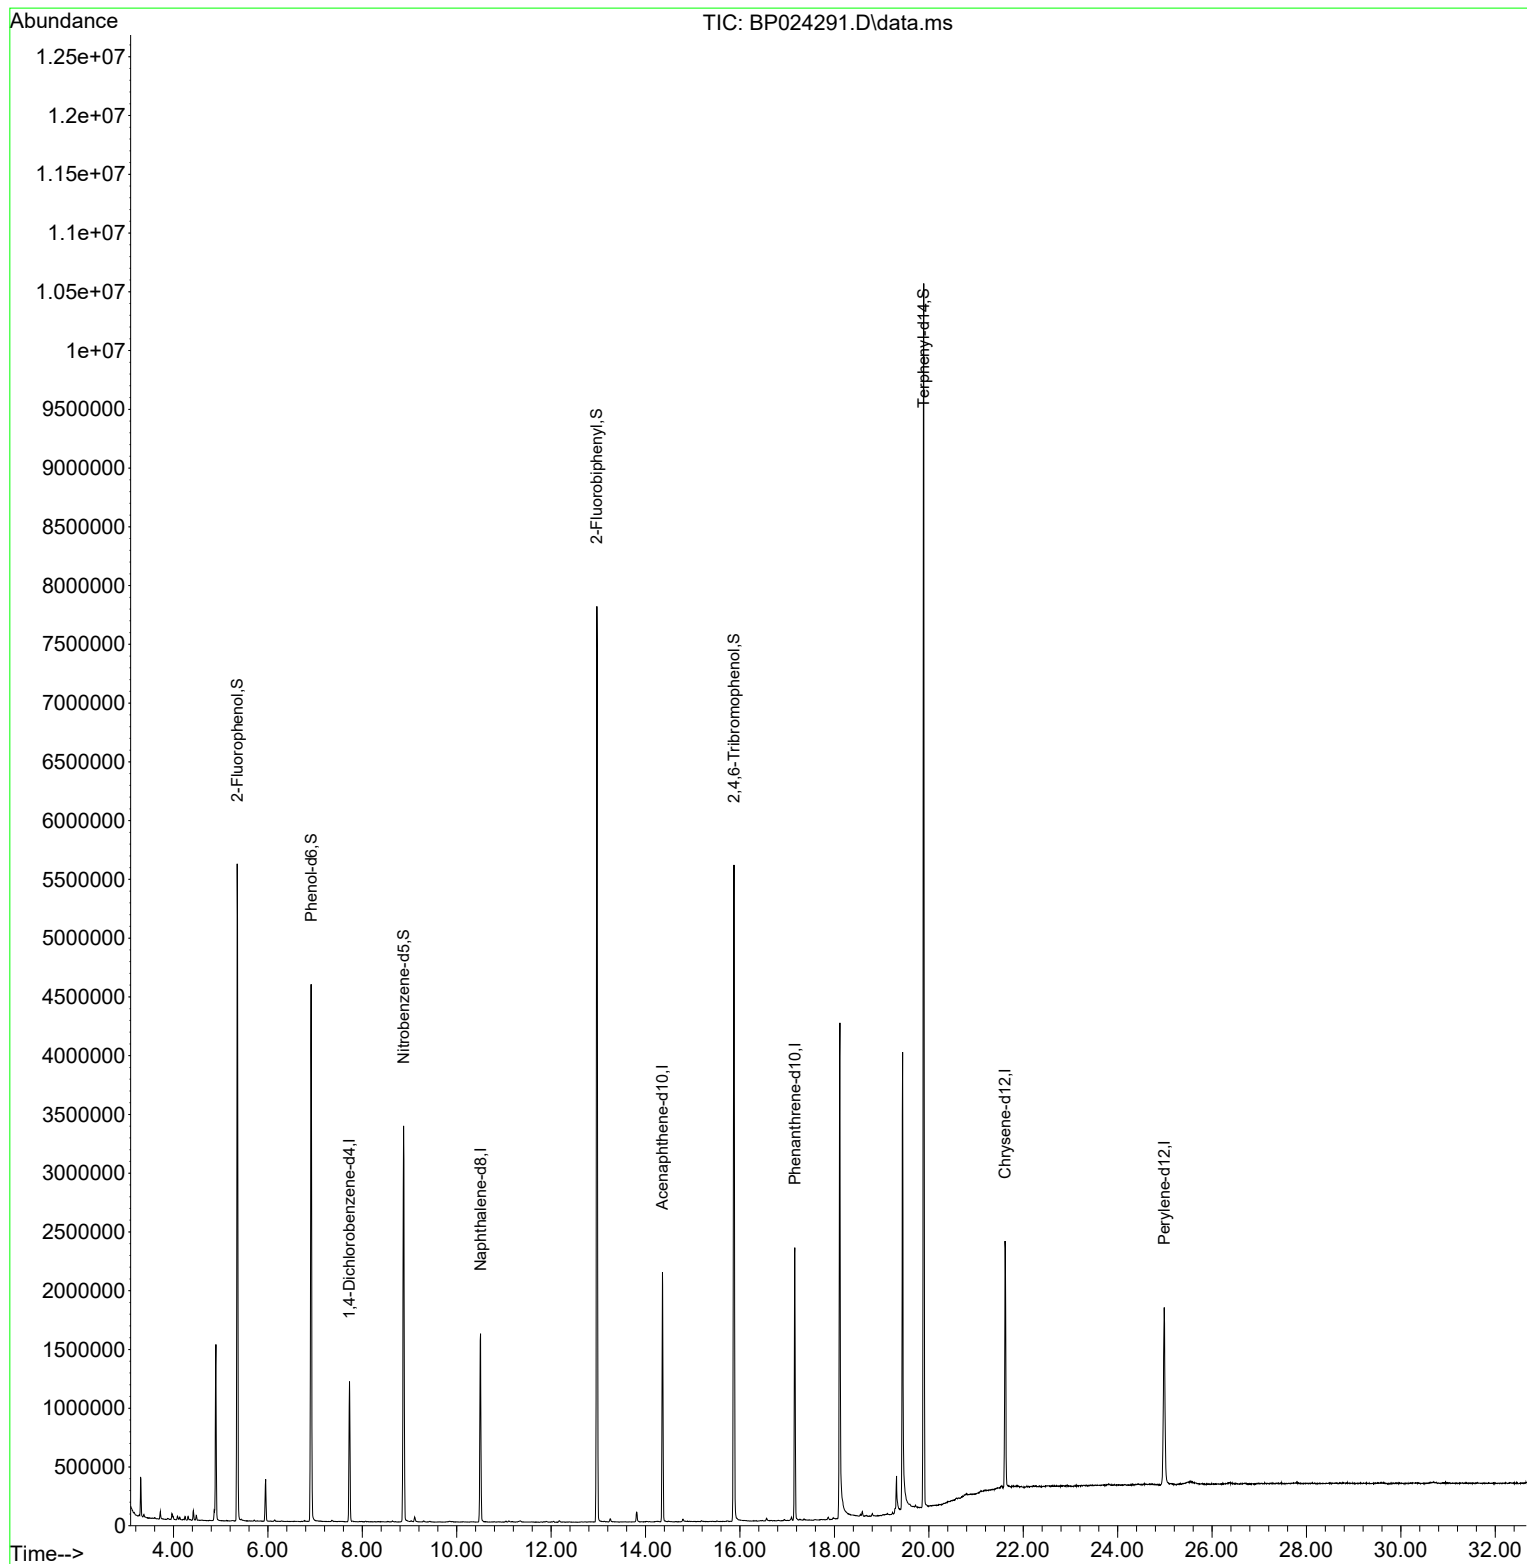




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.728 min Scan# 790
Delta R.T. 0.000 min
Lab File: BP024291.D
Acq: 15 Apr 2025 12:43




Instrument :
BNA_P
ClientSampleId :
TP-7C


Tgt Ion:152 Resp: 329036
Ion Ratio Lower Upper
152 100
150 159.5 124.9 187.3
115 62.7 47.7 71.5

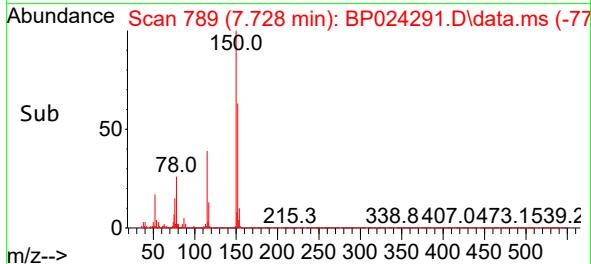

#5
2-Fluorophenol
Concen: 121.901 ng
RT: 5.352 min Scan# 385
Delta R.T. 0.000 min
Lab File: BP024291.D
Acq: 15 Apr 2025 12:43

Tgt Ion:112 Resp: 2425826
Ion Ratio Lower Upper
112 100
64 54.6 41.1 61.7
63 27.4 20.6 30.8


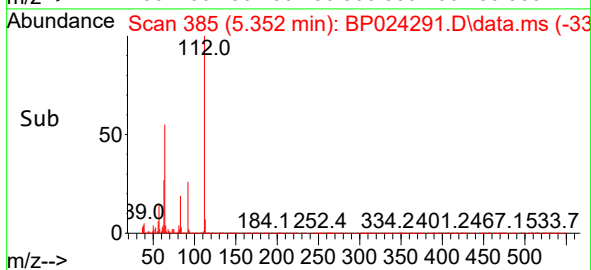

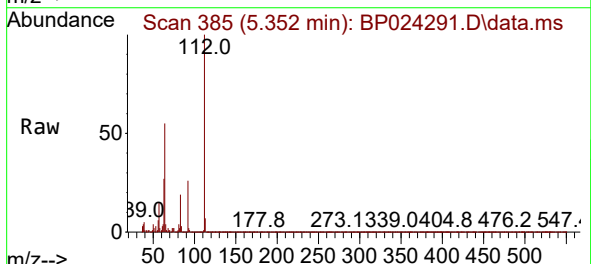




#7
Phenol-d6
Concen: 101.202 ng
RT: 6.916 min Scan# 651
Delta R.T. 0.000 min
Lab File: BP024291.D
Acq: 15 Apr 2025 12:43




Instrument :
BNA_P
ClientSampleId :
TP-7C


Tgt Ion: 99 Resp: 2757596
Ion Ratio Lower Upper
99 100
42 14.2 10.6 16.0
71 31.5 23.7 35.5

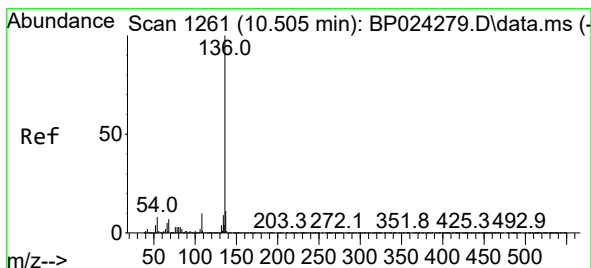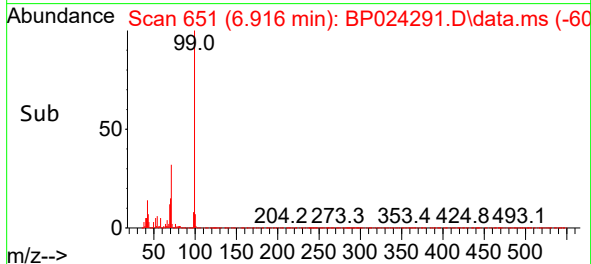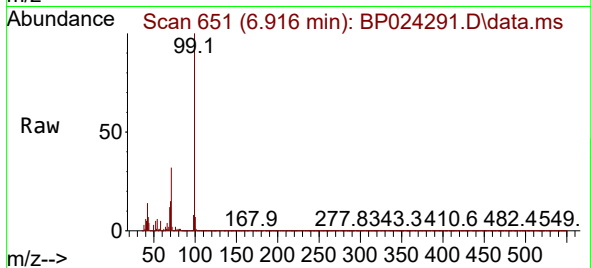

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.504 min Scan# 1261
Delta R.T. 0.000 min
Lab File: BP024291.D
Acq: 15 Apr 2025 12:43

Tgt Ion: 136 Resp: 1266138
Ion Ratio Lower Upper
136 100
137 10.7 9.2 13.8
54 7.0 6.0 9.0
68 6.5 5.5 8.3


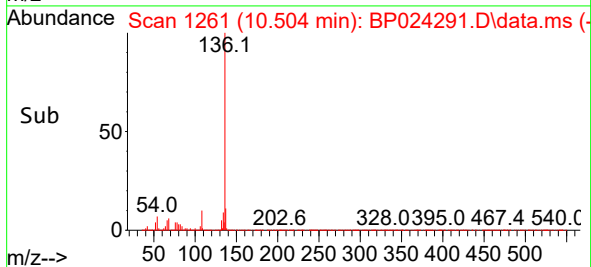

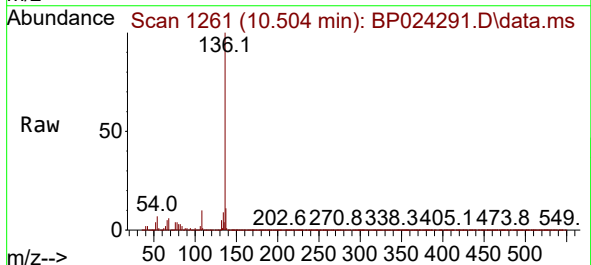




#23
Nitrobenzene-d5
Concen: 93.227 ng
RT: 8.875 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP024291.D
Acq: 15 Apr 2025 12:43




Instrument :
BNA_P
ClientSampleId :
TP-7C


Tgt Ion: 82 Resp: 2070069
Ion Ratio Lower Upper
82 100
128 45.2 36.5 54.7
54 42.4 33.4 50.2

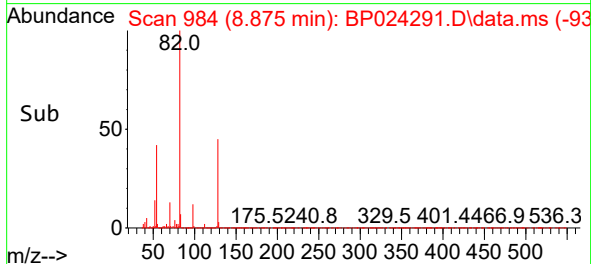

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.357 min Scan# 1916
Delta R.T. -0.012 min
Lab File: BP024291.D
Acq: 15 Apr 2025 12:43

Tgt Ion: 164 Resp: 701826
Ion Ratio Lower Upper
164 100
162 101.8 80.6 120.8
160 45.9 35.3 52.9


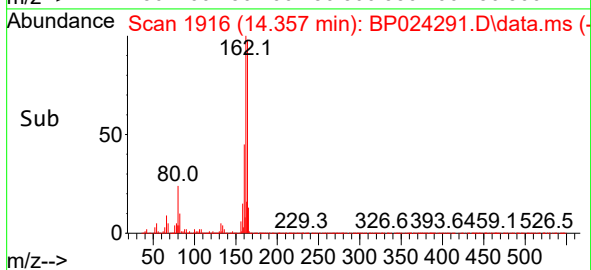

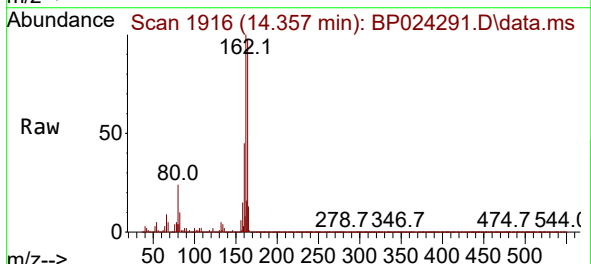




#42
2,4,6-Tribromophenol
Concen: 124.602 ng
RT: 15.875 min Scan# 2174
Delta R.T. -0.018 min
Lab File: BP024291.D
Acq: 15 Apr 2025 12:43




Instrument :
BNA_P
ClientSampleId :
TP-7C


Tgt Ion:330 Resp: 1209901
Ion Ratio Lower Upper
330 100
332 96.7 77.1 115.7
141 31.8 24.7 37.1

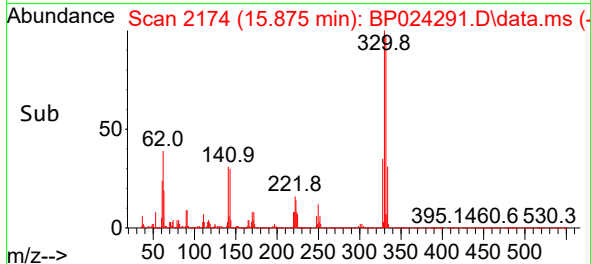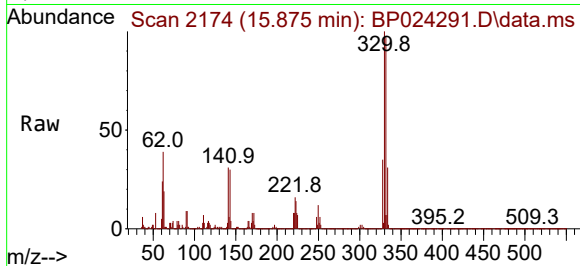

#45
2-Fluorobiphenyl
Concen: 87.423 ng
RT: 12.969 min Scan# 1680
Delta R.T. -0.012 min
Lab File: BP024291.D
Acq: 15 Apr 2025 12:43

Tgt Ion:172 Resp: 4007272
Ion Ratio Lower Upper
172 100
171 35.4 28.2 42.2
170 23.7 18.6 27.8

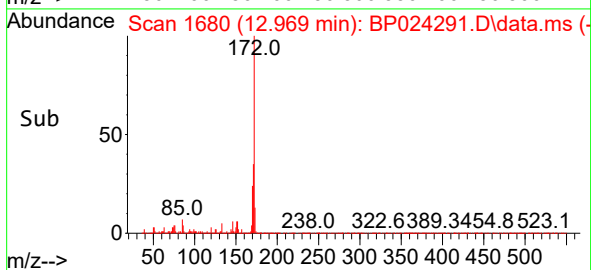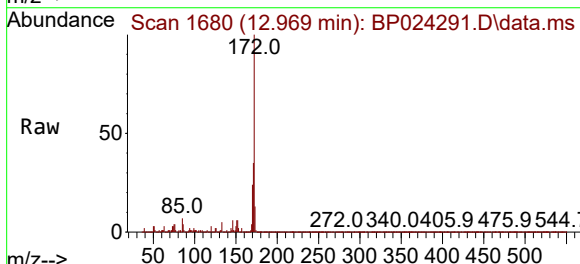

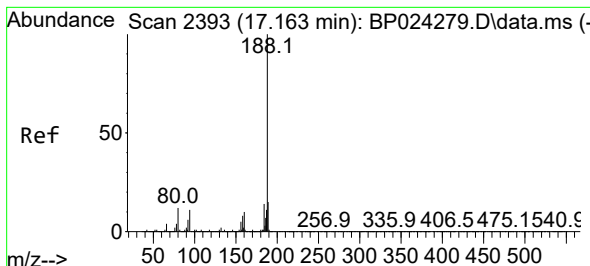

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.163 min Scan# 21

Delta R.T. -0.018 min

Lab File: BP024291.D

Acq: 15 Apr 2025 12:43

Instrument :

BNA_P

ClientSampleId :

TP-7C





Tgt Ion:188 Resp: 1267211

Ion Ratio Lower Upper

188 100

94 10.8 8.6 13.0

80 11.7 9.8 14.6

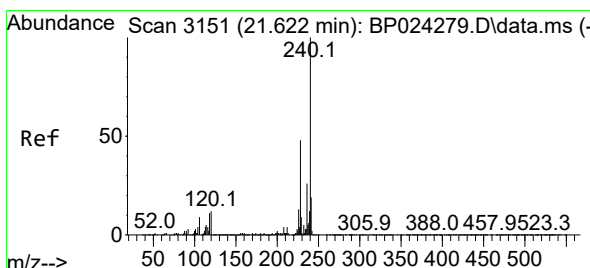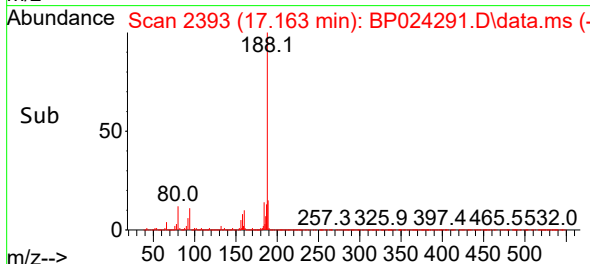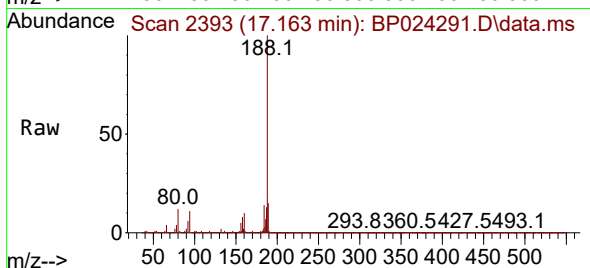

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.616 min Scan# 3150

Delta R.T. -0.006 min

Lab File: BP024291.D

Acq: 15 Apr 2025 12:43




Tgt Ion:240 Resp: 1201894


Ion Ratio Lower Upper

240 100

120 12.9 9.8 14.8

236 25.7 20.9 31.3

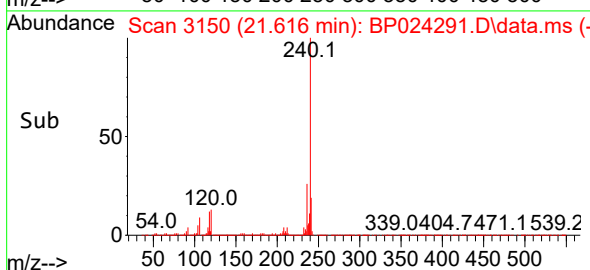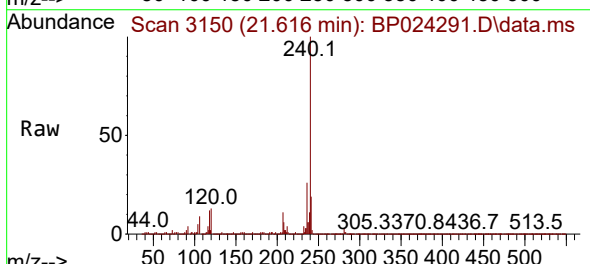



#79

Terphenyl-d14

Concen: 89.579 ng

RT: 19.892 min Scan# 2857

Delta R.T. -0.029 min

Lab File: BP024291.D

Acq: 15 Apr 2025 12:43

Instrument :

BNA_P

ClientSampleId :

TP-7C





Tgt Ion:244 Resp: 5341472

Ion Ratio Lower Upper

244 100

212 7.0 5.6 8.4

122 11.1 9.4 14.0

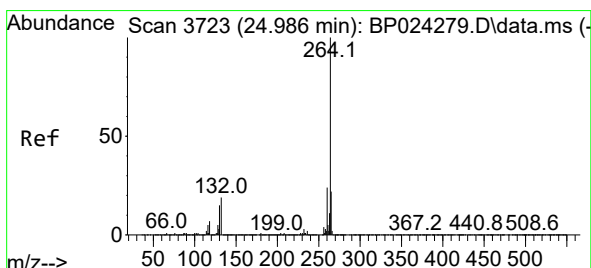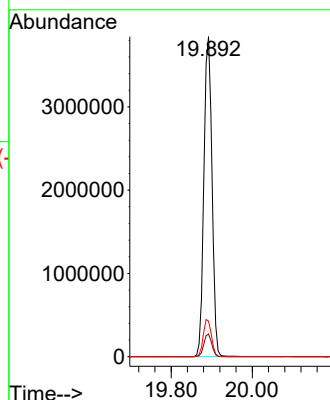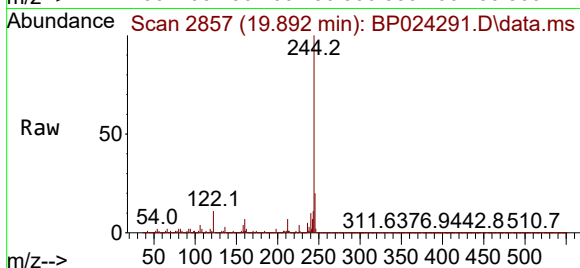

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.986 min Scan# 3723

Delta R.T. 0.000 min

Lab File: BP024291.D

Acq: 15 Apr 2025 12:43

Tgt Ion:264 Resp: 1296224

Ion Ratio Lower Upper

264 100

260 23.3 18.9 28.3

265 22.5 17.8 26.6

