
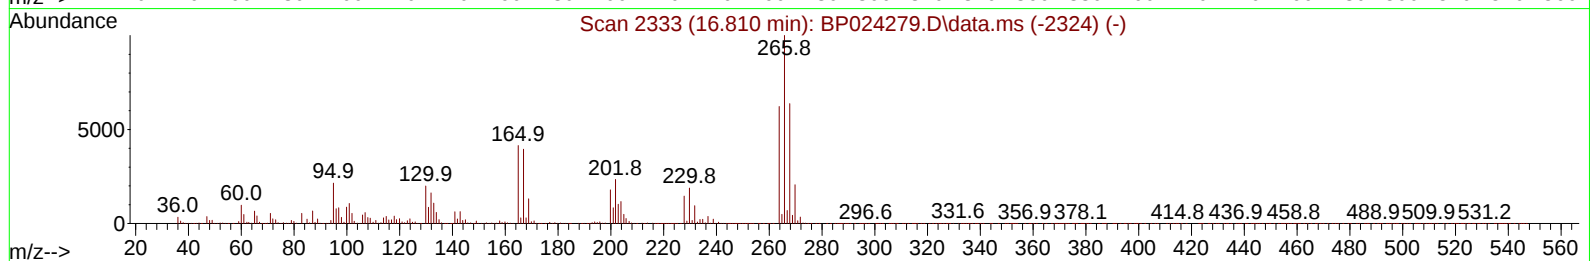
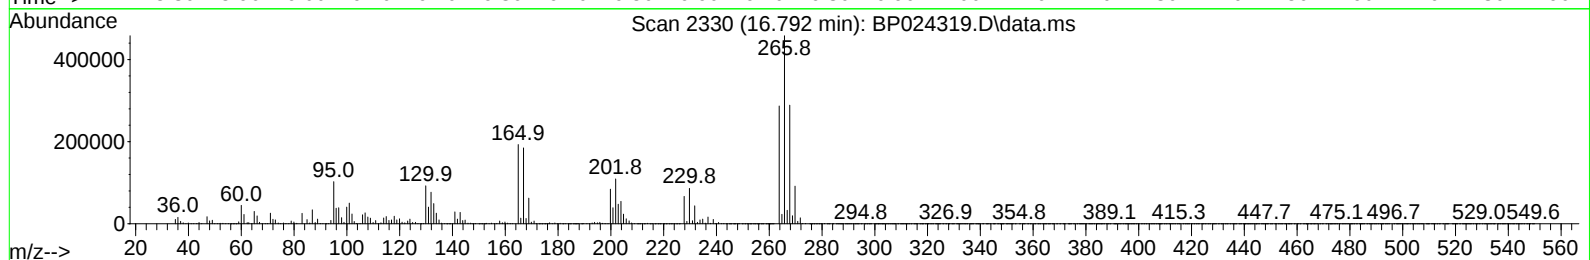


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041725\
Data File : BP024319.D
Acq On : 17 Apr 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 12:47:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

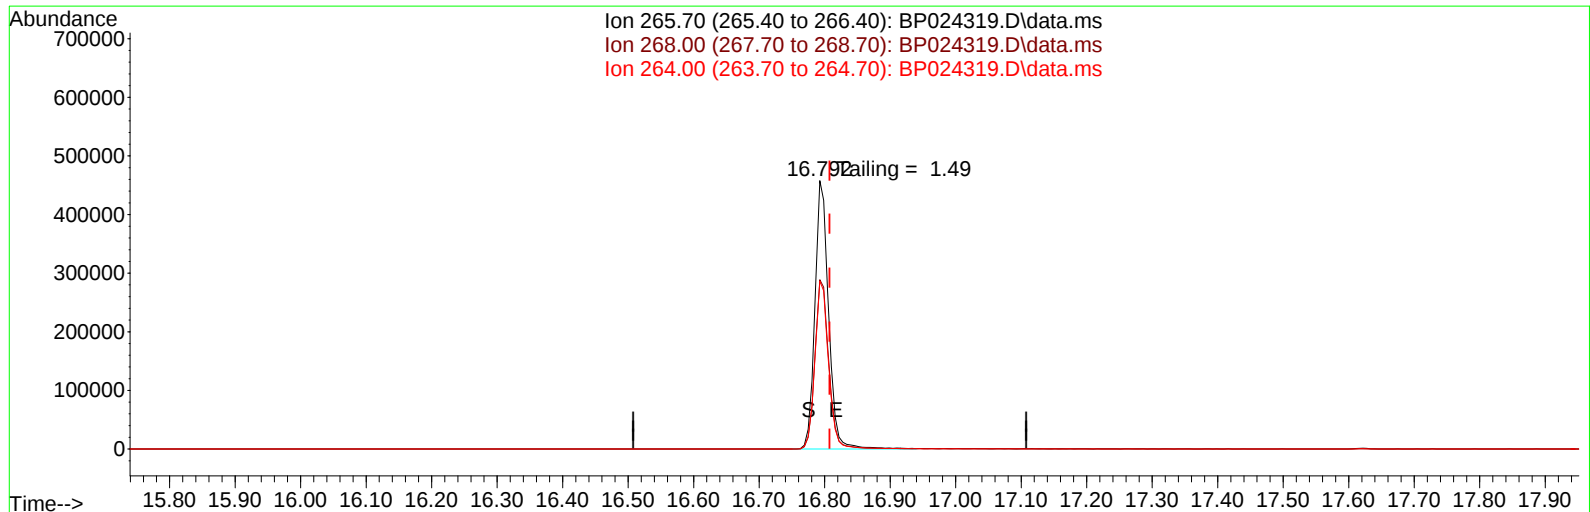

TIC: BP024319.D\data.ms

(70) Pentachlorophenol (C)




16.792min (-0.015) 3494703.78 ng

response 665367

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.09
264.00	62.20	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041725\
Data File : BP024319.D
Acq On : 17 Apr 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 12:47:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

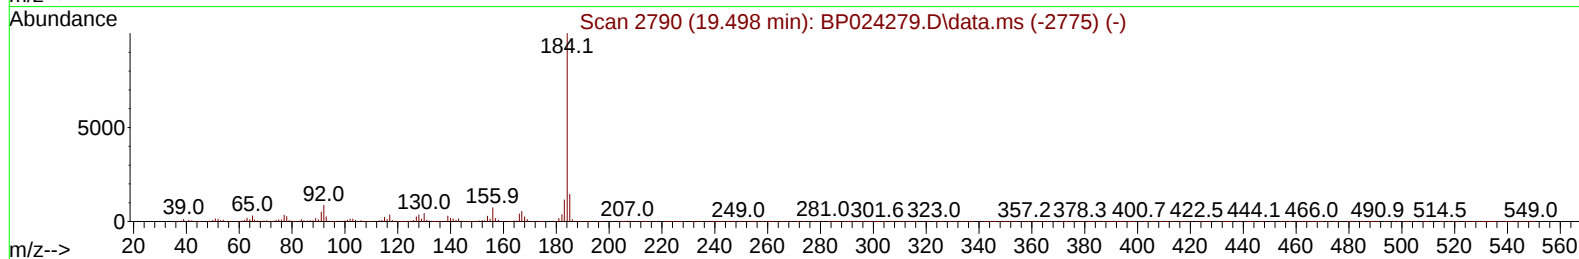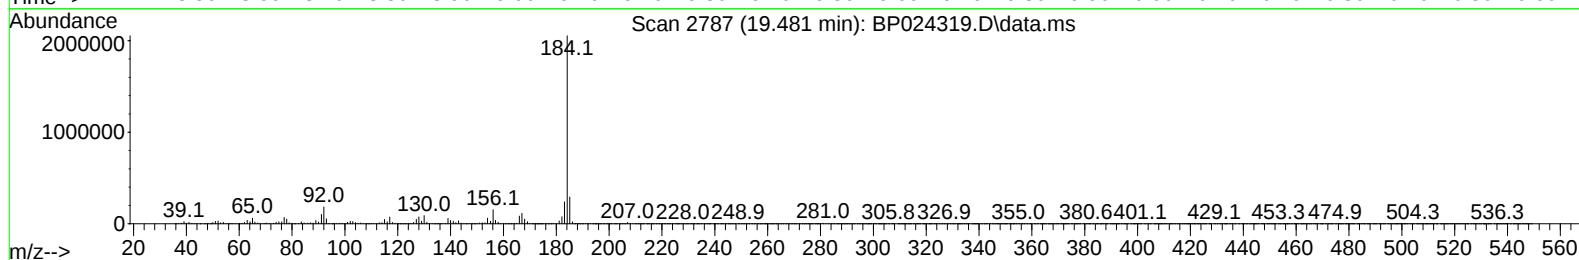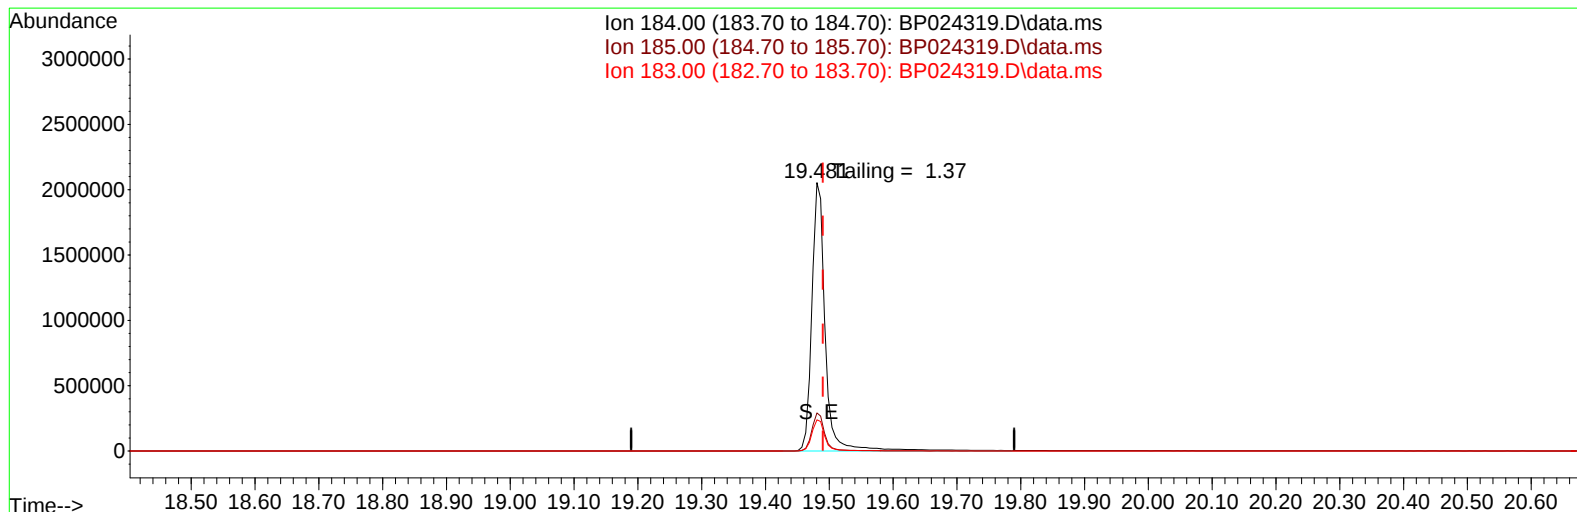

TIC: BP024319.D\data.ms

(77) Benzidine**19.481min (-0.009) 4514488.36 ng****response 2975698**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.21
183.00	11.50	11.67
0.00	0.00	0.00