
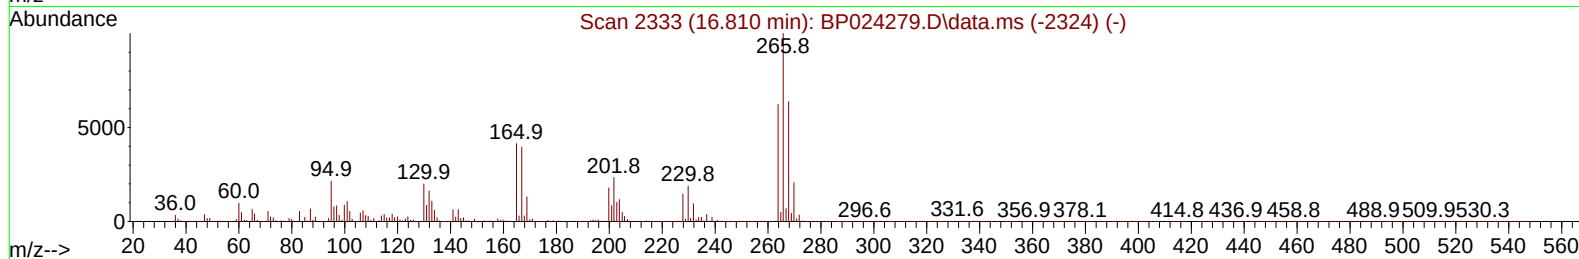
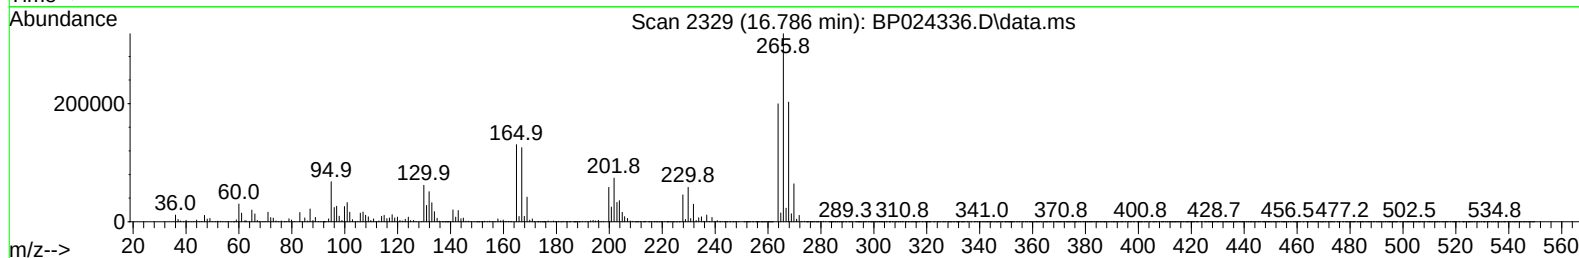


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041825\
Data File : BP024336.D
Acq On : 18 Apr 2025 10:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 12:10:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

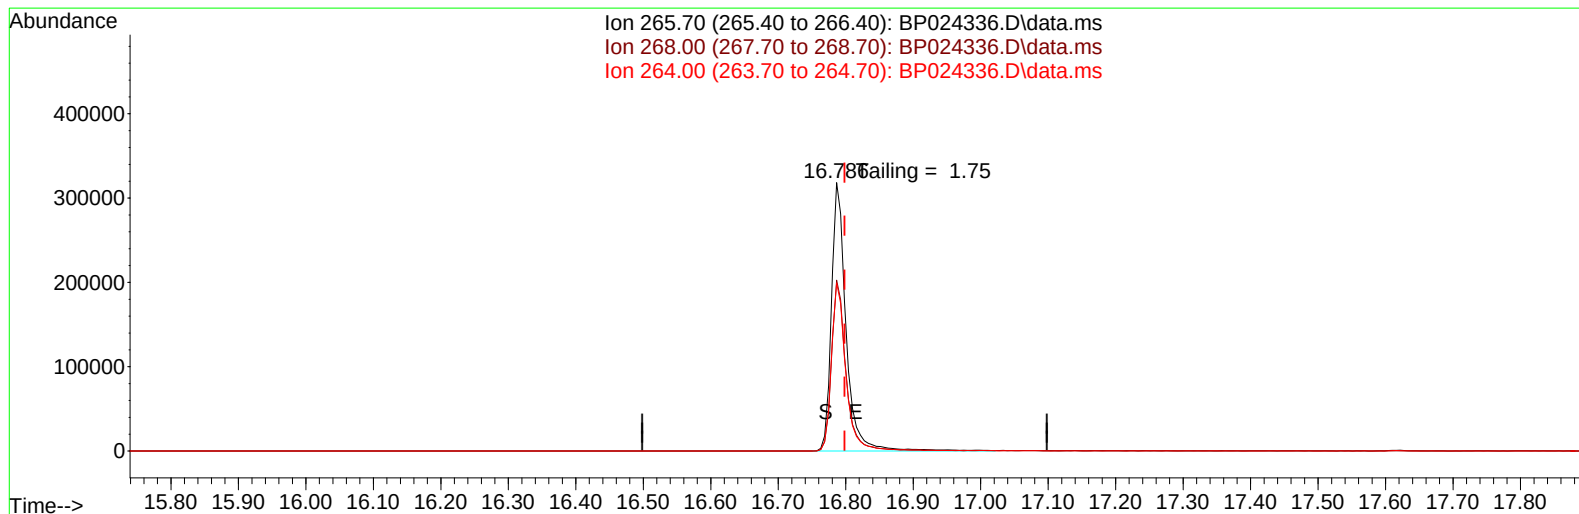

TIC: BP024336.D\data.ms

(70) Pentachlorophenol (C)




16.786min (-0.012) 2010562.17 ng

response 473939

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.69
264.00	62.20	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041825\
Data File : BP024336.D
Acq On : 18 Apr 2025 10:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 12:10:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

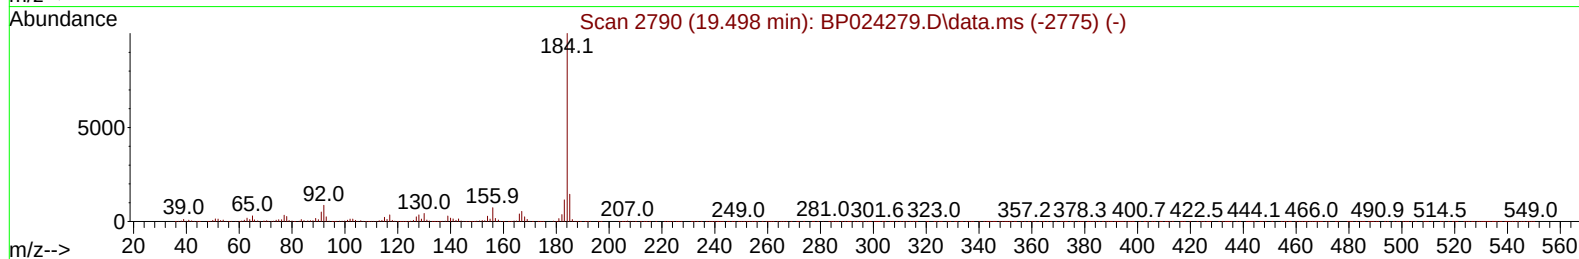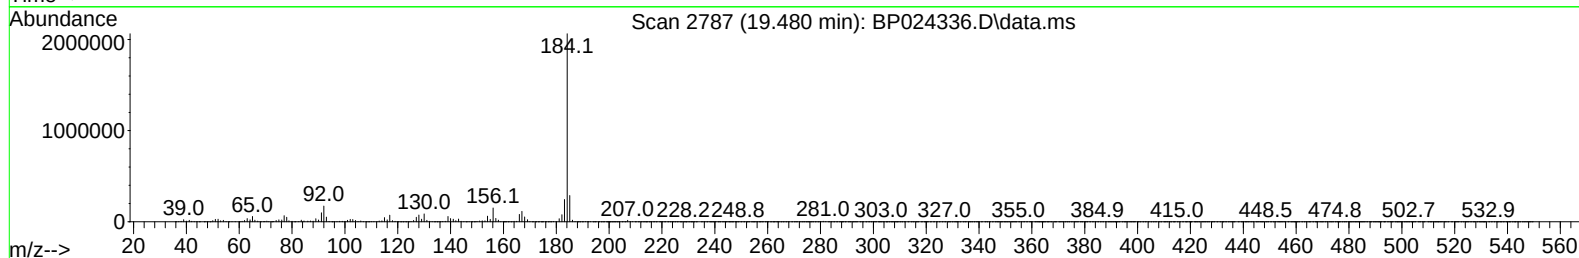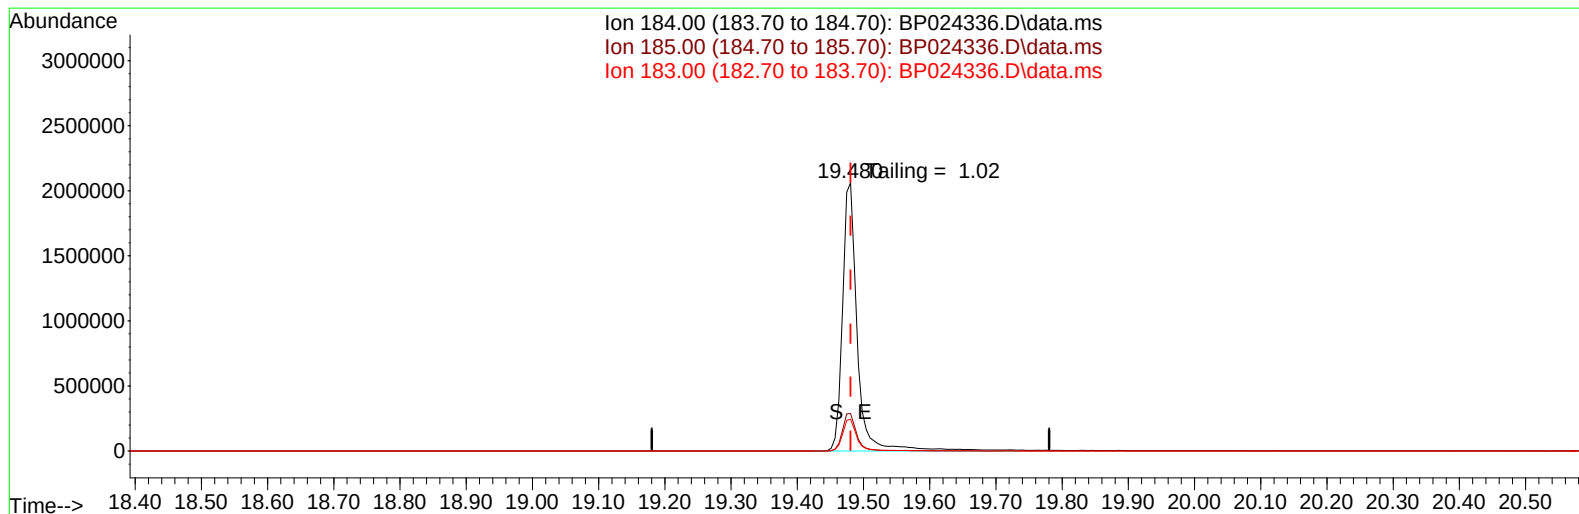

TIC: BP024336.D\data.ms

(77) Benzidine**19.480min (+ 0.000) 1458069.24 ng****response 3105020**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.99
183.00	11.50	11.86
0.00	0.00	0.00