




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009961.D
 Acq On : 20 Apr 2022 00:14
 Operator : CG/JU
 Sample : N2422-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J14

Manual IntegrationsAPPROVED

Quant Time: Apr 20 01:35:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/25/2022

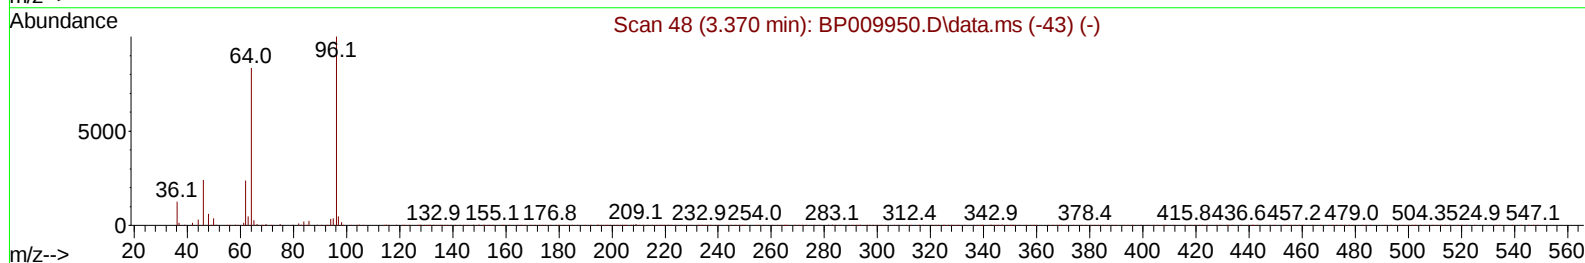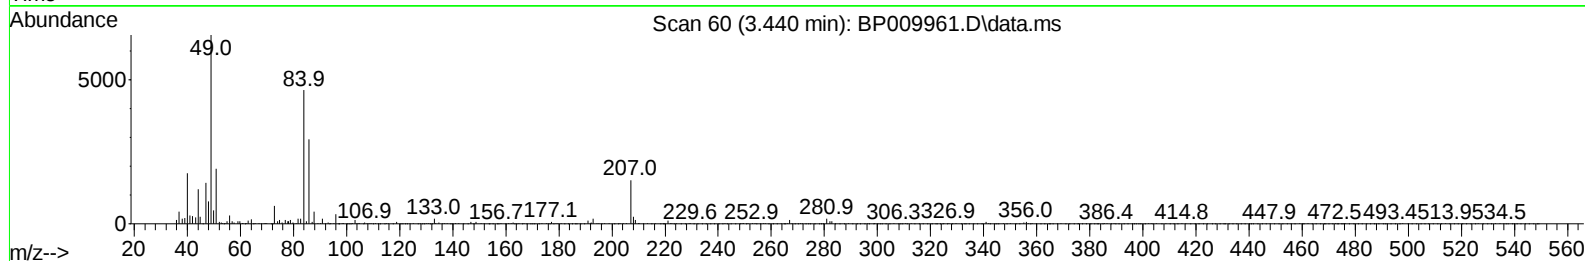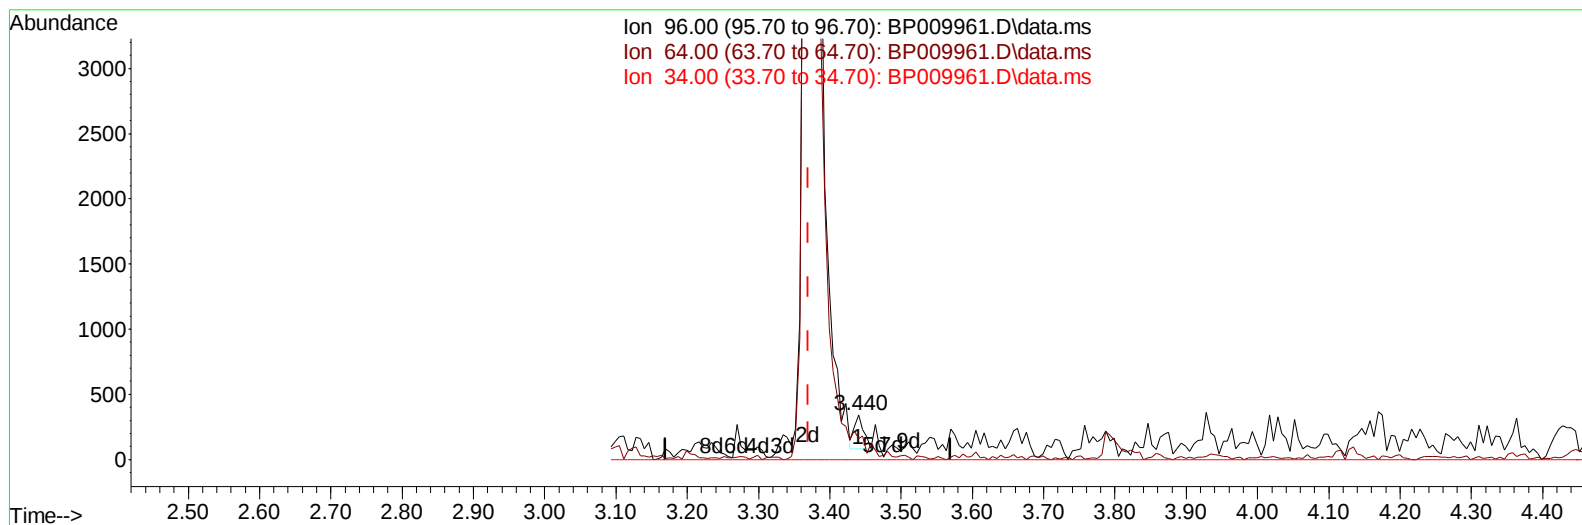

TIC: BP009961.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.440min (+ 0.070) 0.08 ng/uL

response 238

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	46.51
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009961.D
Acq On : 20 Apr 2022 00:14
Operator : CG/JU
Sample : N2422-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J14

Manual IntegrationsAPPROVED

Quant Time: Apr 20 01:35:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/25/2022

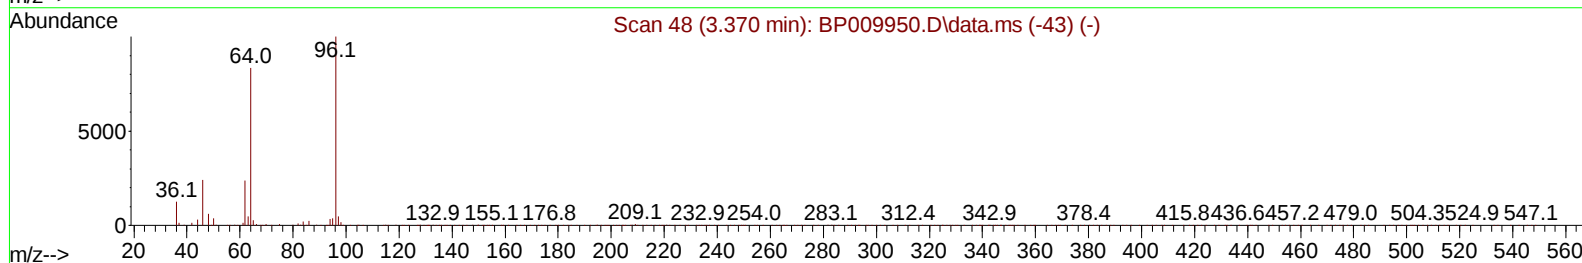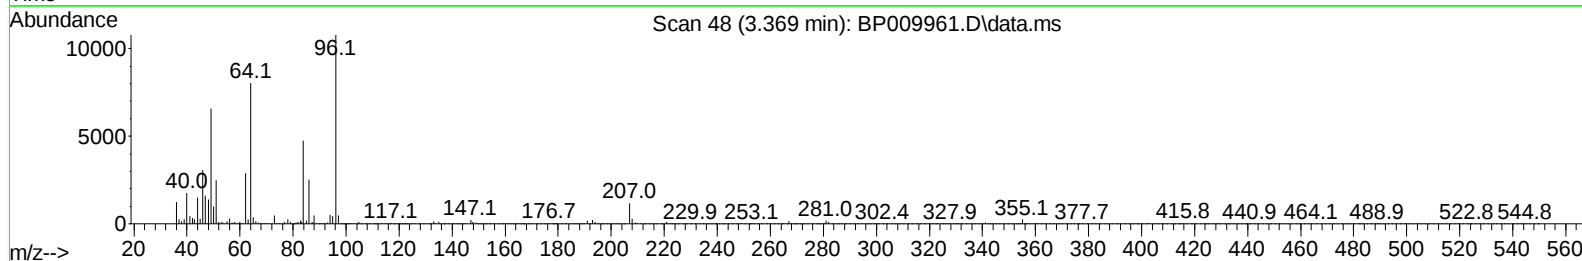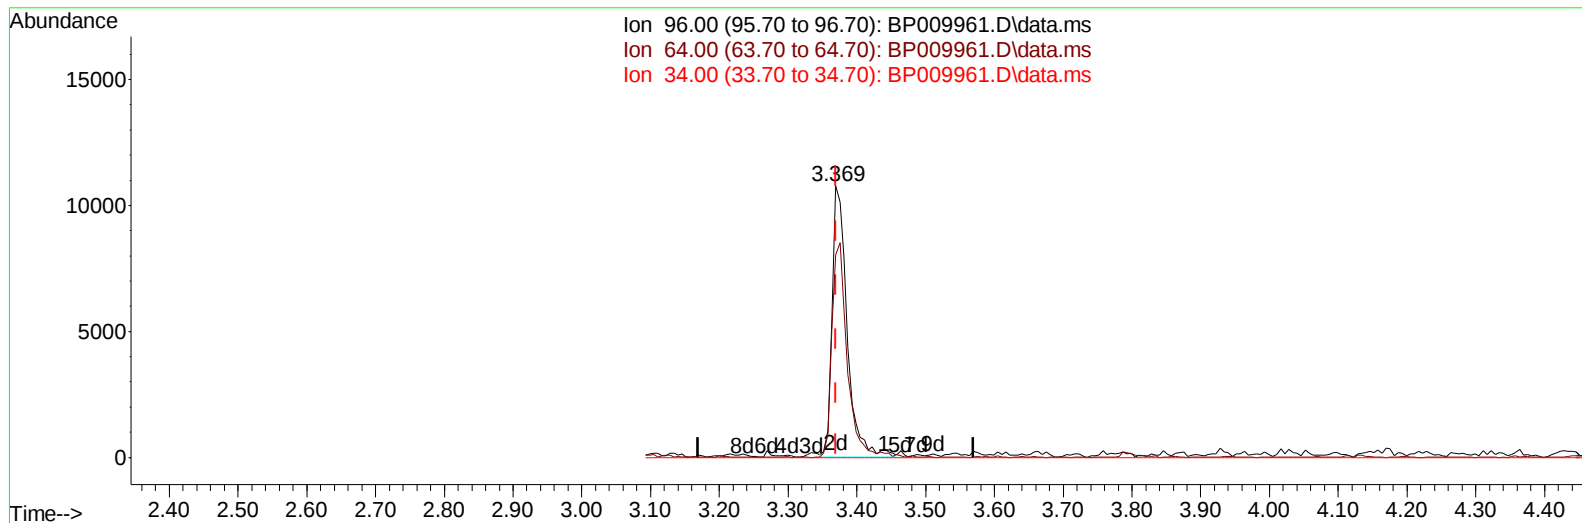

TIC: BP009961.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (-0.000) 5.41 ng/uL m

response 16191

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	74.58#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009961.D
 Acq On : 20 Apr 2022 00:14
 Operator : CG/JU
 Sample : N2422-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J14

Manual IntegrationsAPPROVED

Quant Time: Apr 20 01:35:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/25/2022

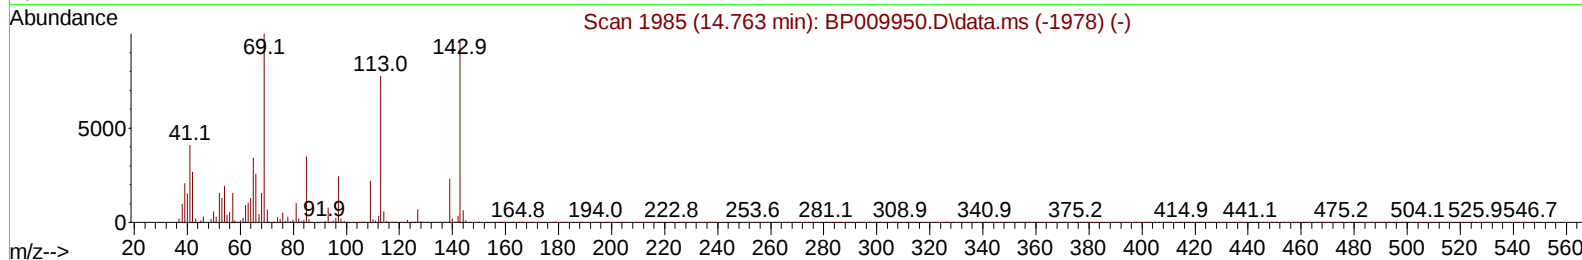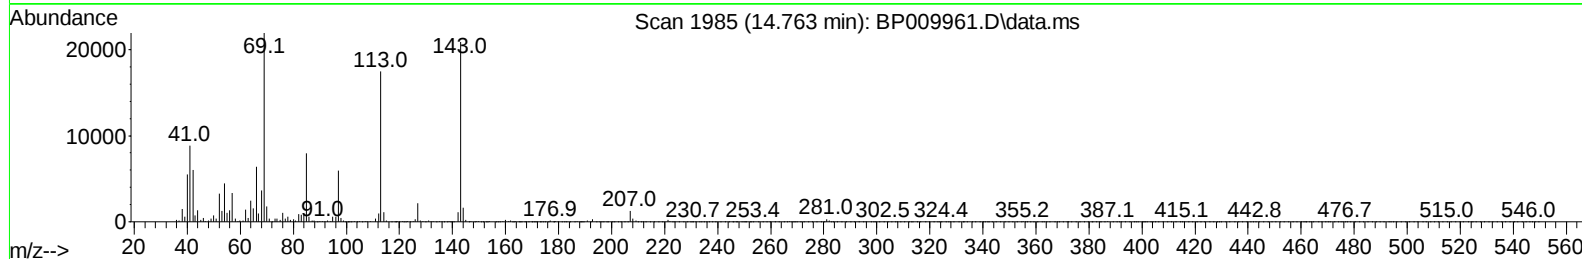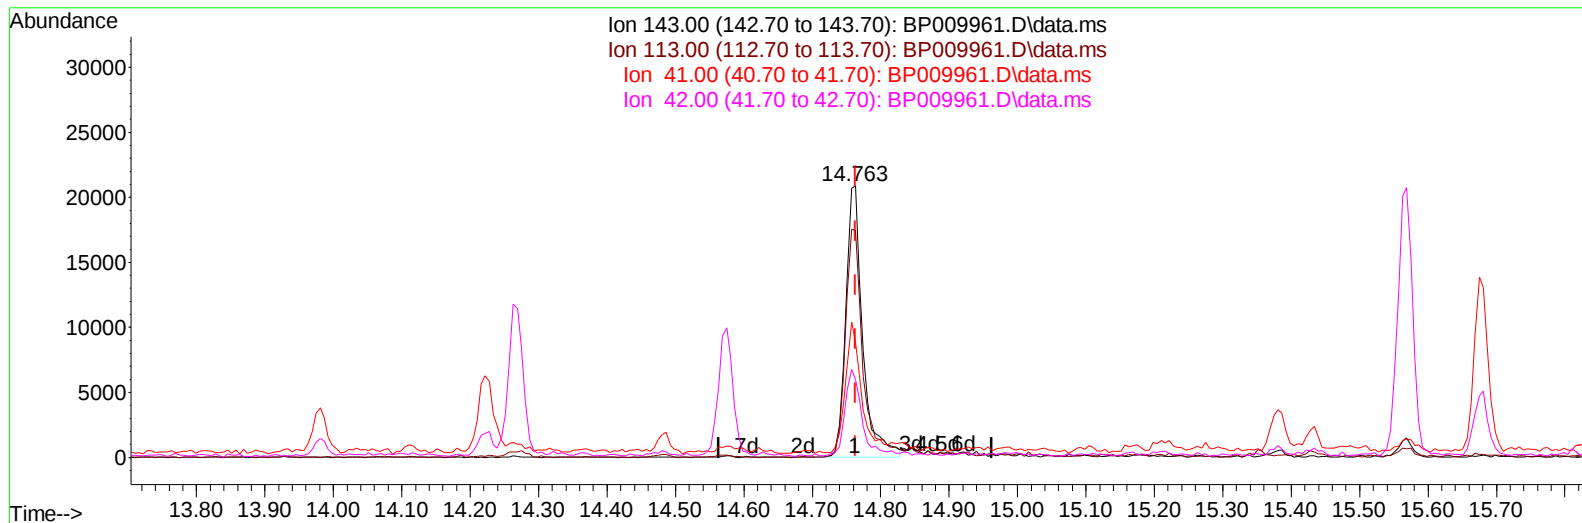

TIC: BP009961.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.000) 5.82 ng/u1

response 35787

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.56#
41.00	23.20	42.24#
42.00	18.00	28.77#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009961.D
Acq On : 20 Apr 2022 00:14
Operator : CG/JU
Sample : N2422-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J14

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 20 01:35:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

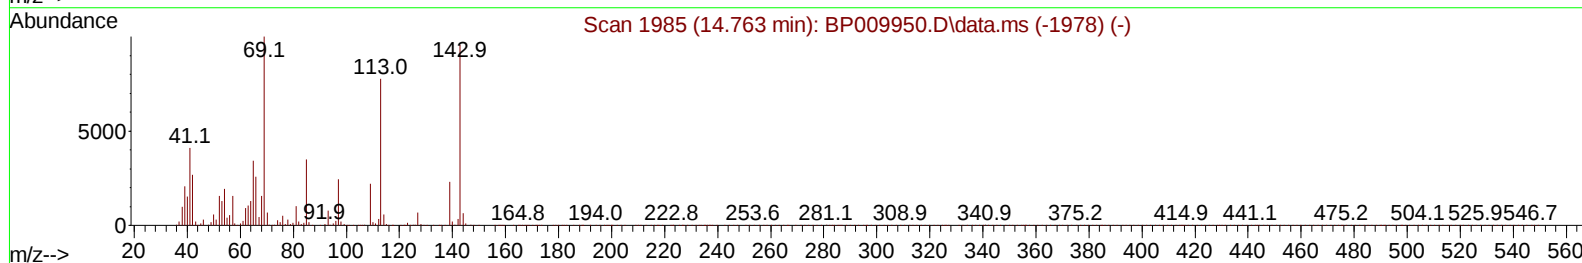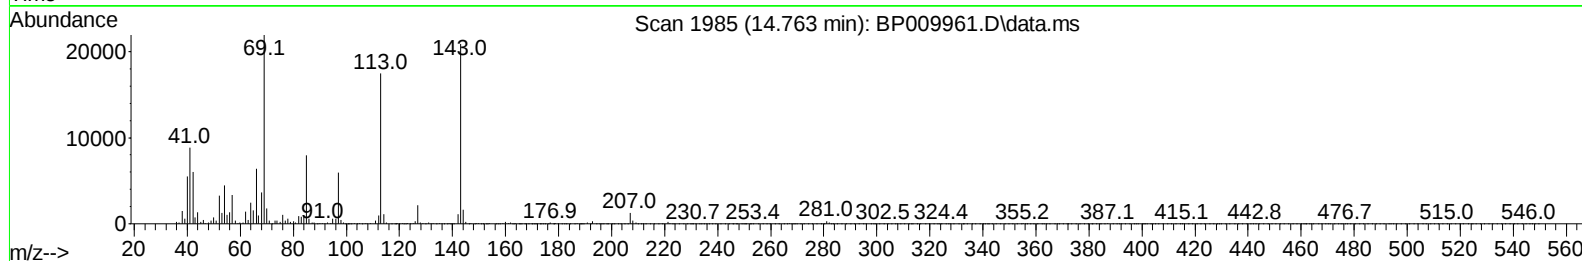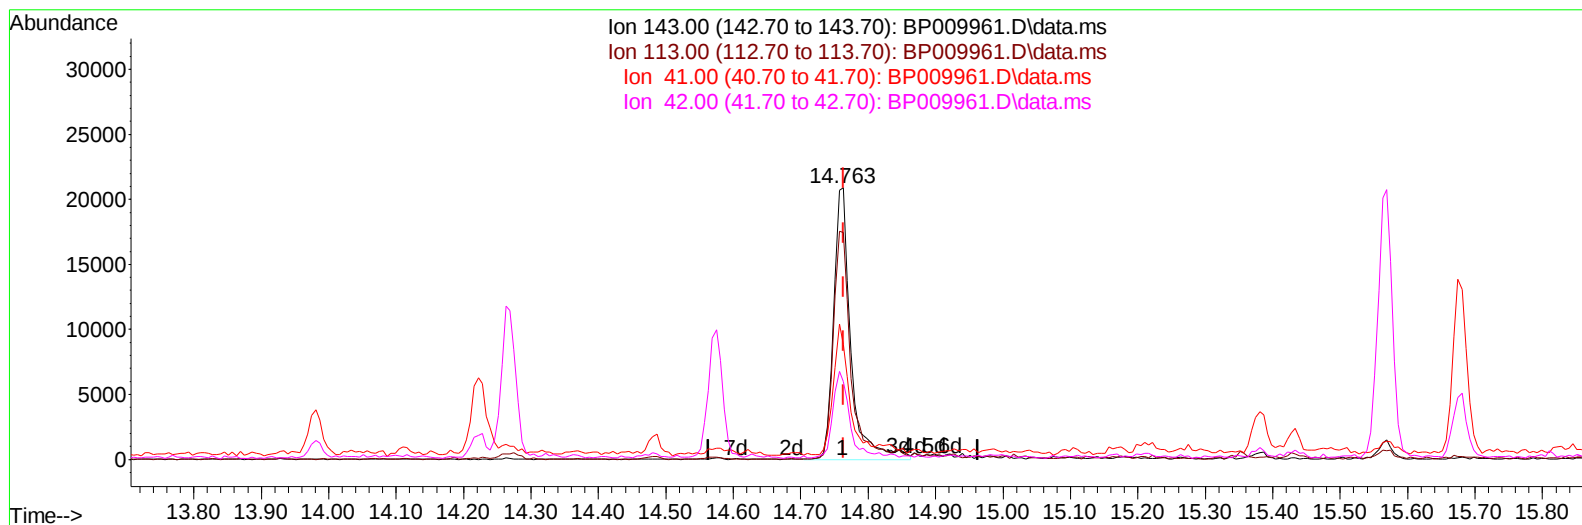

TIC: BP009961.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.000) 6.03 ng/ul m

response 37101

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.56#
41.00	23.20	42.24#
42.00	18.00	28.77#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009961.D
 Acq On : 20 Apr 2022 00:14
 Operator : CG/JU
 Sample : N2422-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J14

Manual IntegrationsAPPROVED

Quant Time: Apr 20 01:35:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	133455	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.751	136	590702	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	432001	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	934769	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.410	240	882902	20.000	ng/ul	# 0.00
88) Perylene-d12	23.862	264	803467	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	16191m	5.415	ng/uL	0.00
4) Pyridine-d5	3.793	84	83298	10.103	ng/ul	0.00
7) Phenol-d5	7.099	99	76242	6.507	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	250999	35.984	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	232860	26.348	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	163106	16.676	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	161241	37.852	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	174224	37.306	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	296381	30.328	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	381423	27.403	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	1293046	38.104	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1377360	34.260	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	37101m	6.029	ng/ul	0.00
60) Fluorene-d10	15.569	176	1119281	39.209	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	216375	39.074	ng/ul	0.00
73) Anthracene-d10	17.428	188	1906343	42.594	ng/ul	0.00
81) Pyrene-d10	19.657	212	2300740	47.713	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	1854381	44.319	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.128	94	14652	1.249	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009961.D
Acq On : 20 Apr 2022 00:14
Operator : CG/JU
Sample : N2422-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J14

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 20 01:35:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

