




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009965.D
 Acq On : 20 Apr 2022 02:29
 Operator : CG/JU
 Sample : N2422-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J42

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 20 05:23:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

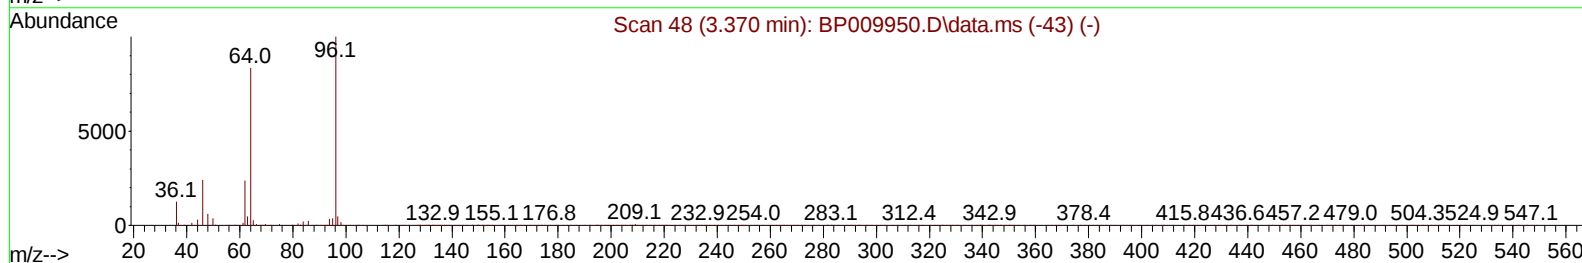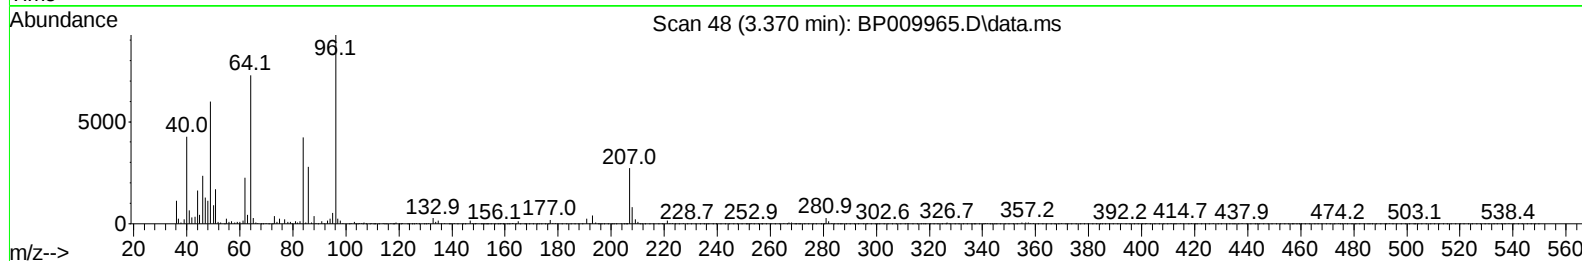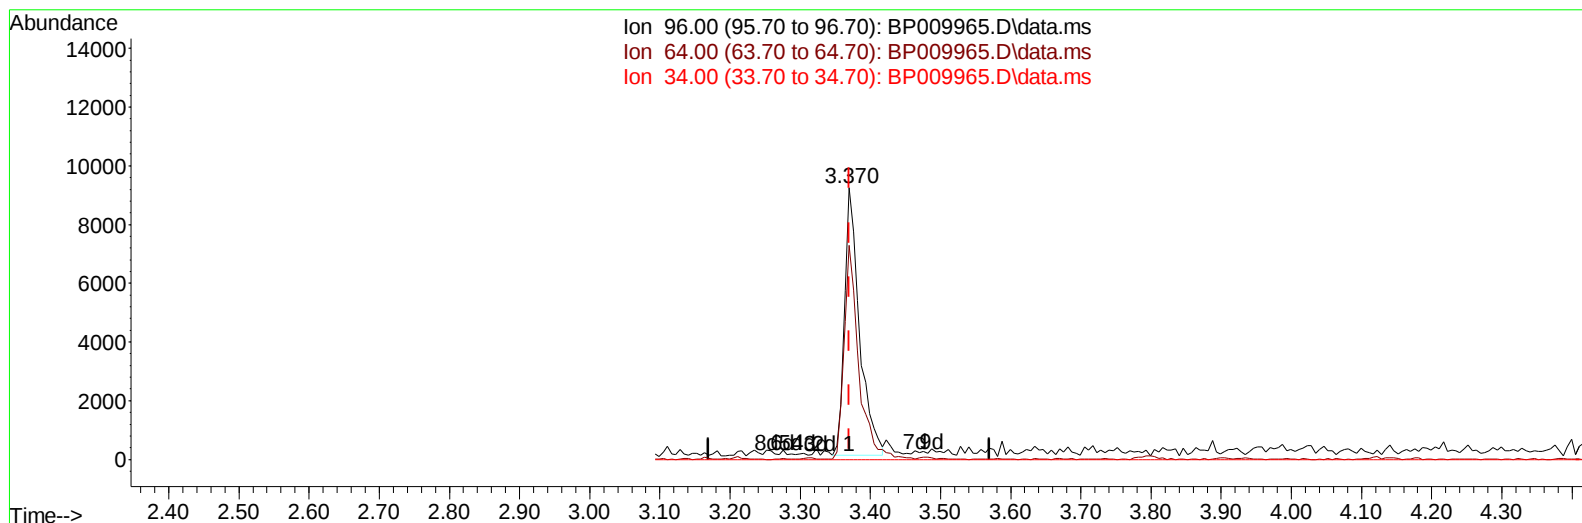

TIC: BP009965.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.370min (+ 0.000) 5.34 ng/uL

response 13596

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	78.76#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009965.D
 Acq On : 20 Apr 2022 02:29
 Operator : CG/JU
 Sample : N2422-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J42

Manual IntegrationsAPPROVED

Quant Time: Apr 20 05:23:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/25/2022

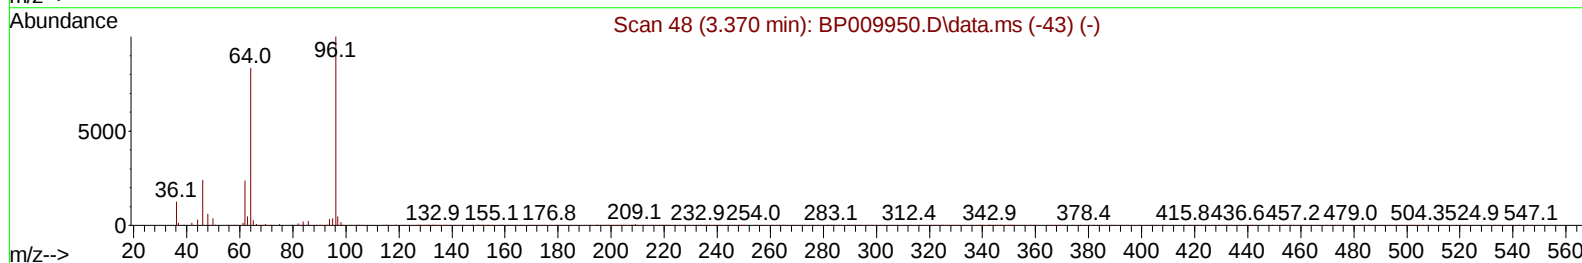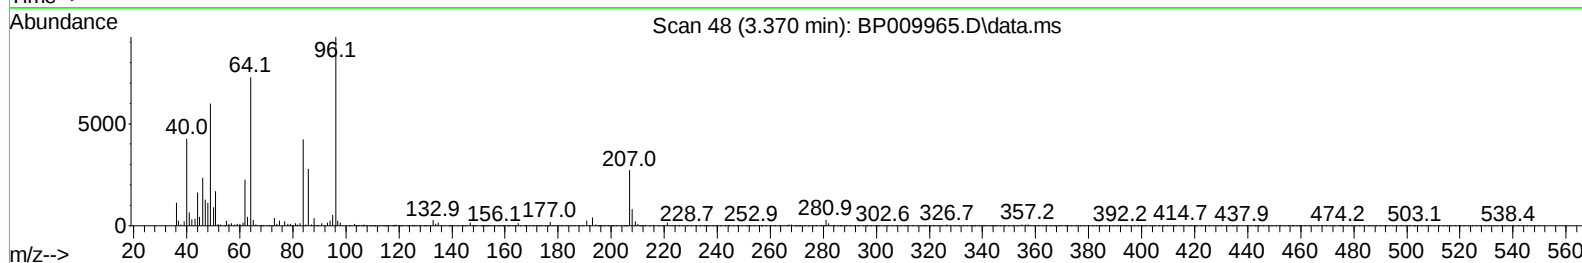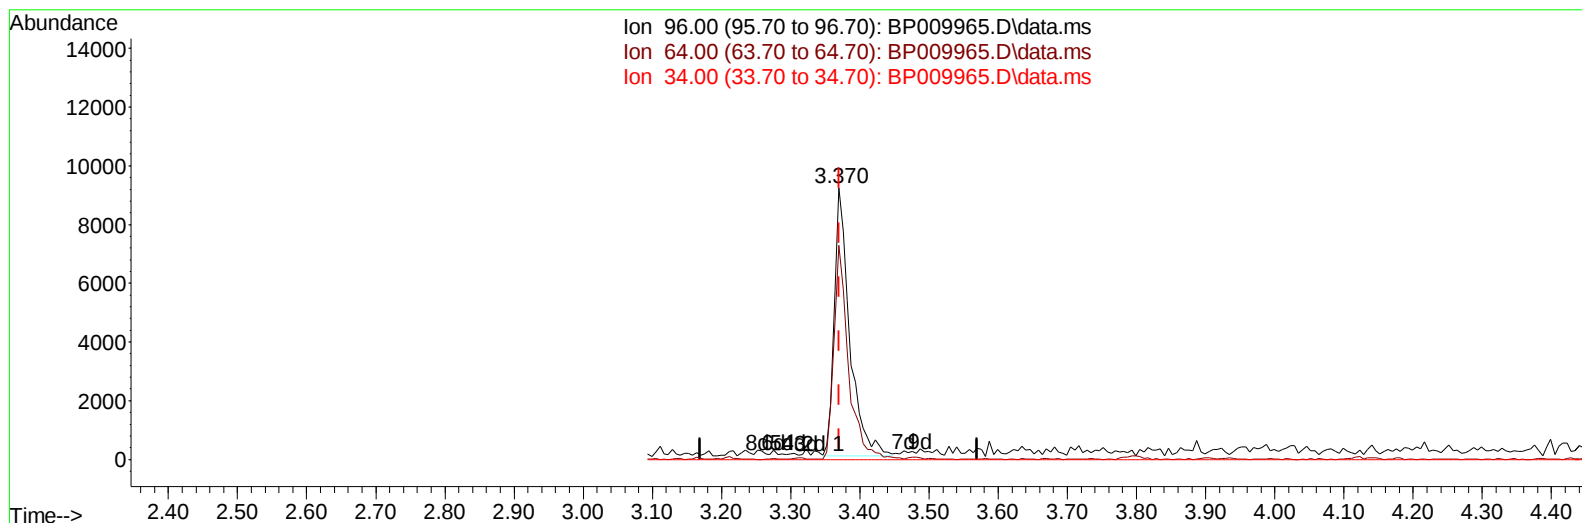

TIC: BP009965.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.370min (+ 0.000) 5.54 ng/uL m

response 14095

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	78.76#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009965.D
 Acq On : 20 Apr 2022 02:29
 Operator : CG/JU
 Sample : N2422-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J42

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 20 05:23:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	113642	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	503329	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	365548	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	804786	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	837120	20.000	ng/ul	# 0.00
88) Perylene-d12	23.857	264	832119	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	14095m	5.535	ng/uL	0.00
4) Pyridine-d5	3.793	84	64412	9.175	ng/ul	0.00
7) Phenol-d5	7.105	99	50361	5.048	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	141431	23.811	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	129988	17.272	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	96270	11.559	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	86599	23.859	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	87291	21.936	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	158868	19.078	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	323101	27.243	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	690897	24.061	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	729242	21.437	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	22751	4.369	ng/ul	0.00
60) Fluorene-d10	15.569	176	590065	24.428	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	86494	18.142	ng/ul	0.00
73) Anthracene-d10	17.428	188	1003304	26.038	ng/ul	0.00
81) Pyrene-d10	19.651	212	1298268	28.396	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	1206886	27.851	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.128	94	18313	1.834	ng/ul#	94
78) Di-n-butylphthalate	18.281	149	187522	3.874	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009965.D
Acq On : 20 Apr 2022 02:29
Operator : CG/JU
Sample : N2422-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J42

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 20 05:23:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

