




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009975.D
 Acq On : 20 Apr 2022 14:29
 Operator : CG/JU
 Sample : PB144175BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK175

Manual IntegrationsAPPROVED

Quant Time: Apr 21 01:05:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

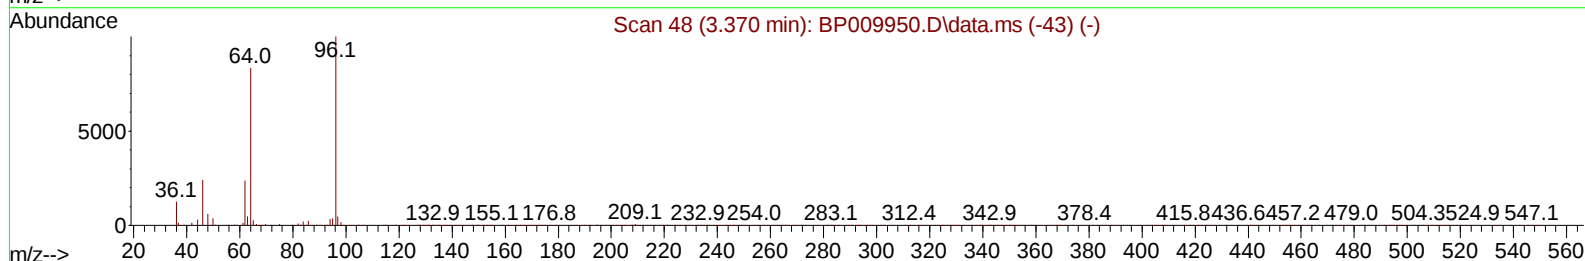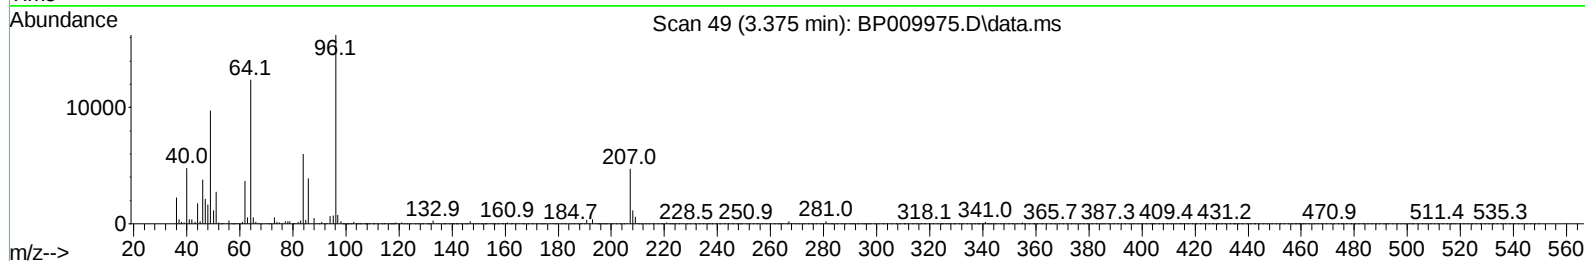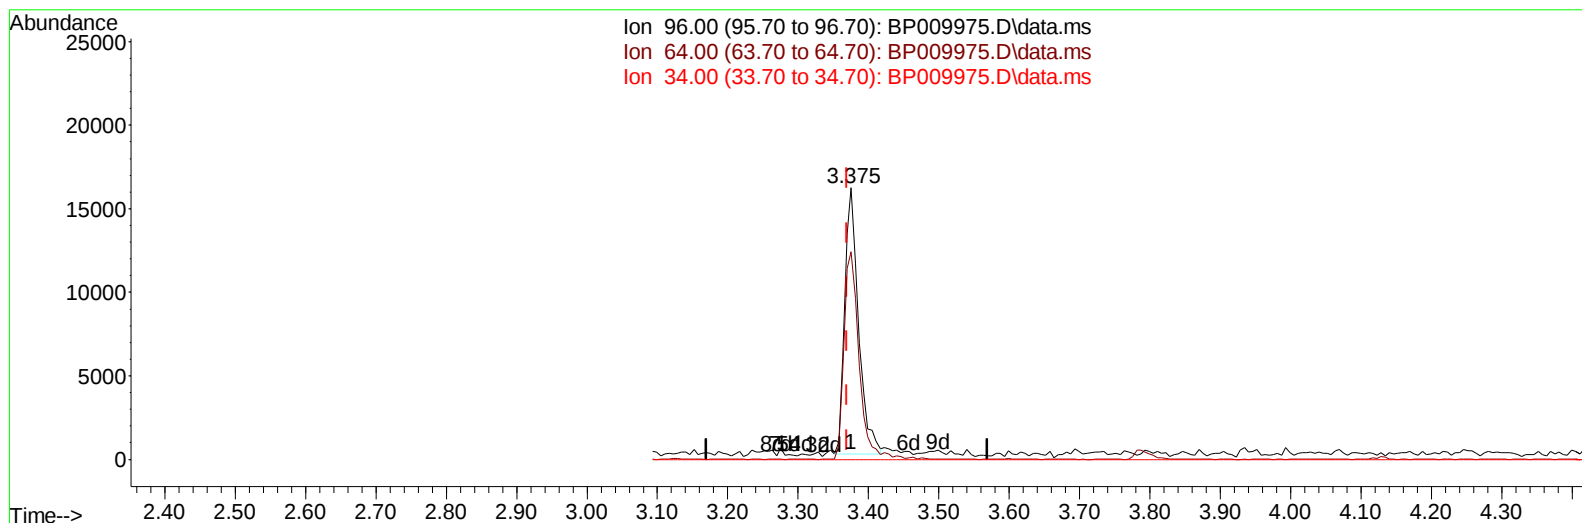

TIC: BP009975.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.006) 5.65 ng/uL

response 21617

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	76.42#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009975.D
 Acq On : 20 Apr 2022 14:29
 Operator : CG/JU
 Sample : PB144175BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK175

Manual IntegrationsAPPROVED

Quant Time: Apr 21 01:05:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

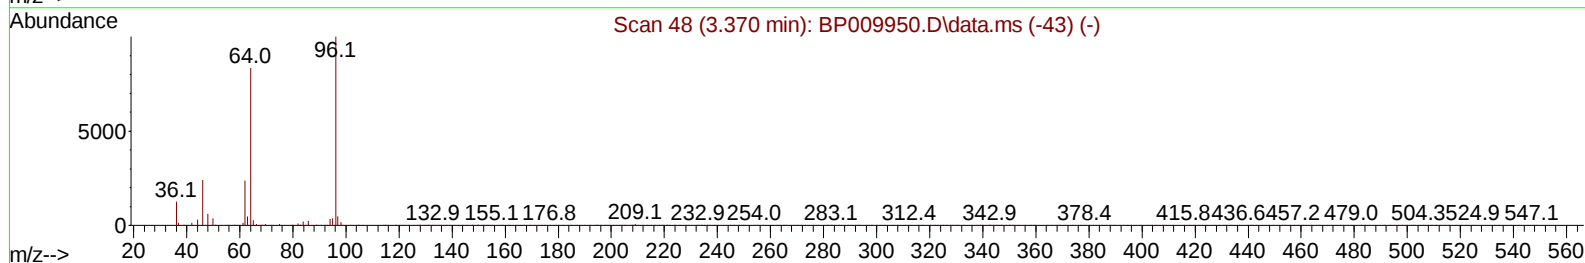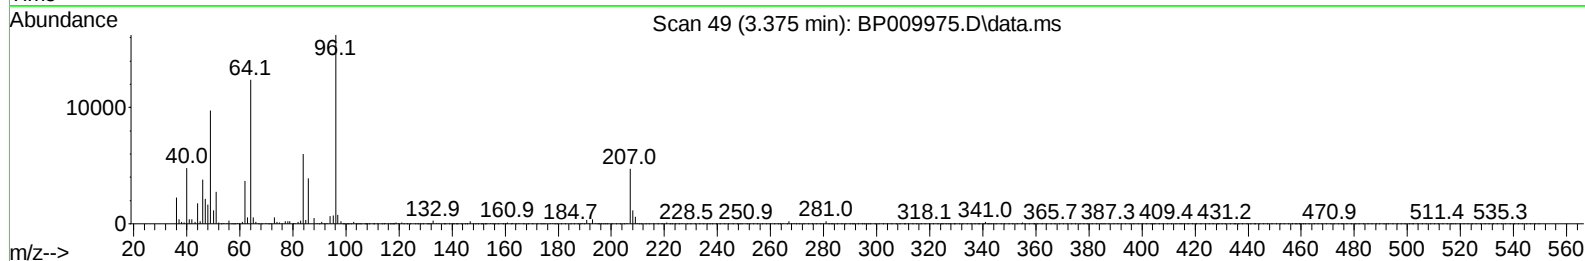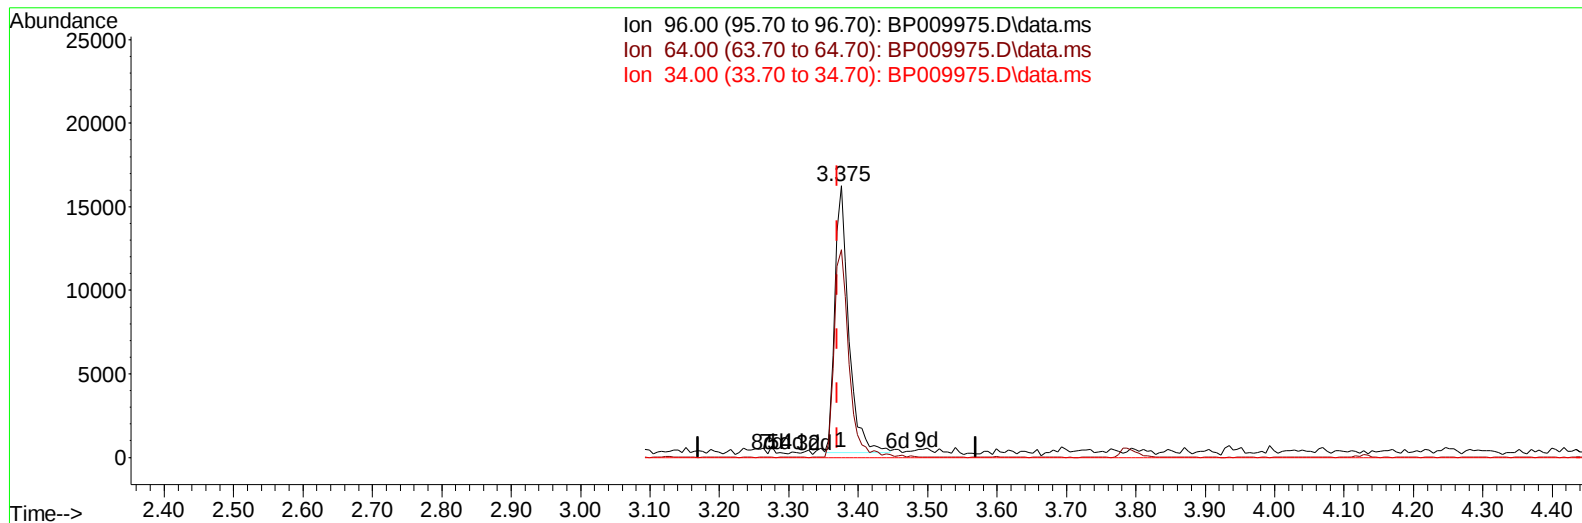

TIC: BP009975.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.006) 5.80 ng/uL m

response 22197

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	76.42#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009975.D
 Acq On : 20 Apr 2022 14:29
 Operator : CG/JU
 Sample : PB144175BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK175

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 01:05:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	170668	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	740830	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	538324	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.334	188	1181537	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.410	240	1062921	20.000	ng/ul	# 0.00
88) Perylene-d12	23.868	264	865573	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	22197m	5.805	ng/uL	0.00
4) Pyridine-d5	3.787	84	289905	27.496	ng/ul	0.00
7) Phenol-d5	7.105	99	383519	25.596	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	264300	29.629	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	318269	28.160	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	332092	26.550	ng/ul	0.00
21) Nitrobenzene-d5	9.105	128	166126	31.096	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	182141	31.098	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	316142	25.794	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	471808	27.028	ng/ul	0.00
46) Dimethylphthalate-d6	13.987	166	1283907	30.362	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1369507	27.337	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	182045	23.738	ng/ul	0.00
60) Fluorene-d10	15.575	176	1057565	29.730	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	179268	25.612	ng/ul	0.00
73) Anthracene-d10	17.428	188	1710232	30.232	ng/ul	0.00
81) Pyrene-d10	19.657	212	2012305	34.664	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.710	264	1387776	30.787	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009975.D
Acq On : 20 Apr 2022 14:29
Operator : CG/JU
Sample : PB144175BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK175

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 01:05:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

