




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009997.D
 Acq On : 21 Apr 2022 03:22
 Operator : CG/JU
 Sample : N2472-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:20:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

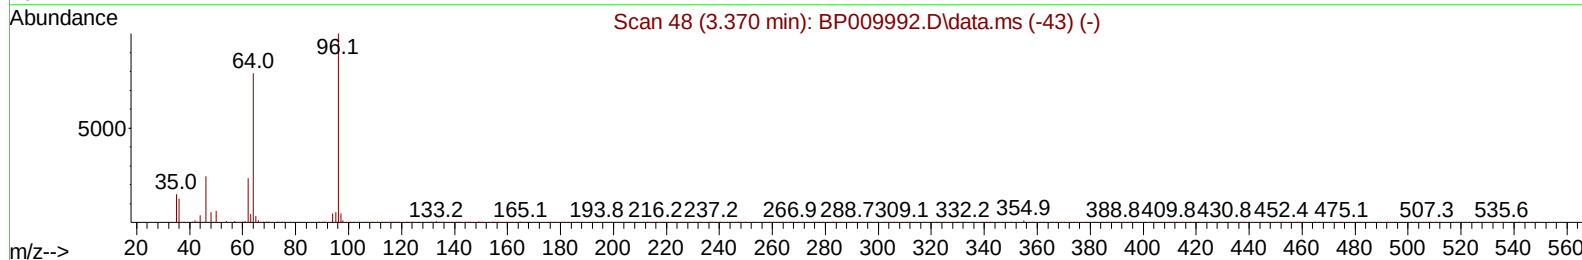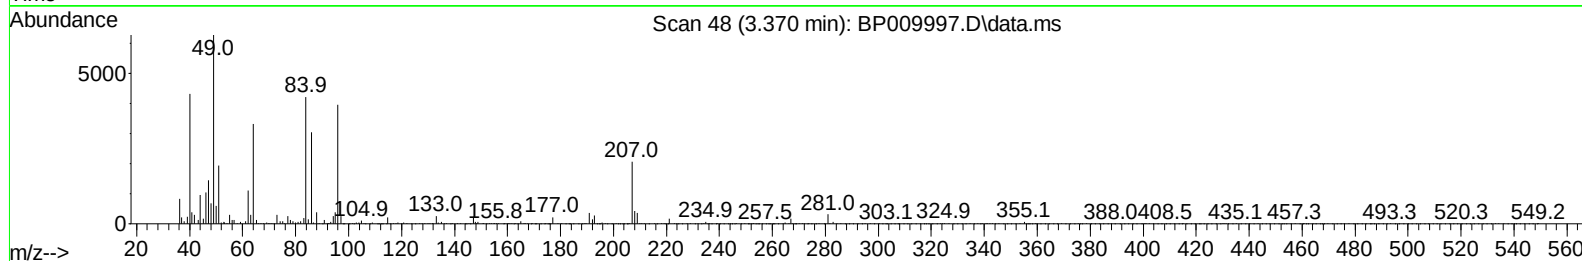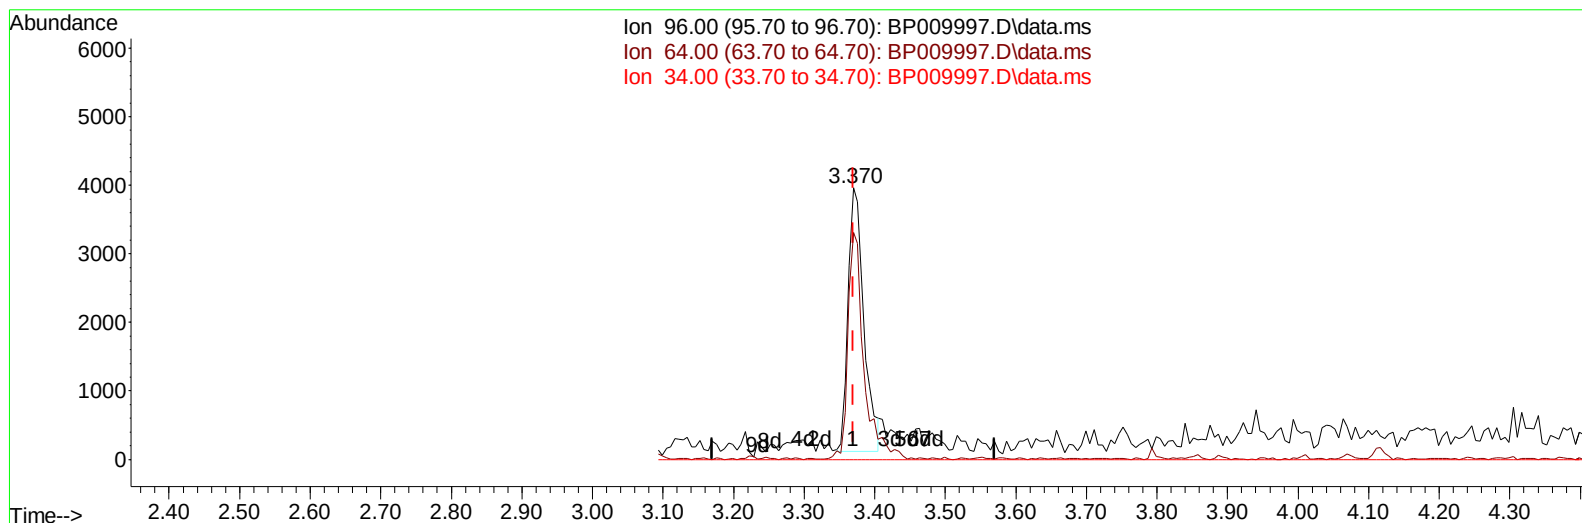

TIC: BP009997.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.370min (-0.000) 2.48 ng/uL

response 6056

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	83.64#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009997.D
Acq On : 21 Apr 2022 03:22
Operator : CG/JU
Sample : N2472-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HX6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:20:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

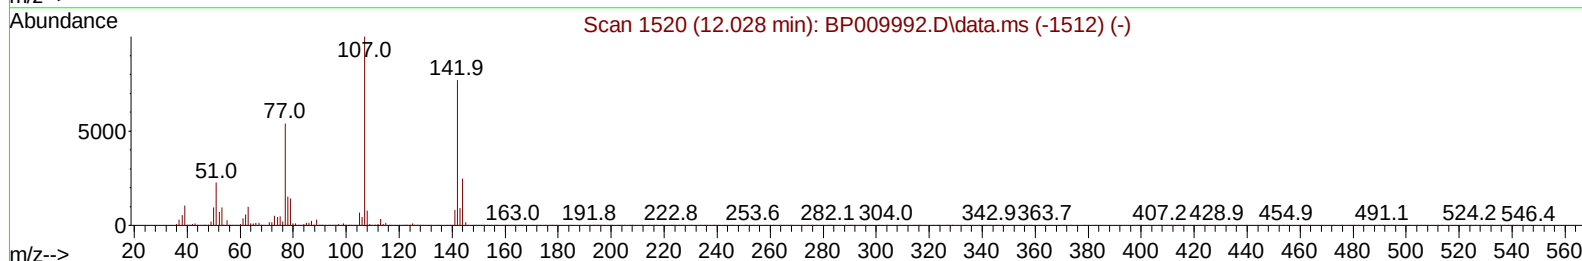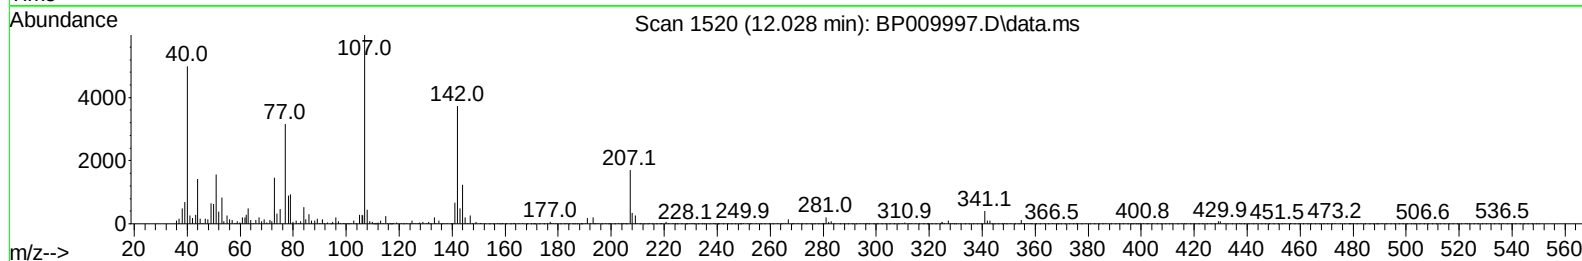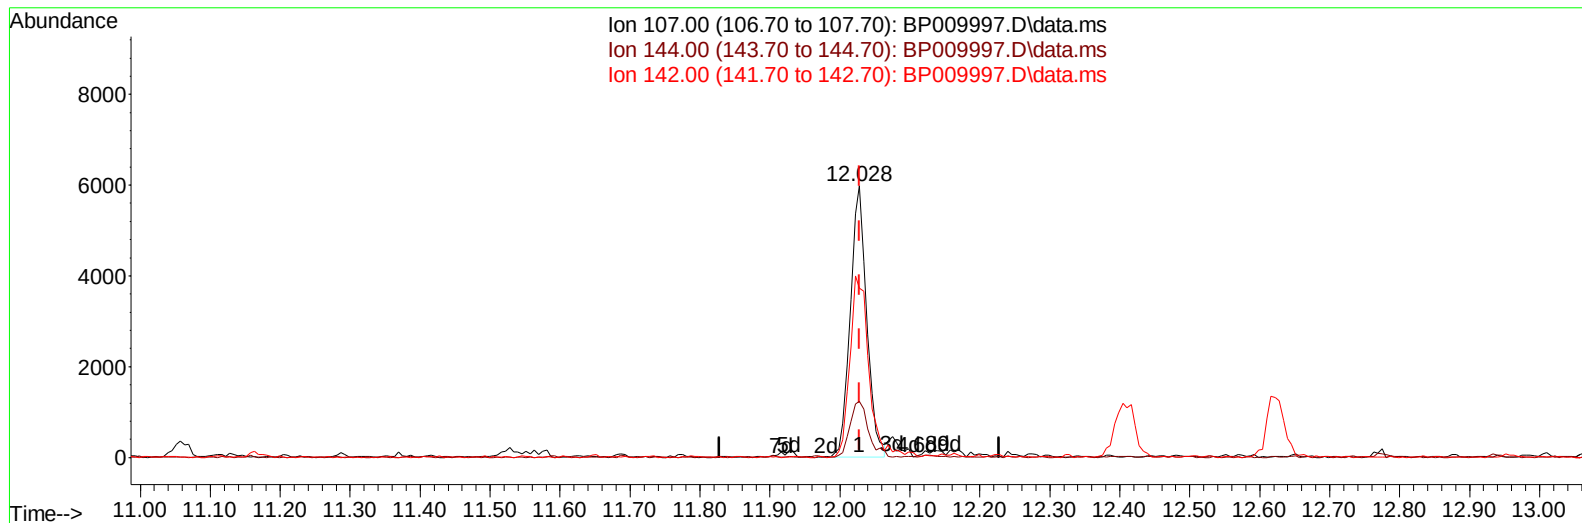

TIC: BP009997.D\data.ms

(35) 4-Chloro-3-methylphenol (C)

12.028min (-0.000) 1.00 ng/ul

response 9652

Ion	Exp%	Act%
107.00	100.00	100.00
144.00	19.80	20.54
142.00	48.60	62.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009997.D
 Acq On : 21 Apr 2022 03:22
 Operator : CG/JU
 Sample : N2472-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:20:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

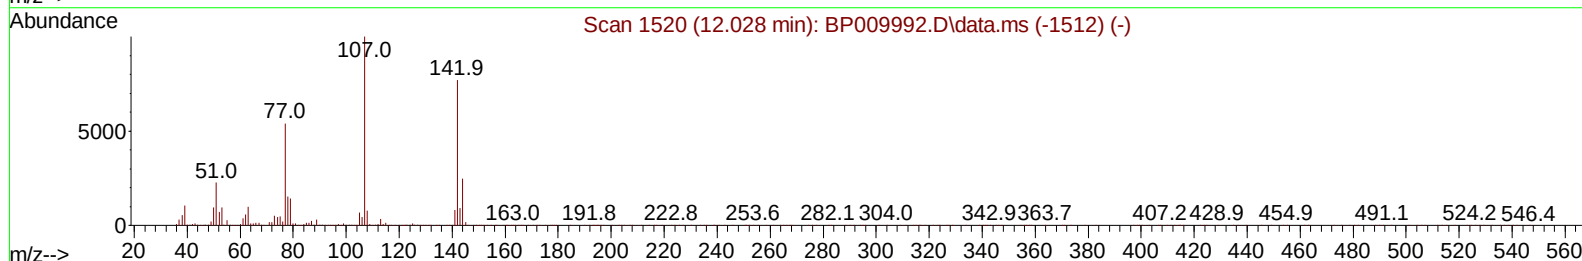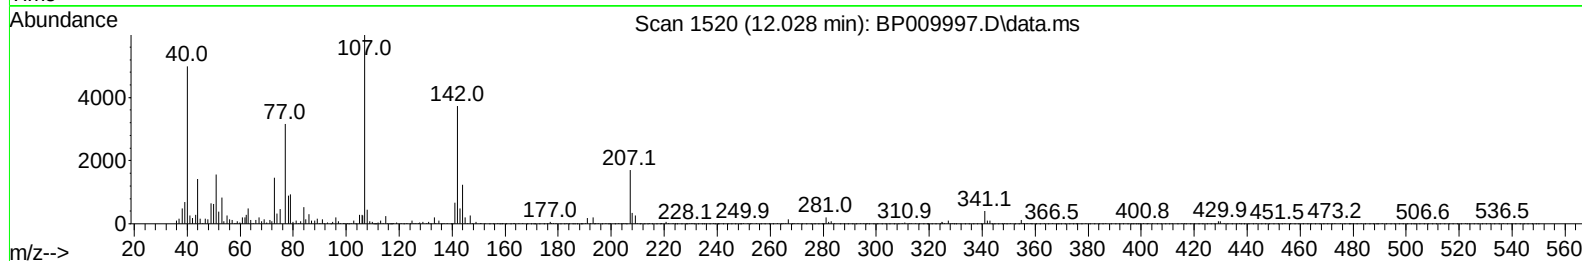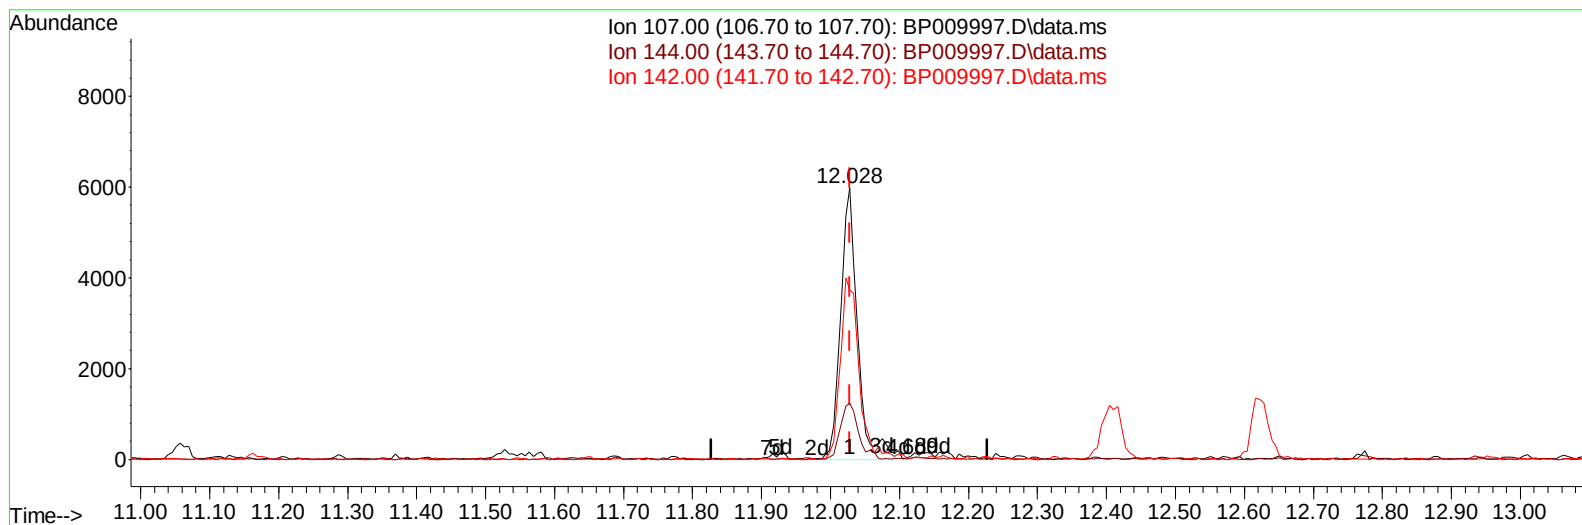

TIC: BP009997.D\data.ms

(35) 4-Chloro-3-methylphenol (C)

12.028min (-0.000) 1.07 ng/ul m

response 10236

Ion	Exp%	Act%
107.00	100.00	100.00
144.00	19.80	20.54
142.00	48.60	62.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009997.D
Acq On : 21 Apr 2022 03:22
Operator : CG/JU
Sample : N2472-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HX6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:20:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

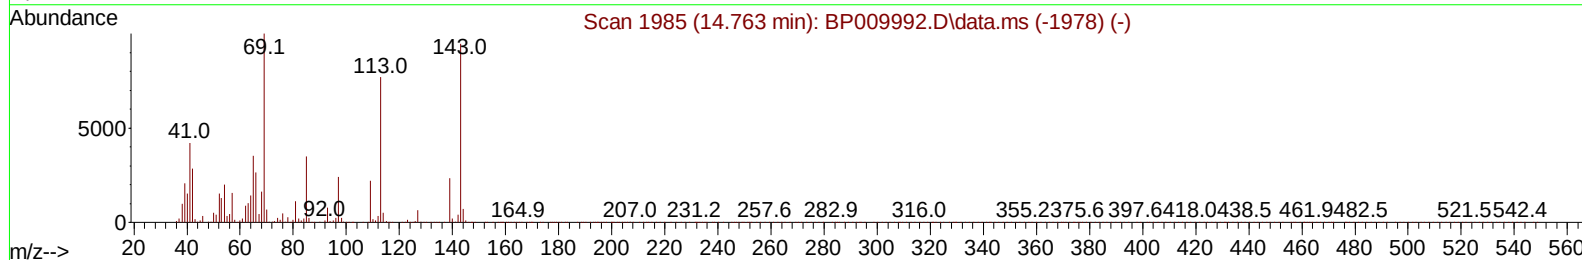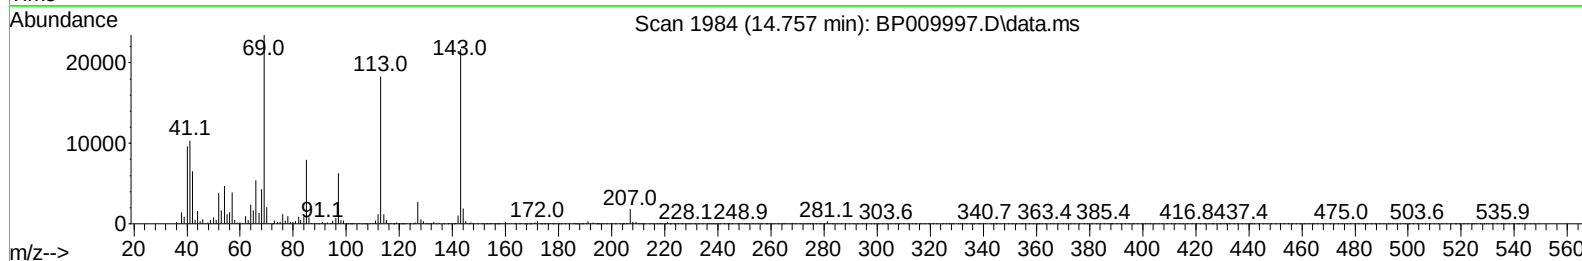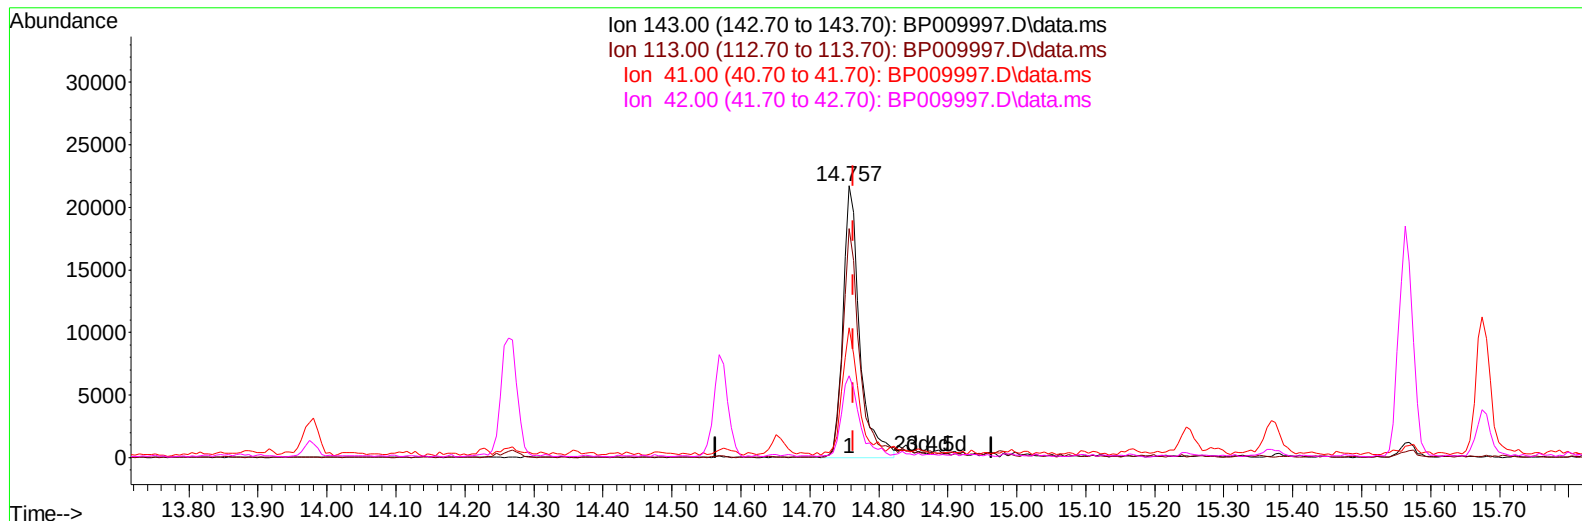

TIC: BP009997.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.006) 7.15 ng/ul

response 36562

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	84.23#
41.00	23.20	47.75#
42.00	18.00	30.13#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009997.D
Acq On : 21 Apr 2022 03:22
Operator : CG/JU
Sample : N2472-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COHX6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:20:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

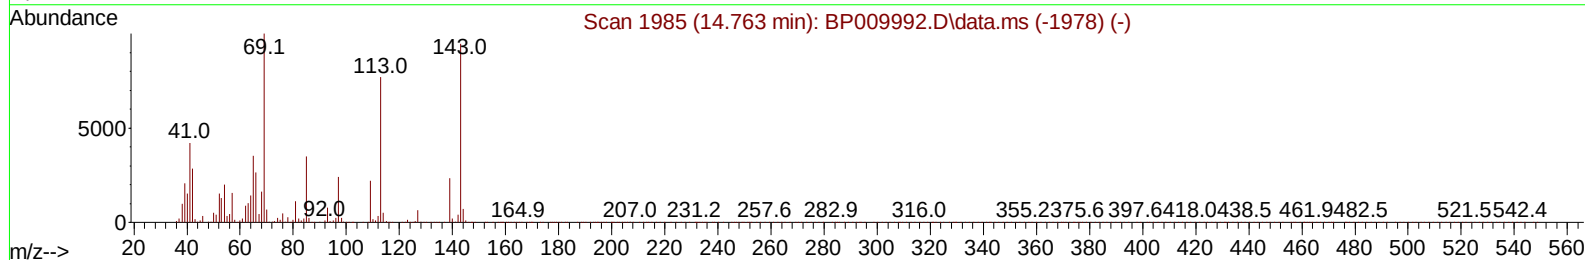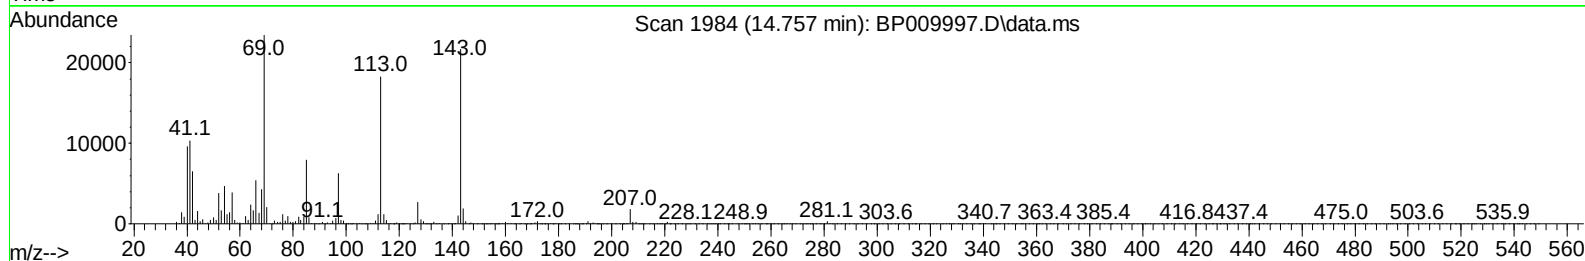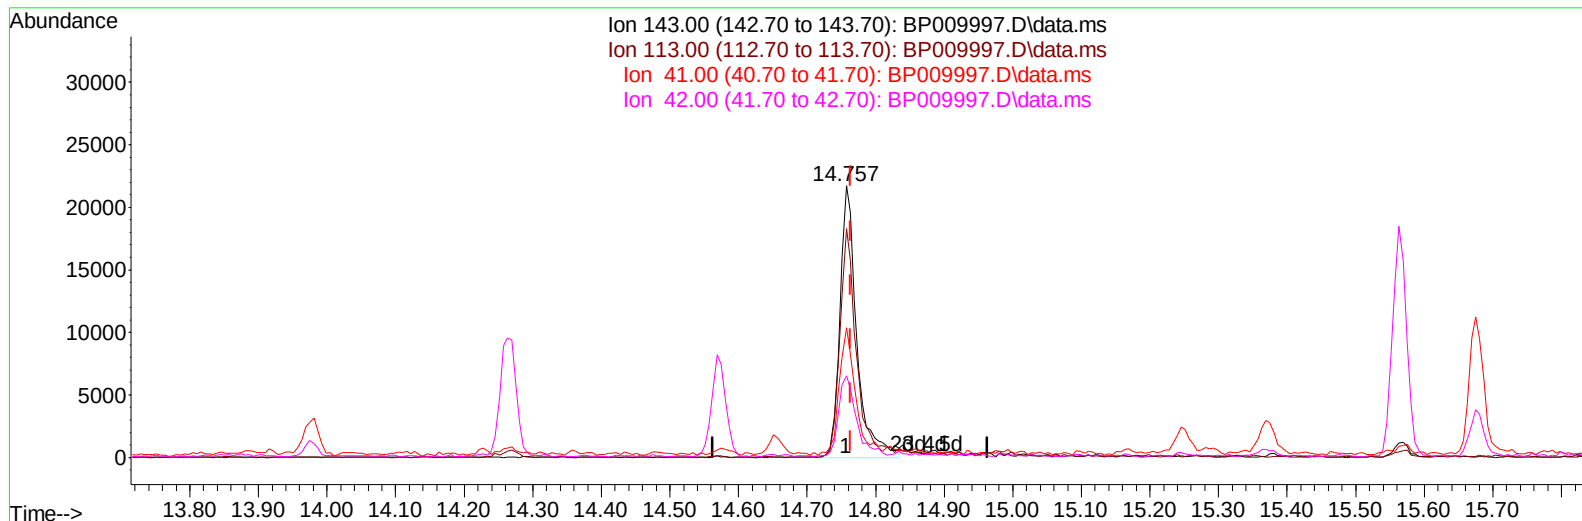

TIC: BP009997.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.006) 7.27 ng/ul m

response 37170

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	84.23#
41.00	23.20	47.75#
42.00	18.00	30.13#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009997.D
 Acq On : 21 Apr 2022 03:22
 Operator : CG/JU
 Sample : N2472-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 05:20:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	108974	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	494280	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	358912	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	803125	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	809529	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	716808	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	6363m	2.606	ng/uL	0.00
4) Pyridine-d5	3.799	84	31389	4.662	ng/ul	0.01
7) Phenol-d5	7.099	99	70395	7.358	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	222294	39.028	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	210840	29.216	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	147688	18.492	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	148977	41.796	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	157379	40.273	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	266125	32.544	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	339312	29.133	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	1097481	38.927	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	1228438	36.779	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	37170m	7.270	ng/ul	0.00
60) Fluorene-d10	15.563	176	966634	40.757	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	180831	38.008	ng/ul	-0.01
73) Anthracene-d10	17.422	188	1791863	46.599	ng/ul	0.00
81) Pyrene-d10	19.651	212	2201706	49.798	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1801000	48.247	ng/ul	-0.01
Target Compounds						
35) 4-Chloro-3-methylphenol	12.028	107	10236m	1.066	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009997.D
Acq On : 21 Apr 2022 03:22
Operator : CG/JU
Sample : N2472-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HX6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 05:20:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

