




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009998.D
 Acq On : 21 Apr 2022 03:56
 Operator : CG/JU
 Sample : N2472-05
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J01

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:20:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

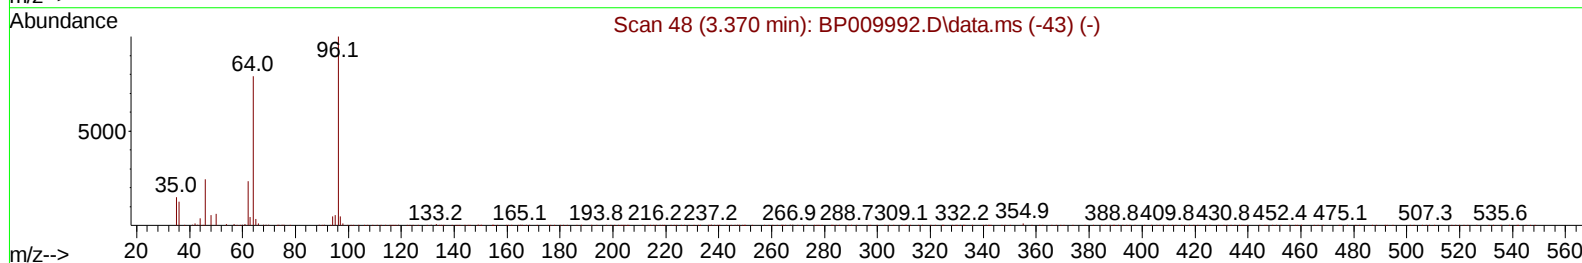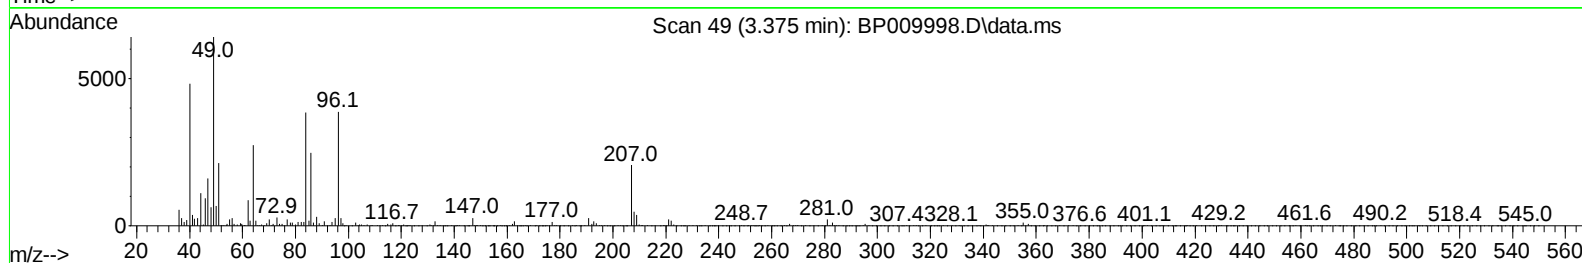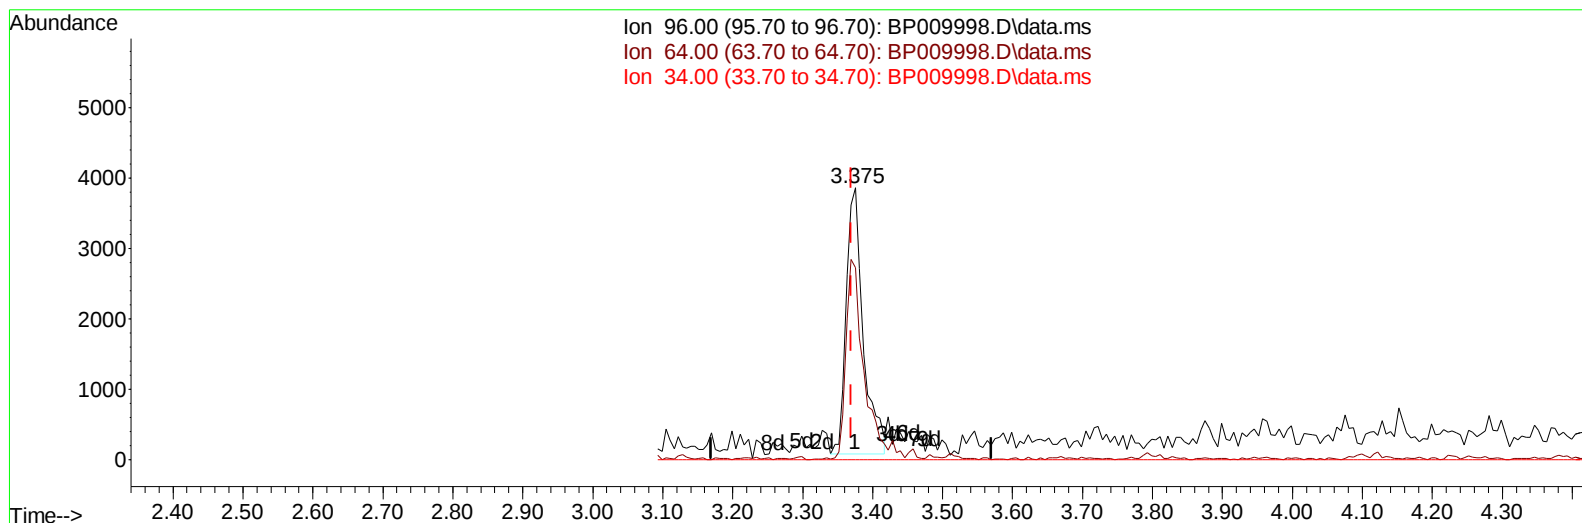

TIC: BP009998.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.006) 2.48 ng/uL

response 6314

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	70.72#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009998.D
 Acq On : 21 Apr 2022 03:56
 Operator : CG/JU
 Sample : N2472-05
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J01

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:20:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

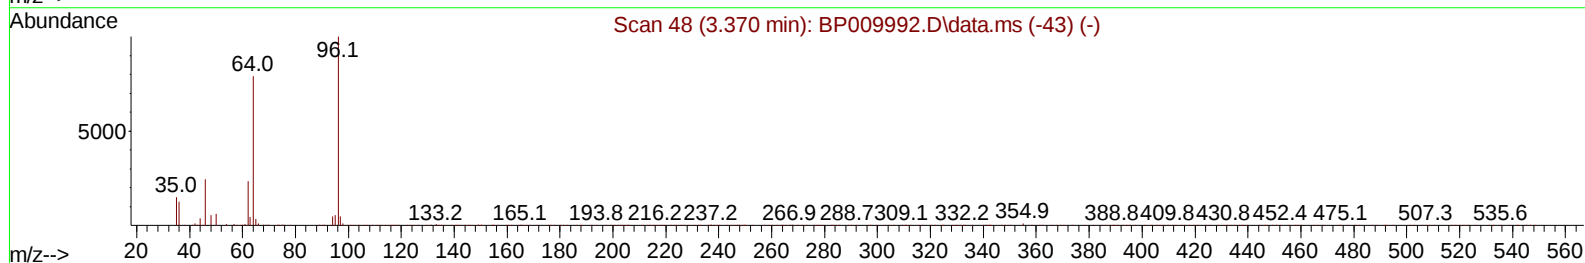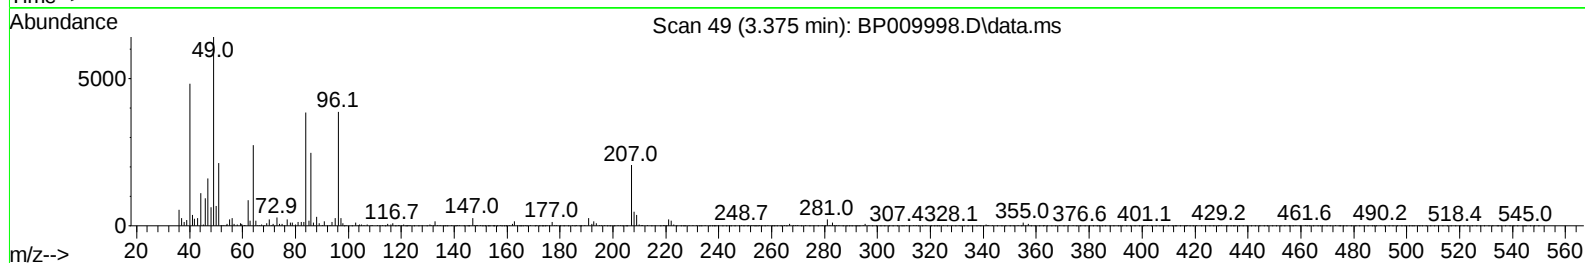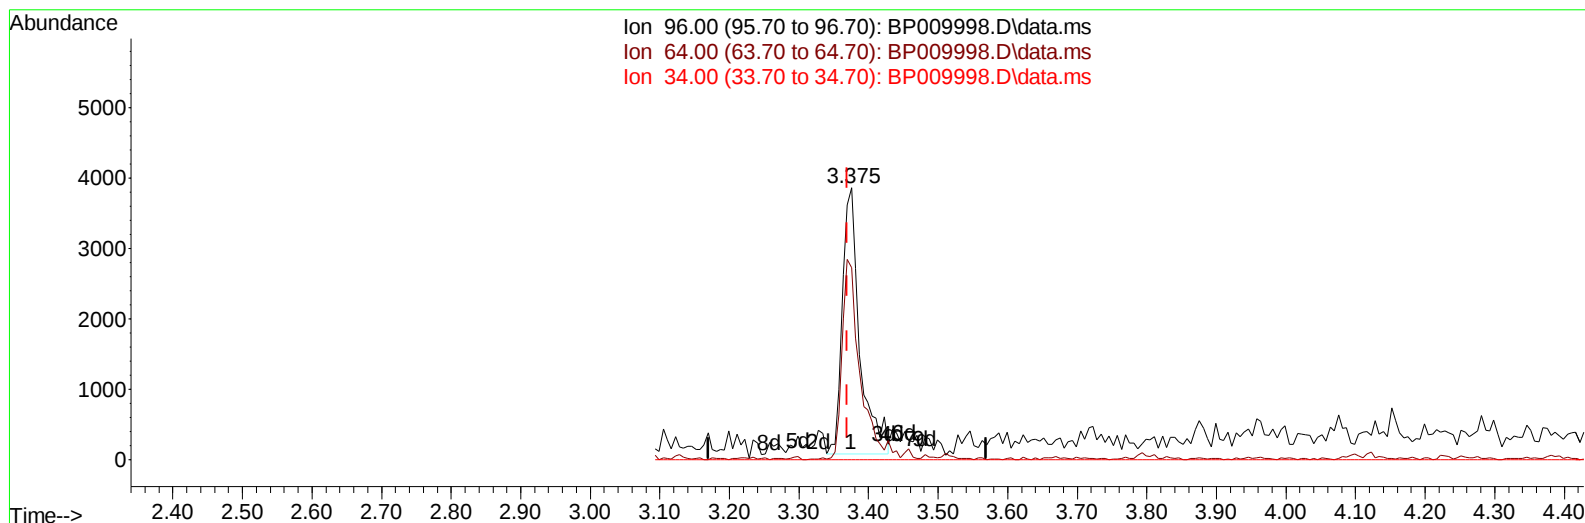

TIC: BP009998.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.006) 2.59 ng/uL m

response 6578

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	70.72#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009998.D
Acq On : 21 Apr 2022 03:56
Operator : CG/JU
Sample : N2472-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J01

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:20:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

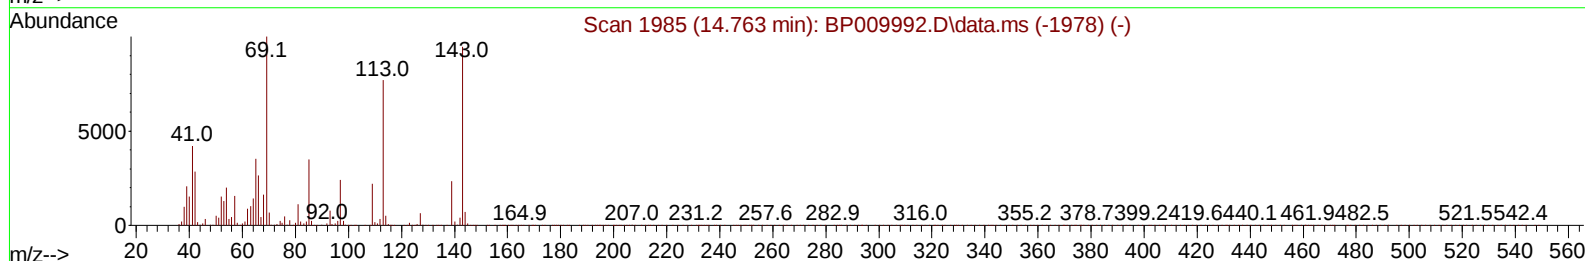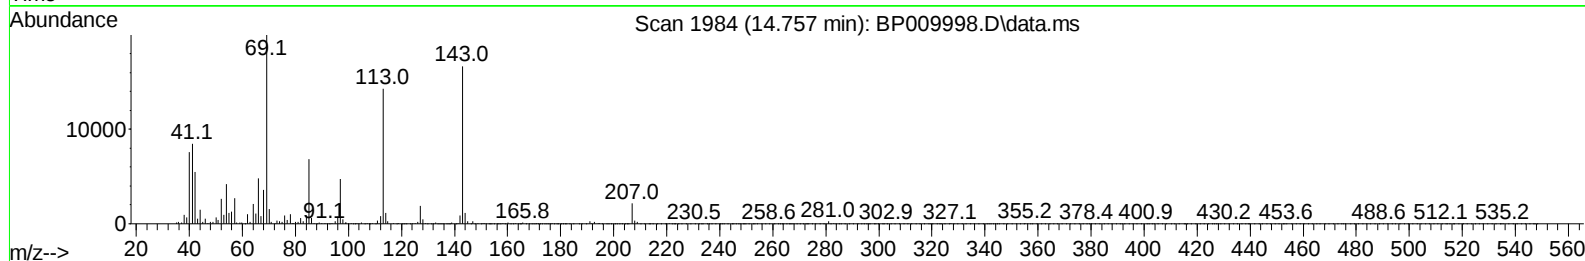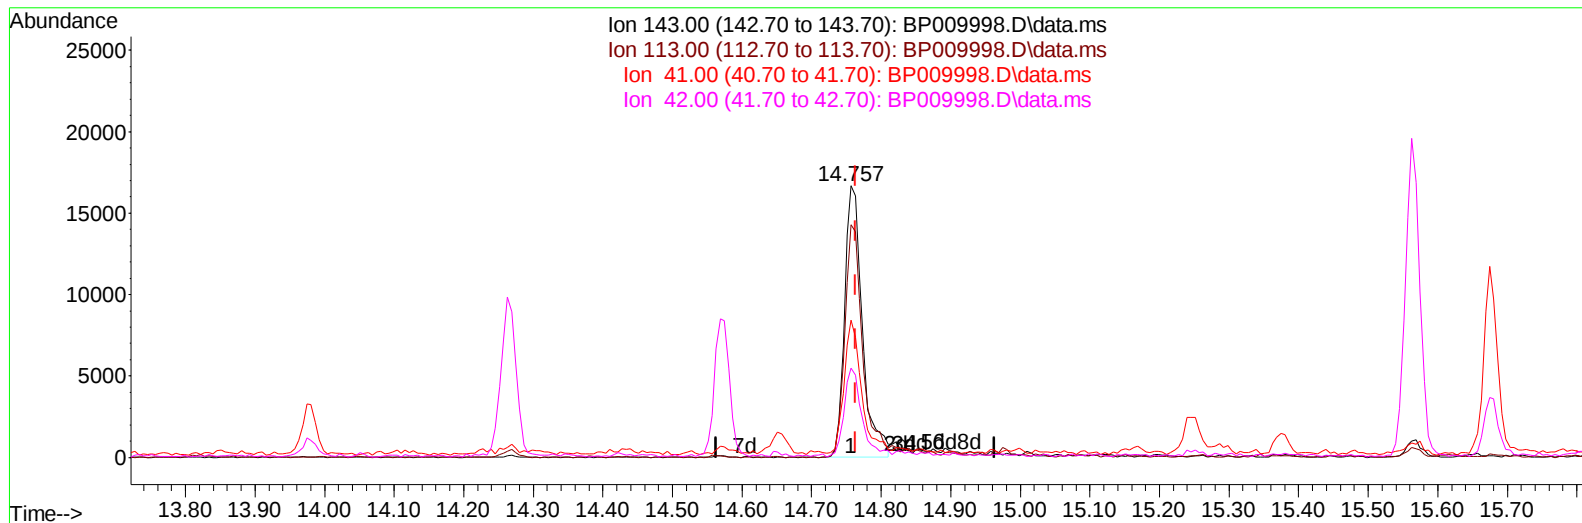

TIC: BP009998.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.006) 5.81 ng/u1

response 29699

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	85.78#
41.00	23.20	50.62#
42.00	18.00	32.80#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009998.D
Acq On : 21 Apr 2022 03:56
Operator : CG/JU
Sample : N2472-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J01

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 05:20:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

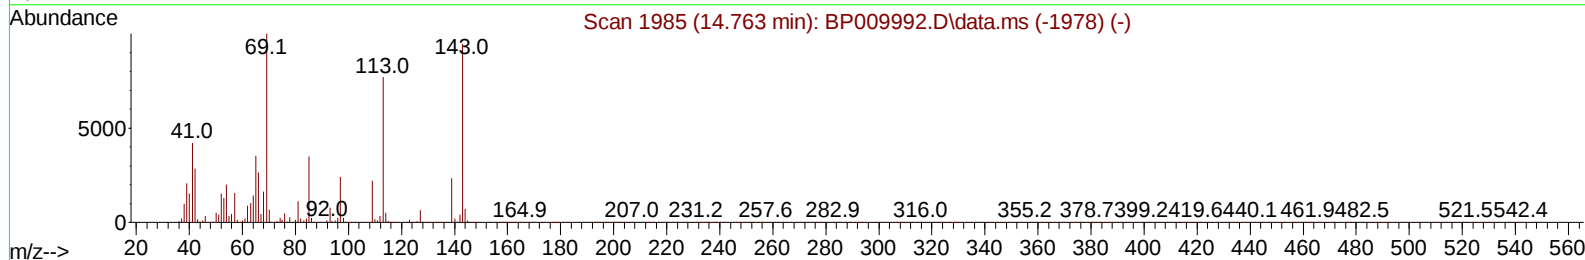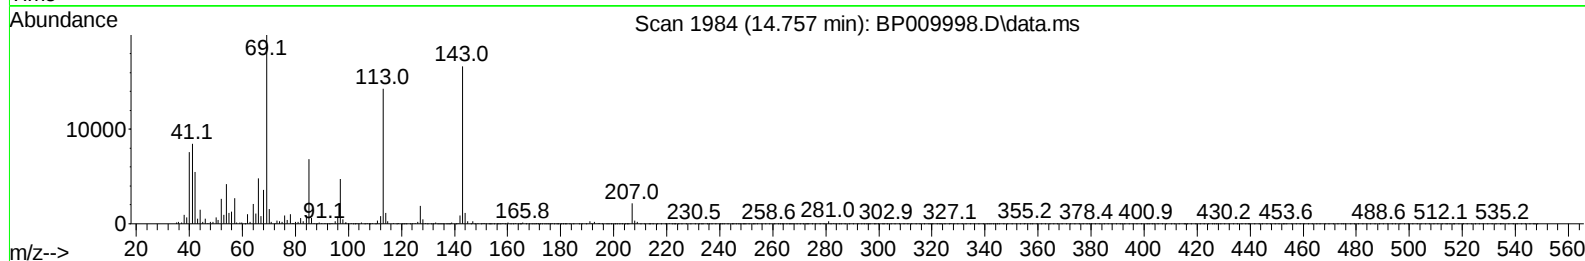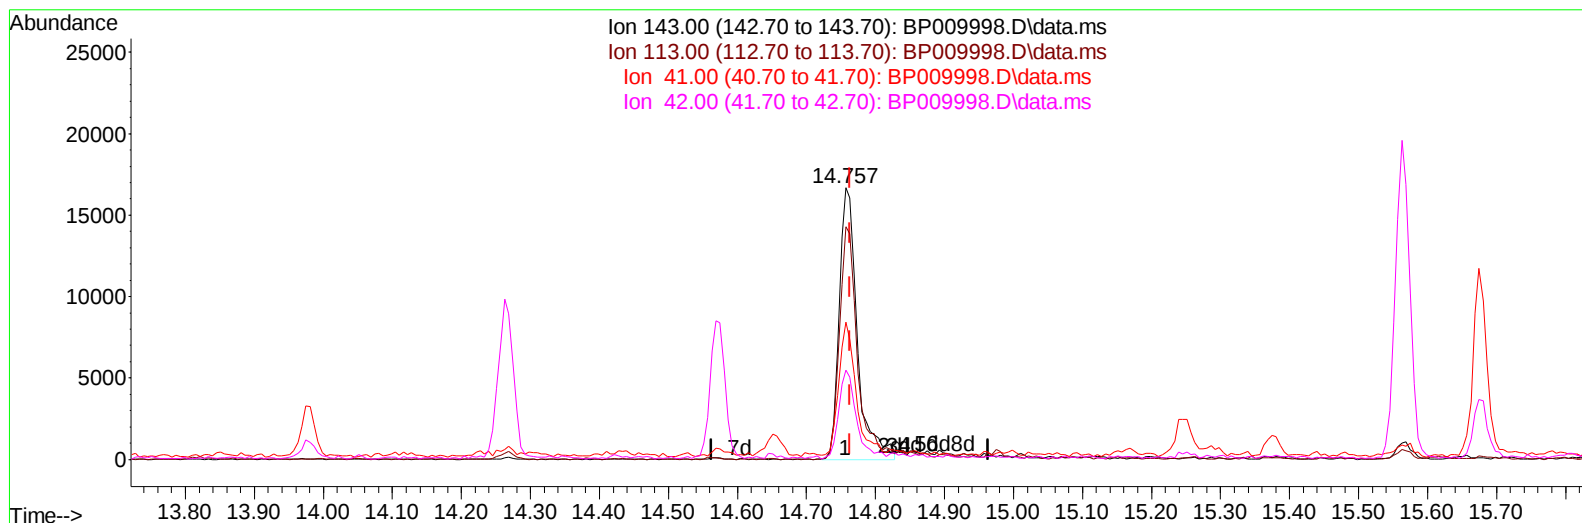

TIC: BP009998.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.757min (-0.006) 5.97 ng/u1 m****response 30517**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	85.78#
41.00	23.20	50.62#
42.00	18.00	32.80#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009998.D
 Acq On : 21 Apr 2022 03:56
 Operator : CG/JU
 Sample : N2472-05
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J01

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:20:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.940	152		113514	20.000	ng/ul	0.00
20) Naphthalene-d8	10.745	136		497081	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164		359110	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188		805253	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240		825124	20.000	ng/ul	# 0.00
88) Perylene-d12	23.851	264		756421	20.000	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.375	96		6578m	2.586	ng/uL	0.00
4) Pyridine-d5	3.793	84		36129	5.152	ng/ul	0.00
7) Phenol-d5	7.099	99		64332	6.455	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67		223462	37.664	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132		206773	27.506	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113		137523	16.530	ng/ul	0.00
21) Nitrobenzene-d5	9.098	128		147229	41.073	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143		152908	38.908	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165		254826	30.987	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131		342739	29.262	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166		1163915	41.261	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160		1221280	36.544	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143		30517m	5.965	ng/ul	0.00
60) Fluorene-d10	15.563	176		998317	42.070	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200		166523	34.908	ng/ul	0.00
73) Anthracene-d10	17.422	188		1683387	43.662	ng/ul	0.00
81) Pyrene-d10	19.651	212		2076066	46.069	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264		1784300	45.296	ng/ul	-0.01
Target Compounds							
35) 4-Chloro-3-methylphenol	12.028	107		19338	2.002	ng/ul#	Qvalue 72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009998.D
Acq On : 21 Apr 2022 03:56
Operator : CG/JU
Sample : N2472-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J01

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 05:20:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

