




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009999.D
Acq On : 21 Apr 2022 04:30
Operator : CG/JU
Sample : N2472-07
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J46

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 05:21:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

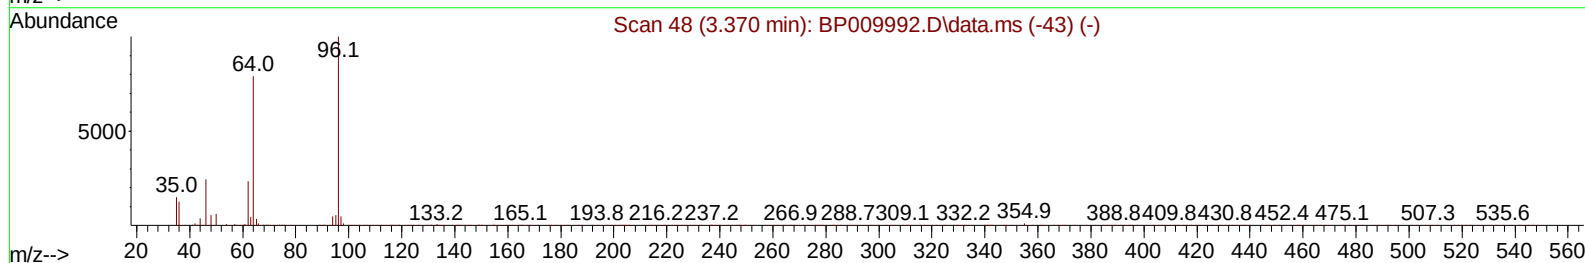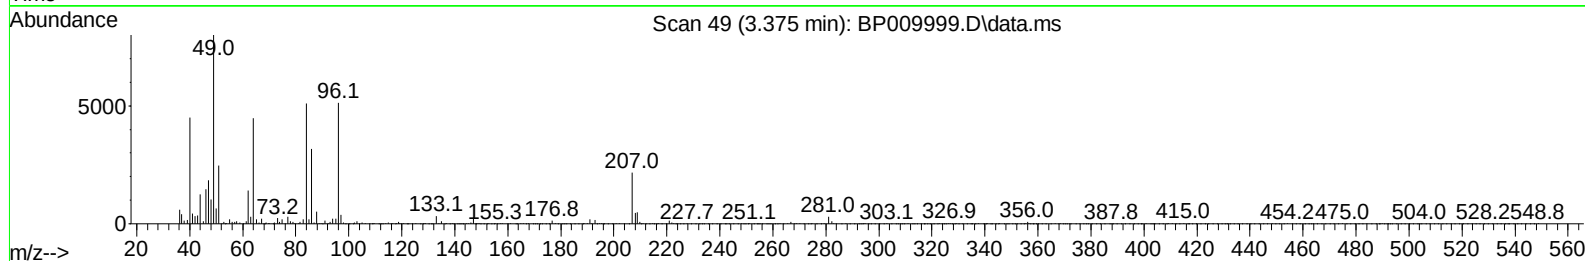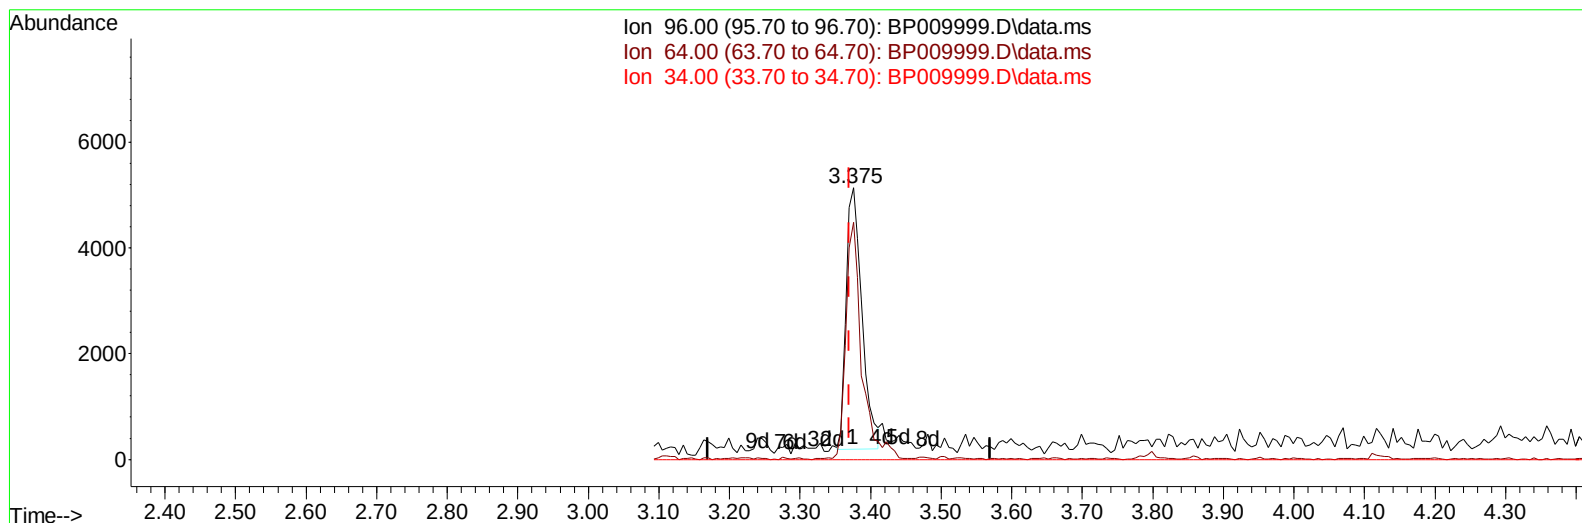

TIC: BP009999.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.006) 2.18 ng/uL

response 7817

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	87.37#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009999.D
 Acq On : 21 Apr 2022 04:30
 Operator : CG/JU
 Sample : N2472-07
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J46

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:21:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

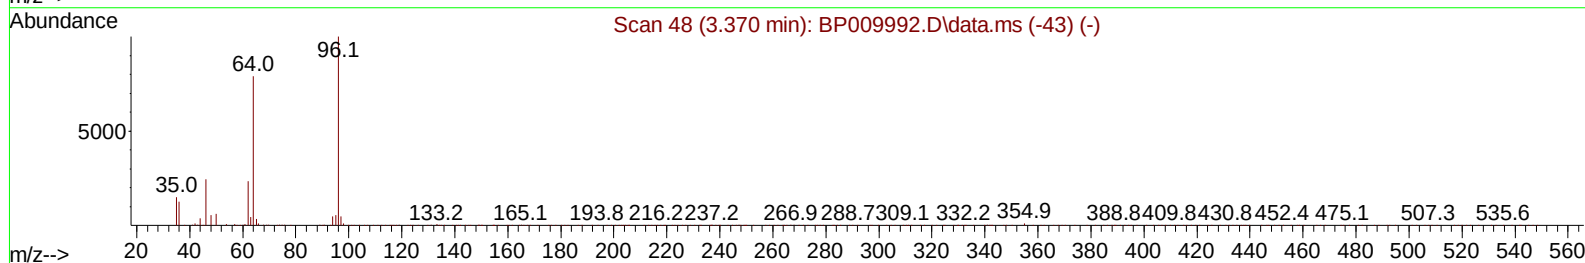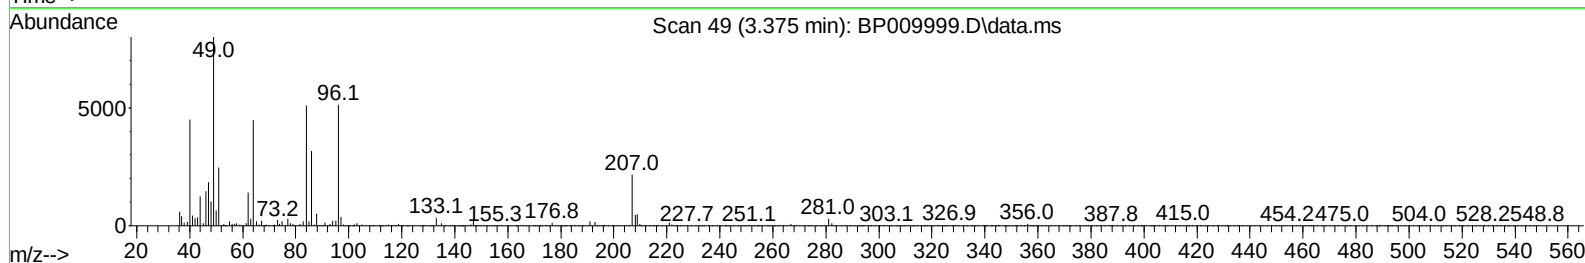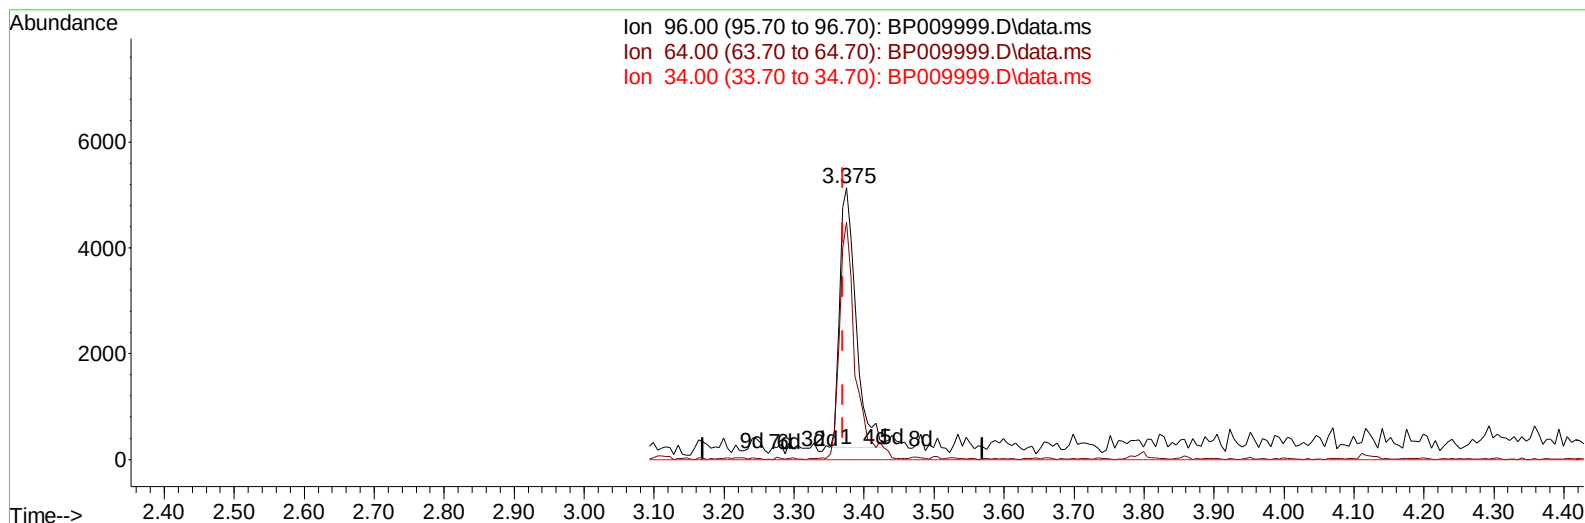

TIC: BP009999.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.006) 2.23 ng/uL m

response 7984

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	87.37#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009999.D
 Acq On : 21 Apr 2022 04:30
 Operator : CG/JU
 Sample : N2472-07
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J46

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:21:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

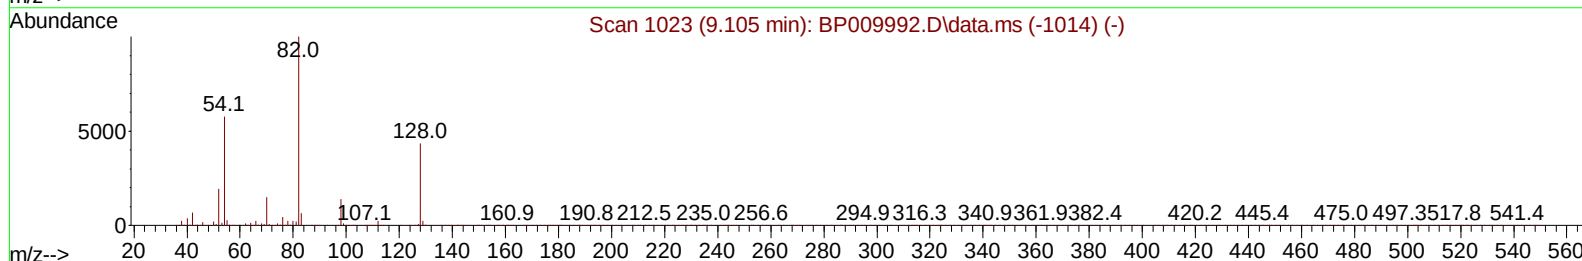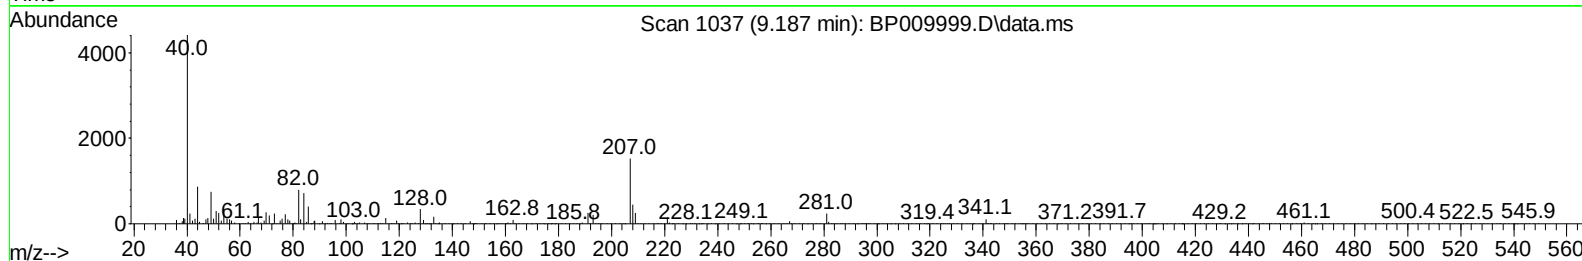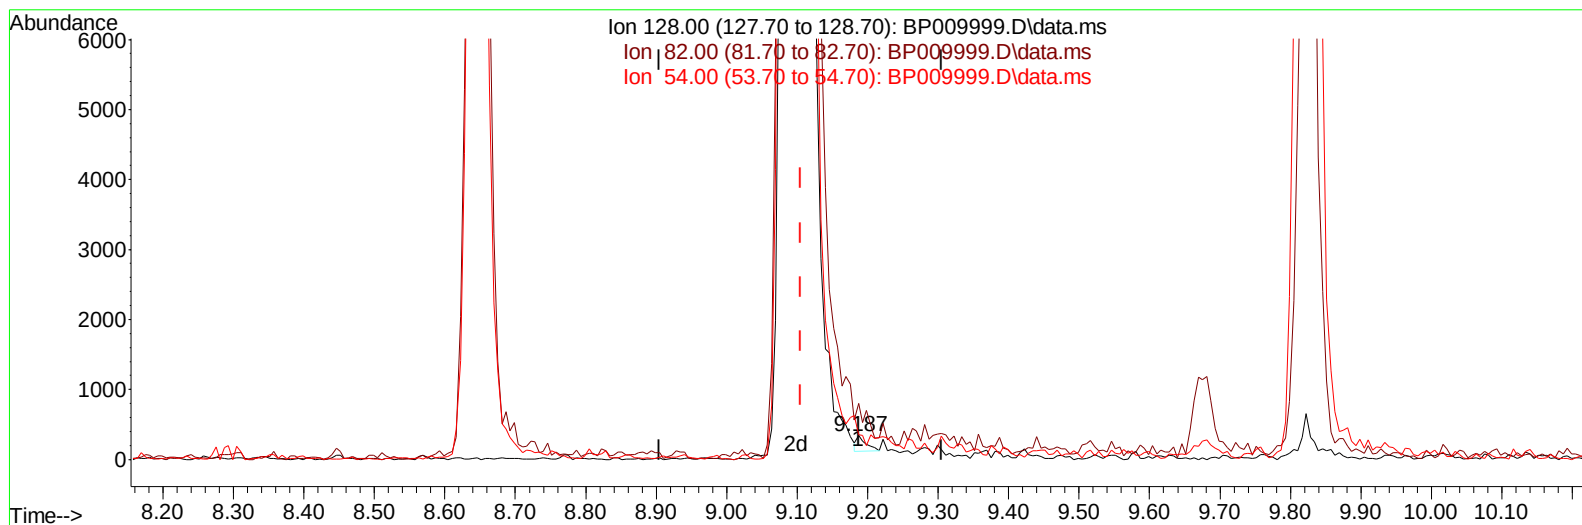

TIC: BP009999.D\data.ms

(21) Nitrobenzene-d5 (S)

9.187min (+ 0.082) 0.04 ng/u1

response	211	
Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	233.24
54.00	120.20	103.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009999.D
 Acq On : 21 Apr 2022 04:30
 Operator : CG/JU
 Sample : N2472-07
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J46

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:21:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

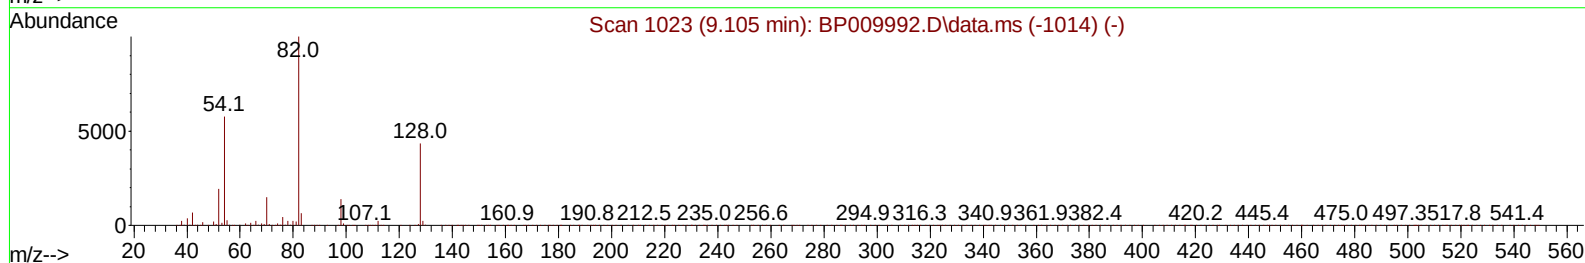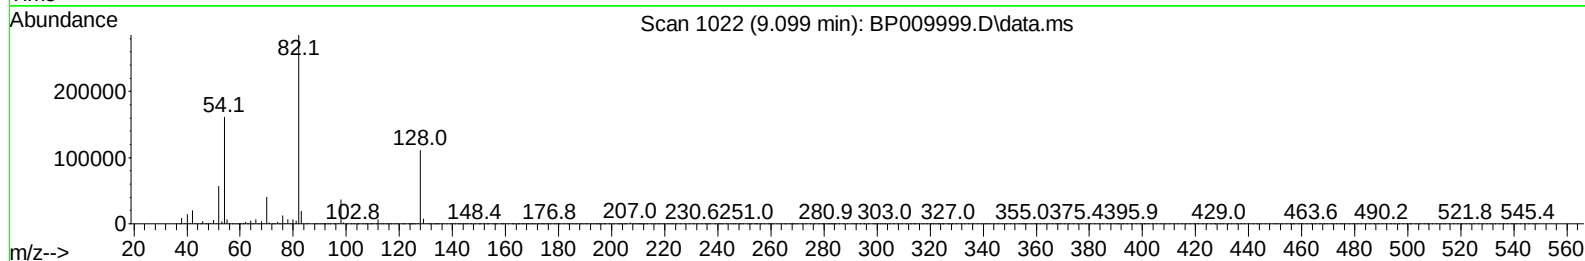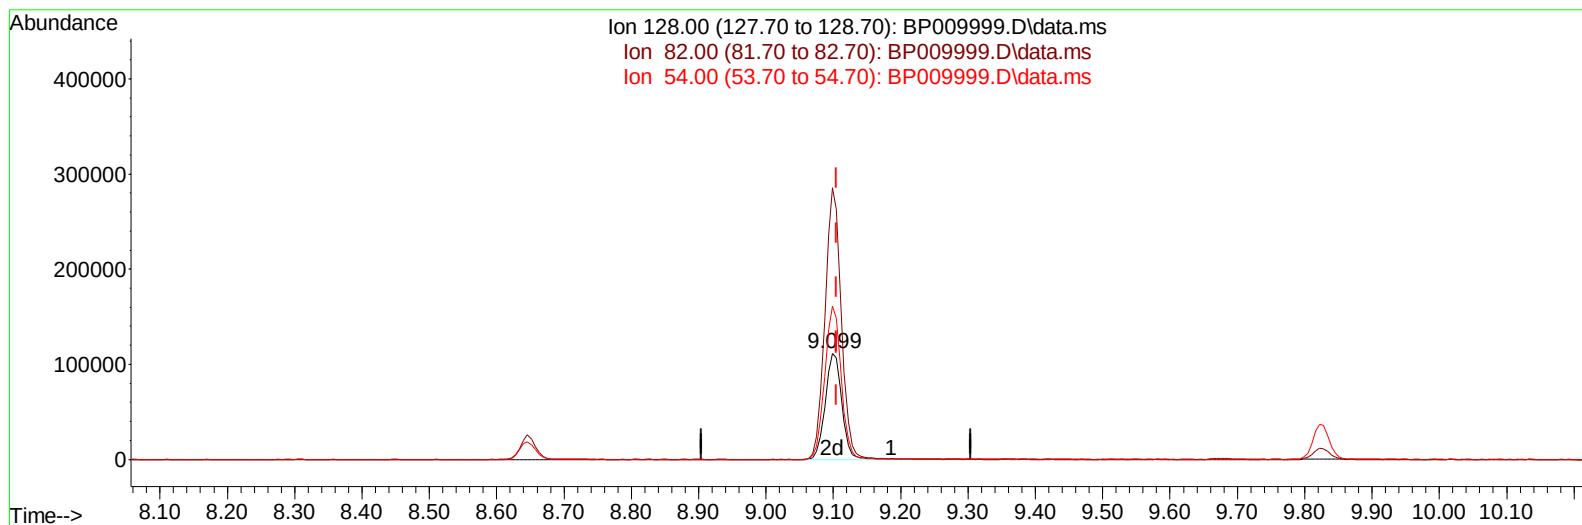

TIC: BP009999.D\data.ms

(21) Nitrobenzene-d5 (S)

9.099min (-0.006) 36.90 ng/ul m

response 192148

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	256.21
54.00	120.20	144.80#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009999.D
 Acq On : 21 Apr 2022 04:30
 Operator : CG/JU
 Sample : N2472-07
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J46

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:21:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	159764	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	722049	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	530507	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1178225	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	1088192	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	964130	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	7984m	2.230	ng/uL	0.00
4) Pyridine-d5	3.793	84	77764	7.879	ng/ul	0.00
7) Phenol-d5	7.099	99	86561	6.171	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	287111	34.383	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	268363	25.365	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	183991	15.714	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	192148m	36.903	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	207495	36.348	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	343493	28.755	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	473008	27.801	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	1528520	36.680	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1644593	33.312	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	39138	5.179	ng/ul	0.00
60) Fluorene-d10	15.563	176	1302542	37.156	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	249495	35.745	ng/ul	0.00
73) Anthracene-d10	17.422	188	2186330	38.756	ng/ul	0.00
81) Pyrene-d10	19.651	212	2600746	43.760	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	2003897	39.912	ng/ul	-0.01
Target Compounds						
75) 1,2,3,4-Tetrachloroben...	13.375	216	32646	1.916	ng/uL	Qvalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009999.D
Acq On : 21 Apr 2022 04:30
Operator : CG/JU
Sample : N2472-07
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J46

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 05:21:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

