




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP010000.D
 Acq On : 21 Apr 2022 05:03
 Operator : CG/JU
 Sample : N2472-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J00

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:51:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

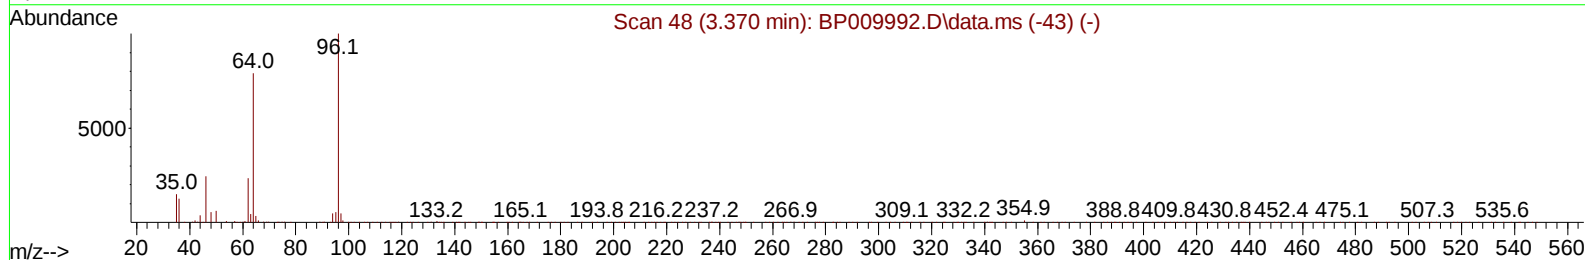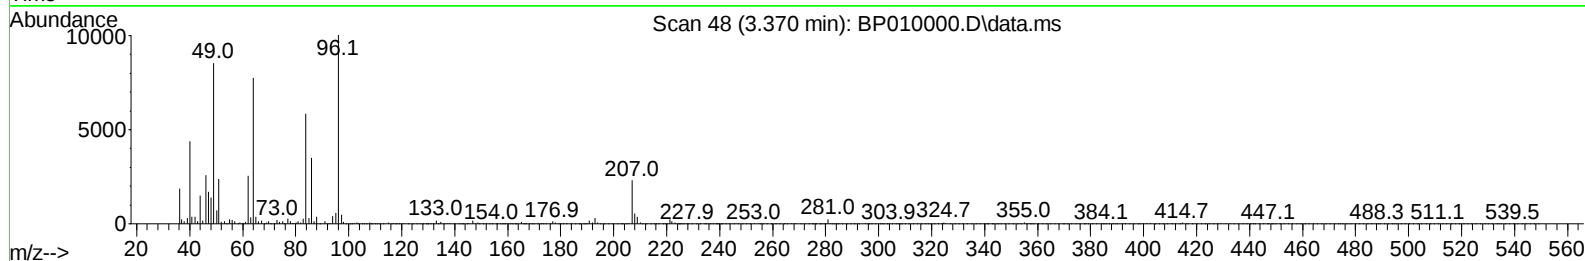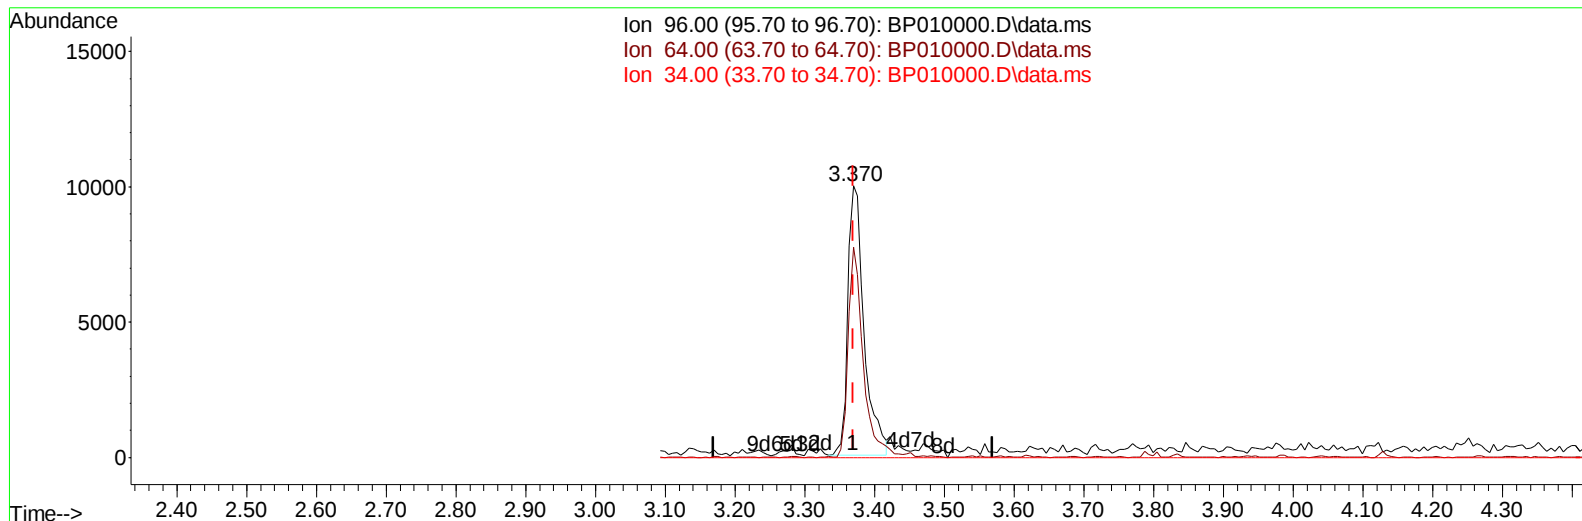

TIC: BP010000.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.370min (-0.000) 4.79 ng/uL

response 16089

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	77.39#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP010000.D
 Acq On : 21 Apr 2022 05:03
 Operator : CG/JU
 Sample : N2472-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J00

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:51:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

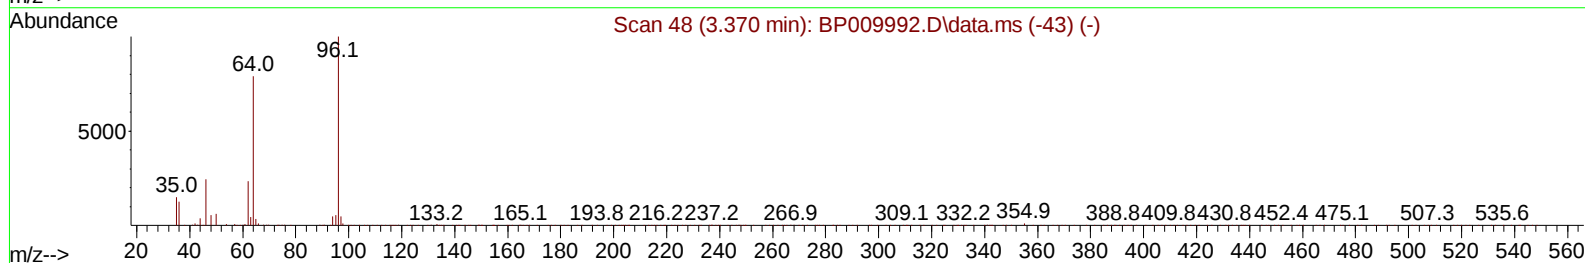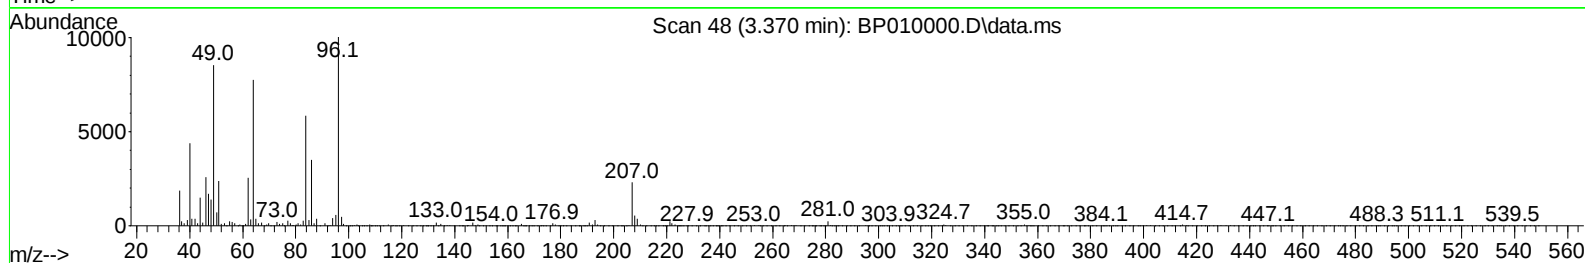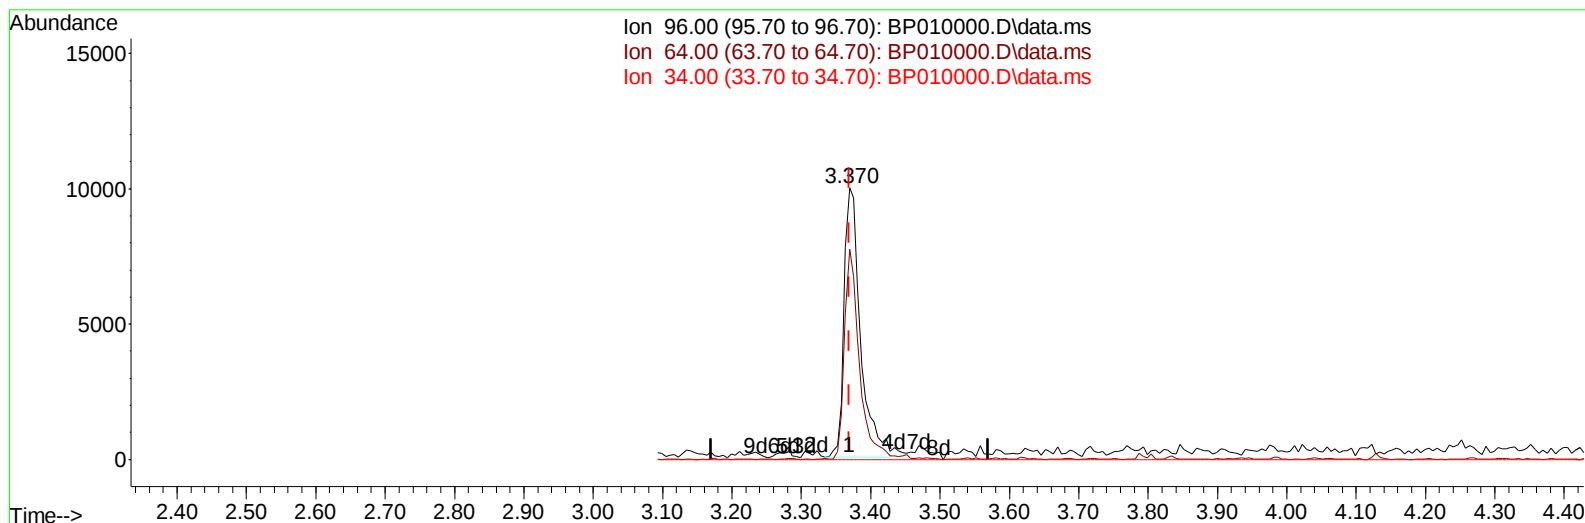

TIC: BP010000.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.370min (-0.000) 4.91 ng/uL m

response 16505

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	77.39#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP010000.D
 Acq On : 21 Apr 2022 05:03
 Operator : CG/JU
 Sample : N2472-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J00

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:51:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

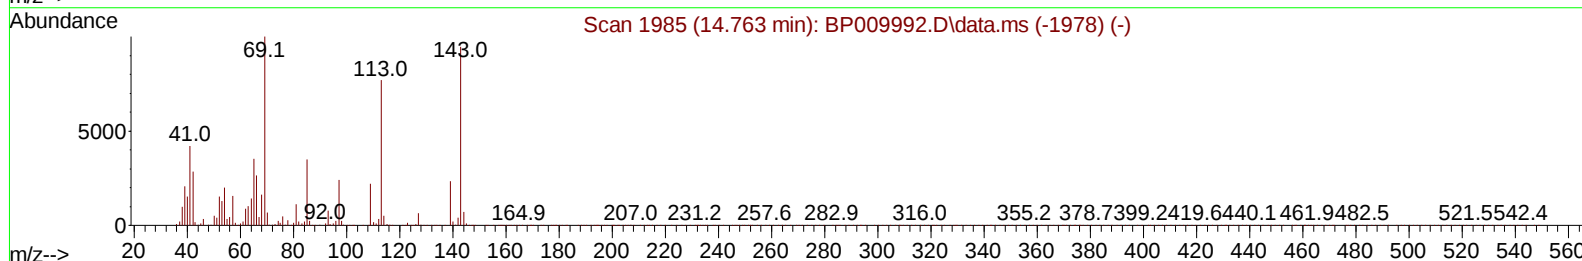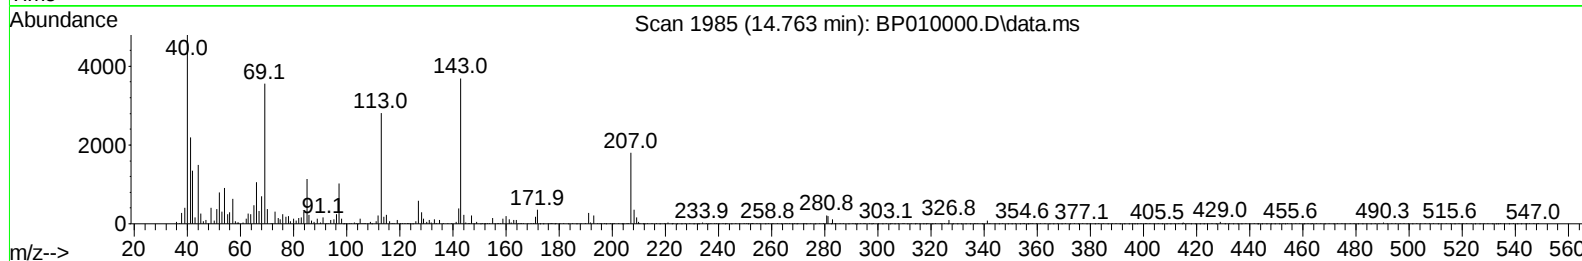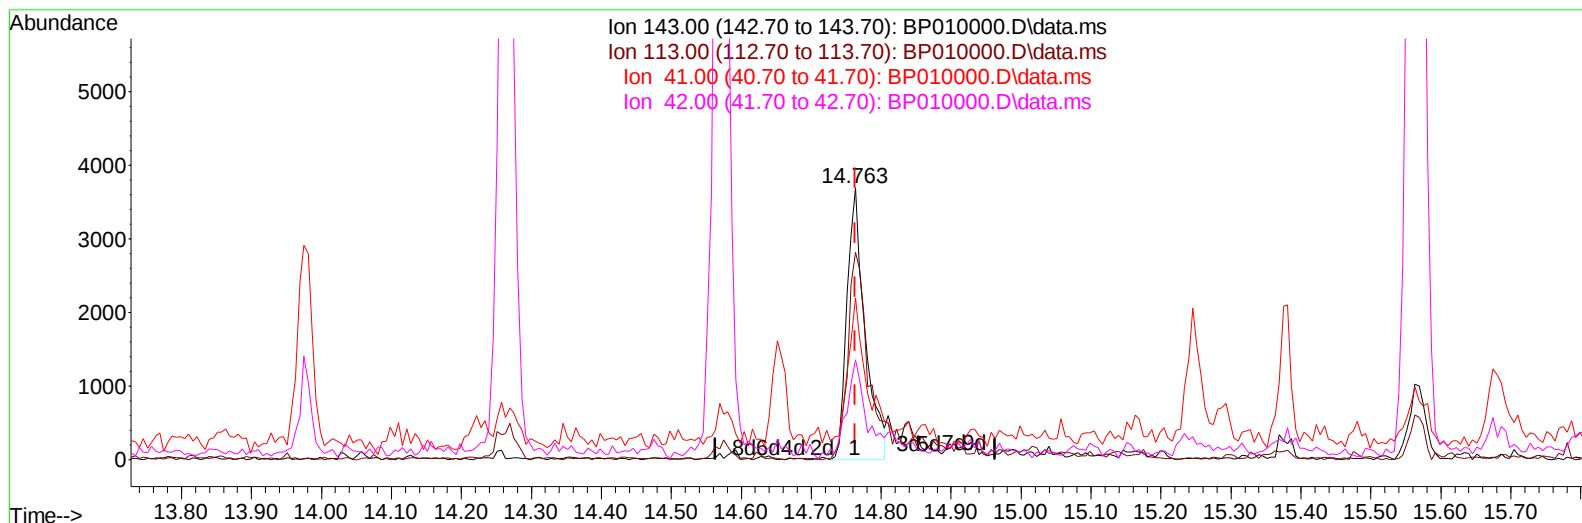

TIC: BP010000.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.000) 0.90 ng/u1

response 6596

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	76.23#
41.00	23.20	59.49#
42.00	18.00	36.75#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP010000.D
Acq On : 21 Apr 2022 05:03
Operator : CG/JU
Sample : N2472-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J00

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:51:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

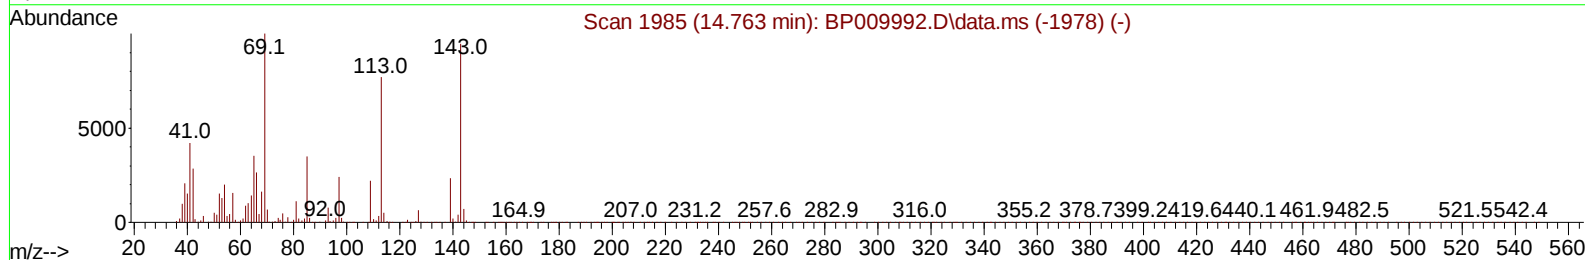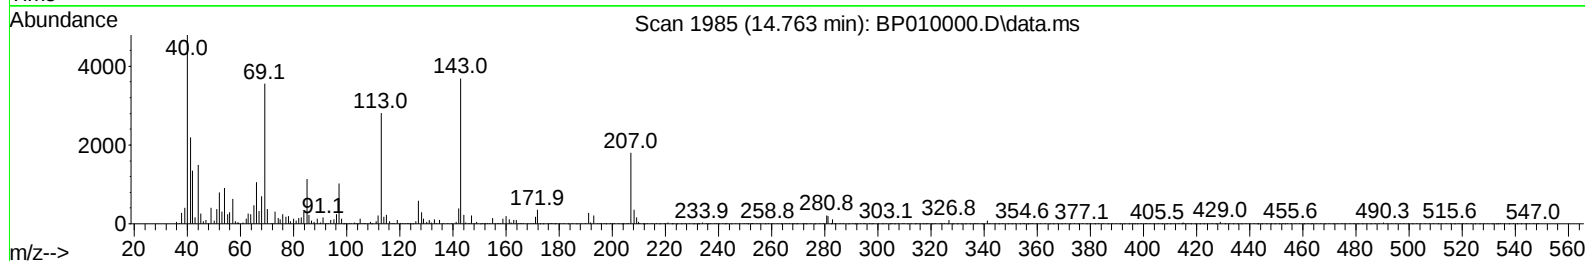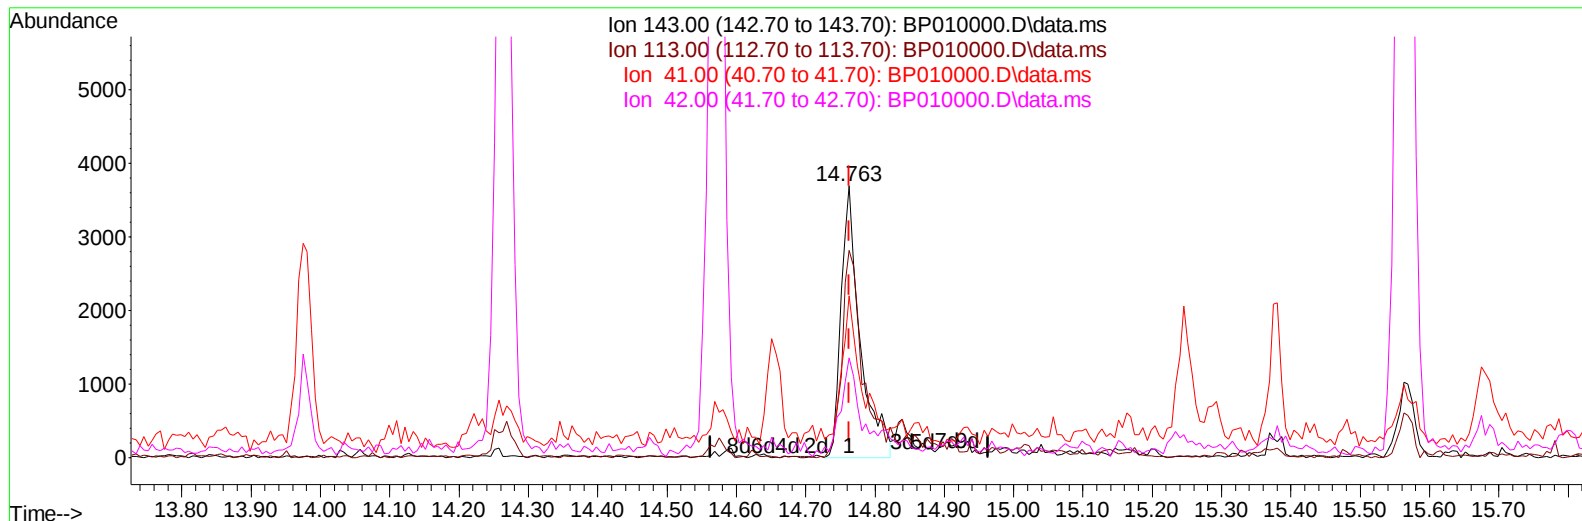

TIC: BP010000.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.000) 0.96 ng/ul m

response 7011

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	76.23#
41.00	23.20	59.49#
42.00	18.00	36.75#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP010000.D
Acq On : 21 Apr 2022 05:03
Operator : CG/JU
Sample : N2472-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J00

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:51:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

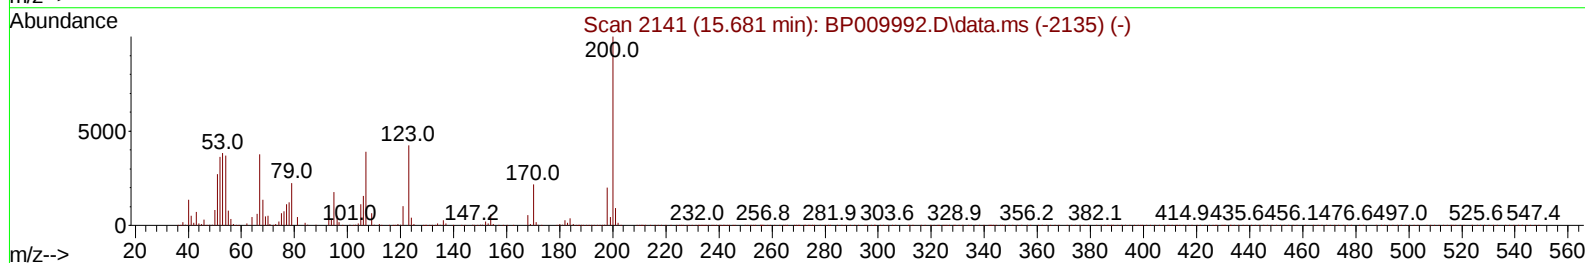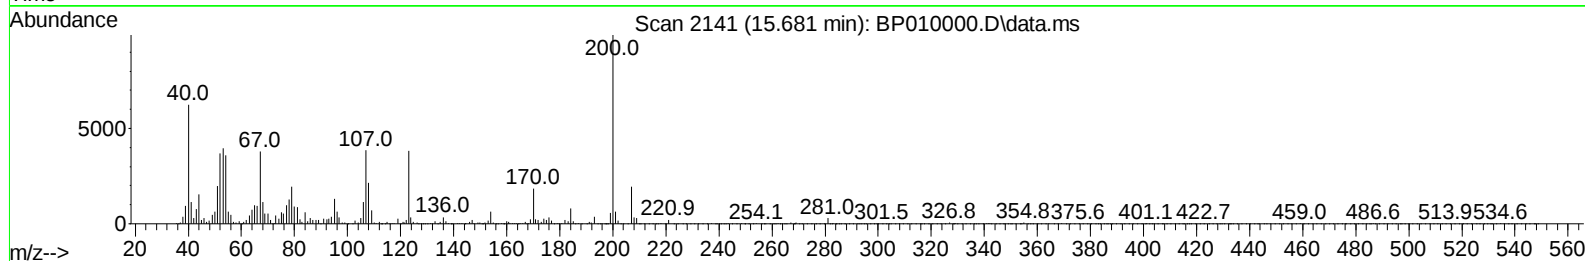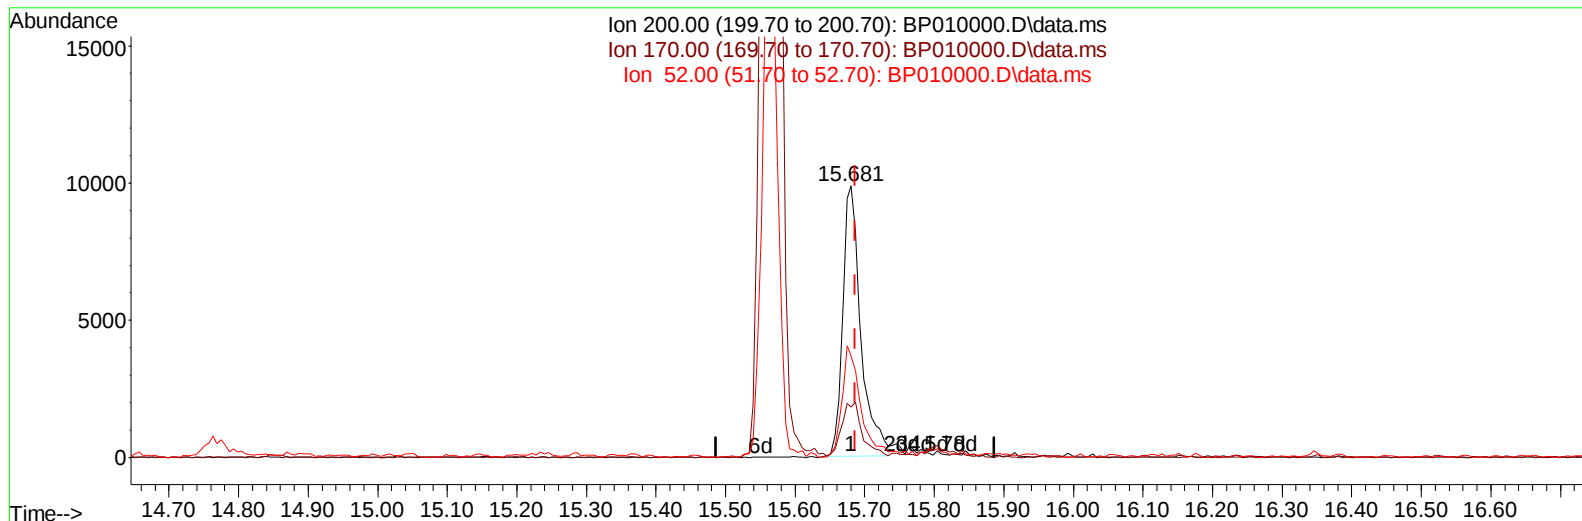

TIC: BP010000.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.681min (-0.006) 2.59 ng/u1

response 17790

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.00	18.51
52.00	21.20	37.27#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP010000.D
 Acq On : 21 Apr 2022 05:03
 Operator : CG/JU
 Sample : N2472-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J00

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:51:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

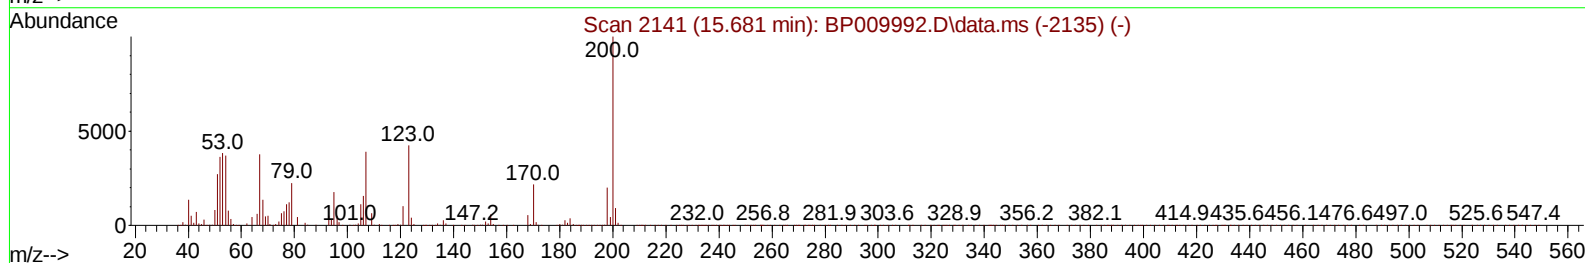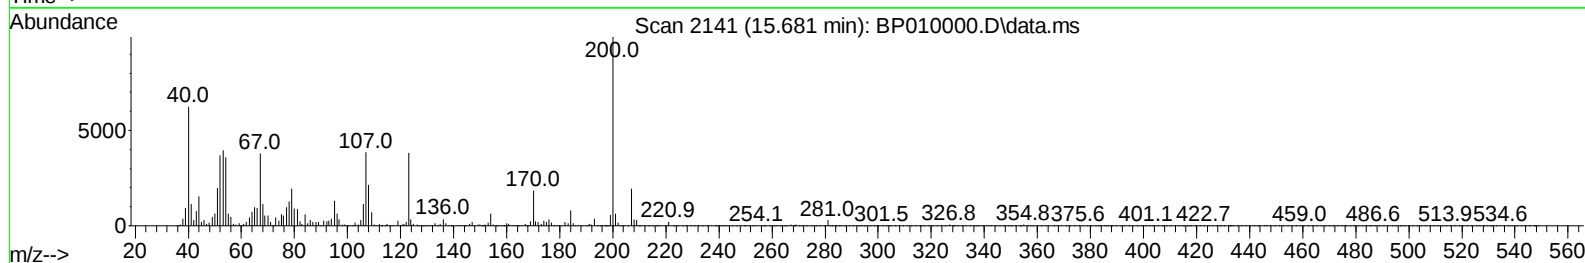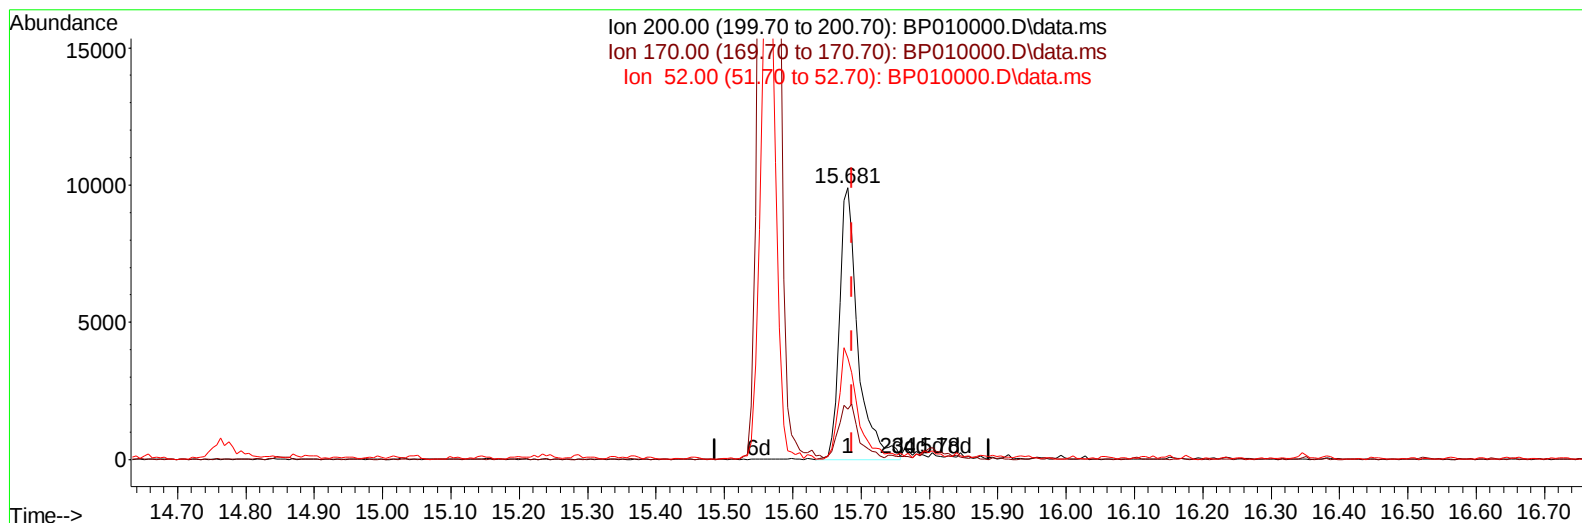

TIC: BP010000.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.681min (-0.006) 2.70 ng/ul m

response 18552

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.00	18.51
52.00	21.20	37.27#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP010000.D
 Acq On : 21 Apr 2022 05:03
 Operator : CG/JU
 Sample : N2472-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J00

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 05:51:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	149912	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	683869	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	511856	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1160081	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	1149148	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	950172	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	16505m	4.914	ng/uL	0.00
4) Pyridine-d5	3.793	84	90842	9.809	ng/ul	0.00
7) Phenol-d5	7.099	99	69386	5.272	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	224082	28.599	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	200241	20.170	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	141477	12.877	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	146938	29.795	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	128919	23.844	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	243399	21.513	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	443863	27.545	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	1136140	28.257	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	1232399	25.872	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	7011m	0.961	ng/ul	0.00
60) Fluorene-d10	15.563	176	982207	29.039	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	18552m	2.700	ng/ul	0.00
73) Anthracene-d10	17.422	188	1718927	30.947	ng/ul	0.00
81) Pyrene-d10	19.651	212	2090685	33.312	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1551356	31.352	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP010000.D
Acq On : 21 Apr 2022 05:03
Operator : CG/JU
Sample : N2472-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J00

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 05:51:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

