

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009955.D
 Acq On : 19 Apr 2022 20:52
 Operator : CG/JU
 Sample : N2388-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFE1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 20 01:33:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	115729	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.751	136	511341	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	369126	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	811257	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.410	240	883619	20.000	ng/ul	# 0.00
88) Perylene-d12	23.862	264	852561	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	14036m	5.413	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.099	99	55909	5.503	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	192494	31.824	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	184405	24.061	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	112196	13.228	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	121680	32.999	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	128441	31.771	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	225540	26.661	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	7429m	0.617	ng/ul	0.01
46) Dimethylphthalate-d6	13.981	166	914085	31.525	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	599535	17.453	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	30175m	5.738	ng/ul	0.00
60) Fluorene-d10	15.569	176	756108	30.998	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	133384	27.754	ng/ul	0.00
73) Anthracene-d10	17.428	188	1050709	27.051	ng/ul	0.00
81) Pyrene-d10	19.657	212	1383334	28.665	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	1016872	22.903	ng/ul	0.00
Target Compounds						
8) Phenol	7.128	94	20580m	2.024	ng/ul	Qvalue
78) Di-n-butylphthalate	18.280	149	132333	2.712	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009955.D
Acq On : 19 Apr 2022 20:52
Operator : CG/JU
Sample : N2388-01
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
BFFE1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 20 01:33:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

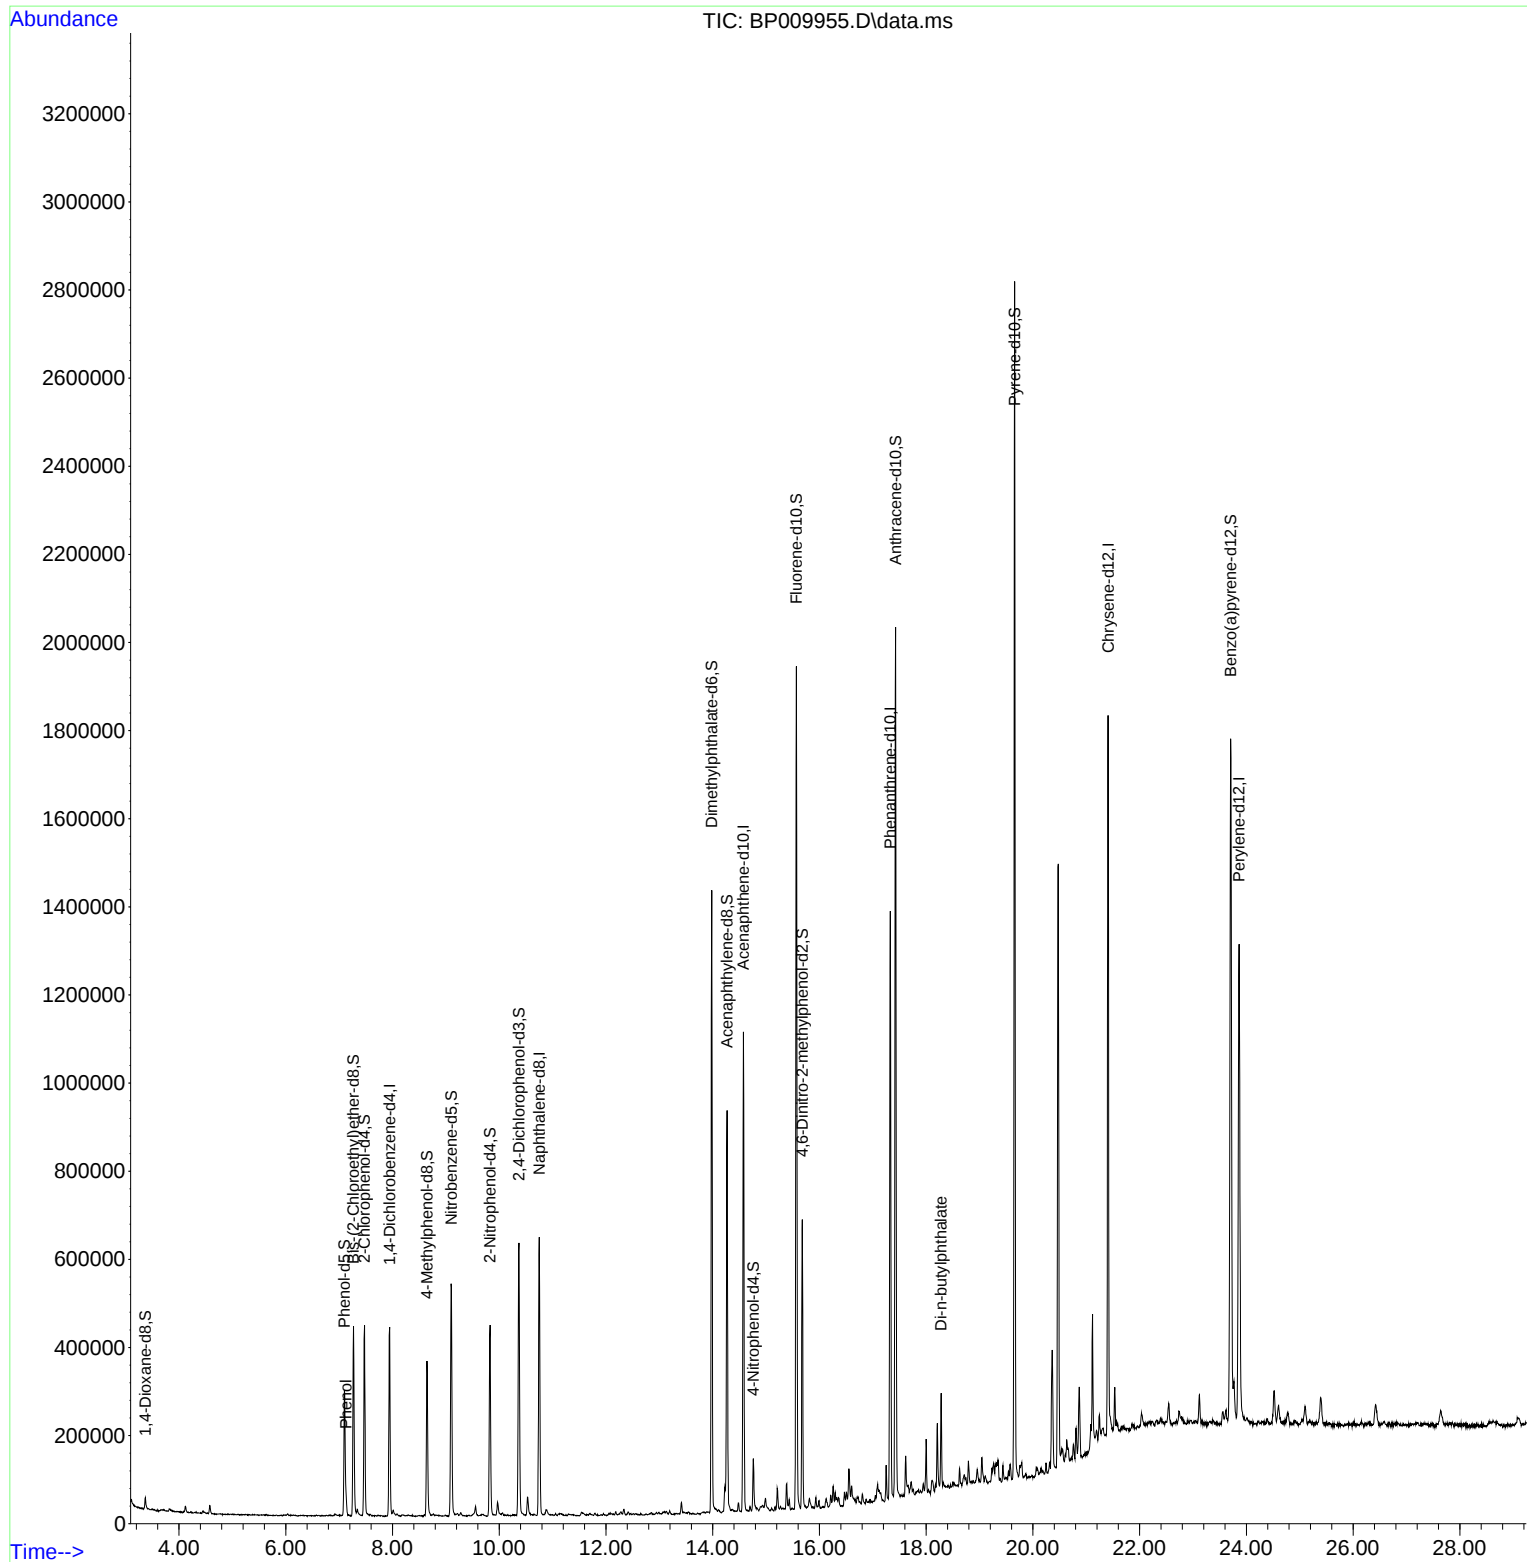

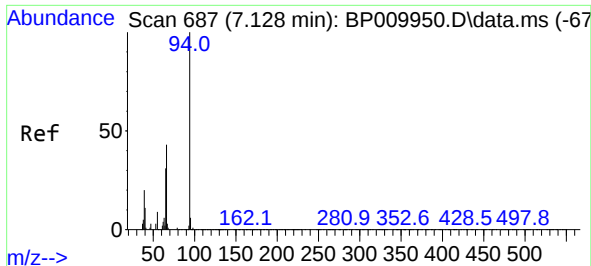





#8
Phenol
Concen: 2.024 ng/ul m
RT: 7.128 min Scan# 687
Delta R.T. -0.000 min
Lab File: BP009955.D
Acq: 19 Apr 2022 20:52

Instrument :
BNA_P
ClientSampleId :
BFFE1

Tgt Ion: 94 Resp: 20580
Ion Ratio Lower Upper
94 100
65 36.0 19.0 28.6
66 46.4 34.6 51.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/25/2022

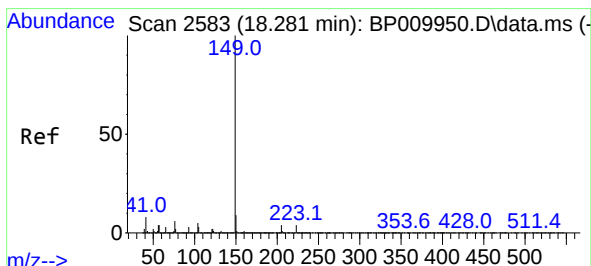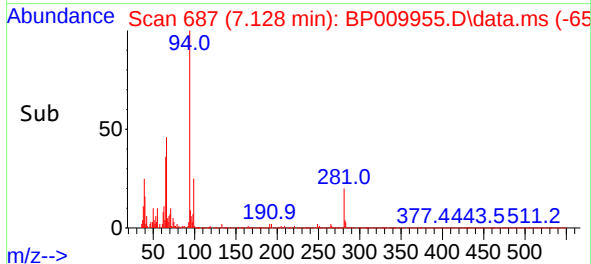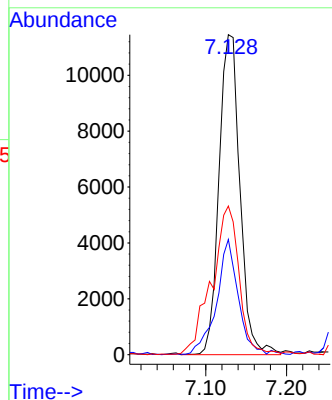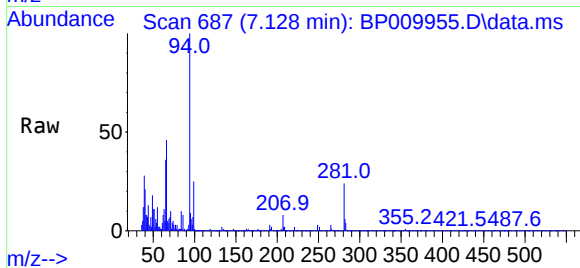

#78
Di-n-butylphthalate
Concen: 2.712 ng/ul
RT: 18.280 min Scan# 2583
Delta R.T. -0.000 min
Lab File: BP009955.D
Acq: 19 Apr 2022 20:52

Tgt Ion:149 Resp: 132333
Ion Ratio Lower Upper
149 100
150 9.2 9.6 14.4#
104 6.0 6.2 9.4#

