

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009998.D
 Acq On : 21 Apr 2022 03:56
 Operator : CG/JU
 Sample : N2472-05
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J01

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 21 05:20:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 01:32:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	113514	20.000	ng/u1	0.00
20) Naphthalene-d8	10.745	136	497081	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.575	164	359110	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.322	188	805253	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.404	240	825124	20.000	ng/u1	# 0.00
88) Perylene-d12	23.851	264	756421	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	6578m	2.586	ng/uL	0.00
4) Pyridine-d5	3.793	84	36129	5.152	ng/u1	0.00
7) Phenol-d5	7.099	99	64332	6.455	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	223462	37.664	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	206773	27.506	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	137523	16.530	ng/u1	0.00
21) Nitrobenzene-d5	9.098	128	147229	41.073	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	152908	38.908	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	254826	30.987	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	342739	29.262	ng/u1	0.00
46) Dimethylphthalate-d6	13.981	166	1163915	41.261	ng/u1	0.00
49) Acenaphthylene-d8	14.263	160	1221280	36.544	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	30517m	5.965	ng/u1	0.00
60) Fluorene-d10	15.563	176	998317	42.070	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	166523	34.908	ng/u1	0.00
73) Anthracene-d10	17.422	188	1683387	43.662	ng/u1	0.00
81) Pyrene-d10	19.651	212	2076066	46.069	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.698	264	1784300	45.296	ng/u1	-0.01
Target Compounds					Qvalue	
35) 4-Chloro-3-methylphenol	12.028	107	19338	2.002	ng/u1#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009998.D
Acq On : 21 Apr 2022 03:56
Operator : CG/JU
Sample : N2472-05
Misc :
ALS Vial : 52 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0J01

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
Supervised By :Yogesh Patel 04/25/2022


Quant Time: Apr 21 05:20:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 01:32:14 2022
Response via : Initial Calibration

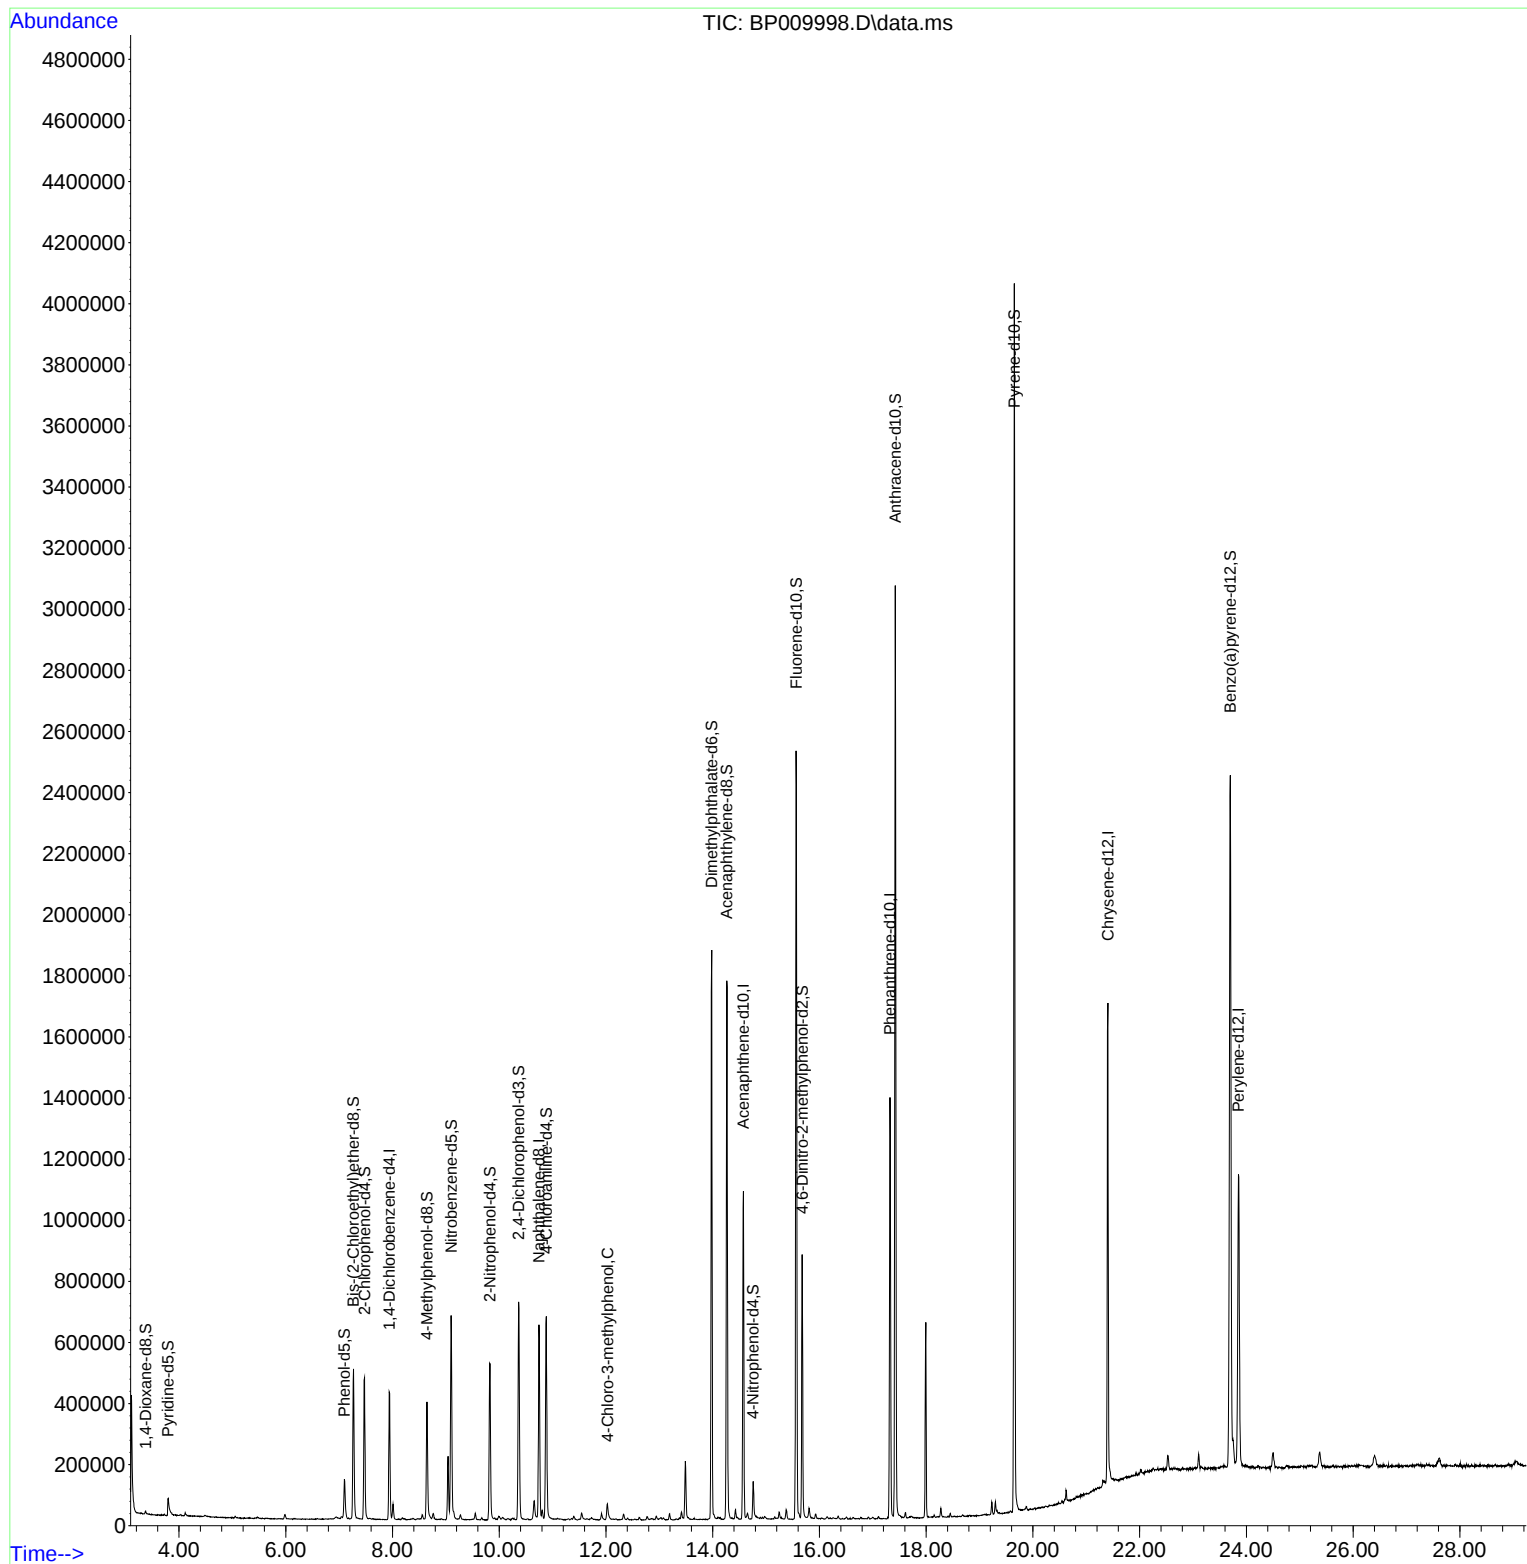

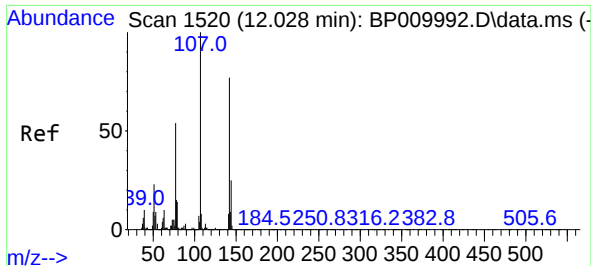

#35
 4-Chloro-3-methylphenol
 Concen: 2.002 ng/ul
 RT: 12.028 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: BP009998.D
 Acq: 21 Apr 2022 03:56

Instrument :
 BNA_P
 ClientSampleId :
 C0J01

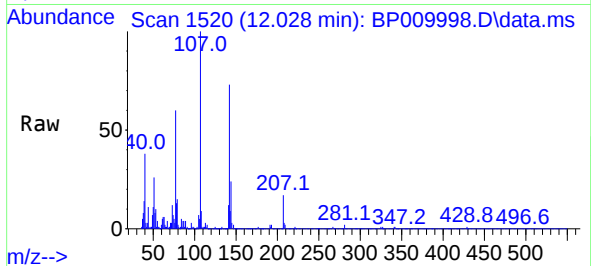

Tgt Ion:107 Resp: 19338
 Ion Ratio Lower Upper
 107 100
 144 24.1 15.8 23.8
 142 72.9 38.9 58.3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/21/2022
 Supervised By :Yogesh Patel 04/25/2022

