

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009959.D
 Acq On : 19 Apr 2022 23:07
 Operator : CG/JU
 Sample : N2388-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	57	rVB	32369	49621	0.83%	0.101%
2	3.793	117	120	135	rBV	93649	166613	2.79%	0.338%
3	4.123	172	176	181	rBV	18696	27072	0.45%	0.055%
4	4.487	234	238	242	rVB7	4676	6815	0.11%	0.014%
5	4.628	260	262	268	rVB5	5736	7902	0.13%	0.016%
6	5.052	331	334	338	rBV4	5190	6370	0.11%	0.013%
7	6.487	575	578	582	rBV5	4021	6498	0.11%	0.013%
8	7.099	676	682	691	rVB	143288	242854	4.07%	0.492%
9	7.269	703	711	723	rBV	558005	907734	15.20%	1.840%
10	7.475	739	746	756	rBV	551842	873144	14.62%	1.770%
11	7.946	817	826	833	rBV	494174	792821	13.27%	1.607%
12	8.011	833	837	846	rVB	32360	54770	0.92%	0.111%
13	8.646	938	945	959	rBV	460738	779986	13.06%	1.581%
14	8.763	963	965	971	rVB3	8096	12745	0.21%	0.026%
15	9.046	1008	1013	1015	rBV6	4008	6319	0.11%	0.013%
16	9.099	1015	1022	1034	rVV	734448	1265052	21.18%	2.564%
17	9.205	1037	1040	1047	rVV9	6891	14438	0.24%	0.029%
18	9.275	1047	1052	1059	rVB9	9669	18944	0.32%	0.038%
19	9.828	1136	1146	1162	rBV	584248	1015108	17.00%	2.057%
20	10.216	1208	1212	1218	rBV5	9264	17524	0.29%	0.036%
21	10.369	1230	1238	1255	rBV	827298	1426378	23.88%	2.891%
22	10.540	1261	1267	1275	rVB10	12364	24480	0.41%	0.050%
23	10.657	1285	1287	1295	rVB9	3310	6259	0.10%	0.013%
24	10.752	1295	1303	1317	rBV	719656	1266700	21.21%	2.567%
25	10.881	1317	1325	1340	rBV	764133	1339618	22.43%	2.715%
26	11.304	1390	1397	1400	rBV9	3796	9052	0.15%	0.018%
27	11.404	1410	1414	1419	rVB4	6898	11978	0.20%	0.024%
28	11.546	1433	1438	1442	rBV6	6951	13651	0.23%	0.028%
29	12.340	1566	1573	1578	rBV2	17719	33444	0.56%	0.068%
30	12.893	1662	1667	1671	rBV2	15895	22229	0.37%	0.045%
31	12.946	1671	1676	1683	rVB2	15742	27590	0.46%	0.056%
32	13.193	1712	1718	1722	rBV	34435	50317	0.84%	0.102%
33	13.422	1752	1757	1761	rVB	21629	30265	0.51%	0.061%
34	13.481	1761	1767	1774	rBV	72779	118345	1.98%	0.240%
35	13.981	1846	1852	1858	rBV	2109030	2851273	47.74%	5.779%
36	14.269	1889	1901	1919	rBV	2108837	3109911	52.07%	6.303%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009959.D
 Acq On : 19 Apr 2022 23:07
 Operator : CG/JU
 Sample : N2388-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	14.575	1946	1953	1963	rBV	1287829	1862031	31.18%	3.774%
38	14.657	1963	1967	1972	rVB5	9310	14694	0.25%	0.030%
39	14.757	1977	1984	1995	rBV	143460	259164	4.34%	0.525%
40	14.993	2019	2024	2027	rBV7	6677	10298	0.17%	0.021%
41	15.251	2065	2068	2075	rVB6	8458	15407	0.26%	0.031%
42	15.381	2084	2090	2096	rVB3	26104	41993	0.70%	0.085%
43	15.569	2114	2122	2134	rBV	2959875	4139493	69.31%	8.390%
44	15.681	2134	2141	2151	rVV	995604	1390221	23.28%	2.818%
45	15.810	2158	2163	2169	rVB2	31143	51054	0.85%	0.103%
46	15.934	2180	2184	2192	rVB5	14477	25983	0.44%	0.053%
47	16.140	2214	2219	2221	rBV6	4316	6614	0.11%	0.013%
48	16.251	2234	2238	2242	rBV6	3355	6040	0.10%	0.012%
49	16.357	2251	2256	2263	rVB5	12817	21858	0.37%	0.044%
50	16.651	2299	2306	2307	rBV7	3744	6253	0.10%	0.013%
51	16.728	2316	2319	2324	rVB7	4857	6346	0.11%	0.013%
52	16.839	2331	2338	2342	rBV9	5491	11175	0.19%	0.023%
53	16.928	2349	2353	2359	rBV7	4797	8823	0.15%	0.018%
54	17.004	2362	2366	2371	rBV8	7298	11615	0.19%	0.024%
55	17.116	2382	2385	2390	rVB3	7006	11282	0.19%	0.023%
56	17.328	2411	2421	2431	rBV	1645334	2337136	39.13%	4.737%
57	17.428	2431	2438	2453	rVV	3409578	4904987	82.12%	9.941%
58	17.616	2466	2470	2474	rBV	9743	14133	0.24%	0.029%
59	17.910	2517	2520	2522	rBV3	6845	7409	0.12%	0.015%
60	17.992	2529	2534	2544	rBV	290628	359679	6.02%	0.729%
61	18.210	2567	2571	2575	rBV	53192	72527	1.21%	0.147%
62	18.281	2579	2583	2592	rVB	31079	41344	0.69%	0.084%
63	18.457	2610	2613	2616	rBV5	4793	6099	0.10%	0.012%
64	18.816	2671	2674	2679	rBV7	7355	10036	0.17%	0.020%
65	19.039	2707	2712	2717	rBV7	14472	22318	0.37%	0.045%
66	19.233	2740	2745	2750	rBV	46800	62950	1.05%	0.128%
67	19.304	2752	2757	2764	rVV2	42581	67713	1.13%	0.137%
68	19.439	2777	2780	2784	rVB2	24062	27968	0.47%	0.057%
69	19.586	2802	2805	2808	rBV4	10826	12643	0.21%	0.026%
70	19.657	2811	2817	2831	rVV	4543054	5972660	100.00%	12.105%
71	21.410	3109	3115	3121	rBV	1827332	2554242	42.77%	5.177%
72	22.539	3302	3307	3317	rVB3	293206	498632	8.35%	1.011%
73	23.704	3497	3505	3513	rBV2	2571722	5401448	90.44%	10.947%
74	23.863	3525	3532	3543	rVB3	1163287	2452073	41.05%	4.970%

Sum of corrected areas: 49340161




Instrument :
BNA_P
ClientSampleId :
BFFE8

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009959.D
Acq On : 19 Apr 2022 23:07
Operator : CG/JU
Sample : N2388-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

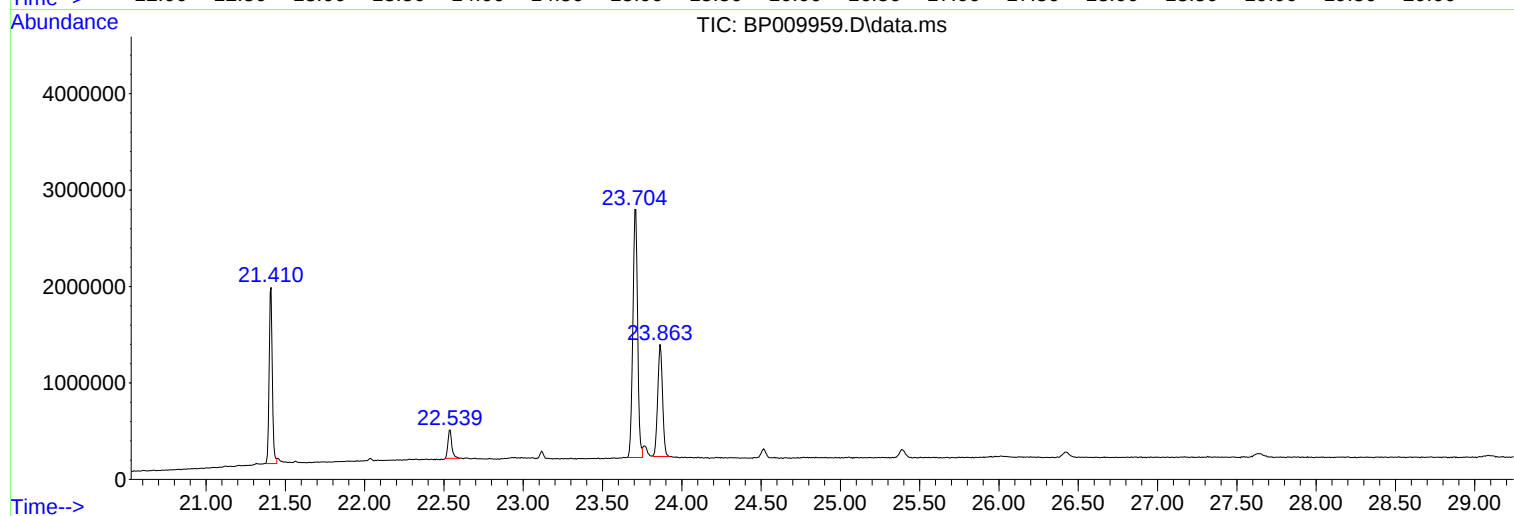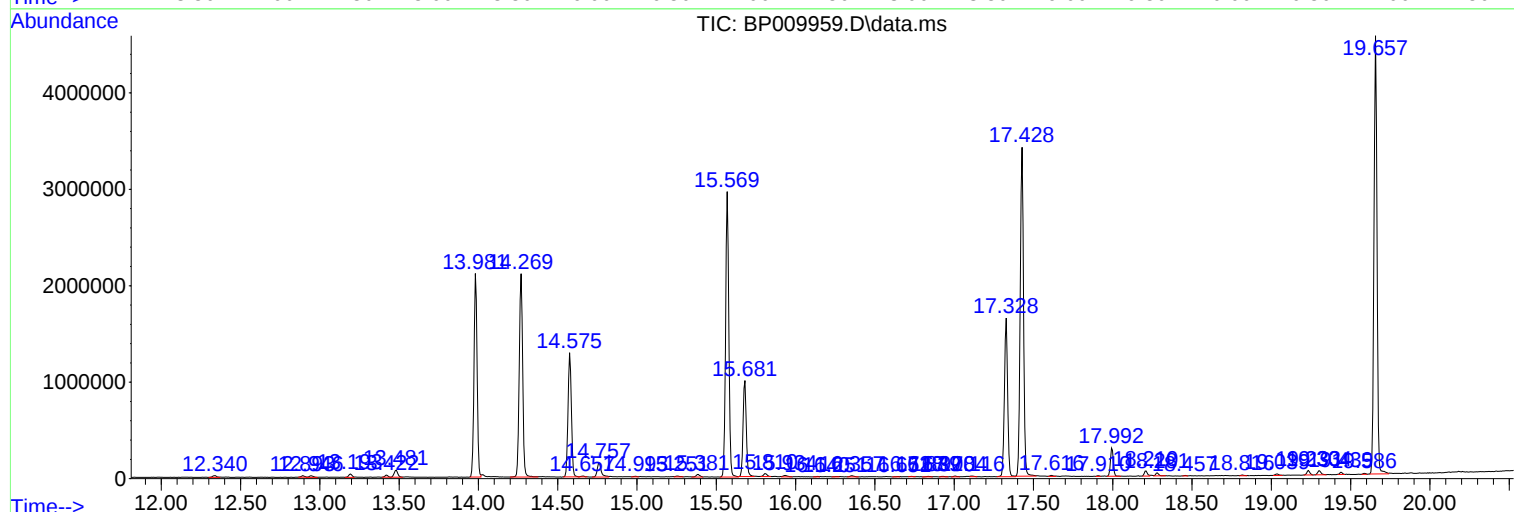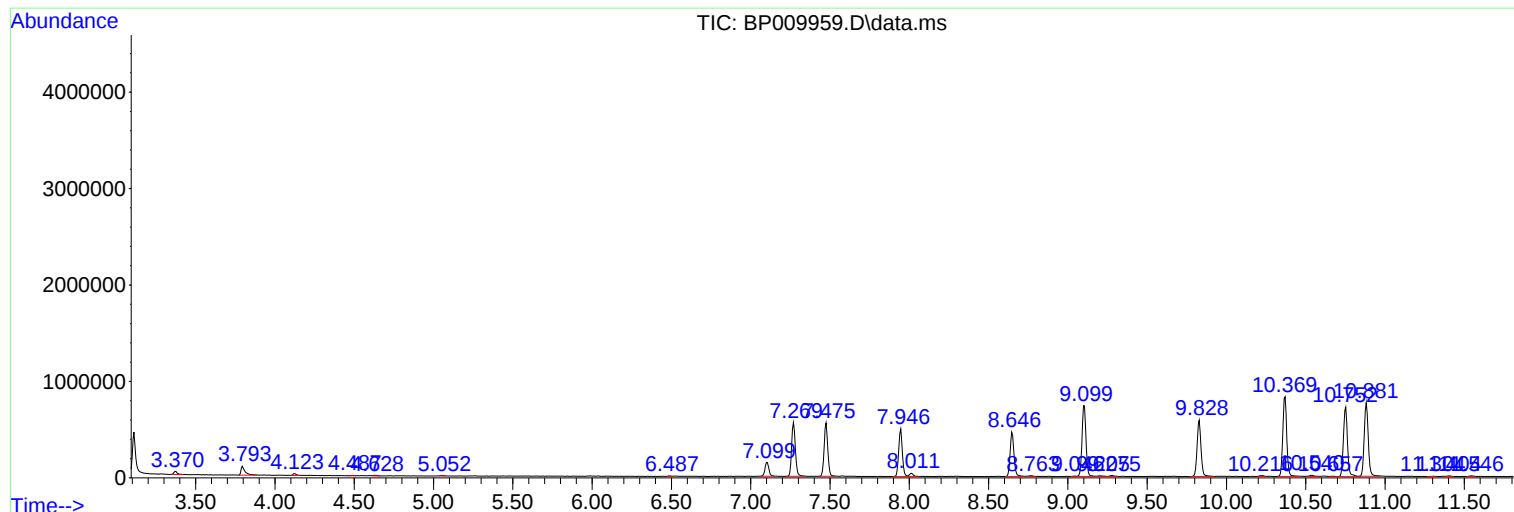

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009959.D
Acq On : 19 Apr 2022 23:07
Operator : CG/JU
Sample : N2388-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFE8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.992	3.08 ng/ul	359679	Phenanthrene-d10	17.328

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	99		
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	95		
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	91		
4	2,5-di-tert-Butyl-1,4-benzoquinone	220	C14H20O2	002460-77-7	50		
5	Silane, tert-butyldichlorophenyl-	232	C10H14Cl2Si	017887-41-1	35		

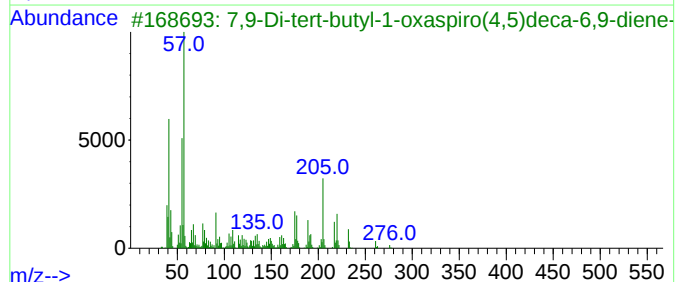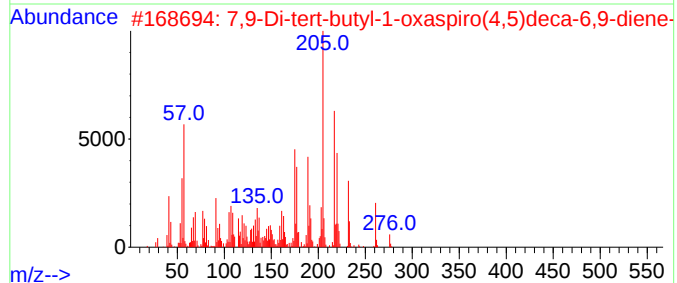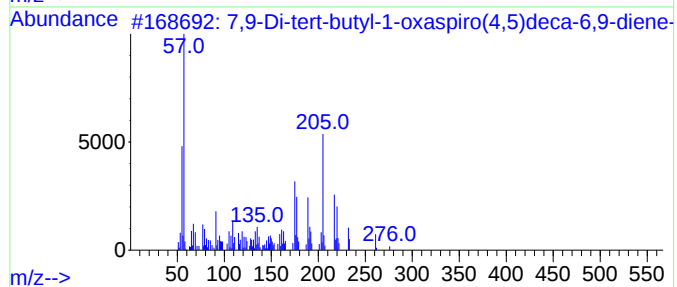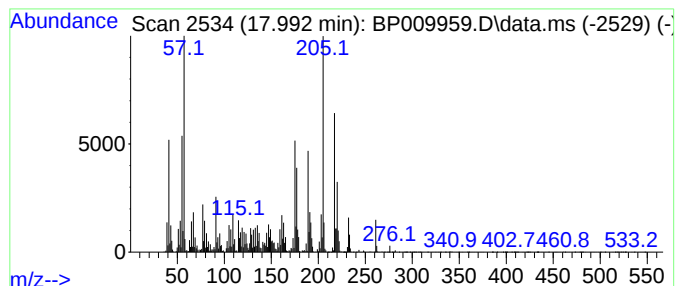

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009959.D
Acq On : 19 Apr 2022 23:07
Operator : CG/JU
Sample : N2388-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFE8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 9-Octadecenamide, (Z)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.539	3.90 ng/ul	498632	Chrysene-d12	21.410

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			9-Octadecenamide, (Z)-	281	C18H35NO	000301-02-0	90
2			13-Docosenamide, (Z)-	337	C22H43NO	000112-84-5	87
3			9-Octadecenamide, (Z)-	281	C18H35NO	000301-02-0	87
4			13-Docosenamide, (Z)-	337	C22H43NO	000112-84-5	81
5			13-Docosenamide, (Z)-	337	C22H43NO	000112-84-5	68

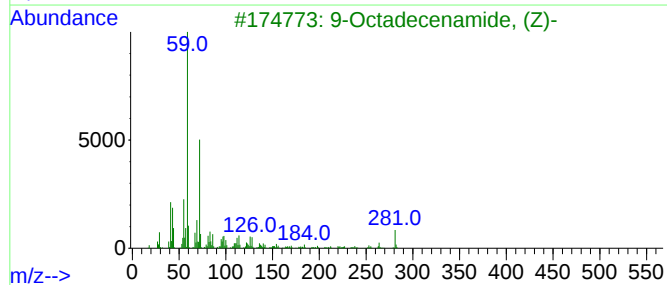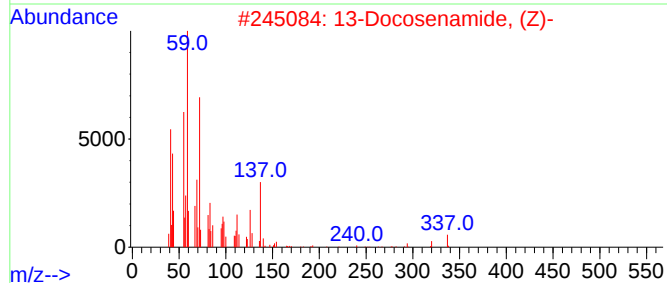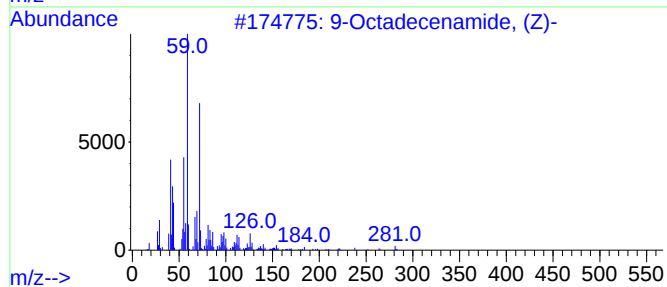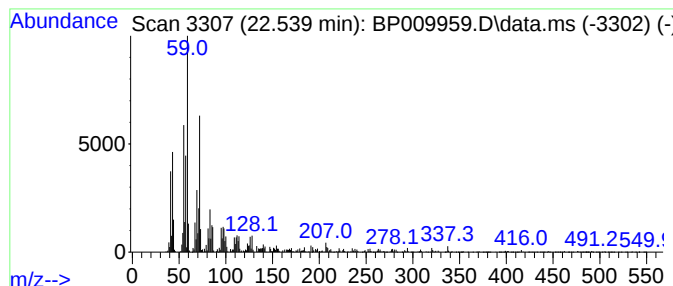

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009959.D
Acq On : 19 Apr 2022 23:07
Operator : CG/JU
Sample : N2388-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	17.992	3.1	ng/u1	359679	4	17.328	2337140	20.0
9-Octadecenamid...	22.539	3.9	ng/u1	498632	5	21.410	2554240	20.0