

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009968.D
 Acq On : 20 Apr 2022 08:53
 Operator : CG/JU
 Sample : PB144232BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	59	rVB	31009	54183	1.31%	0.135%
2	3.787	116	119	140	rBV	355857	659697	15.99%	1.642%
3	4.122	174	176	180	rVB3	6835	7517	0.18%	0.019%
4	4.975	317	321	325	rVB7	2801	4459	0.11%	0.011%
5	7.105	676	683	699	rBV	505968	830873	20.14%	2.069%
6	7.275	705	712	725	rVB	423316	679033	16.46%	1.691%
7	7.481	736	747	756	rBV	518998	854512	20.72%	2.127%
8	7.952	819	827	836	rBV	439546	740720	17.96%	1.844%
9	8.652	939	946	960	rBV	661365	1113399	26.99%	2.772%
10	9.104	1016	1023	1036	rBV	515890	901880	21.86%	2.245%
11	9.834	1138	1147	1159	rBV	432144	743844	18.03%	1.852%
12	10.375	1231	1239	1249	rBV	653686	1100599	26.68%	2.740%
13	10.757	1296	1304	1318	rBV	671467	1122758	27.22%	2.795%
14	10.887	1318	1326	1338	rBV	679777	1179135	28.59%	2.936%
15	12.346	1568	1574	1578	rBV3	13871	25052	0.61%	0.062%
16	12.945	1674	1676	1681	rVB6	3613	5129	0.12%	0.013%
17	13.869	1831	1833	1840	rVB8	2876	4782	0.12%	0.012%
18	13.987	1846	1853	1867	rBV	1449082	2046993	49.63%	5.096%
19	14.275	1895	1902	1911	rBV	1478713	2134661	51.75%	5.315%
20	14.581	1947	1954	1965	rVV	1148480	1697024	41.14%	4.225%
21	14.769	1979	1986	2005	rBV	677796	1039955	25.21%	2.589%
22	14.940	2011	2015	2016	rBV4	5864	6555	0.16%	0.016%
23	15.016	2026	2028	2035	rVB2	10146	14845	0.36%	0.037%
24	15.228	2057	2064	2066	rBV8	8815	18426	0.45%	0.046%
25	15.263	2068	2070	2074	rVB4	8790	10601	0.26%	0.026%
26	15.387	2088	2091	2098	rVB9	5861	7041	0.17%	0.018%
27	15.575	2115	2123	2135	rBV	1973248	2896415	70.22%	7.211%
28	15.687	2136	2142	2152	rVV	714092	955212	23.16%	2.378%
29	15.816	2160	2164	2174	rVB5	24848	45104	1.09%	0.112%
30	16.010	2191	2197	2204	rVB6	9284	21585	0.52%	0.054%
31	16.139	2214	2219	2221	rBV6	2937	4908	0.12%	0.012%
32	16.292	2241	2245	2249	rVB7	5330	9860	0.24%	0.025%
33	16.363	2249	2257	2264	rBV6	9839	20885	0.51%	0.052%
34	16.657	2303	2307	2311	rVB6	6440	9153	0.22%	0.023%
35	16.798	2324	2331	2334	rBV9	4934	7779	0.19%	0.019%
36	16.845	2334	2339	2346	rVV5	9344	18400	0.45%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009968.D
 Acq On : 20 Apr 2022 08:53
 Operator : CG/JU
 Sample : PB144232BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	16.910	2346	2350	2352	rVV5	4441	6898	0.17%	0.017%
38	17.122	2379	2386	2390	rBV3	9226	16432	0.40%	0.041%
39	17.210	2397	2401	2406	rBV7	8090	14668	0.36%	0.037%
40	17.333	2415	2422	2432	rBV	1491496	2181224	52.88%	5.430%
41	17.433	2432	2439	2450	rVV	2228550	3295018	79.88%	8.203%
42	17.763	2492	2495	2499	rBV6	4719	6856	0.17%	0.017%
43	17.922	2516	2522	2524	rBV6	8149	14573	0.35%	0.036%
44	17.951	2524	2527	2531	rVB3	12139	15895	0.39%	0.040%
45	18.098	2549	2552	2557	rBV7	4639	5687	0.14%	0.014%
46	18.216	2568	2572	2578	rBV8	9581	21983	0.53%	0.055%
47	18.286	2580	2584	2591	rVB2	19379	31836	0.77%	0.079%
48	18.716	2652	2657	2662	rVB7	7257	15476	0.38%	0.039%
49	18.828	2672	2676	2679	rBV6	8924	11380	0.28%	0.028%
50	18.969	2698	2700	2704	rVB2	7028	7433	0.18%	0.019%
51	19.116	2720	2725	2732	rBV2	5640	11787	0.29%	0.029%
52	19.239	2742	2746	2751	rVB	30225	45144	1.09%	0.112%
53	19.310	2754	2758	2763	rVB	31127	43369	1.05%	0.108%
54	19.592	2803	2806	2809	rVB3	11125	11163	0.27%	0.028%
55	19.663	2812	2818	2823	rBV	3117498	4124801	100.00%	10.269%
56	21.416	3111	3116	3132	rVB	1931722	2635739	63.90%	6.562%
57	23.716	3499	3507	3515	rBV2	1936834	4047369	98.12%	10.076%
58	23.880	3527	3535	3548	rVB2	1221988	2608724	63.24%	6.495%




Sum of corrected areas: 40166429

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009968.D
Acq On : 20 Apr 2022 08:53
Operator : CG/JU
Sample : PB144232BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK232

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

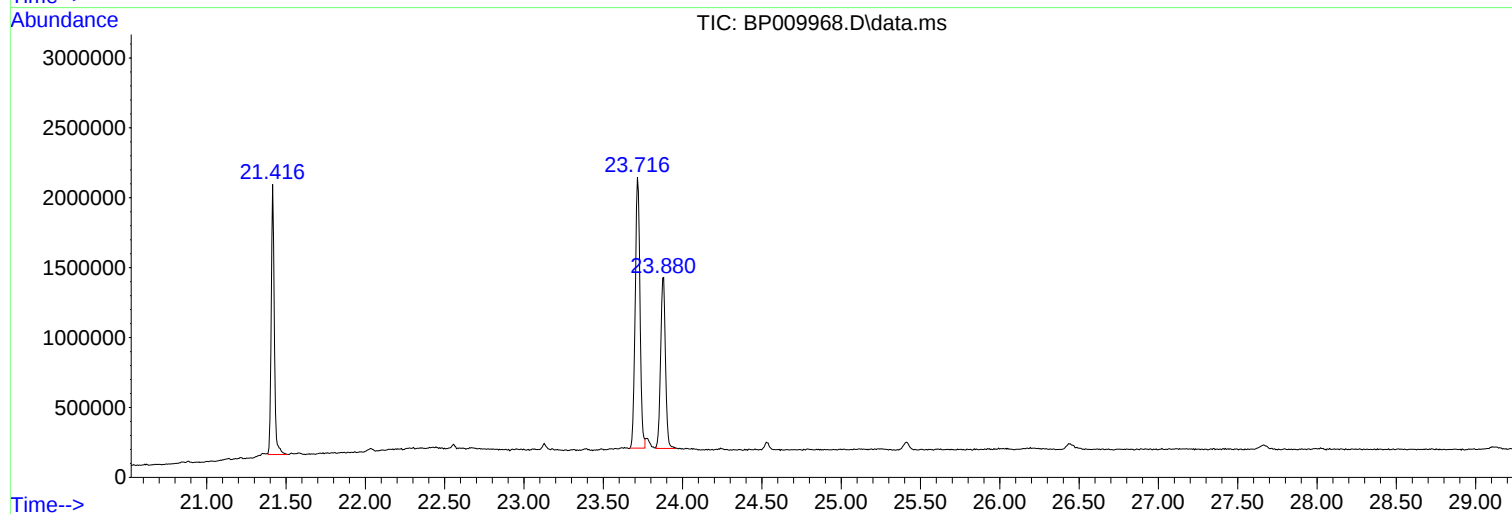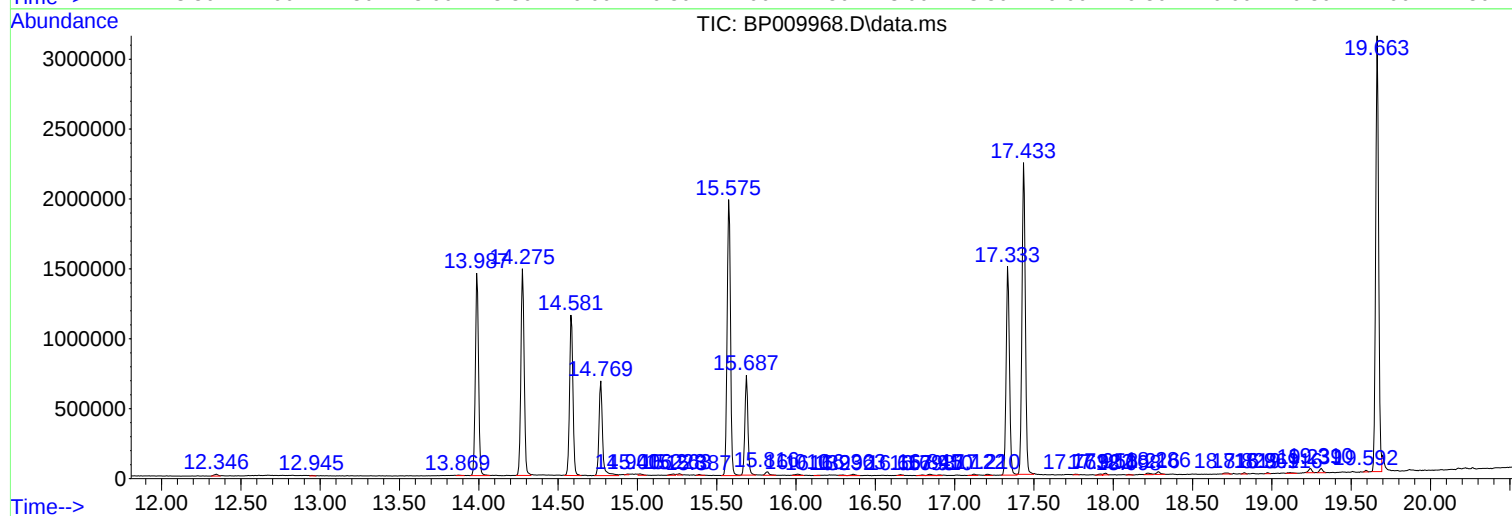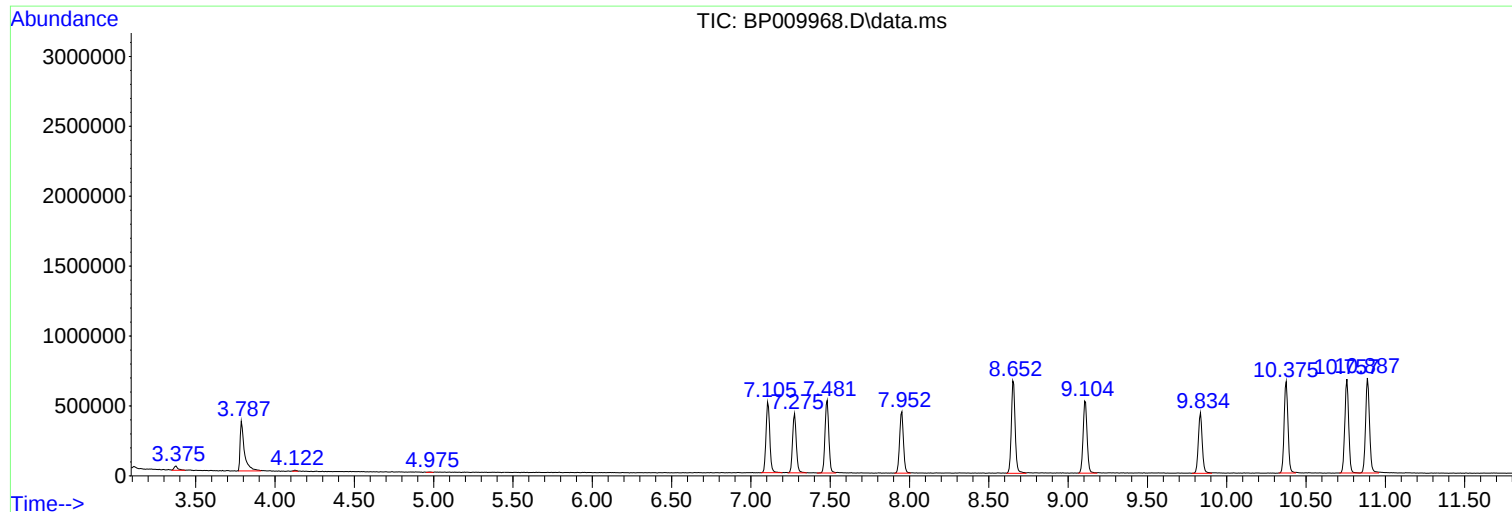

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009968.D
Acq On : 20 Apr 2022 08:53
Operator : CG/JU
Sample : PB144232BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK232

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009968.D
Acq On : 20 Apr 2022 08:53
Operator : CG/JU
Sample : PB144232BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK232

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------