

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009983.D
 Acq On : 20 Apr 2022 18:57
 Operator : CG/JU
 Sample : N2472-10
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.376	45	49	55	rVB	16816	23208	0.39%	0.043%
2	3.787	116	119	136	rBV	187682	340278	5.78%	0.627%
3	4.123	172	176	181	rVB	9783	14694	0.25%	0.027%
4	4.340	210	213	219	rVB5	9114	12453	0.21%	0.023%
5	4.752	281	283	290	rVB5	5973	8176	0.14%	0.015%
6	5.052	331	334	339	rVB5	5785	8197	0.14%	0.015%
7	6.946	653	656	660	rBV5	4834	7441	0.13%	0.014%
8	7.099	675	682	697	rBV	203381	379615	6.45%	0.700%
9	7.269	704	711	721	rBV	626578	1011234	17.17%	1.864%
10	7.352	721	725	730	rVB3	8991	17918	0.30%	0.033%
11	7.475	738	746	756	rBV	657544	1108348	18.82%	2.042%
12	7.946	816	826	833	rBV	609865	1031541	17.51%	1.901%
13	8.011	833	837	842	rVB	13973	22041	0.37%	0.041%
14	8.193	862	868	873	rVB9	3412	6643	0.11%	0.012%
15	8.299	880	886	891	rBV10	3585	8153	0.14%	0.015%
16	8.381	898	900	905	rVB6	4534	6931	0.12%	0.013%
17	8.463	908	914	916	rBV7	3247	6414	0.11%	0.012%
18	8.646	937	945	959	rBV	610338	1042626	17.70%	1.921%
19	8.746	959	962	963	rVV3	7313	9373	0.16%	0.017%
20	8.758	963	964	969	rVB3	9166	11847	0.20%	0.022%
21	9.099	1015	1022	1036	rBV	837089	1430050	24.28%	2.635%
22	9.228	1040	1044	1047	rVV6	5184	9512	0.16%	0.018%
23	9.281	1047	1053	1057	rVB7	6143	11645	0.20%	0.021%
24	9.552	1093	1099	1108	rBV	58459	94364	1.60%	0.174%
25	9.675	1115	1120	1124	rBV4	5571	10055	0.17%	0.019%
26	9.828	1137	1146	1158	rBV	673365	1182754	20.08%	2.180%
27	9.916	1160	1161	1166	rVB5	6192	7256	0.12%	0.013%
28	10.363	1229	1237	1250	rBV	1112172	1916634	32.54%	3.532%
29	10.534	1259	1266	1275	rBV	29707	56177	0.95%	0.104%
30	10.693	1288	1293	1296	rBV5	5663	9711	0.16%	0.018%
31	10.746	1296	1302	1317	rVB	926585	1616930	27.45%	2.980%
32	10.881	1317	1325	1341	rBV	891624	1622807	27.55%	2.991%
33	11.099	1358	1362	1366	rVB7	4548	7153	0.12%	0.013%
34	11.552	1432	1439	1443	rBV10	3879	8916	0.15%	0.016%
35	11.687	1459	1462	1470	rBV10	4425	10681	0.18%	0.020%
36	11.787	1473	1479	1483	rVV8	5785	10149	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009983.D
 Acq On : 20 Apr 2022 18:57
 Operator : CG/JU
 Sample : N2472-10
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COJ10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	12.052	1515	1524	1533	rVB5	12661	30207	0.51%	0.056%
38	12.175	1541	1545	1554	rBV3	18167	29501	0.50%	0.054%
39	12.275	1558	1562	1566	rVV6	6803	11314	0.19%	0.021%
40	12.334	1566	1572	1579	rVV	21763	41274	0.70%	0.076%

41	12.410	1579	1585	1592	rVB7	11315	23506	0.40%	0.043%
42	12.622	1615	1621	1625	rBV3	8825	13823	0.23%	0.025%
43	12.769	1639	1646	1650	rBV6	8006	16073	0.27%	0.030%
44	12.946	1672	1676	1679	rBV4	8219	10740	0.18%	0.020%
45	13.075	1693	1698	1704	rBV9	9176	20986	0.36%	0.039%

46	13.134	1704	1708	1713	rVB7	6208	8885	0.15%	0.016%
47	13.193	1713	1718	1722	rBV2	13909	19314	0.33%	0.036%
48	13.375	1745	1749	1751	rBV5	6450	9434	0.16%	0.017%
49	13.410	1751	1755	1760	rVV	44393	66027	1.12%	0.122%
50	13.481	1760	1767	1774	rVV	90444	156660	2.66%	0.289%

51	13.546	1774	1778	1783	rVB7	5813	7556	0.13%	0.014%
52	13.981	1845	1852	1858	rBV	2312604	3215229	54.59%	5.925%
53	14.110	1870	1874	1879	rVB8	5746	8869	0.15%	0.016%
54	14.222	1888	1893	1895	rBV3	45170	62220	1.06%	0.115%
55	14.269	1895	1901	1913	rVB	2424343	3673366	62.37%	6.769%

56	14.481	1933	1937	1942	rVB4	15806	23182	0.39%	0.043%
57	14.575	1946	1953	1961	rBV	1595665	2318861	39.37%	4.273%
58	14.634	1961	1963	1971	rVB6	13163	22480	0.38%	0.041%
59	14.757	1979	1984	1996	rBV	176734	299809	5.09%	0.552%
60	14.916	2003	2011	2017	rBV8	17298	43816	0.74%	0.081%

61	14.975	2017	2021	2026	rVB4	11464	19137	0.32%	0.035%
62	15.210	2055	2061	2068	rVB2	24252	46779	0.79%	0.086%
63	15.381	2085	2090	2096	rVV2	68595	113156	1.92%	0.209%
64	15.434	2096	2099	2105	rVB2	16156	20754	0.35%	0.038%
65	15.569	2115	2122	2128	rBV	3111040	4657416	79.08%	8.583%

66	15.681	2135	2141	2150	rBV	1000577	1400845	23.79%	2.581%
67	15.804	2158	2162	2171	rVB2	38240	71084	1.21%	0.131%
68	15.928	2178	2183	2188	rVB5	14376	23745	0.40%	0.044%
69	15.987	2190	2193	2197	rBV5	6896	9868	0.17%	0.018%
70	16.116	2211	2215	2218	rBV6	9696	14008	0.24%	0.026%

71	16.140	2218	2219	2224	rVV5	7840	8456	0.14%	0.016%
72	16.210	2228	2231	2234	rVV5	10606	13359	0.23%	0.025%
73	16.251	2234	2238	2242	rVV4	22238	37705	0.64%	0.069%
74	16.293	2242	2245	2248	rVV4	23041	32376	0.55%	0.060%
75	16.357	2252	2256	2261	rVB4	16743	29419	0.50%	0.054%

76	16.469	2270	2275	2277	rBV3	18094	25266	0.43%	0.047%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009983.D
 Acq On : 20 Apr 2022 18:57
 Operator : CG/JU
 Sample : N2472-10
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

77	16.569	2289	2292	2295	rBV4	5592	6708	0.11%	0.012%
78	16.634	2300	2303	2307	rBV5	14459	20437	0.35%	0.038%
79	16.781	2325	2328	2329	rBV3	8080	7511	0.13%	0.014%
80	16.804	2329	2332	2335	rVB4	12169	14244	0.24%	0.026%
81	16.875	2340	2344	2346	rBV3	7062	10749	0.18%	0.020%
82	16.975	2358	2361	2362	rBV3	7780	7461	0.13%	0.014%
83	17.087	2375	2380	2387	rBV6	35059	67347	1.14%	0.124%
84	17.140	2387	2389	2394	rVB6	13766	18298	0.31%	0.034%
85	17.192	2396	2398	2403	rVB6	7952	7676	0.13%	0.014%
86	17.251	2404	2408	2412	rBV	41437	50261	0.85%	0.093%
87	17.328	2414	2421	2431	rBV	1880636	2802122	47.58%	5.164%
88	17.428	2431	2438	2450	rVV	3350839	4975782	84.48%	9.169%
89	17.639	2468	2474	2481	rVB8	18798	43661	0.74%	0.080%
90	17.992	2531	2534	2539	rVB3	31146	42790	0.73%	0.079%
91	18.204	2566	2570	2578	rBV	153316	239352	4.06%	0.441%
92	18.275	2580	2582	2587	rVB	37996	42749	0.73%	0.079%
93	19.228	2741	2744	2748	rBV2	50859	60367	1.02%	0.111%
94	19.298	2753	2756	2759	rVV	41851	46177	0.78%	0.085%
95	19.439	2777	2780	2784	rBV5	22745	29662	0.50%	0.055%
96	19.657	2810	2817	2828	rBV	4076815	5889575	100.00%	10.853%
97	21.110	3060	3064	3073	rBV	538862	691843	11.75%	1.275%
98	21.404	3109	3114	3120	rBV	2040202	2685862	45.60%	4.950%
99	23.698	3497	3504	3511	rBV2	2154102	4384215	74.44%	8.079%
100	23.857	3524	3531	3540	rVB2	1144328	2381752	40.44%	4.389%




Sum of corrected areas: 54265031

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009983.D
Acq On : 20 Apr 2022 18:57
Operator : CG/JU
Sample : N2472-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

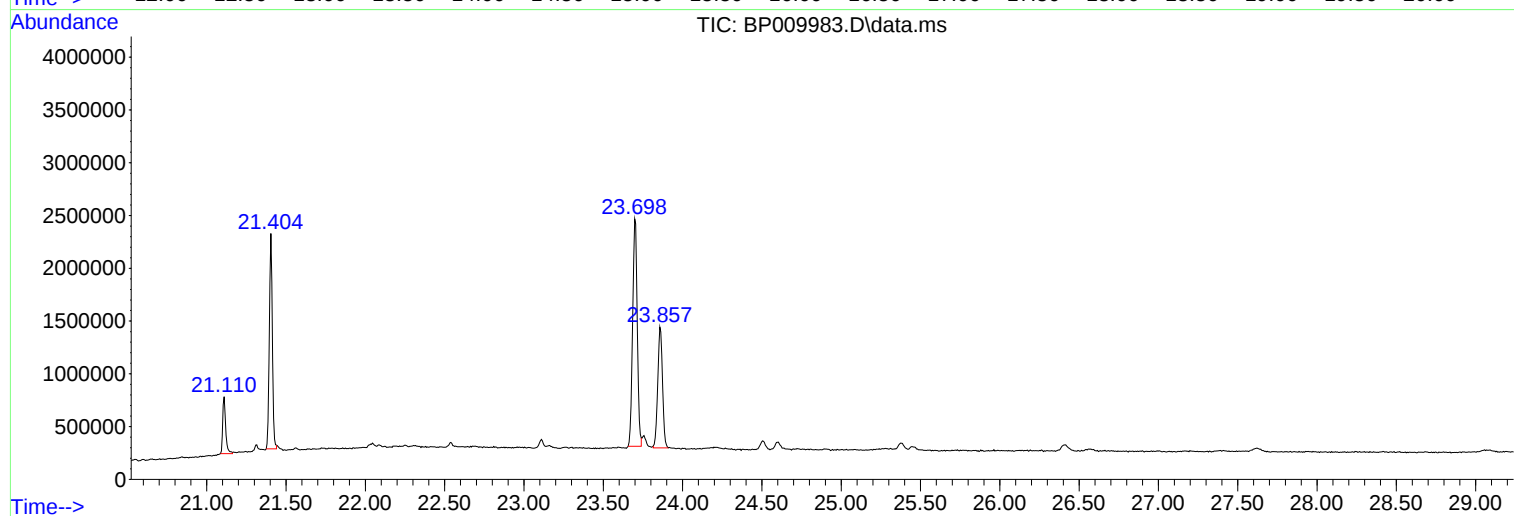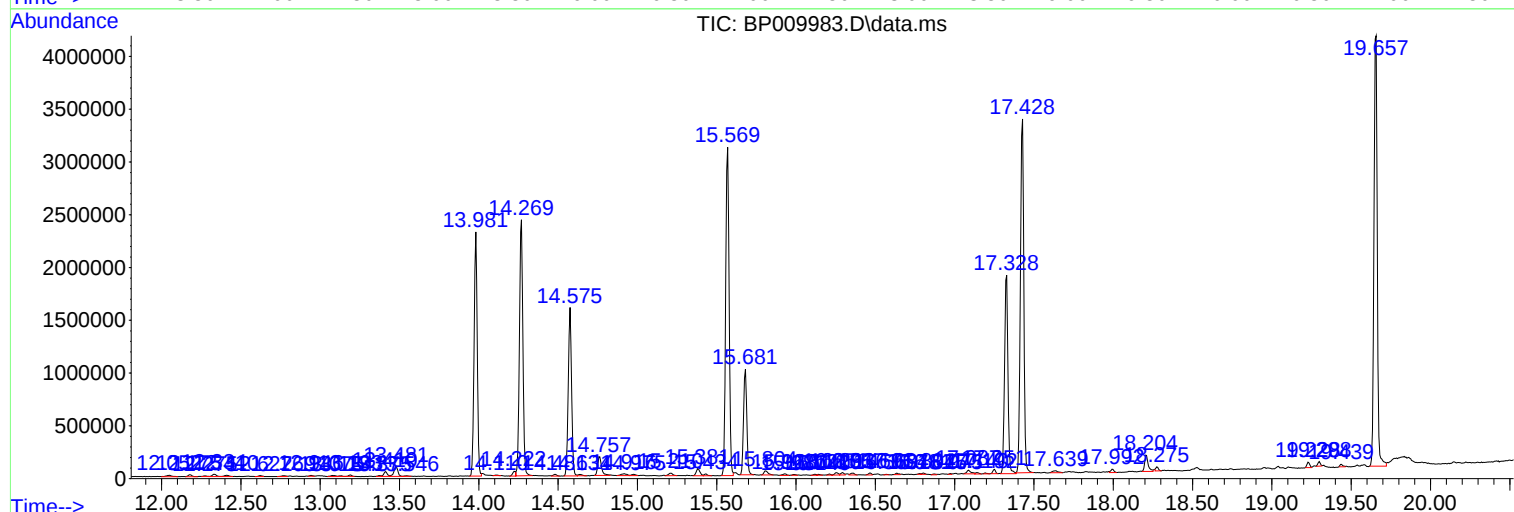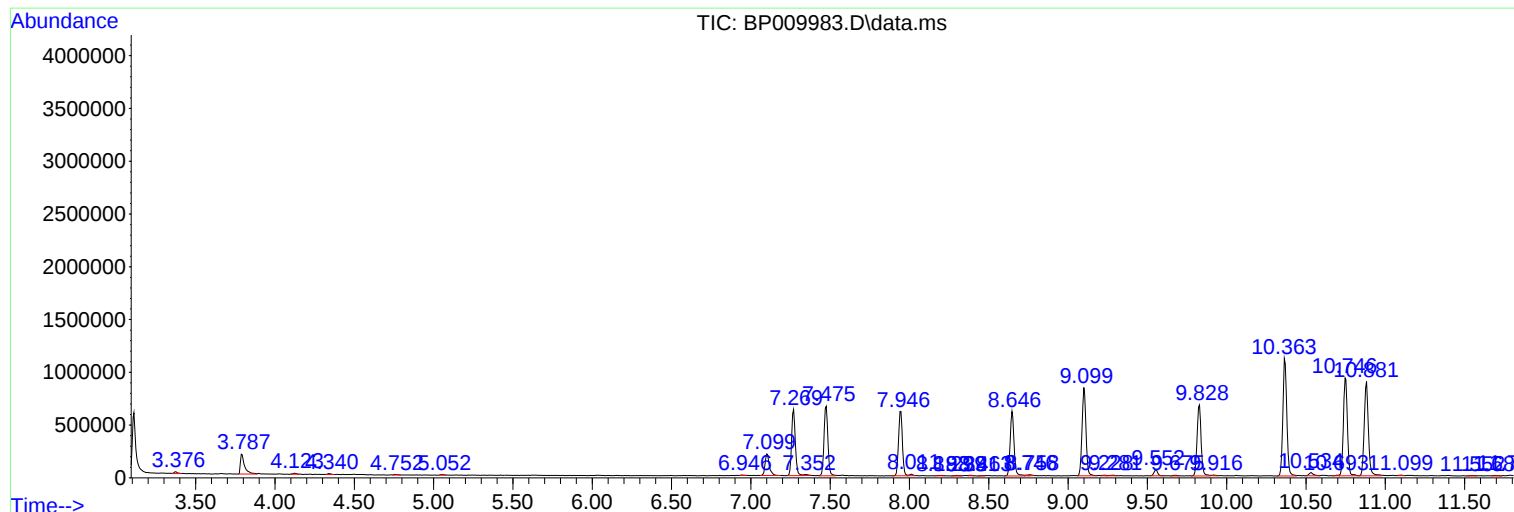

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009983.D
Acq On : 20 Apr 2022 18:57
Operator : CG/JU
Sample : N2472-10
Misc :
ALS Vial : 36 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0J10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.110	5.15 ng/ul	691843	Chrysene-d12		21.404	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	9-Tricosene, (Z)-		322	C23H46	027519-02-4	98
2	Cycloeicosane		280	C20H40	000296-56-0	98
3	1-Tetracosene		336	C24H48	010192-32-2	94
4	Pentacos-1-ene		350	C25H50	016980-85-1	94
5	Nonacos-1-ene		406	C29H58	018835-35-3	94

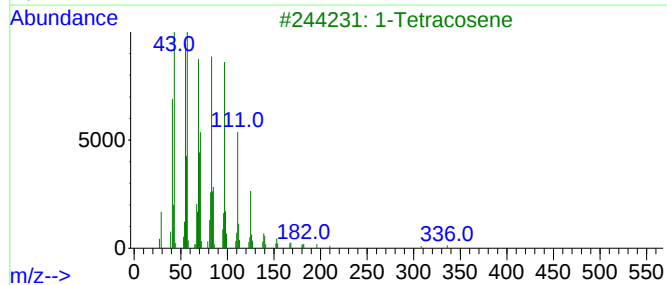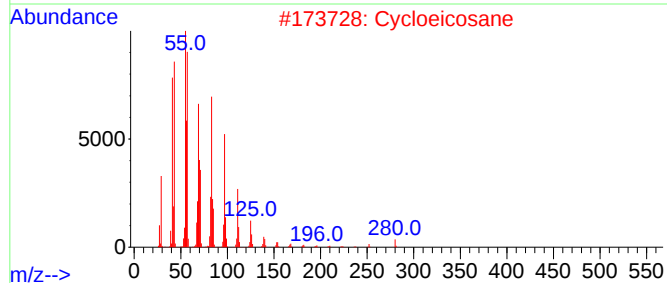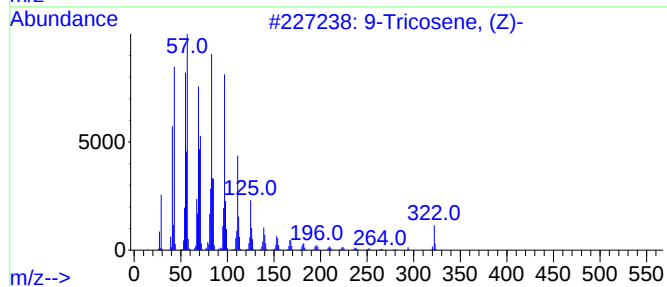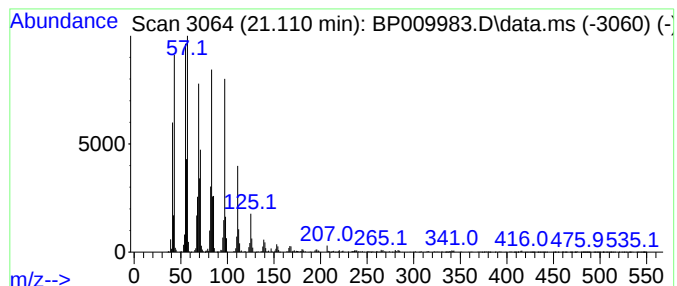

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009983.D
Acq On : 20 Apr 2022 18:57
Operator : CG/JU
Sample : N2472-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.110	5.2	ng/u1	691843	5	21.404	2685860	20.0