

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009987.D
 Acq On : 20 Apr 2022 21:12
 Operator : CG/JU
 Sample : N2472-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	54	rVB3	12556	16487	0.31%	0.042%
2	3.787	116	119	130	rBV	134744	226840	4.27%	0.579%
3	4.122	173	176	181	rVB3	9617	14345	0.27%	0.037%
4	5.046	328	333	343	rBV2	27966	46283	0.87%	0.118%
5	6.946	649	656	659	rBV8	3796	7758	0.15%	0.020%
6	7.105	677	683	691	rBV	69419	118117	2.22%	0.302%
7	7.269	704	711	722	rBV	448290	737028	13.87%	1.882%
8	7.475	739	746	757	rBV	260793	433494	8.16%	1.107%
9	7.940	817	825	834	rBV	444712	751760	14.15%	1.920%
10	8.010	836	837	844	rVB7	7901	8665	0.16%	0.022%
11	8.646	939	945	954	rBV	242869	410168	7.72%	1.048%
12	9.099	1014	1022	1034	rBV	611547	1048764	19.74%	2.678%
13	9.551	1089	1099	1105	rBV3	22961	40377	0.76%	0.103%
14	9.675	1114	1120	1126	rBV9	3372	5972	0.11%	0.015%
15	9.828	1139	1146	1156	rBV	265200	468976	8.83%	1.198%
16	9.922	1158	1162	1169	rVB10	4754	9779	0.18%	0.025%
17	10.369	1230	1238	1250	rBV	403638	703421	13.24%	1.796%
18	10.746	1295	1302	1317	rVB	657831	1148403	21.61%	2.933%
19	10.881	1317	1325	1337	rBV	621038	1125959	21.19%	2.876%
20	12.181	1540	1546	1550	rBV5	8077	12551	0.24%	0.032%
21	12.269	1556	1561	1568	rBV	59514	104792	1.97%	0.268%
22	12.334	1568	1572	1578	rVV2	14981	27346	0.51%	0.070%
23	12.410	1579	1585	1590	rVB7	5058	9415	0.18%	0.024%
24	12.616	1613	1620	1627	rBV10	5572	10841	0.20%	0.028%
25	12.775	1644	1647	1651	rBV6	4913	6896	0.13%	0.018%
26	13.092	1694	1701	1703	rBV8	4130	7638	0.14%	0.020%
27	13.410	1750	1755	1760	rVV3	18922	31118	0.59%	0.079%
28	13.451	1760	1762	1767	rVB4	5688	7493	0.14%	0.019%
29	13.981	1845	1852	1865	rBV	1712972	2383548	44.86%	6.087%
30	14.269	1892	1901	1914	rBV	1715442	2586760	48.68%	6.606%
31	14.481	1933	1937	1941	rVB7	3859	5485	0.10%	0.014%
32	14.575	1947	1953	1960	rBV	1157347	1686645	31.74%	4.307%
33	14.634	1962	1963	1968	rVB3	7942	7774	0.15%	0.020%
34	14.763	1979	1985	1999	rBV2	42256	94802	1.78%	0.242%
35	14.898	2004	2008	2010	rVV5	6303	8997	0.17%	0.023%
36	14.934	2010	2014	2018	rVV7	5474	11010	0.21%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009987.D
 Acq On : 20 Apr 2022 21:12
 Operator : CG/JU
 Sample : N2472-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	14.975	2018	2021	2029	rVB4	7492	13326	0.25%	0.034%
38	15.204	2056	2060	2067	rVB9	2930	5891	0.11%	0.015%
39	15.381	2084	2090	2097	rBV3	17941	33317	0.63%	0.085%
40	15.569	2114	2122	2129	rBV	2418640	3629956	68.31%	9.270%
41	15.681	2135	2141	2154	rVB	344875	505630	9.52%	1.291%
42	15.810	2158	2163	2173	rVB3	31176	53826	1.01%	0.137%
43	16.139	2214	2219	2222	rBV5	3045	5803	0.11%	0.015%
44	16.269	2235	2241	2242	rBV6	3260	5380	0.10%	0.014%
45	16.357	2249	2256	2258	rBV5	10928	14225	0.27%	0.036%
46	16.516	2275	2283	2287	rVB8	10127	15987	0.30%	0.041%
47	16.633	2298	2303	2308	rBV8	5945	10246	0.19%	0.026%
48	16.780	2321	2328	2332	rBV10	6886	11641	0.22%	0.030%
49	17.110	2380	2384	2392	rVB4	8345	19443	0.37%	0.050%
50	17.322	2414	2420	2431	rBV	1467374	2181968	41.06%	5.572%
51	17.422	2431	2437	2449	rVV	2952825	4351863	81.90%	11.114%
52	17.516	2449	2453	2458	rVB8	11435	20607	0.39%	0.053%
53	17.992	2532	2534	2538	rVB4	5864	6895	0.13%	0.018%
54	18.204	2567	2570	2576	rBV6	20394	27280	0.51%	0.070%
55	18.275	2576	2582	2588	rVB2	11960	20322	0.38%	0.052%
56	19.233	2740	2745	2749	rBV2	37786	55632	1.05%	0.142%
57	19.298	2752	2756	2760	rBV	39634	54741	1.03%	0.140%
58	19.651	2810	2816	2831	rBV	3895881	5313786	100.00%	13.571%
59	21.110	3060	3064	3073	rBV2	136494	191337	3.60%	0.489%
60	21.404	3109	3114	3131	rBV	1735769	2363618	44.48%	6.036%
61	23.704	3497	3505	3512	rBV	1981681	3949077	74.32%	10.085%
62	23.857	3524	3531	3543	rVB2	943010	1968655	37.05%	5.028%




Sum of corrected areas: 39156159

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009987.D
Acq On : 20 Apr 2022 21:12
Operator : CG/JU
Sample : N2472-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J29

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

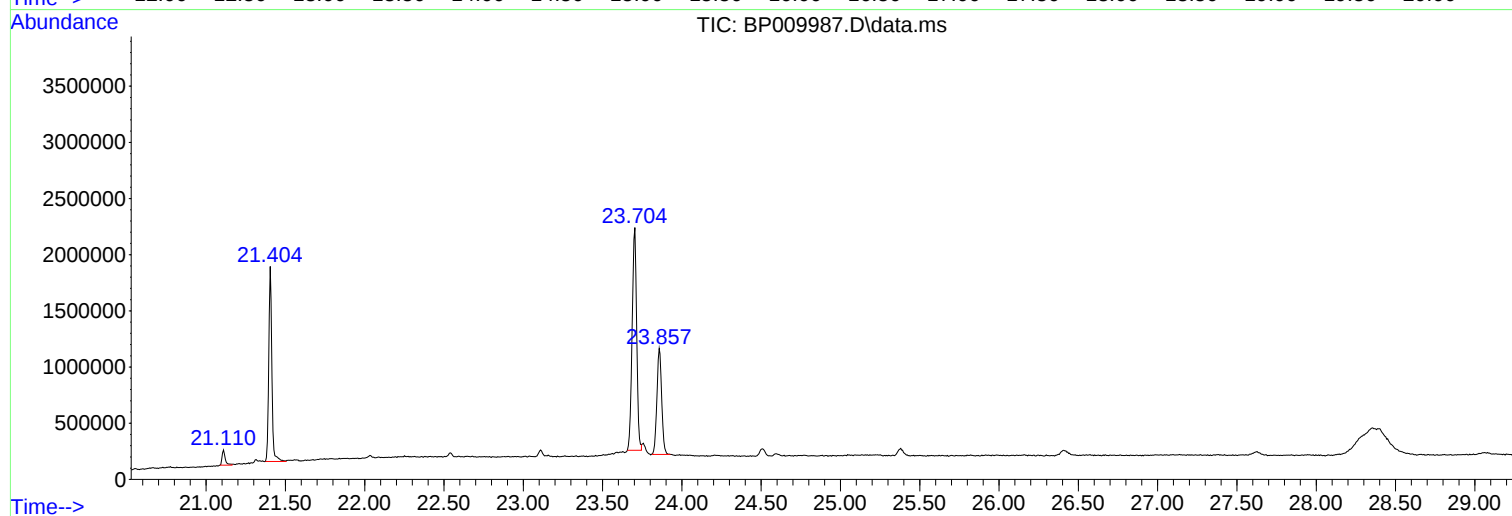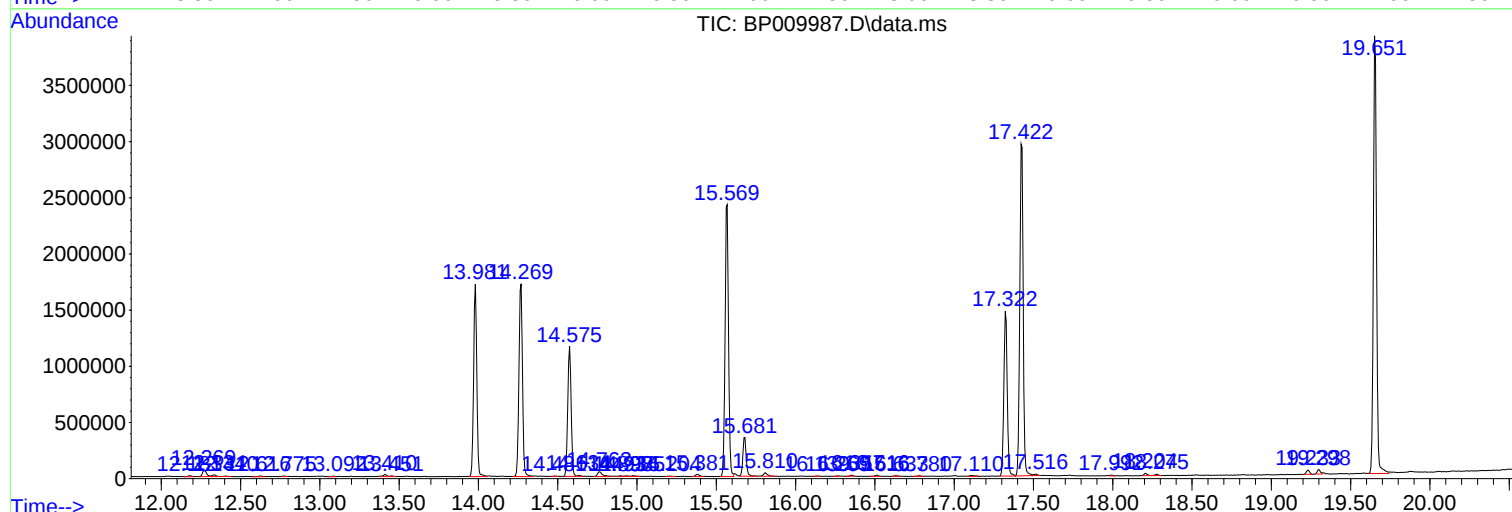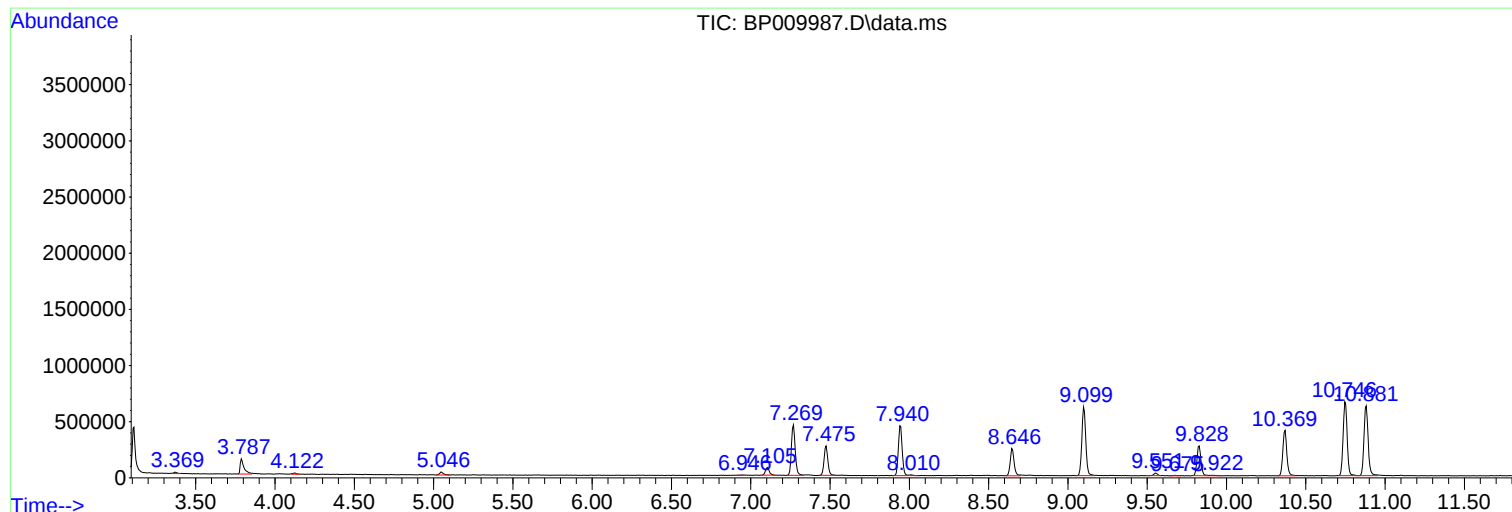

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009987.D
Acq On : 20 Apr 2022 21:12
Operator : CG/JU
Sample : N2472-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J29

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009987.D
Acq On : 20 Apr 2022 21:12
Operator : CG/JU
Sample : N2472-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J29

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc