

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009994.D
 Acq On : 21 Apr 2022 01:41
 Operator : CG/JU
 Sample : PB144243BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK243

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	45	48	55	rBV	33428	41965	0.91%	0.098%
2	3.781	115	118	139	rBV	381204	708096	15.29%	1.646%
3	4.122	173	176	186	rVB7	7915	13844	0.30%	0.032%
4	7.099	676	682	699	rVB	568745	947457	20.46%	2.202%
5	7.269	704	711	721	rVV	456525	735071	15.87%	1.709%
6	7.475	738	746	755	rBV	583809	968819	20.92%	2.252%
7	7.940	817	825	835	rBV	456642	762863	16.47%	1.773%
8	8.646	938	945	960	rBV	780730	1272566	27.48%	2.958%
9	9.099	1014	1022	1034	rBV	623765	1062043	22.93%	2.469%
10	9.822	1136	1145	1158	rBV	511712	899568	19.42%	2.091%
11	10.363	1229	1237	1250	rBV	761632	1327467	28.66%	3.086%
12	10.746	1295	1302	1314	rVB	695758	1193505	25.77%	2.774%
13	10.881	1316	1325	1340	rBV	768646	1391934	30.05%	3.236%
14	12.334	1567	1572	1577	rBV2	14594	26689	0.58%	0.062%
15	12.546	1604	1608	1611	rBV5	3034	5004	0.11%	0.012%
16	13.981	1845	1852	1864	rBV	1635712	2290097	49.45%	5.324%
17	14.269	1892	1901	1916	rBV	1618580	2539630	54.83%	5.904%
18	14.575	1946	1953	1964	rBV	1183770	1787662	38.60%	4.156%
19	14.757	1977	1984	2009	rBV	750803	1183495	25.55%	2.751%
20	14.987	2018	2023	2026	rBV7	3039	5483	0.12%	0.013%
21	15.563	2113	2121	2133	rBV	2198940	3307294	71.41%	7.688%
22	15.675	2133	2140	2151	rVV	748244	1062874	22.95%	2.471%
23	15.804	2157	2162	2169	rVB	24676	40223	0.87%	0.094%
24	16.351	2250	2255	2259	rBV7	9673	14516	0.31%	0.034%
25	17.004	2363	2366	2371	rBV7	4725	7815	0.17%	0.018%
26	17.110	2376	2384	2387	rBV6	6976	16315	0.35%	0.038%
27	17.322	2414	2420	2429	rBV	1564924	2278065	49.19%	5.296%
28	17.422	2430	2437	2451	rVV2	2537946	3754572	81.06%	8.728%
29	17.698	2482	2484	2490	rVB7	3424	5376	0.12%	0.012%
30	19.151	2729	2731	2734	rBV4	4161	4883	0.11%	0.011%
31	19.228	2740	2744	2751	rBV3	35156	49739	1.07%	0.116%
32	19.298	2751	2756	2763	rVV	31941	48272	1.04%	0.112%
33	19.580	2801	2804	2807	rBV5	5303	5757	0.12%	0.013%
34	19.651	2810	2816	2834	rBV	3503737	4631565	100.00%	10.767%
35	21.404	3108	3114	3126	rBV	1861304	2557575	55.22%	5.945%
36	23.698	3496	3504	3511	rBV2	1852549	3817519	82.42%	8.874%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009994.D
Acq On : 21 Apr 2022 01:41
Operator : CG/JU
Sample : PB144243BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK243

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION

37	23.857	3523	3531	3542	rVB2	1100791	2252375	48.63%	5.236%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 43017993

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009994.D
Acq On : 21 Apr 2022 01:41
Operator : CG/JU
Sample : PB144243BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK243

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

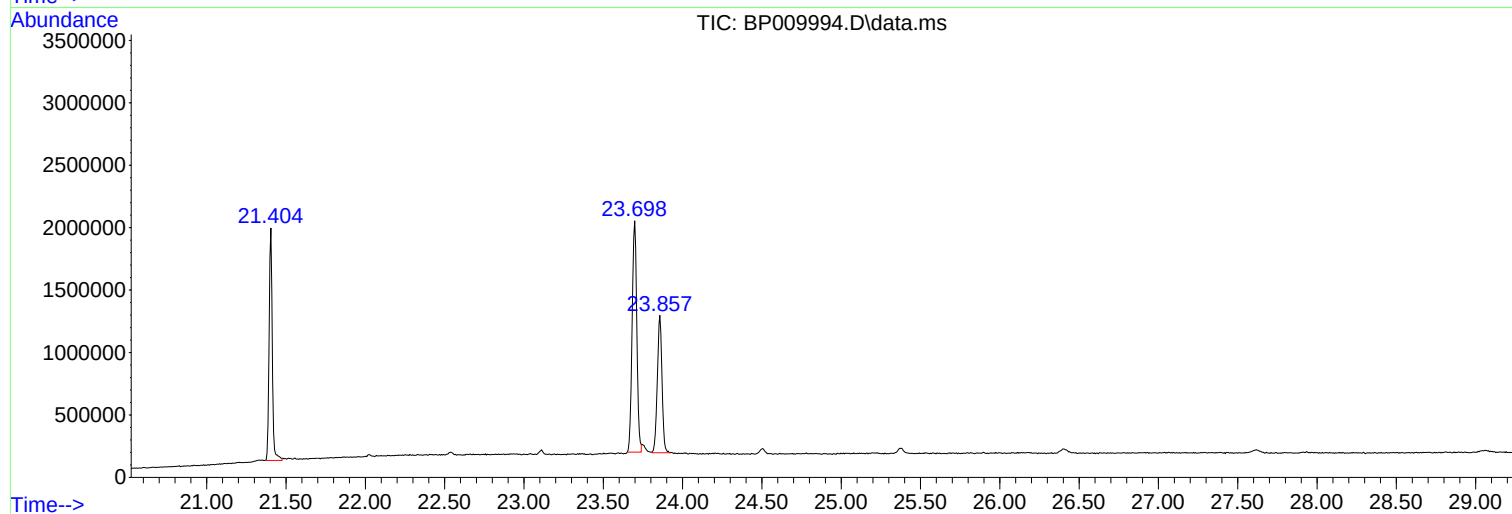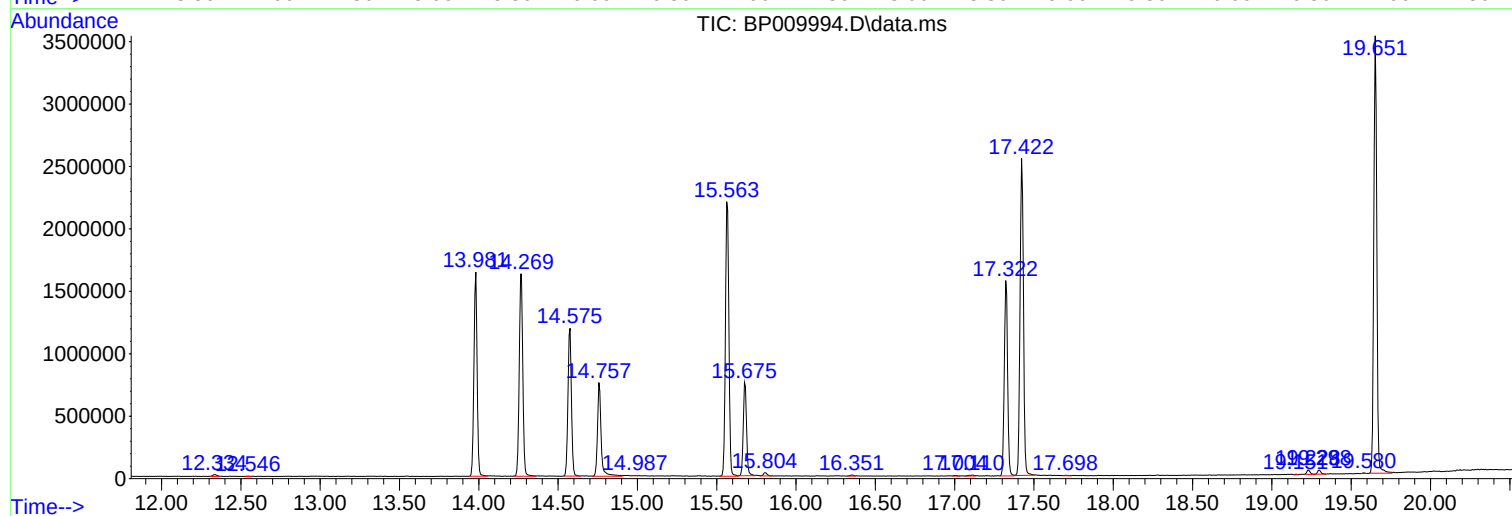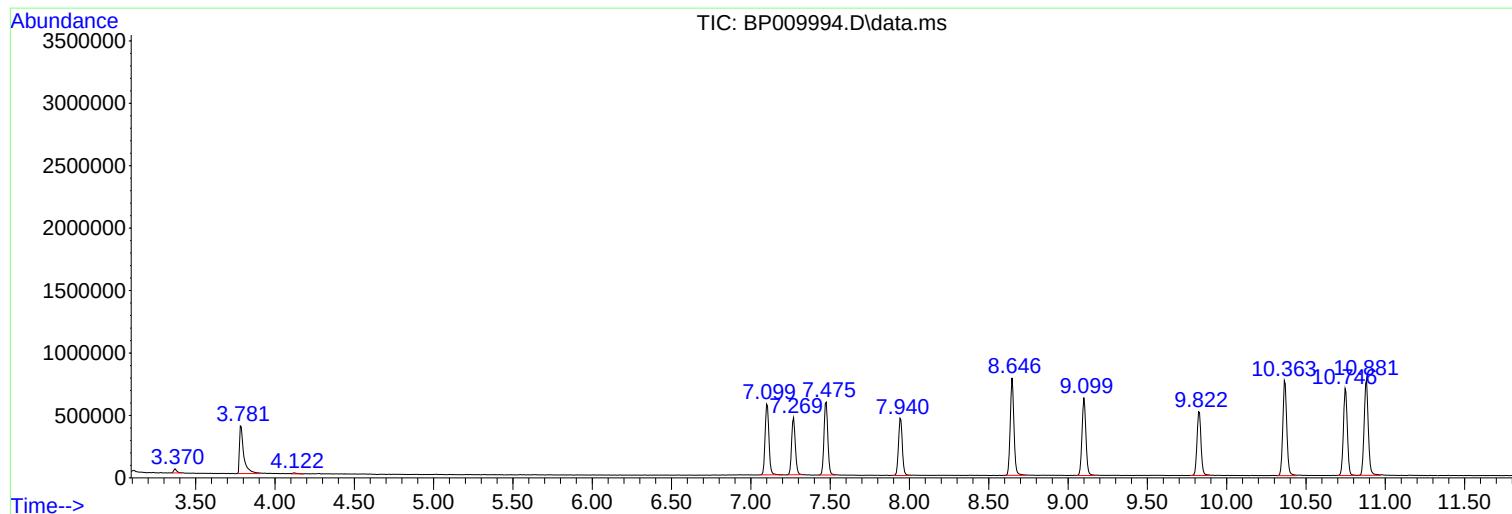

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009994.D
Acq On : 21 Apr 2022 01:41
Operator : CG/JU
Sample : PB144243BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK243

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009994.D
Acq On : 21 Apr 2022 01:41
Operator : CG/JU
Sample : PB144243BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK243

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc