

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009996.D
 Acq On : 21 Apr 2022 02:49
 Operator : CG/JU
 Sample : N2472-04
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	46	49	53	rVB3	10542	12160	0.22%	0.028%
2	3.799	118	121	136	rBV	65020	137428	2.50%	0.312%
3	4.128	173	177	182	rVB5	8182	14772	0.27%	0.034%
4	5.052	333	334	340	rVB6	4550	6350	0.12%	0.014%
5	7.099	676	682	695	rVB	120292	216428	3.93%	0.492%
6	7.269	703	711	722	rBV	523798	857453	15.57%	1.949%
7	7.352	722	725	730	rVB6	5170	9719	0.18%	0.022%
8	7.475	738	746	757	rBV	493424	828707	15.05%	1.883%
9	7.940	818	825	833	rBV	438461	739594	13.43%	1.681%
10	8.011	835	837	843	rVB5	8182	11887	0.22%	0.027%
11	8.305	881	887	890	rBV7	3504	6530	0.12%	0.015%
12	8.646	937	945	958	rBV	391755	658542	11.96%	1.497%
13	8.763	963	965	971	rVB7	4350	5938	0.11%	0.013%
14	9.099	1013	1022	1035	rBV	720664	1218010	22.11%	2.768%
15	9.269	1047	1051	1056	rVB8	2802	5754	0.10%	0.013%
16	9.552	1092	1099	1107	rVB	33007	53786	0.98%	0.122%
17	9.822	1138	1145	1169	rBV	556100	983147	17.85%	2.234%
18	10.363	1228	1237	1251	rBV	769426	1334713	24.23%	3.033%
19	10.746	1294	1302	1316	rVB	652097	1148466	20.85%	2.610%
20	10.881	1317	1325	1342	rBV	679578	1245514	22.61%	2.830%
21	12.181	1539	1546	1551	rVB3	14348	22942	0.42%	0.052%
22	12.328	1564	1571	1577	rBV	18666	34545	0.63%	0.079%
23	12.404	1580	1584	1589	rVB6	5377	8924	0.16%	0.020%
24	12.628	1615	1622	1625	rBV7	4649	8971	0.16%	0.020%
25	12.769	1640	1646	1651	rBV10	4966	11057	0.20%	0.025%
26	12.863	1658	1662	1668	rVB9	4144	5814	0.11%	0.013%
27	12.993	1680	1684	1686	rBV5	3859	6140	0.11%	0.014%
28	13.069	1694	1697	1703	rVB7	5148	9489	0.17%	0.022%
29	13.122	1703	1706	1711	rBV6	4854	7936	0.14%	0.018%
30	13.199	1713	1719	1725	rVB10	6584	13266	0.24%	0.030%
31	13.381	1743	1750	1751	rBV6	8477	12159	0.22%	0.028%
32	13.410	1751	1755	1759	rVB2	26174	35379	0.64%	0.080%
33	13.851	1826	1830	1833	rBV6	7205	11289	0.20%	0.026%
34	13.981	1845	1852	1864	rVV	1884622	2692053	48.88%	6.118%
35	14.110	1870	1874	1881	rVB9	8073	16445	0.30%	0.037%
36	14.269	1892	1901	1914	rBV	1934495	2976303	54.04%	6.764%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP009996.D
 Acq On : 21 Apr 2022 02:49
 Operator : CG/JU
 Sample : N2472-04
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	14.416	1922	1926	1931	rVB7	12861	25256	0.46%	0.057%
38	14.481	1933	1937	1942	rBV7	10474	16549	0.30%	0.038%
39	14.575	1944	1953	1962	rBV	1143741	1772935	32.19%	4.029%
40	14.757	1979	1984	1992	rBV	117814	206431	3.75%	0.469%
41	15.369	2085	2088	2094	rBV8	24143	45266	0.82%	0.103%
42	15.563	2115	2121	2128	rBV	2565002	3876375	70.38%	8.809%
43	15.675	2135	2140	2148	rBV	924852	1309177	23.77%	2.975%
44	15.804	2158	2162	2165	rBV3	35615	60703	1.10%	0.138%
45	16.316	2247	2249	2253	rVB2	37432	43494	0.79%	0.099%
46	17.322	2415	2420	2430	rBV	1407248	2052307	37.26%	4.664%
47	17.422	2431	2437	2448	rVB2	3116671	4501163	81.72%	10.229%
48	19.651	2811	2816	2827	rBV	4070835	5507808	100.00%	12.516%
49	21.110	3060	3064	3070	rBV	142348	188139	3.42%	0.428%
50	21.404	3108	3114	3127	rVB	1484461	2168653	39.37%	4.928%
51	22.533	3303	3306	3313	rVB	80370	118252	2.15%	0.269%
52	23.110	3400	3404	3409	rVB	87640	137741	2.50%	0.313%
53	23.698	3496	3504	3511	rBV2	2168078	4466369	81.09%	10.150%
54	23.851	3523	3530	3547	rVB2	918832	1951324	35.43%	4.434%
55	24.504	3636	3641	3649	rVB2	90298	189749	3.45%	0.431%




Sum of corrected areas: 44005301

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009996.D
Acq On : 21 Apr 2022 02:49
Operator : CG/JU
Sample : N2472-04
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

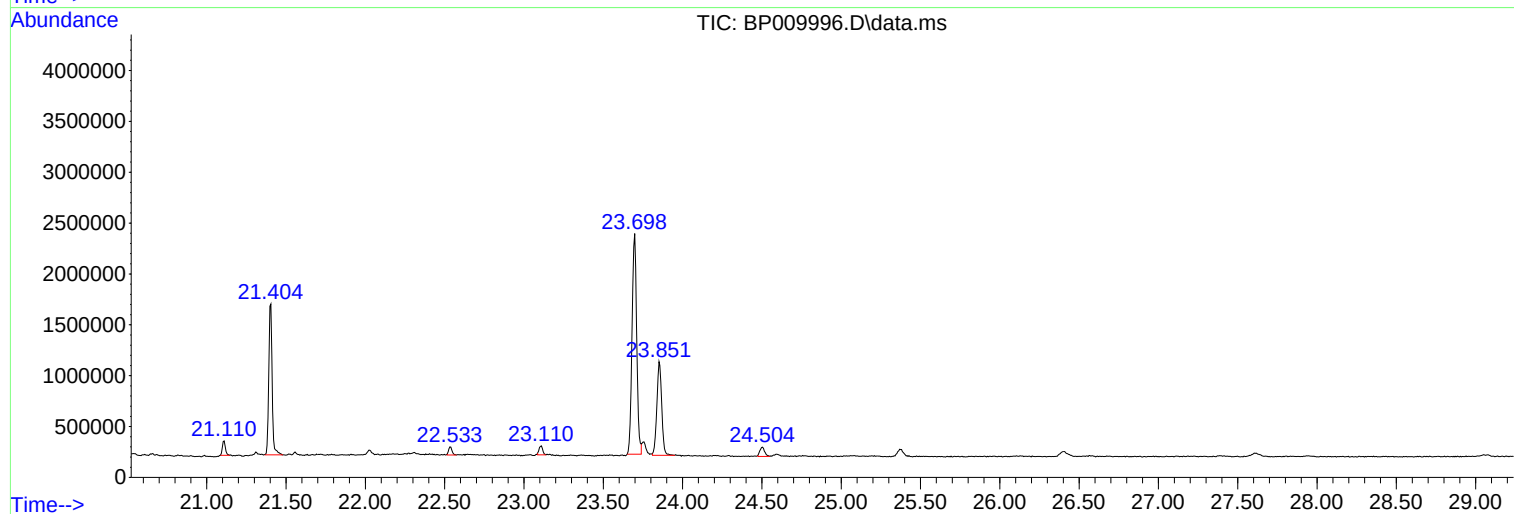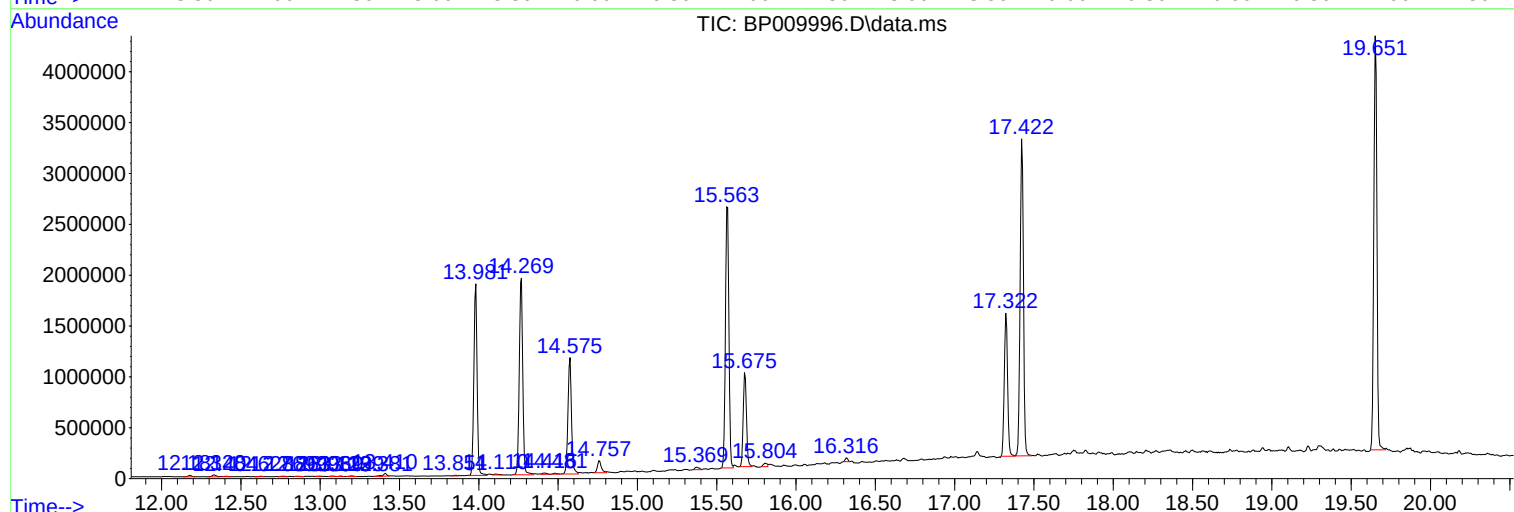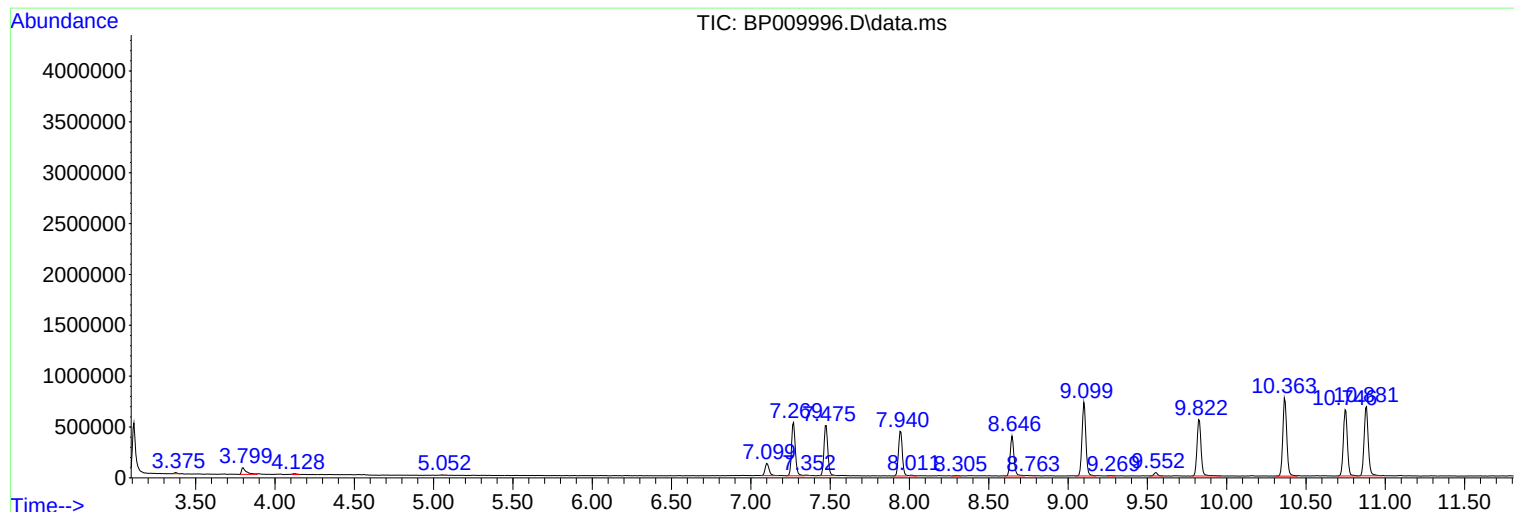

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009996.D
Acq On : 21 Apr 2022 02:49
Operator : CG/JU
Sample : N2472-04
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP009996.D
Acq On : 21 Apr 2022 02:49
Operator : CG/JU
Sample : N2472-04
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc